

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062615\
 Data File : BF080195.D
 Acq On : 26 Jun 2015 18:00
 Operator : TP/IZ
 Sample : G2785-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-6

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	209	212	218	rBV	29008	37349	3.08%	0.574%
2	5.899	244	246	249	rBV	360024	314253	25.90%	4.828%
3	6.893	331	333	336	rBV	251796	204910	16.89%	3.148%
4	7.064	345	348	350	rBV	430298	572292	47.17%	8.792%
5	7.293	366	368	371	rVB	208372	172932	14.25%	2.657%
6	7.453	380	382	384	rBV	741453	586132	48.31%	9.005%
7	7.853	415	417	419	rBV	504038	451840	37.24%	6.942%
8	8.585	479	481	484	rBV	280687	226646	18.68%	3.482%
9	9.659	573	575	578	rBV	1157642	950666	78.36%	14.605%
10	10.356	634	636	639	rBV	314293	263402	21.71%	4.047%
11	11.145	703	705	708	rBV2	509826	547114	45.09%	8.405%
12	11.853	765	767	770	rBV	222763	278338	22.94%	4.276%
13	13.522	910	913	915	rBV	1391246	1213262	100.00%	18.639%
14	14.768	1019	1022	1024	rBV	266096	330162	27.21%	5.072%
15	16.608	1179	1183	1187	rBV	206645	317824	26.20%	4.883%
16	18.163	1313	1319	1328	rVB5	8337	42130	3.47%	0.647%


Sum of corrected areas: 6509252

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062615\
Data File : BF080195.D
Acq On : 26 Jun 2015 18:00
Operator : TP/IZ
Sample : G2785-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-6

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

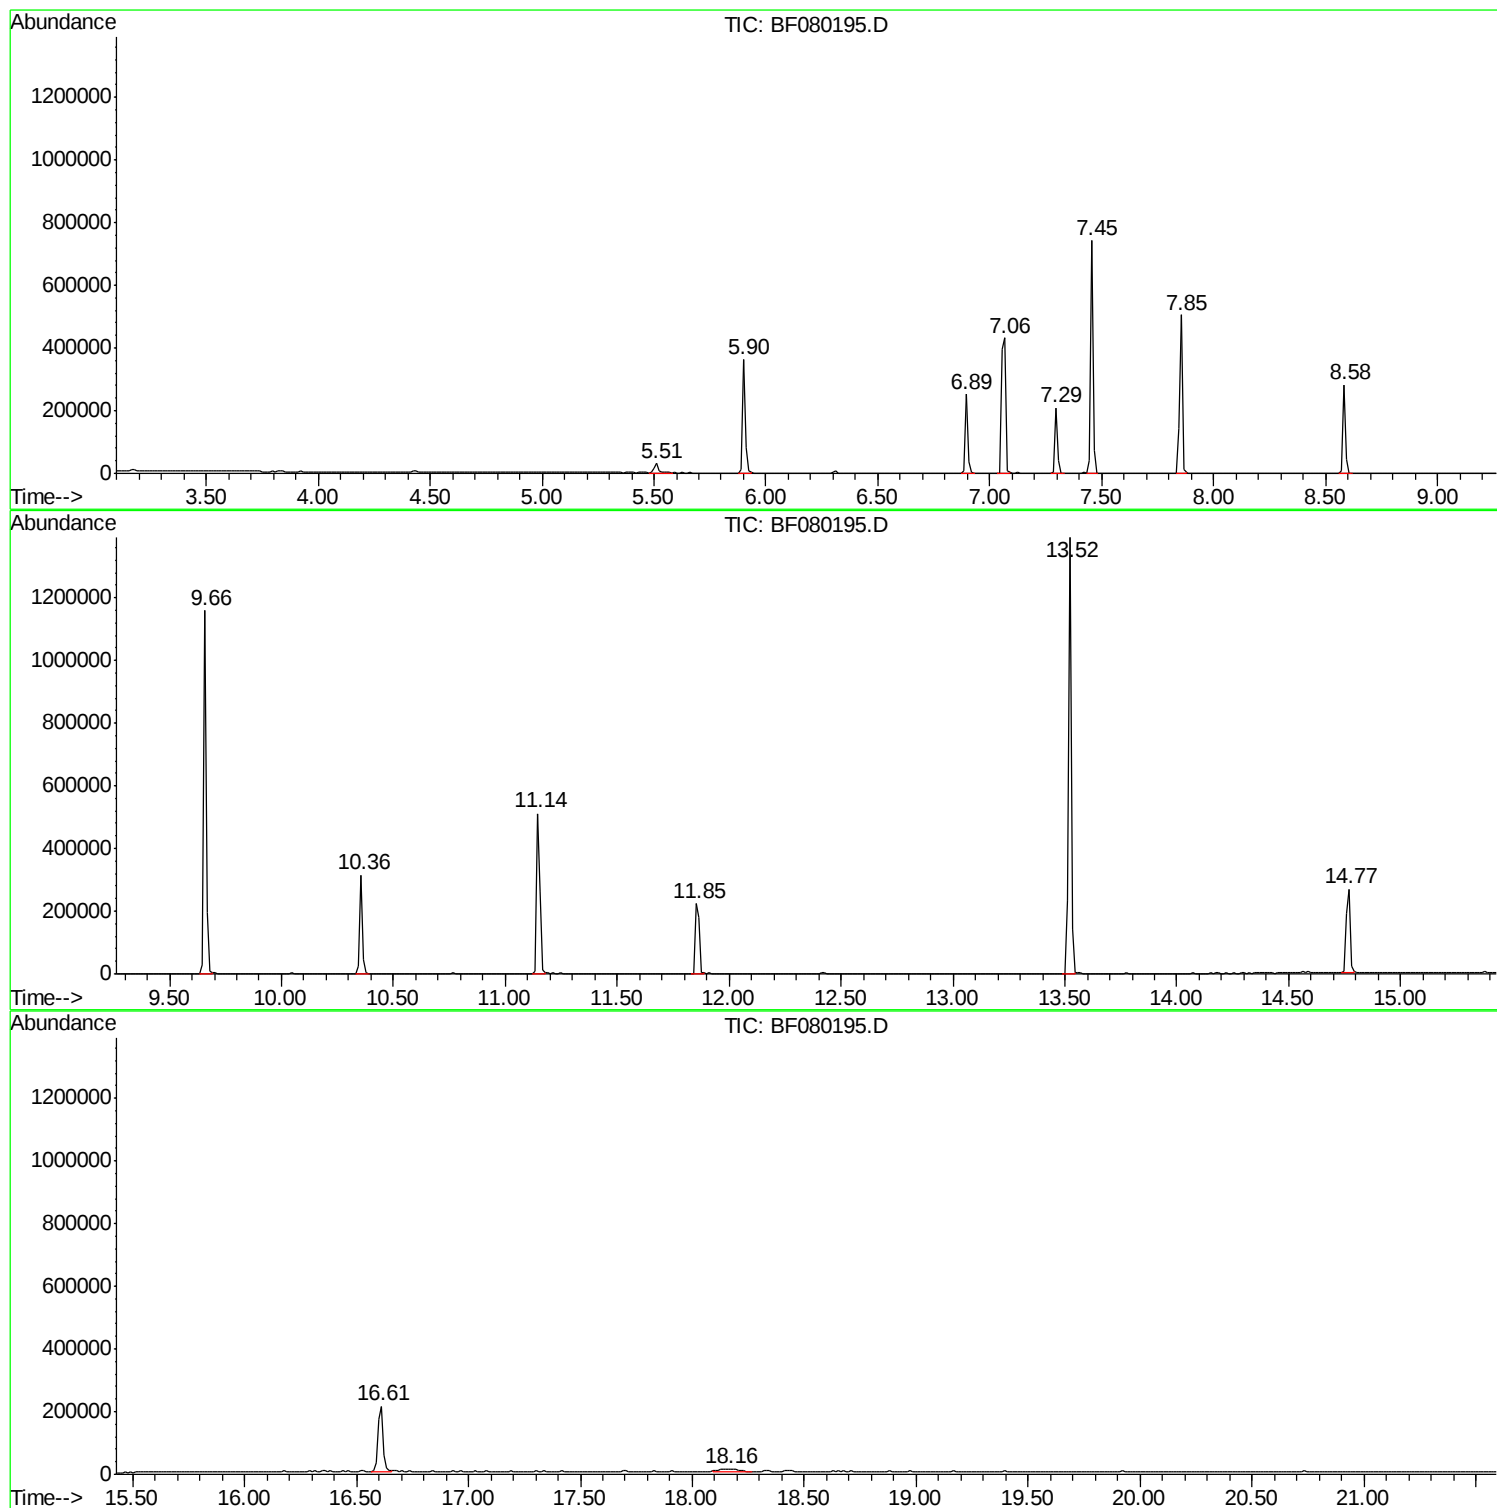

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062615\
Data File : BF080195.D
Acq On : 26 Jun 2015 18:00
Operator : TP/IZ
Sample : G2785-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-6










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.51	4.32 ng	37349	1,4-Dichlorobenzene-d4	7.29

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	42	
2	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	9	
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	7	
4	4-Penten-2-one, 4-methyl-	98	C6H10O	003744-02-3	7	
5	Guanidine	59	CH5N3	000113-00-8	5	

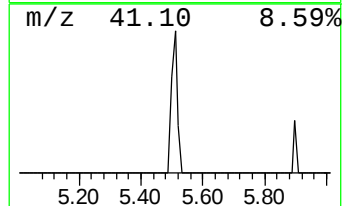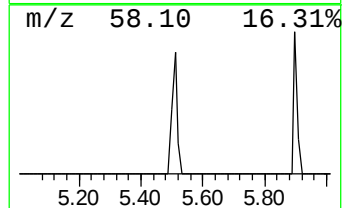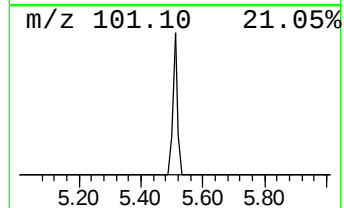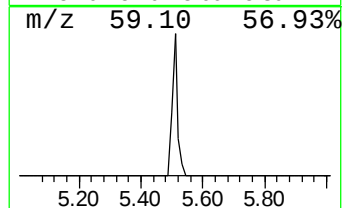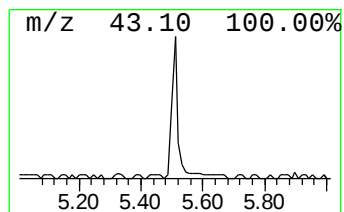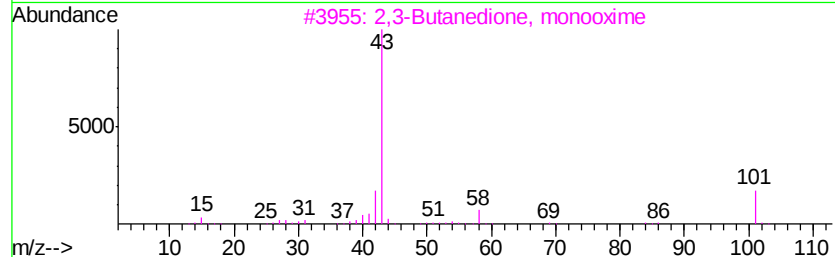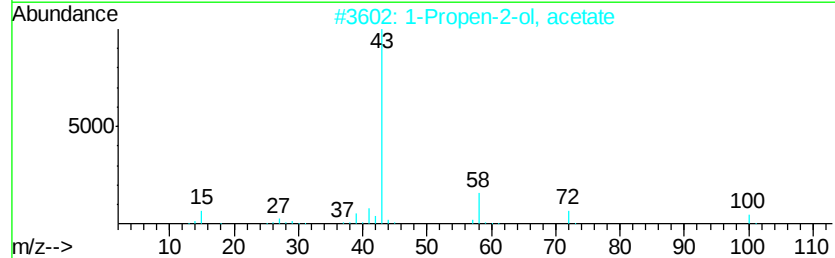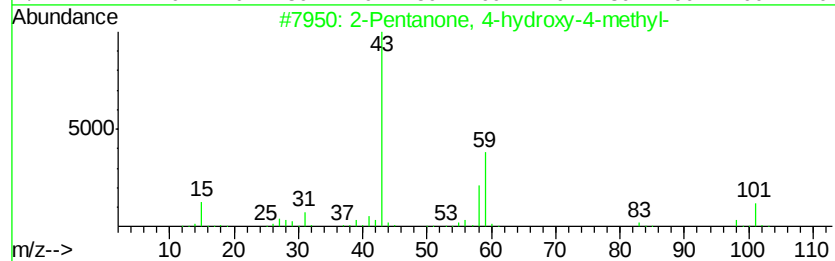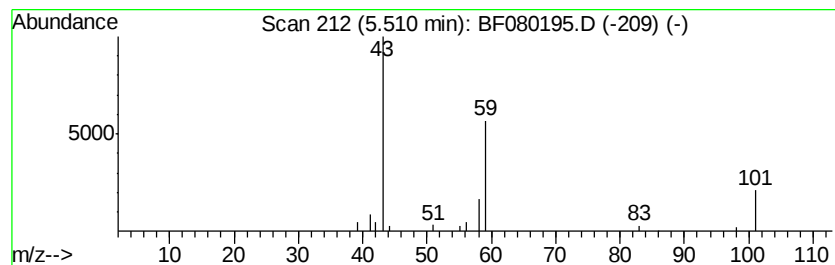

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062615\
Data File : BF080195.D
Acq On : 26 Jun 2015 18:00
Operator : TP/IZ
Sample : G2785-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-6










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 3-Chloro-6-fluoro-pyrazine Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.06	66.19 ng	572292	1,4-Dichlorobenzene-d4	7.29

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	52
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	40
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	37
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9

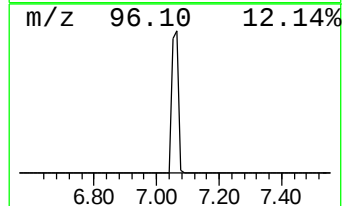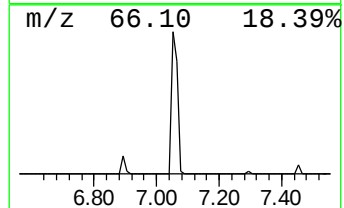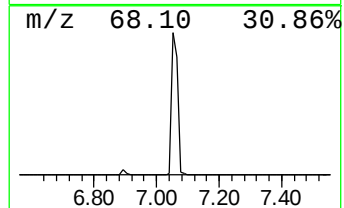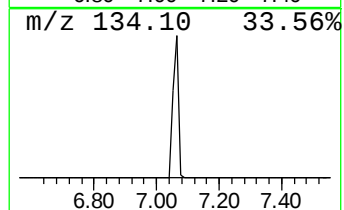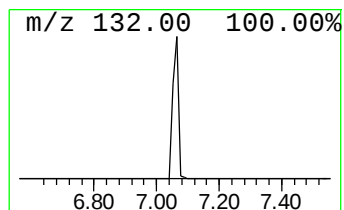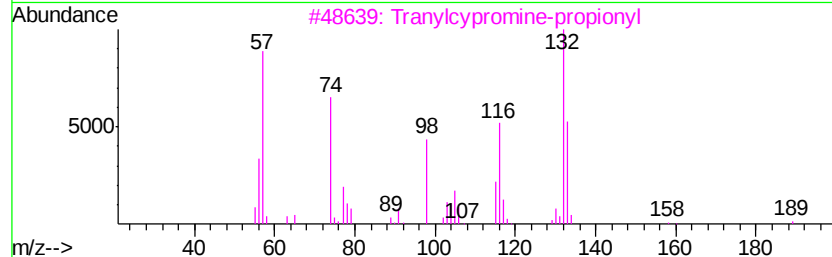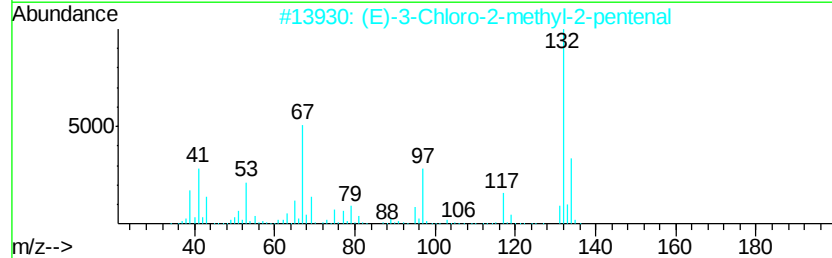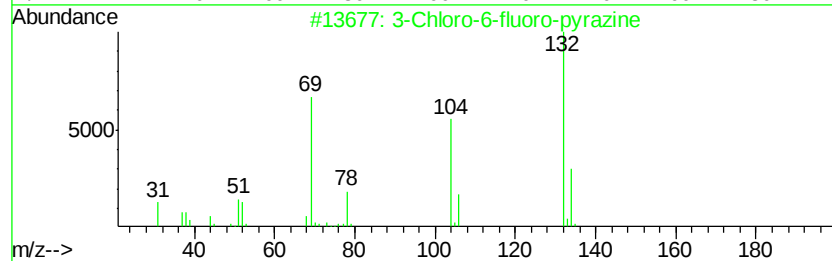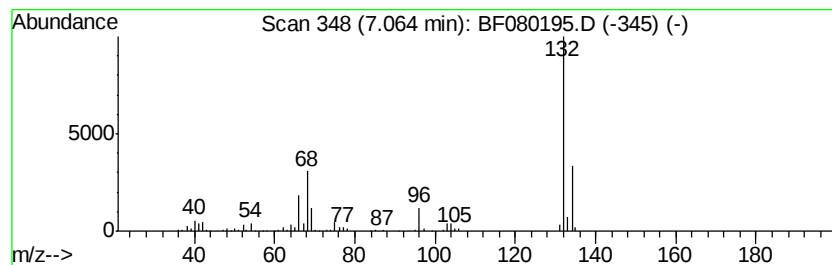

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062615\
Data File : BF080195.D
Acq On : 26 Jun 2015 18:00
Operator : TP/IZ
Sample : G2785-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-6

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.51	4.3	ng	37349	1	7.29	172932	20.0
3-Chloro-6-fluoro...	7.06	66.2	ng	572292	1	7.29	172932	20.0