


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062615\
 Data File : BF080185.D
 Acq On : 26 Jun 2015 9:03
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 23 00:53:56 2015

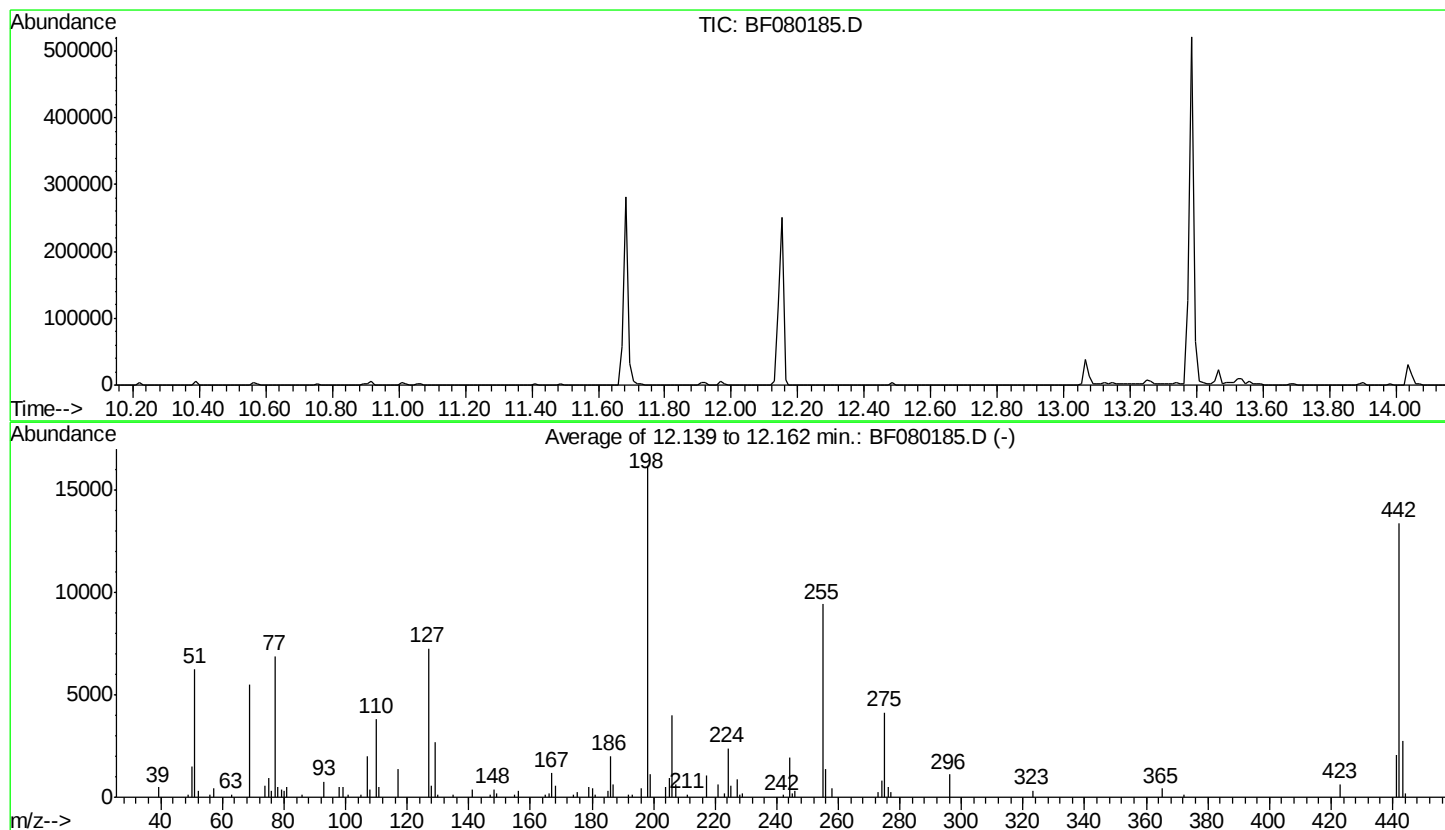

AutoFind: Scans 792, 793, 794; Background Corrected with Scan 789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	6280	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.8	5478	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.9	7275	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16189	PASS
199	198	5	9	7.0	1138	PASS
275	198	10	60	25.5	4135	PASS
365	198	1	100	2.6	420	PASS
441	442	0.01	24	15.4	2061	PASS
442	198	50	100	82.7	13385	PASS
443	442	15	24	20.5	2739	PASS