


Data Path : Z:\HPCHEM1\BNA F\DATA\BF062616\
 Data File : BF088411.D
 Acq On : 26 Jun 2016 11:38
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 27 19:14:18 2016

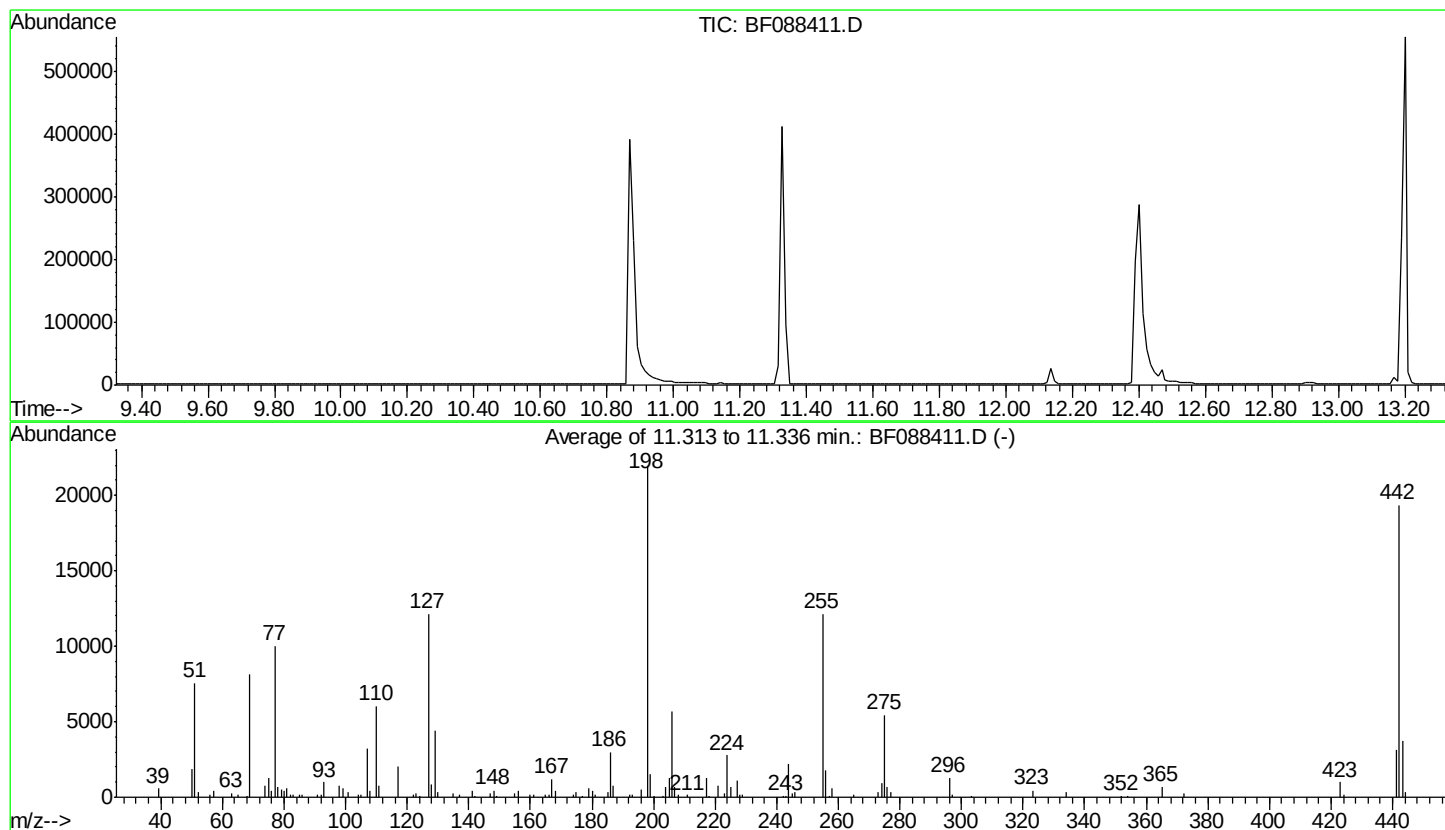

AutoFind: Scans 851, 852, 853; Background Corrected with Scan 848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	7562	PASS
68	69	0.00	2	1.5	118	PASS
69	198	0.00	100	37.0	8129	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.3	12136	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21961	PASS
199	198	5	9	7.0	1539	PASS
275	198	10	60	24.7	5427	PASS
365	198	1	100	3.2	692	PASS
441	442	0.01	24	16.3	3152	PASS
442	198	50	100	88.1	19348	PASS
443	442	15	24	19.1	3697	PASS