

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062619\
 Data File : BF115212.D
 Acq On : 26 Jun 2019 10:41
 Operator : HP/JU
 Sample : K3309-03DL 25X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jun 26 12:13:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 24 04:21:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.61	152	226313	20.00	ng	0.00
21) Naphthalene-d8	7.89	136	902952	20.00	ng	-0.01
39) Acenaphthene-d10	9.64	164	446341	20.00	ng	-0.01
64) Phenanthrene-d10	11.11	188	897944	20.00	ng	-0.01
76) Chrysene-d12	13.72	240	734831	20.00	ng	-0.02
87) Perylene-d12	15.09	264	681506	20.00	ng	-0.02


System Monitoring Compounds

5) 2-Fluorophenol	5.20	112	41452	2.83	ng	0.00
7) Phenol-d6	6.24	99	33647	1.89	ng	-0.02
23) Nitrobenzene-d5	7.17	82	64709	4.41	ng	-0.02
42) 2,4,6-Tribromophenol	10.41	330	30428	6.46	ng	-0.02
45) 2-Fluorobiphenyl	8.97	172	142353	5.42	ng	-0.02
79) Terphenyl-d14	12.68	244	144966	4.19	ng	-0.02

Target Compounds

						Qvalue
2) 1,4-Dioxane	2.20	88	1311262	189.452	ng	99
4) n-Nitrosodimethylamine	2.81	42	71797	9.388	ng	# 1
6) Aniline	6.34	93	269272	11.007	ng	# 57
10) Phenol	6.25	94	154210	7.396	ng	84
11) bis(2-Chloroethyl)ether	6.34	93	269272	17.519	ng	99
12) 1,3-Dichlorobenzene	6.62	146	47909	2.618	ng	97
14) 1,2-Dichlorobenzene	6.78	146	217825	12.817	ng	97
15) Benzyl Alcohol	6.87	79	84406	6.512	ng	# 1
16) 2,2'-oxybis(1-Chloropropan	6.84	45	67666	3.035	ng	75
17) 2-Methylphenol	6.87	107	209160	15.366	ng	100
19) n-Nitroso-di-n-propylamine	7.11	70	69154	6.068	ng	# 33
20) 3+4-Methylphenols	7.03	107	1276783	81.235	ng	# 65
27) 2,4-Dimethylphenol	7.57	122	570709	43.648	ng	# 92
32) Benzoic acid	7.70	122	978698	104.861	ng	# 14
36) 4-Chloro-3-methylphenol	8.45	107	29295	2.144	ng	# 19
51) 2,6-Dinitrotoluene	9.64	165	60335	7.958	ng	# 31
54) 2,4-Dinitrophenol	9.79	184	470	7.453	ng	# 60
57) 2,4-Dinitrotoluene	9.64	165	60335	6.164	ng	# 32
58) Fluorene	10.17	166	139	Below Cal	#	96
65) 4,6-Dinitro-2-methylphenol	10.42	198	440	5.042	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

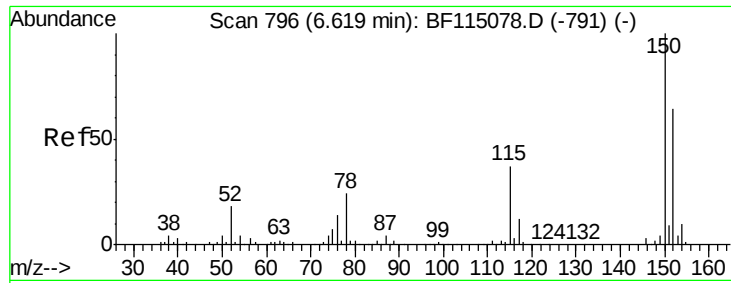


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.61 min Scan# 795
Delta R.T. -0.01 min
Lab File: BF115212.D
Acq: 26 Jun 2019 10:41

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 226313
Ion Ratio Lower Upper
152 100
150 152.6 124.2 186.2
115 55.3 46.1 69.1




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E





#2


1,4-Dioxane
Concen: 189.452 ng
RT: 2.20 min Scan# 44
Delta R.T. -0.00 min
Lab File: BF115212.D
Acq: 26 Jun 2019 10:41

Tgt Ion: 88 Resp: 1311262
Ion Ratio Lower Upper
88 100
58 69.3 56.1 84.1
43 26.2 21.3 31.9



Abundance Ion 88.00 (87.70 to 88.70): BF1
Ion 58.00 (57.70 to 58.70): BF1
Ion 43.00 (42.70 to 43.70): BF1









#4

n-Nitrosodimethylamine
 Concen: 9.388 ng
 RT: 2.81 min Scan# 148
 Delta R.T. 0.01 min
 Lab File: BF115212.D
 Acq: 26 Jun 2019 10:41

Instrument :
 BNA_F
 ClientSampled :




Tot Ion	Ratio	Lower	Upper
42	100		
74	0.0	116.6	175.0#
44	38.7	5.3	7.9#




#5

2-Fluorophenol
 Concen: 2.827 ng
 RT: 5.20 min Scan# 555
 Delta R.T. -0.01 min
 Lab File: BF115212.D
 Acq: 26 Jun 2019 10:41

Tgt Ion	Ratio	Lower	Upper
112	100		
64	54.1	43.8	65.6
63	24.1	22.2	33.4





#6

Aniline

Concen: 11.007 ng

RT: 6.34 min Scan# 749

Delta R.T. 0.06 min

Lab File: BF115212.D

Acq: 26 Jun 2019 10:41

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 93 Resp: 269272

Ion Ratio Lower Upper

93 100

66 0.6 30.0 45.0#




65 23.2 15.6 23.4



Abundance Ion 93.00 (92.70 to 93.70): BF1

Ion 66.00 (65.70 to 66.70): BF1

Ion 65.00 (64.70 to 65.70): BF1



#7

Phenol-d6

Concen: 1.890 ng

RT: 6.24 min Scan# 731

Delta R.T. -0.02 min

Lab File: BF115212.D

Acq: 26 Jun 2019 10:41


Tgt Ion: 99 Resp: 33647

Ion Ratio Lower Upper

99 100

42 22.8 13.6 20.4#



71 33.0 25.5 38.3




Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1





#10

Phenol

Concen: 7.396 ng

RT: 6.25 min Scan# 734

Delta R.T. -0.01 min

Lab File: BF115212.D

Acq: 26 Jun 2019 10:41

Instrument :

BNA_F

ClientSampled :


Tot Ion: 94 Resp: 154210

Ion Ratio Lower Upper




94 100

65 26.0 11.9 51.9

66 32.7 25.2 65.2



Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1



#11

bis(2-Chloroethyl)ether

Concen: 17.519 ng

RT: 6.34 min Scan# 749

Delta R.T. -0.02 min

Lab File: BF115212.D

Acq: 26 Jun 2019 10:41


Tgt Ion: 93 Resp: 269272

Ion Ratio Lower Upper



93 100


63 72.5 51.5 91.5

95 32.7 13.4 53.4



Abundance Ion 93.00 (92.70 to 93.70): BF1
Ion 63.00 (62.70 to 63.70): BF1
Ion 95.00 (94.70 to 95.70): BF1





#12

1,3-Dichlorobenzene

Concen: 2.618 ng

RT: 6.62 min Scan# 797

Delta R.T. 0.06 min

Lab File: BF115212.D

Acq: 26 Jun 2019 10:41

Instrument :

BNA_F

ClientSampleId :


Tot Ion:146 Resp: 47909

Ion Ratio Lower Upper

146 100

148 64.9 52.6 78.8




75 31.5 22.6 34.0



Abundance Ion 146.00 (145.70 to 146.70): E

Ion 148.00 (147.70 to 148.70): E

Ion 75.00 (74.70 to 75.70): BF1



#14

1,2-Dichlorobenzene

Concen: 12.817 ng

RT: 6.78 min Scan# 823

Delta R.T. -0.01 min

Lab File: BF115212.D

Acq: 26 Jun 2019 10:41


Tgt Ion:146 Resp: 217825

Ion Ratio Lower Upper

146 100

148 64.2 51.1 76.7



111 45.4 33.2 49.8






Abundance Ion 146.00 (145.70 to 146.70): E

Ion 148.00 (147.70 to 148.70): E

Ion 111.00 (110.70 to 111.70): E





#15

Benzyl Alcohol

Concen: 6.512 ng

RT: 6.87 min Scan# 839

Delta R.T. 0.11 min

Lab File: BF115212.D

Acq: 26 Jun 2019 10:41

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 79 Resp: 84406

Ion Ratio Lower Upper

79 100

108 281.8 68.7 103.1#

77 103.5 51.7 77.5#



#16

2,2'-oxybis(1-Chloropropane)

Concen: 3.035 ng

RT: 6.84 min Scan# 833

Delta R.T. -0.07 min

Lab File: BF115212.D

Acq: 26 Jun 2019 10:41


Tgt Ion: 45 Resp: 67666


Ion Ratio Lower Upper

45 100

77 3.2 0.0 34.6

79 3.3 0.0 31.2









#17
2-Methylphenol
Concen: 15.366 ng
RT: 6.87 min Scan# 839
Delta R.T. -0.01 min
Lab File: BF115212.D
Acq: 26 Jun 2019 10:41




Instrument :
BNA_F
ClientSampleId :


Tot Ion:107 Resp: 209160
Ion Ratio Lower Upper
107 100
108 113.3 90.9 136.3
77 41.6 33.4 50.2
79 40.2 32.3 48.5



#19
n-Nitroso-di-n-propylamine
Concen: 6.068 ng
RT: 7.11 min Scan# 879
Delta R.T. 0.06 min
Lab File: BF115212.D
Acq: 26 Jun 2019 10:41

Tgt Ion: 70 Resp: 69154
Ion Ratio Lower Upper
70 100
42 96.8 42.6 63.8#
101 61.5 8.0 12.0#
130 0.0 19.4 29.0#









#20
3+4-Methylphenols
Concen: 81.235 ng
RT: 7.03 min Scan# 866
Delta R.T. -0.01 min
Lab File: BF115212.D
Acq: 26 Jun 2019 10:41

Instrument :
BNA_F
ClientSampleId :

Tot Ion:107 Resp: 1276783
Ion Ratio Lower Upper
107 100
108 88.4 75.5 115.5
77 30.7 80.2 120.2#
79 25.4 9.5 49.5




Abundance Ion 107.00 (106.70 to 107.70): E
Ion 108.00 (107.70 to 108.70): E
Ion 77.00 (76.70 to 77.70): BF1
Ion 79.00 (78.70 to 79.70): BF1






#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.89 min Scan# 1012
Delta R.T. -0.01 min
Lab File: BF115212.D
Acq: 26 Jun 2019 10:41

Tgt Ion:136 Resp: 902952
Ion Ratio Lower Upper
136 100
137 11.6 8.9 13.3
54 7.5 5.6 8.4
68 6.3 4.8 7.2



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1









#23
 Nitrobenzene-d5
 Concen: 4.408 ng
 RT: 7.17 min Scan# 889
 Delta R.T. -0.02 min
 Lab File: BF115212.D
 Acq: 26 Jun 2019 10:41

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	82	Resp	64709
Ion Ratio	100	Lower	Upper
128	47.6	40.4	60.6
54	44.9	37.5	56.3




Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF1






#27
 2,4-Dimethylphenol
 Concen: 43.648 ng
 RT: 7.57 min Scan# 958
 Delta R.T. 0.01 min
 Lab File: BF115212.D
 Acq: 26 Jun 2019 10:41

Tgt Ion	122	Resp	570709
Ion Ratio	100	Lower	Upper
107	104.8	85.8	128.6
121	44.2	46.3	69.5#



Abundance Ion 122.00 (121.70 to 122.70): E
 Ion 107.00 (106.70 to 107.70): E
 Ion 121.00 (120.70 to 121.70): E









#32
Benzoic acid
Concen: 104.861 ng
RT: 7.70 min Scan# 979
Delta R.T. 0.01 min
Lab File: BF115212.D
Acq: 26 Jun 2019 10:41




Instrument :
BNA_F
ClientSampleId :


Tot Ion:122 Resp: 978698
Ion Ratio Lower Upper
122 100
105 3.4 98.2 138.2#
77 31.4 67.0 107.0#



#36
4-Chloro-3-methylphenol
Concen: 2.144 ng
RT: 8.45 min Scan# 1108
Delta R.T. -0.00 min
Lab File: BF115212.D
Acq: 26 Jun 2019 10:41

Tgt Ion:107 Resp: 29295
Ion Ratio Lower Upper
107 100
144 0.0 21.7 32.5#
142 2.2 67.0 100.4#









#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.64 min Scan# 1309
Delta R.T. -0.01 min
Lab File: BF115212.D
Acq: 26 Jun 2019 10:41

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
164	100		
162	100.5	81.7	122.5
160	46.0	37.0	55.4




Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E






#42
2,4,6-Tribromophenol
Concen: 6.465 ng
RT: 10.41 min Scan# 1441
Delta R.T. -0.02 min
Lab File: BF115212.D
Acq: 26 Jun 2019 10:41

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.1	77.3	115.9
141	34.7	28.2	42.2



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E









#45
2-Fluorobiphenyl
Concen: 5.417 ng
RT: 8.97 min Scan# 1195
Delta R.T. -0.02 min
Lab File: BF115212.D
Acq: 26 Jun 2019 10:41




Instrument :
BNA_F
ClientSampleId :


Tot Ion:172 Resp: 142353
Ion Ratio Lower Upper
172 100
171 34.4 29.8 44.6
170 22.7 20.3 30.5



#51
2,6-Dinitrotoluene
Concen: 7.958 ng
RT: 9.64 min Scan# 1309
Delta R.T. 0.20 min
Lab File: BF115212.D
Acq: 26 Jun 2019 10:41

Tgt Ion:165 Resp: 60335
Ion Ratio Lower Upper
165 100
63 2.7 39.4 59.2#
89 2.7 42.0 63.0#





#54

2,4-Dinitrophenol

Concen: 7.453 ng

RT: 9.79 min Scan# 1335

Delta R.T. 0.09 min

Lab File: BF115212.D

Acq: 26 Jun 2019 10:41

Instrument :

BNA_F

ClientSampleId :


Tot Ion:184 Resp: 470

Ion Ratio Lower Upper

184 100

63 52.8 41.9 62.9

154 0.0 44.7 67.1#



Abundance Ion 184.00 (183.70 to 184.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 154.00 (153.70 to 154.70): E

9.79

600



400

200

0

9.76 9.78 9.80

Time-->



#57

2,4-Dinitrotoluene

Concen: 6.164 ng

RT: 9.64 min Scan# 1309

Delta R.T. -0.20 min

Lab File: BF115212.D

Acq: 26 Jun 2019 10:41

Tgt Ion:165 Resp: 60335


Ion Ratio Lower Upper

165 100

63 2.7 27.5 41.3#

89 2.7 49.9 74.9#

182 0.0 2.1 3.1#



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

9.64

100000

80000

60000


40000


20000

0

9.55 9.60 9.65 9.70

Time-->









#58
 Fluorene
 Concen: Below Cal
 RT: 10.17 min Scan# 1400
 Delta R.T. -0.02 min
 Lab File: BF115212.D
 Acq: 26 Jun 2019 10:41

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:166 Resp: 139
 Ion Ratio Lower Upper
 166 100
 165 95.7 76.5 114.7
 167 0.0 11.0 16.4#




Abundance Ion 166.00 (165.70 to 166.70): E
 Ion 165.00 (164.70 to 165.70): E
 Ion 167.00 (166.70 to 167.70): E






#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.11 min Scan# 1559
 Delta R.T. -0.01 min
 Lab File: BF115212.D
 Acq: 26 Jun 2019 10:41

Tgt Ion:188 Resp: 897944
 Ion Ratio Lower Upper
 188 100
 94 9.6 8.6 12.8
 80 9.8 8.8 13.2



Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF1
 Ion 80.00 (79.70 to 80.70): BF1





#65

4,6-Dinitro-2-methylphenol

Concen: 5.042 ng

RT: 10.42 min Scan# 1443

Delta R.T. 0.18 min

Lab File: BF115212.D

Acq: 26 Jun 2019 10:41

Instrument :

BNA_F

ClientSampled :


Tot Ion:198 Resp: 440

Ion Ratio Lower Upper

198 100

51 1843.1 11.0 51.0#




105 348.5 17.3 57.3#



Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF1

Ion 105.00 (104.70 to 105.70): E



#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.72 min Scan# 2004

Delta R.T. -0.02 min

Lab File: BF115212.D

Acq: 26 Jun 2019 10:41


Tgt Ion:240 Resp: 734831

Ion Ratio Lower Upper

240 100

120 11.3 9.4 14.2



236 27.0 21.7 32.5




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E





#79

Terphenyl-d14

Concen: 4.194 ng

RT: 12.68 min Scan# 1827

Delta R.T. -0.02 min

Lab File: BF115212.D

Acq: 26 Jun 2019 10:41

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 144966

Ion Ratio Lower Upper

244 100

212 6.2 5.8 8.6




122 12.1 10.4 15.6



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E



#87

Perylene-d12

Concen: 20.000 ng

RT: 15.09 min Scan# 2236

Delta R.T. -0.02 min

Lab File: BF115212.D

Acq: 26 Jun 2019 10:41


Tgt Ion:264 Resp: 681506

Ion Ratio Lower Upper

264 100

260 24.0 19.6 29.4

265 21.6 17.3 25.9



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

