
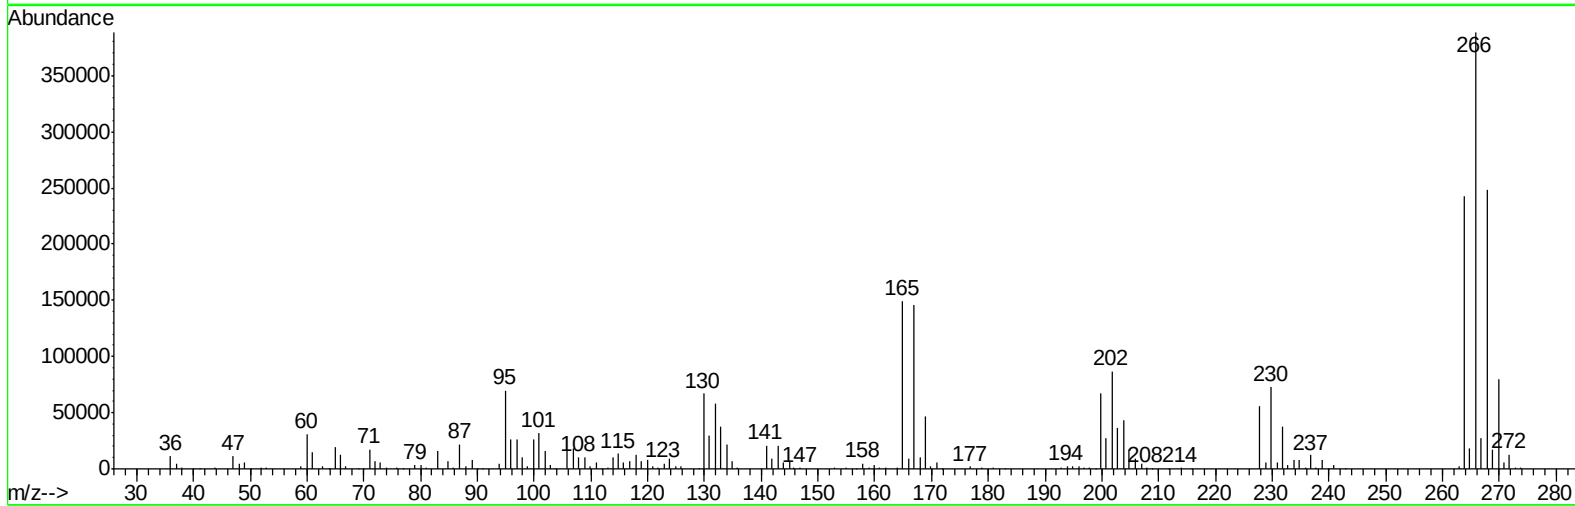


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062619\
Data File : BF115207.D
Acq On : 26 Jun 2019 7:55
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 03:53:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 04:21:29 2019
Response via : Initial Calibration

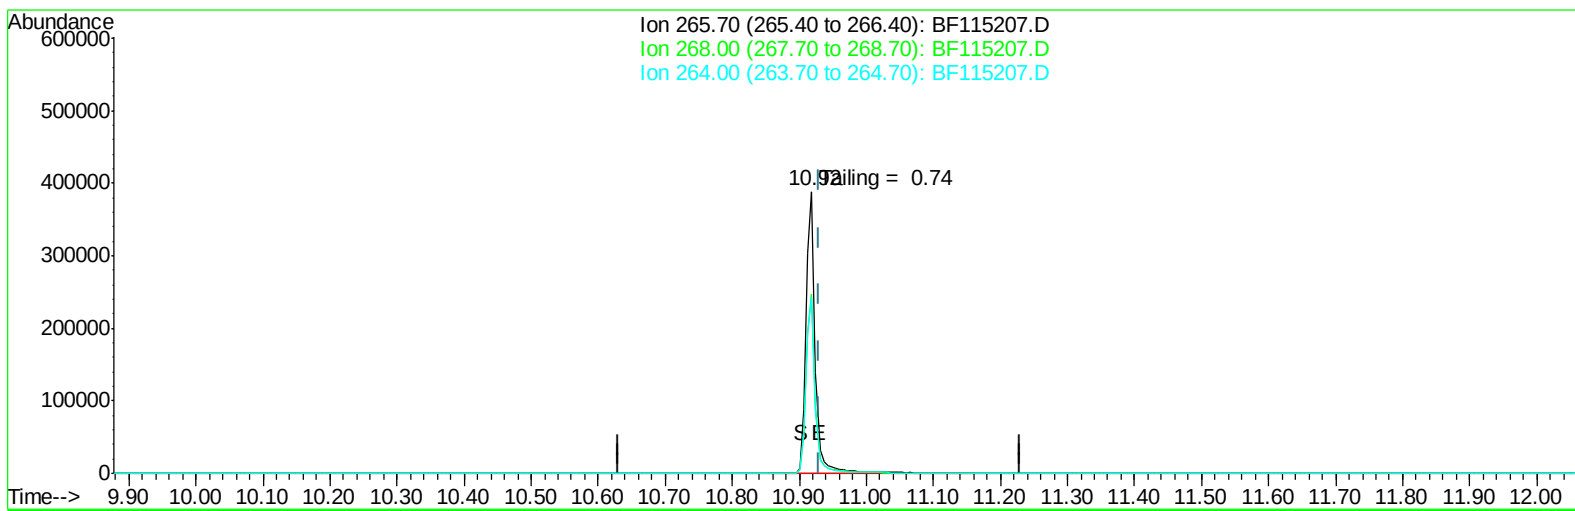

TIC: BF115207.D

(70) Pentachlorophenol (C)



10.919min (-0.012) 333149.65ng

response 369663

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	63.81
264.00	61.60	62.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062619\
Data File : BF115207.D
Acq On : 26 Jun 2019 7:55
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 03:53:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 04:21:29 2019
Response via : Initial Calibration

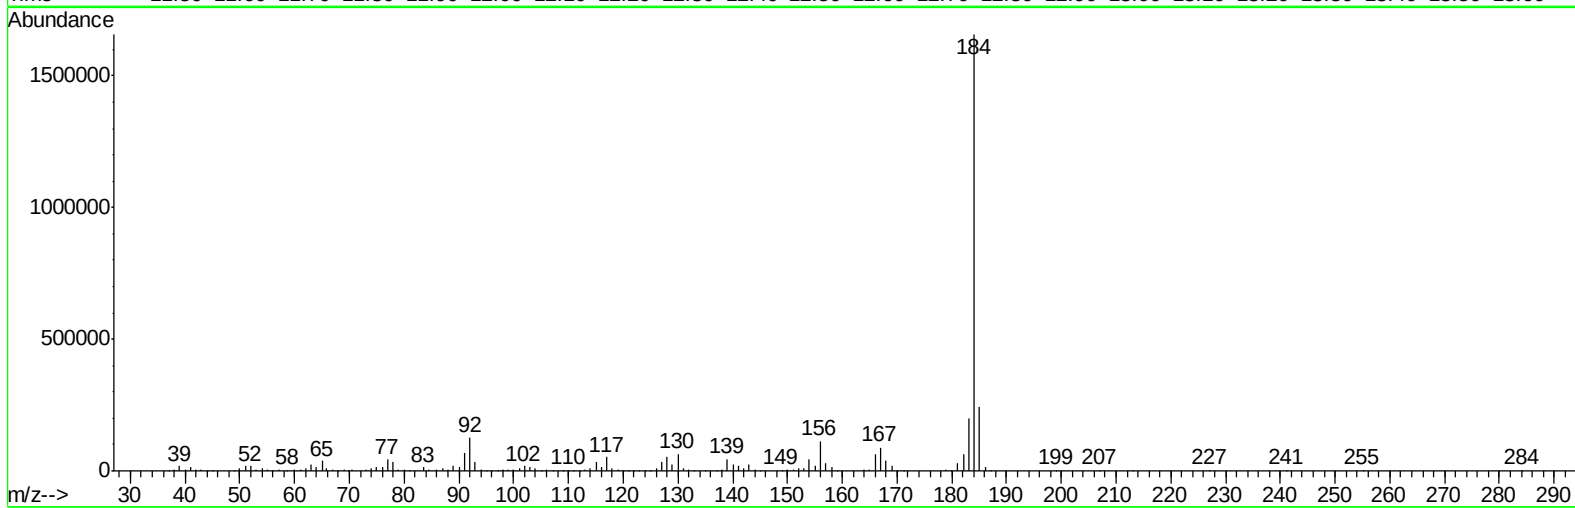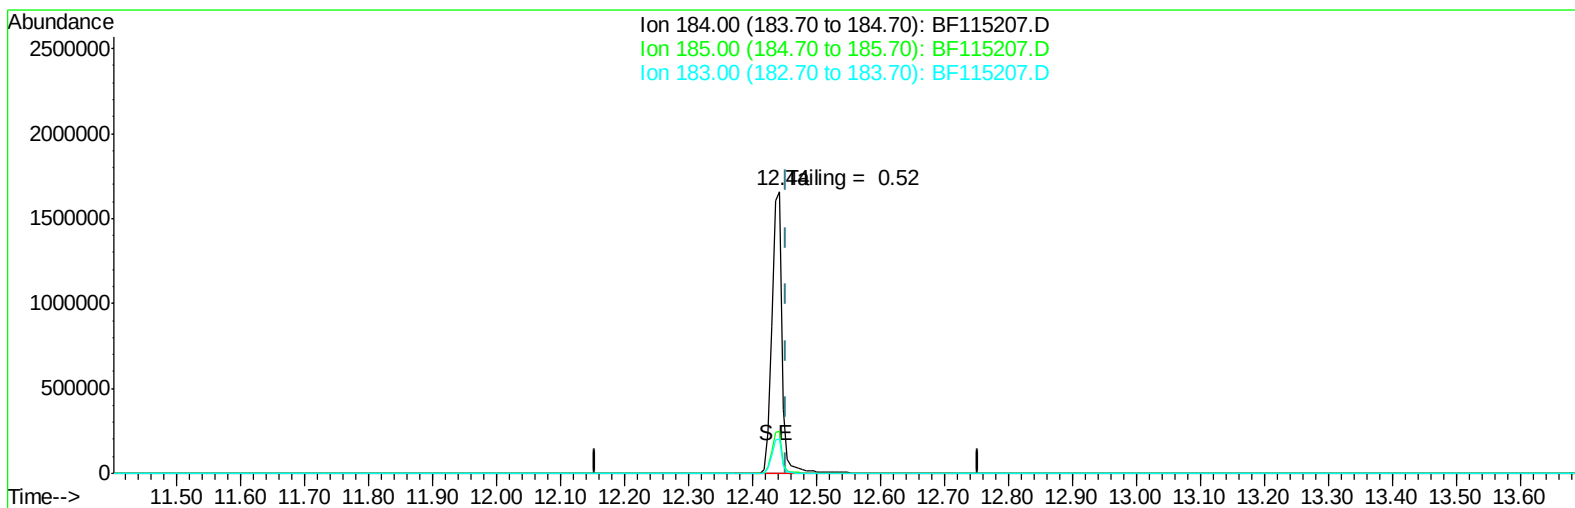

TIC: BF115207.D

(77) Benzidine

12.442min (-0.012) 0.00ng

response 1813884

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.80
183.00	12.00	12.11
0.00	0.00	0.00