
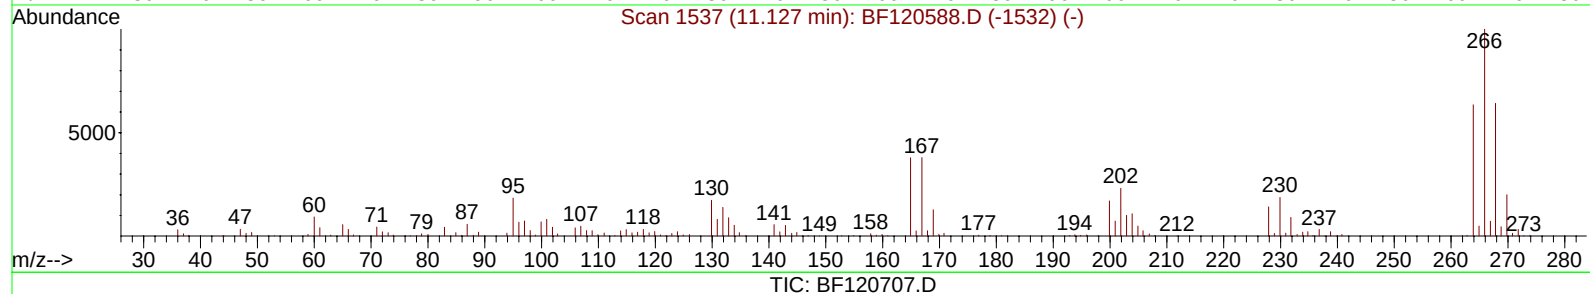
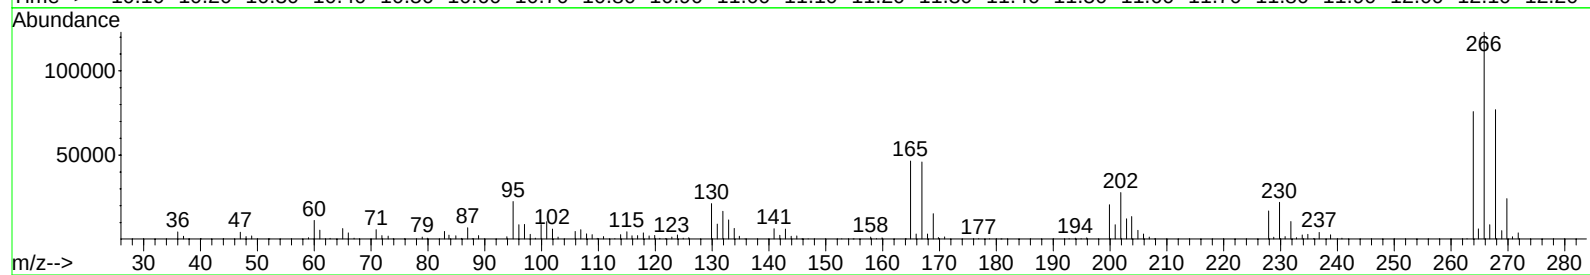


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062620\
 Data File : BF120707.D
 Acq On : 26 Jun 2020 13:54
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 19:07:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 11 11:28:22 2020
 Response via : Initial Calibration

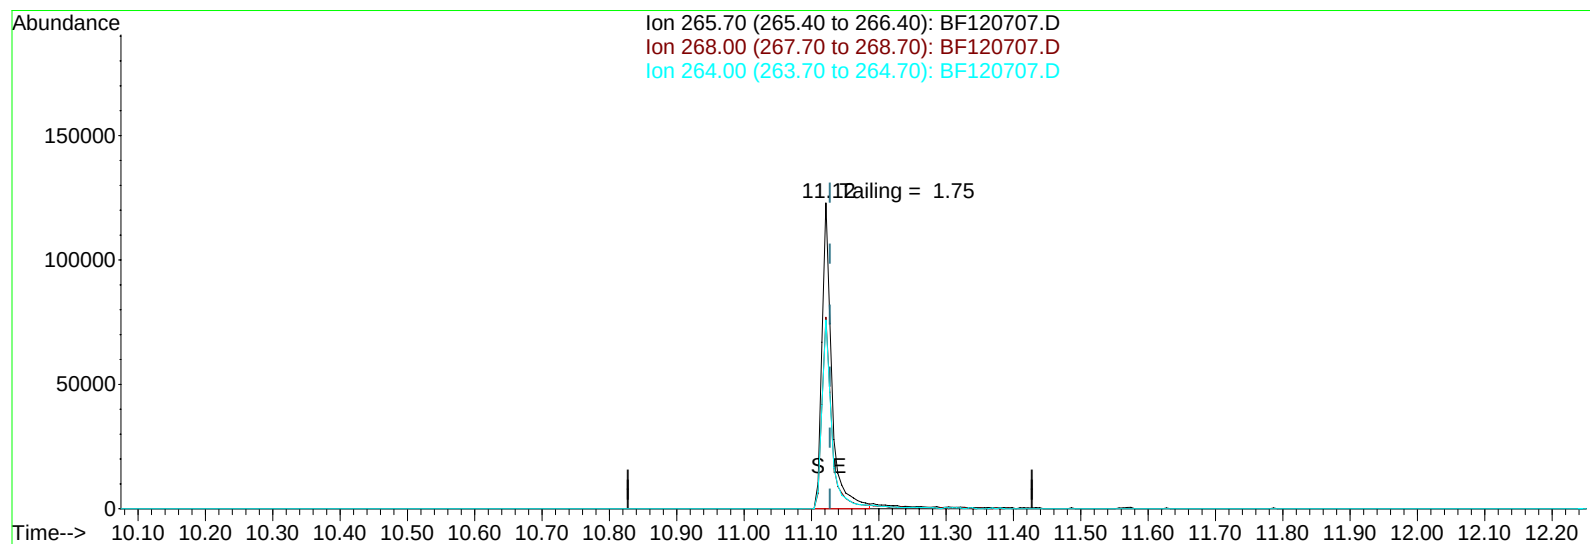

(70) Pentachlorophenol (C)




11.121min (-0.006) 18015.32ng

response 129303

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	62.62
264.00	63.50	61.68
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062620\
 Data File : BF120707.D
 Acq On : 26 Jun 2020 13:54
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 19:07:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 11 11:28:22 2020
 Response via : Initial Calibration

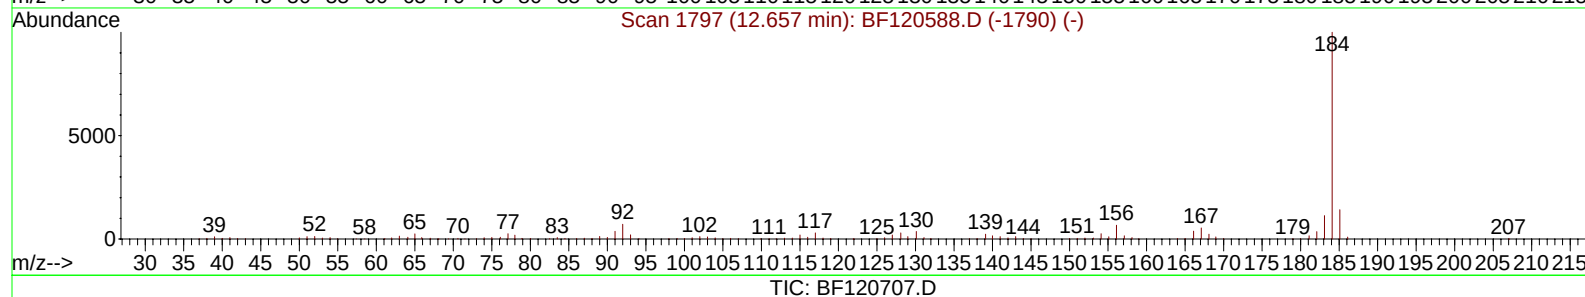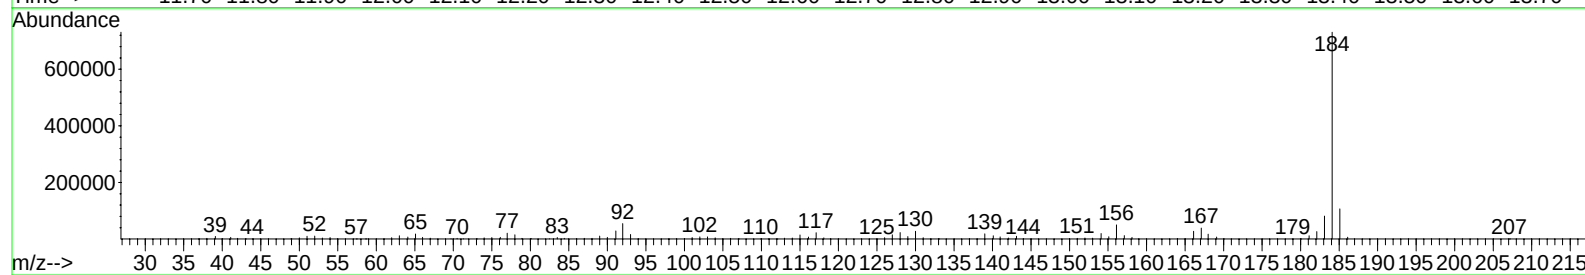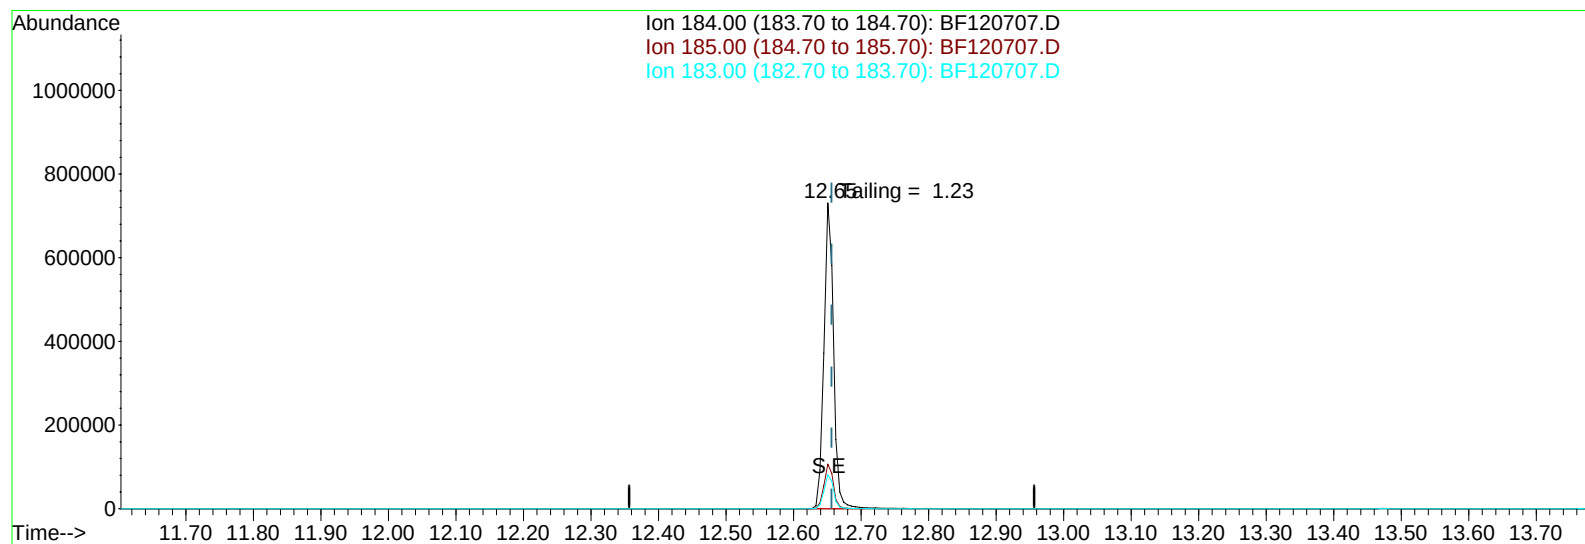

(77) Benzidine

12.651min (-0.006) 15466.76ng

response 722891

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.61
183.00	11.30	11.09
0.00	0.00	0.00