


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062620\
 Data File : BF120707.D
 Acq On : 26 Jun 2020 13:54
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 11 11:28:22 2020

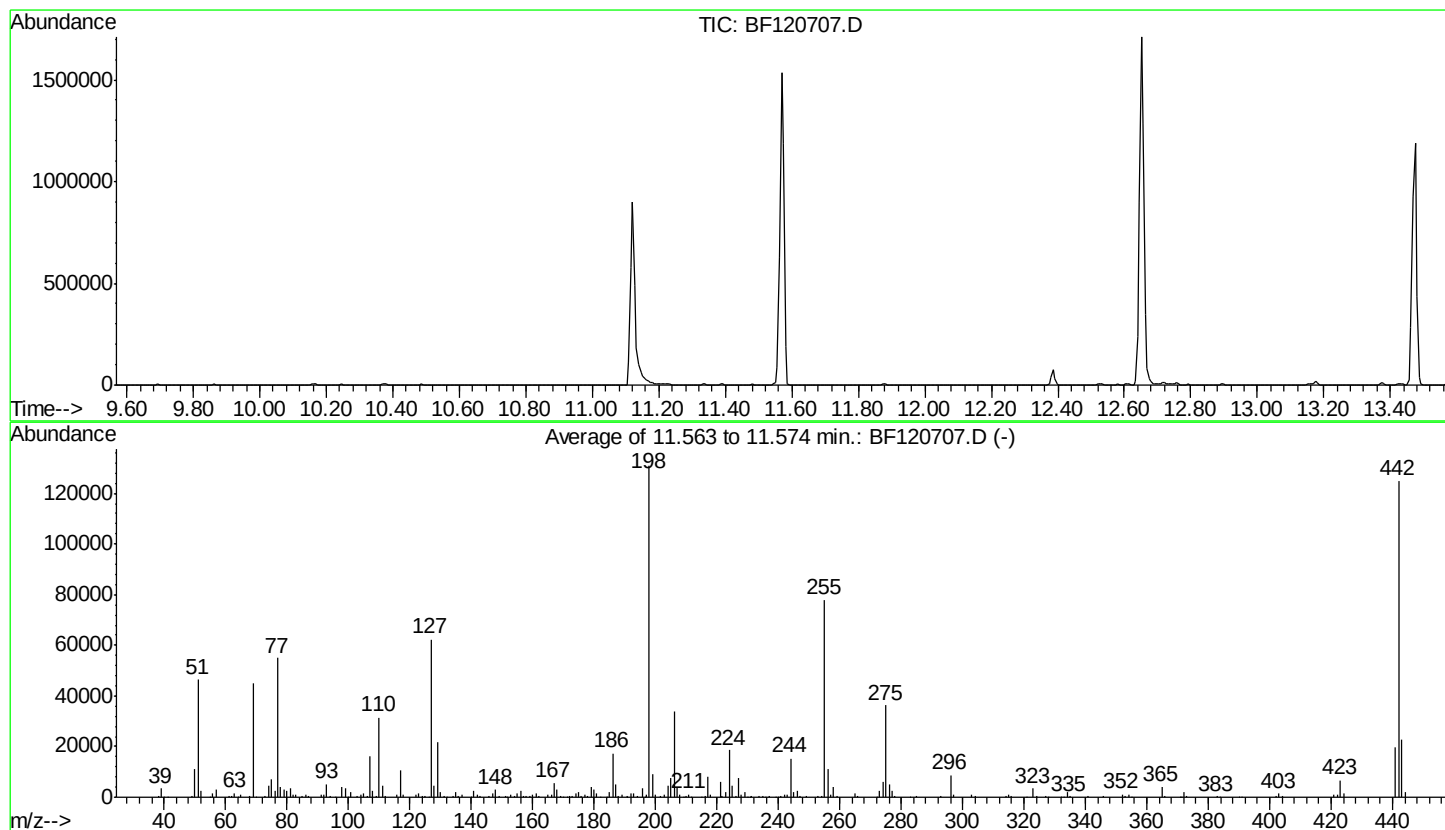

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	46394	PASS
68	69	0.00	2	1.6	733	PASS
69	198	0.00	100	34.5	45157	PASS
70	69	0.00	2	0.2	103	PASS
127	198	10	80	47.6	62322	PASS
197	198	0.00	2	0.6	827	PASS
198	198	100	100	100.0	130944	PASS
199	198	5	9	6.8	8922	PASS
275	198	10	60	27.7	36269	PASS
365	198	1	100	3.2	4182	PASS
441	198	0.01	100	15.0	19671	PASS
442	198	50	100	95.5	125056	PASS
443	442	15	24	18.2	22770	PASS