


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062624\
Data File : BF138347.D
Acq On : 26 Jun 2024 12:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 13 01:52:47 2024

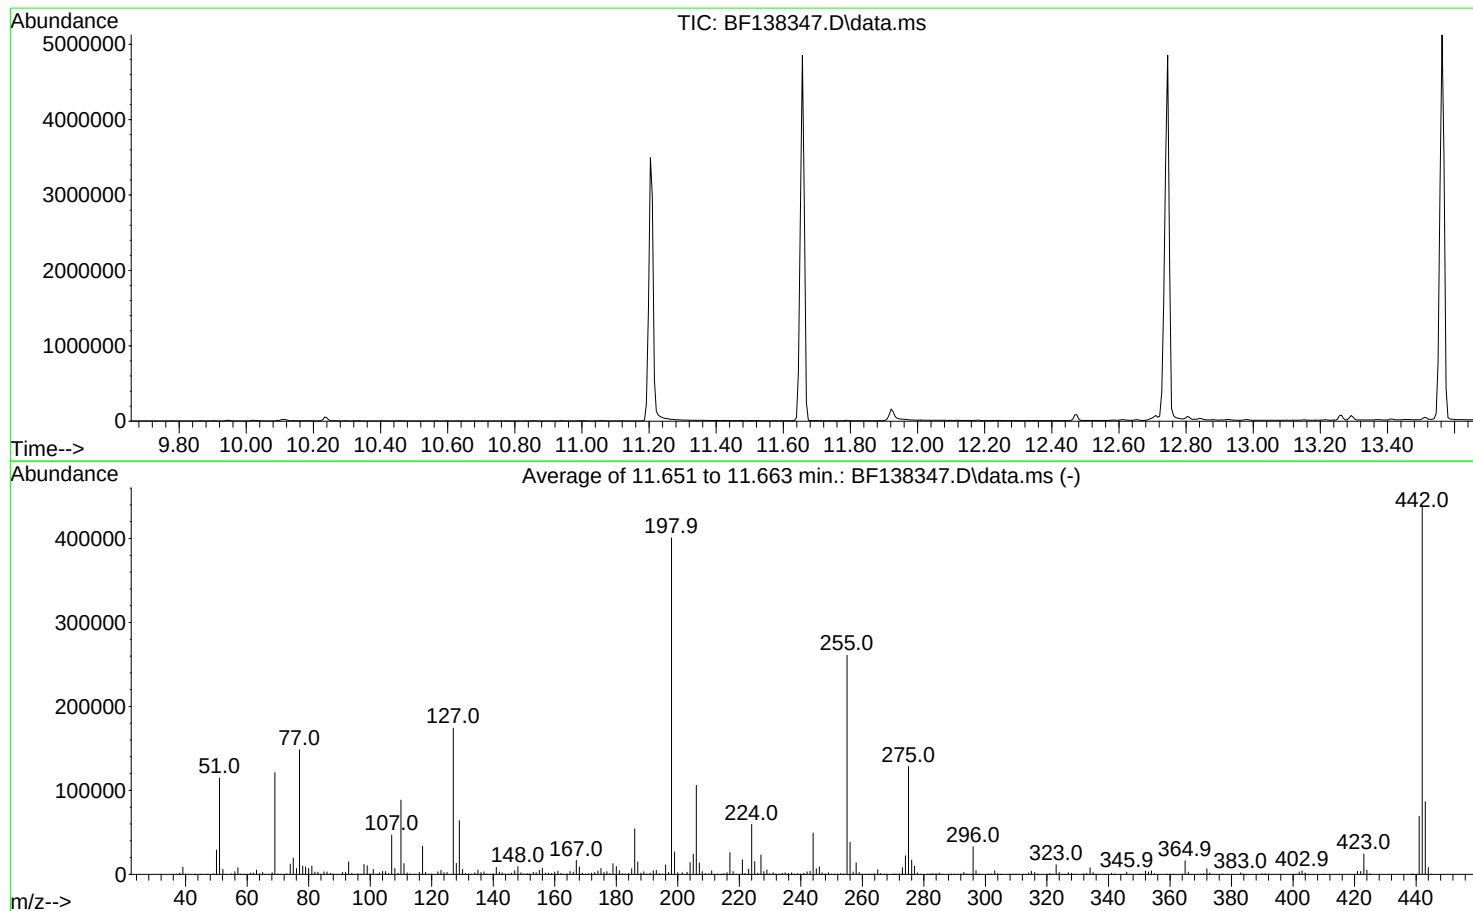




AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.6	114759	PASS
68	69	0.00	2	1.6	1953	PASS
69	198	0.00	100	30.2	121229	PASS
70	69	0.00	2	0.5	649	PASS
127	198	10	80	43.5	174221	PASS
197	198	0.00	2	0.6	2244	PASS
198	198	100	100	100.0	400832	PASS
199	198	5	9	6.7	26699	PASS
275	198	10	60	32.0	128379	PASS
365	198	1	100	4.1	16253	PASS
441	198	0.01	100	17.2	69123	PASS
442	442	50	100	100.0	438123	PASS
443	442	15	24	19.8	86533	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062624\
Data File : BF138347.D
Acq On : 26 Jun 2024 12:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 26 12:50:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

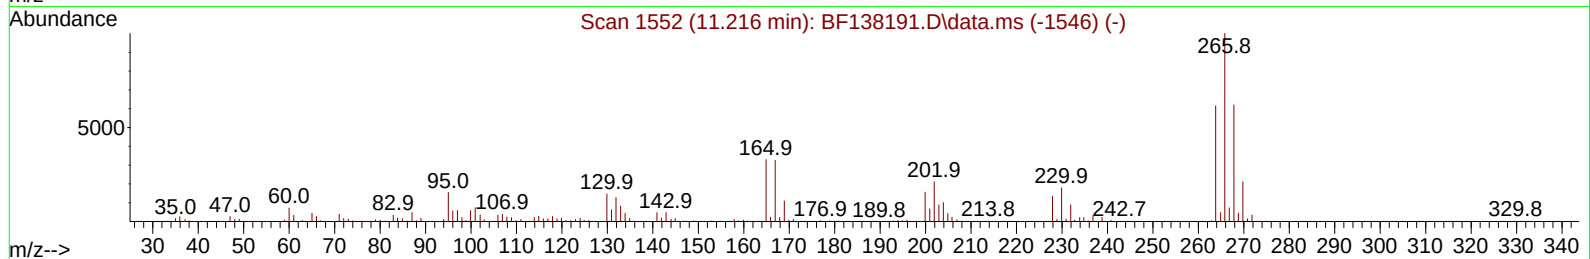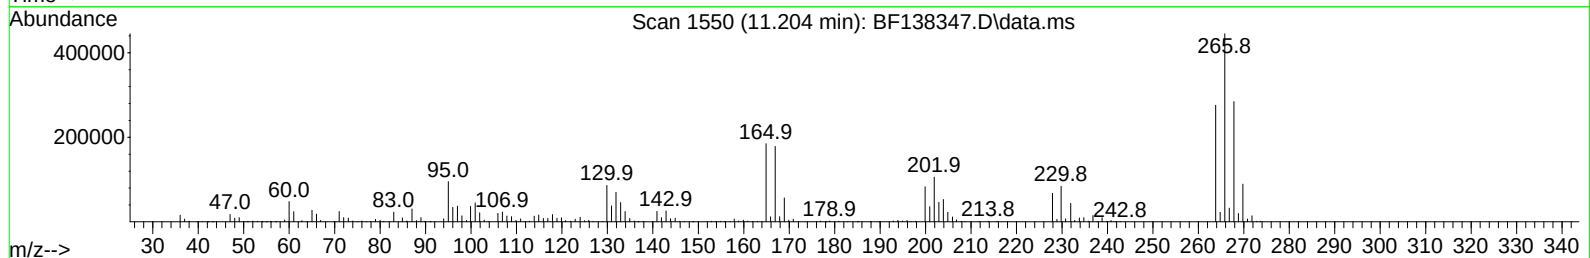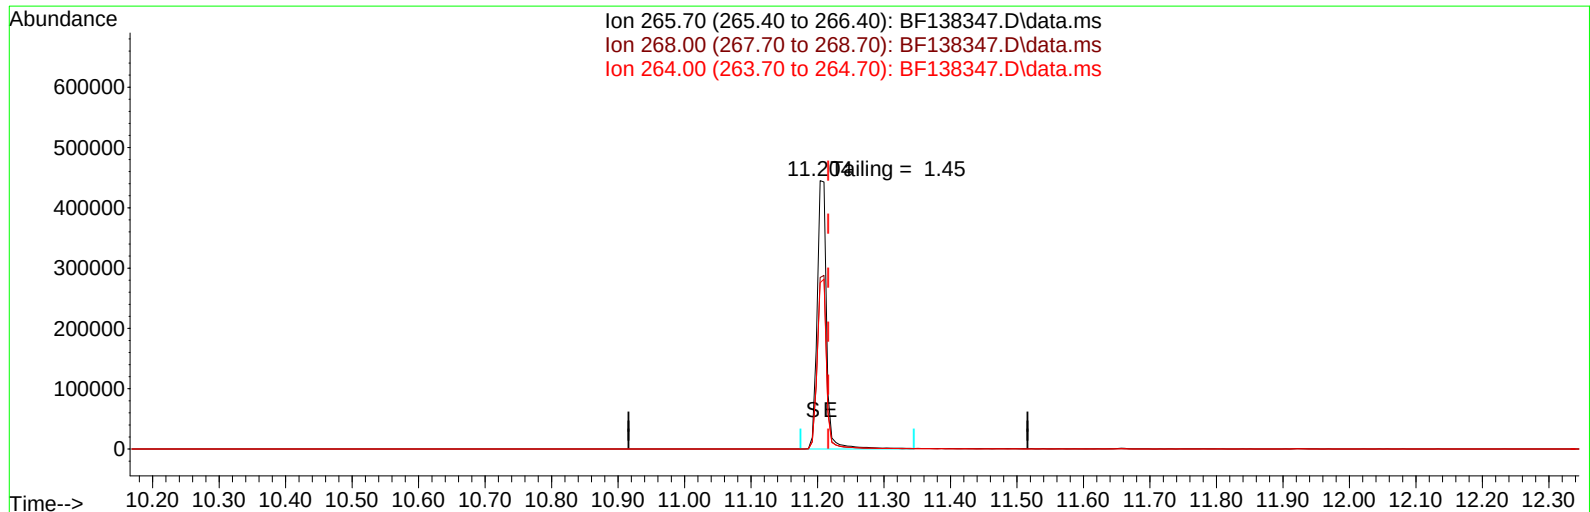

TIC: BF138347.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.012) 112738.39 ng




response 439225

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.91
264.00	61.50	61.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062624\
Data File : BF138347.D
Acq On : 26 Jun 2024 12:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 26 12:50:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

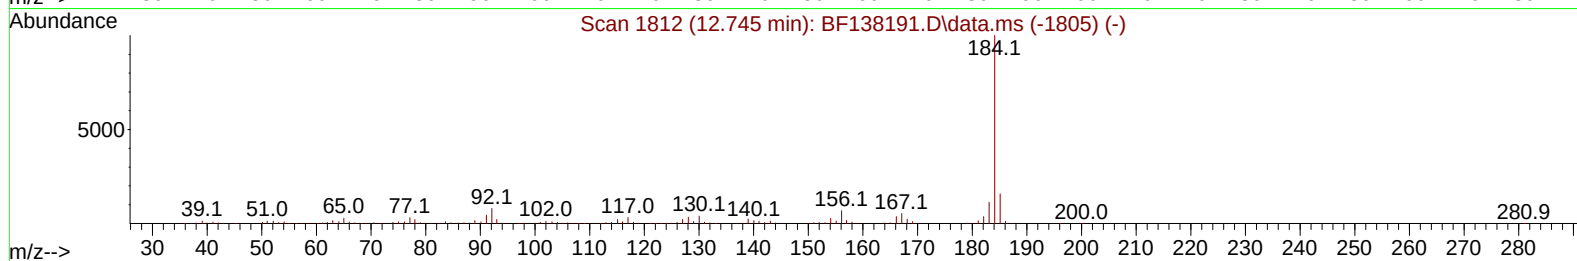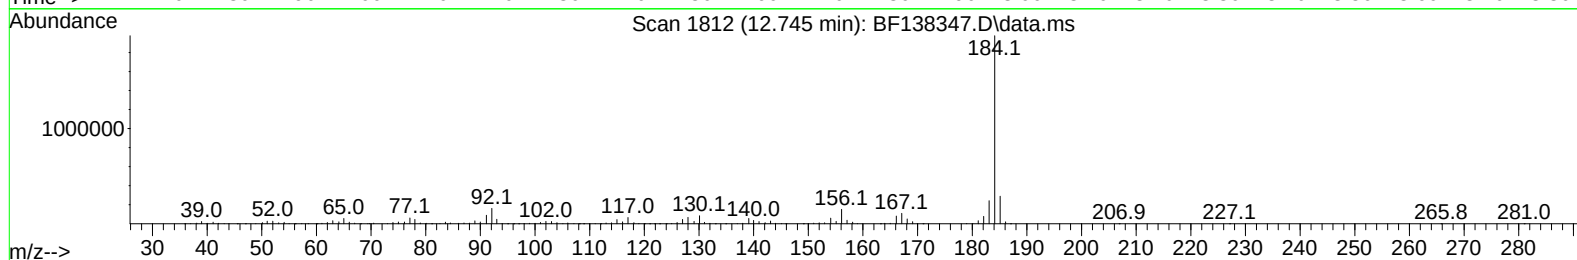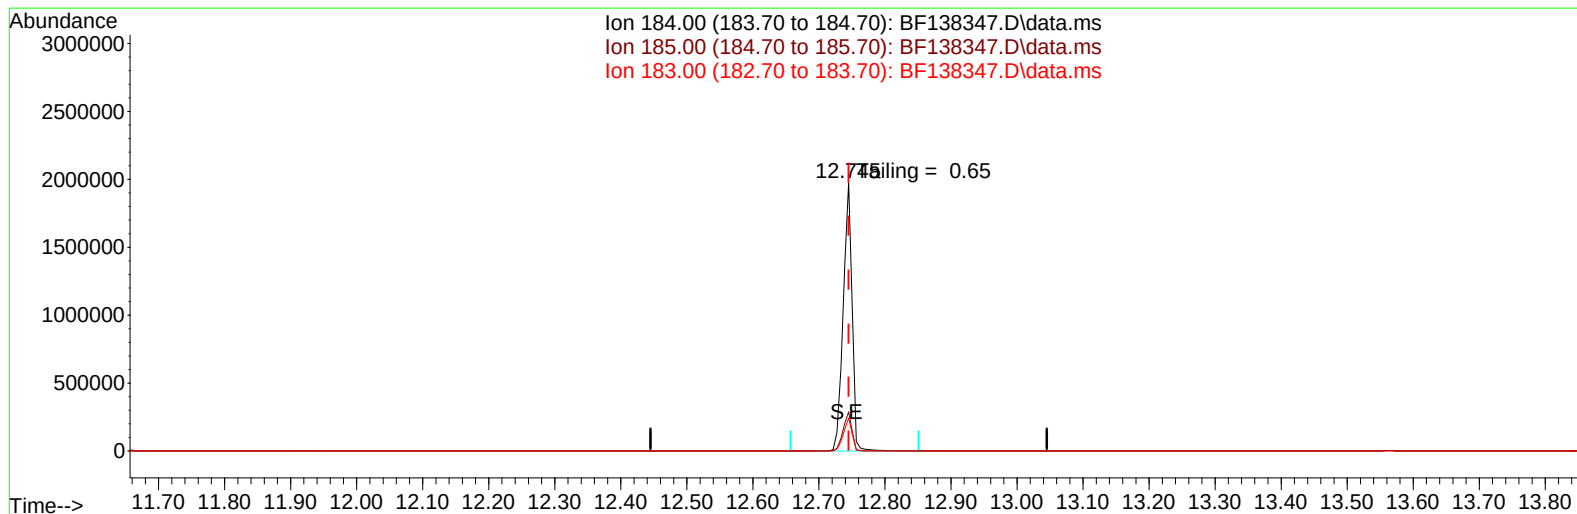

TIC: BF138347.D\data.ms

(77) Benzidine

12.745min (-0.000) 249332.88 ng

response 1863039

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	14.64
183.00	11.30	12.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/26/2024	BNA_F	<u>BF138347.D</u>
Compound Name	Response	Retention Time
DDT	932319	13.563
DDD	21503	13.263
DDE	1306	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22809	955128	2.39

Instrument :
BNA_F
ClientSampleId :
DFTPP