

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062625\
 Data File : BF142874.D
 Acq On : 26 Jun 2025 18:05
 Operator : RC/JU
 Sample : Q2425-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-1

Quant Time: Jun 26 18:26:13 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 24 05:28:21 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	80015	20.000	ng	0.00
21) Naphthalene-d8	8.157	136	306273	20.000	ng	-0.01
39) Acenaphthene-d10	9.916	164	163617	20.000	ng	0.00
64) Phenanthrene-d10	11.404	188	266840	20.000	ng	0.00
76) Chrysene-d12	14.051	240	136110	20.000	ng	0.00
86) Perylene-d12	15.539	264	163547	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.493	112	370830	77.161	ng	0.00
7) Phenol-d6	6.504	99	458335	80.834	ng	0.00
23) Nitrobenzene-d5	7.434	82	281264	50.372	ng	-0.01
42) 2,4,6-Tribromophenol	10.704	330	83075	49.340	ng	-0.01
45) 2-Fluorobiphenyl	9.234	172	636753	51.125	ng	-0.01
79) Terphenyl-d14	12.992	244	496947	50.447	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062625\
Data File : BF142874.D
Acq On : 26 Jun 2025 18:05
Operator : RC/JU
Sample : Q2425-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-1

Quant Time: Jun 26 18:26:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration



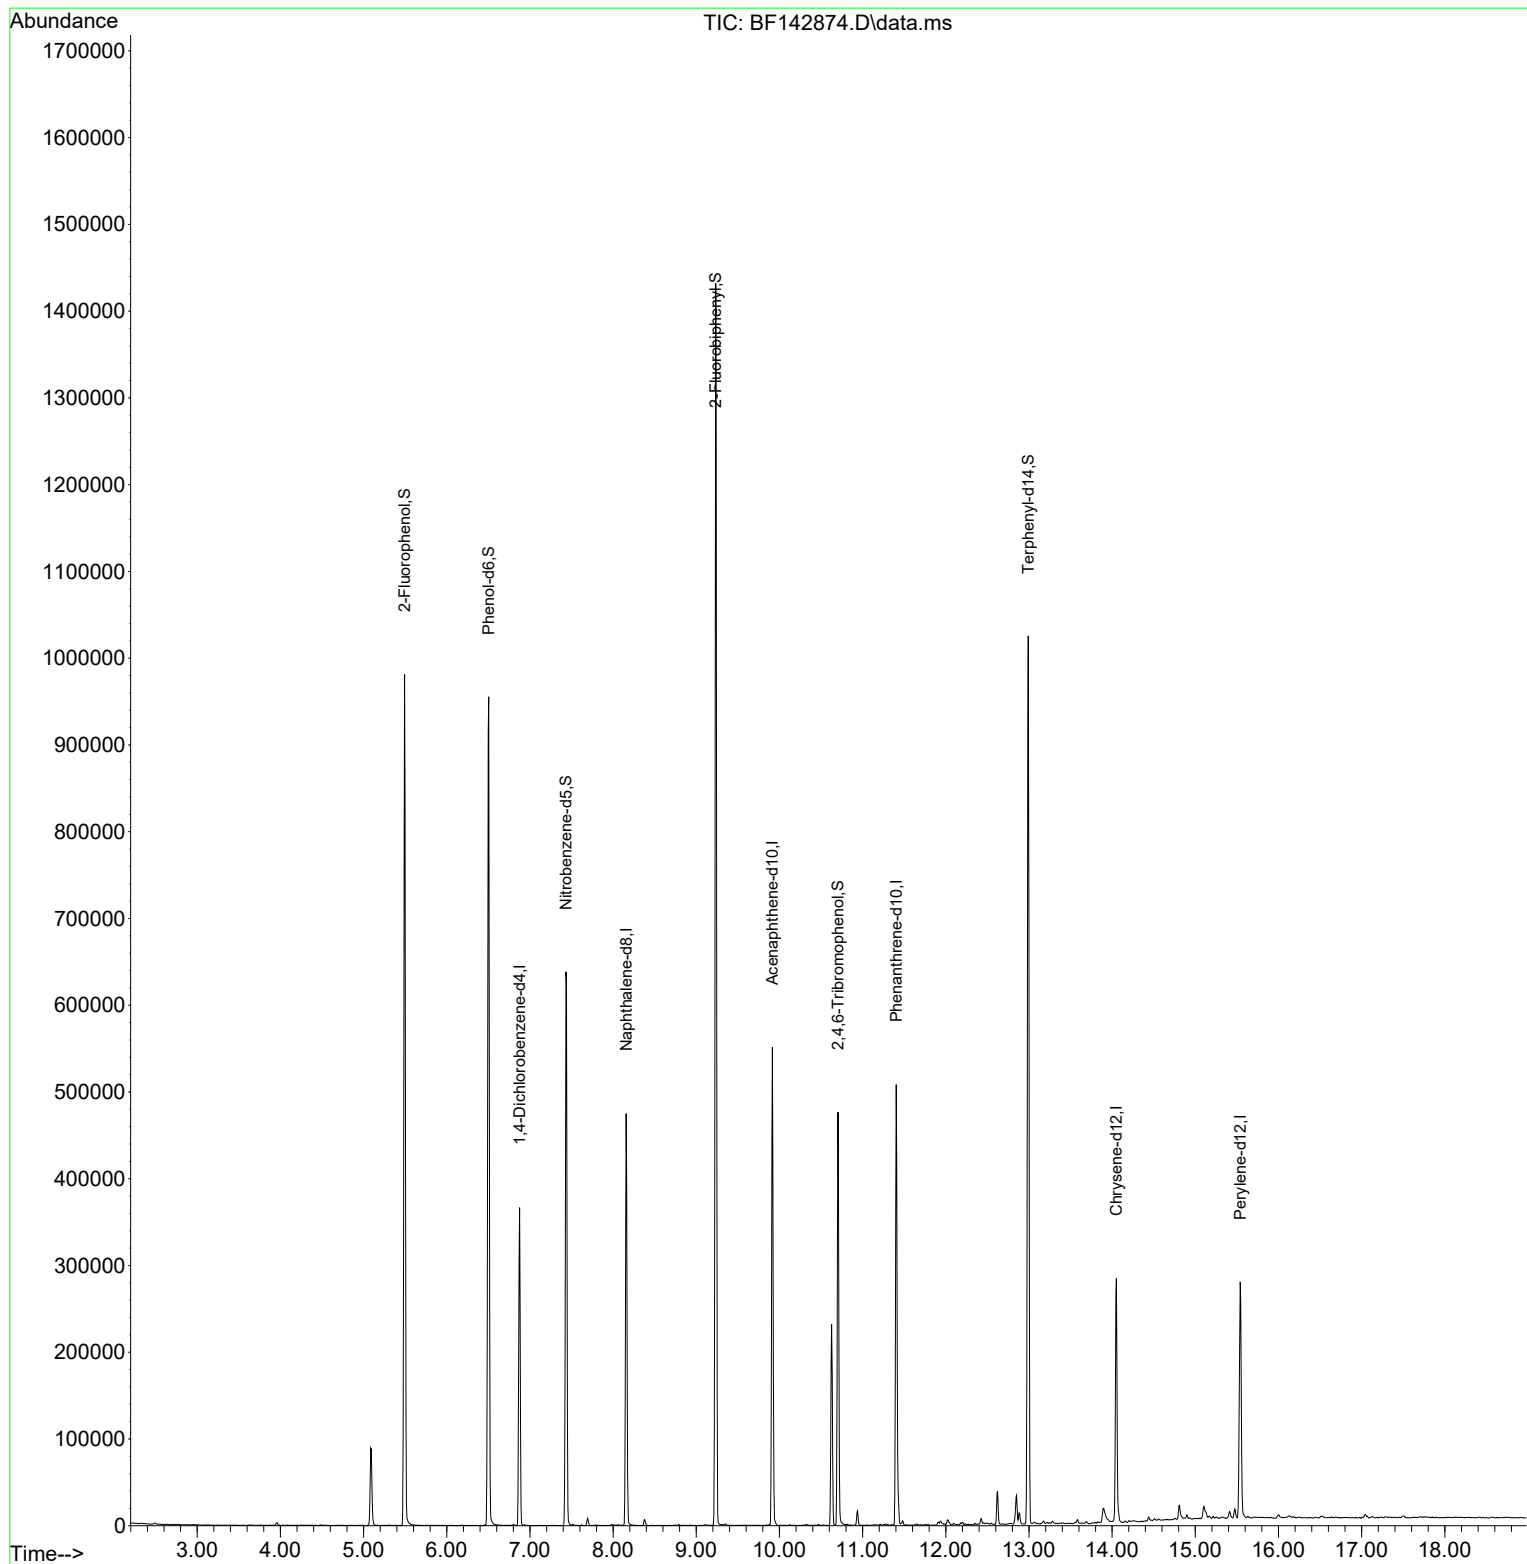




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.875 min Scan# 797
Delta R.T. -0.006 min
Lab File: BF142874.D
Acq: 26 Jun 2025 18:05




Instrument :
BNA_F
ClientSampleId :
COMP-1


Tgt Ion:152 Resp: 80015
Ion Ratio Lower Upper
152 100
150 157.3 127.2 190.8
115 56.5 46.6 69.8

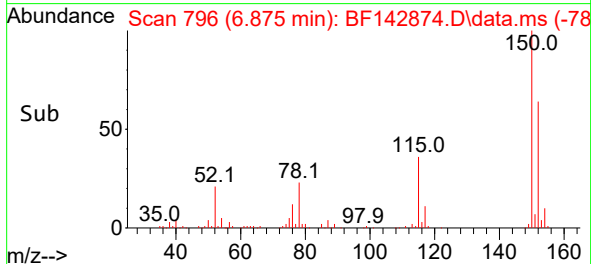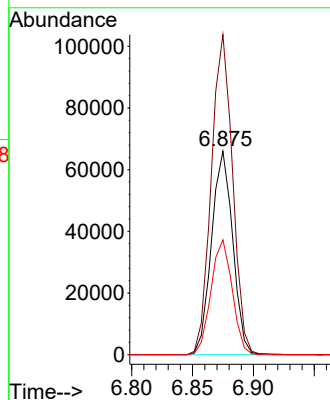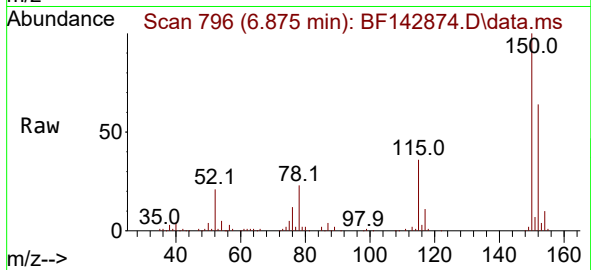

#5
2-Fluorophenol
Concen: 77.161 ng
RT: 5.493 min Scan# 561
Delta R.T. 0.001 min
Lab File: BF142874.D
Acq: 26 Jun 2025 18:05

Tgt Ion:112 Resp: 370830
Ion Ratio Lower Upper
112 100
64 58.4 48.2 72.2
63 30.9 25.7 38.5

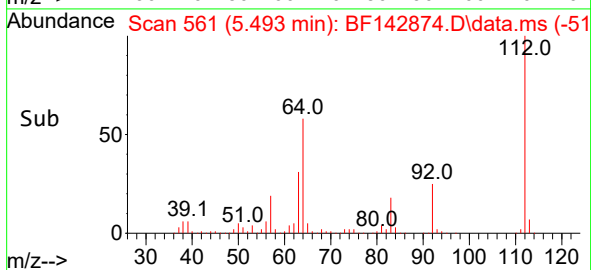
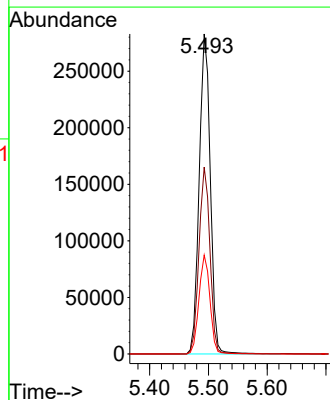
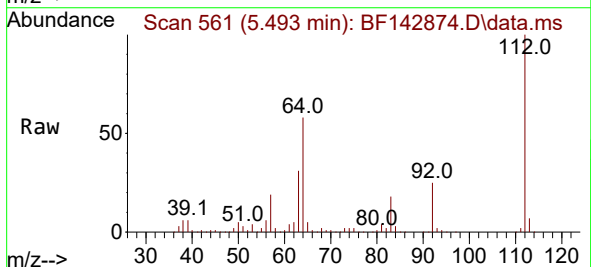


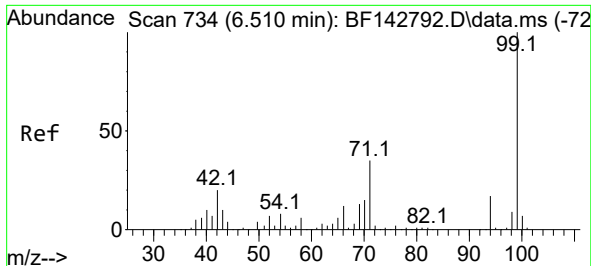

#7
Phenol-d6
Concen: 80.834 ng
RT: 6.504 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF142874.D
Acq: 26 Jun 2025 18:05




Instrument :
BNA_F
ClientSampleId :
COMP-1


Tgt Ion: 99 Resp: 458335
Ion Ratio Lower Upper
99 100
42 19.3 15.9 23.9
71 34.7 27.8 41.8

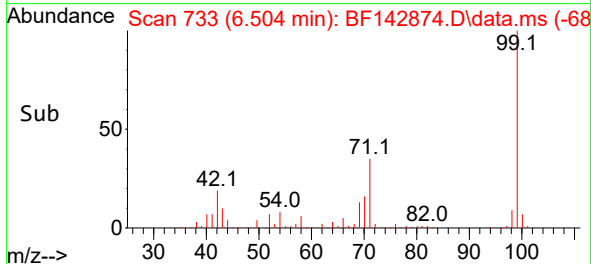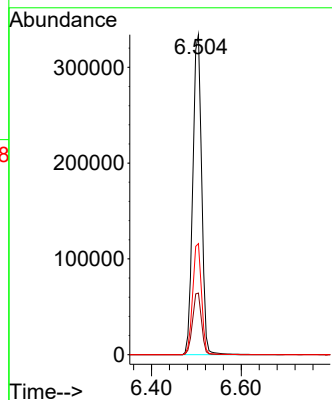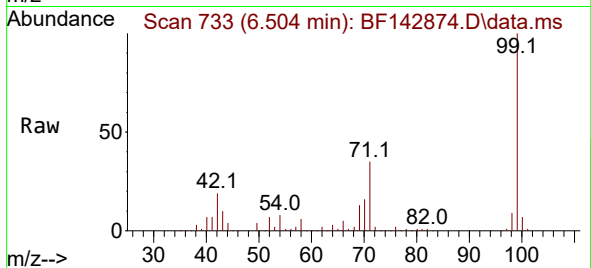

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.157 min Scan# 1014
Delta R.T. -0.012 min
Lab File: BF142874.D
Acq: 26 Jun 2025 18:05

Tgt Ion: 136 Resp: 306273
Ion Ratio Lower Upper
136 100
137 10.8 8.4 12.6
54 8.0 6.3 9.5
68 4.4 3.7 5.5


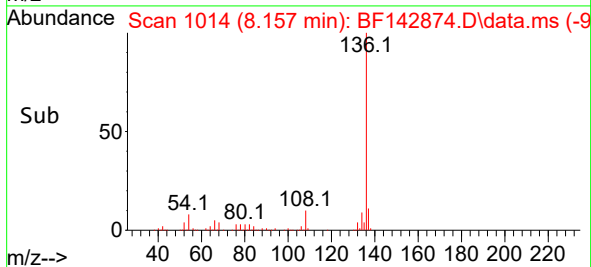
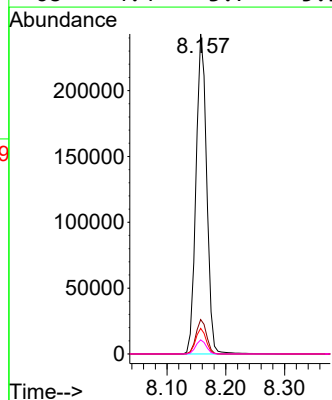
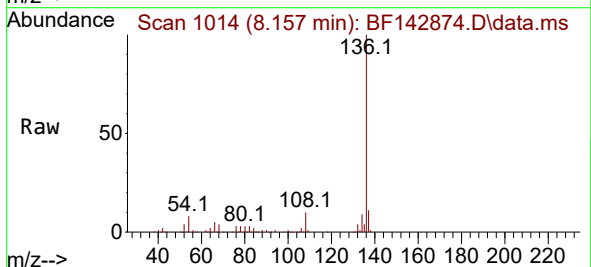


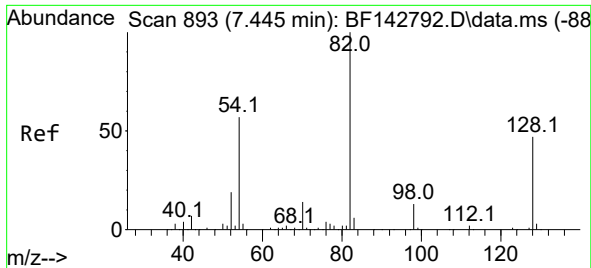

#23
 Nitrobenzene-d5
 Concen: 50.372 ng
 RT: 7.434 min Scan# 891
 Delta R.T. -0.011 min
 Lab File: BF142874.D
 Acq: 26 Jun 2025 18:05




Instrument :
 BNA_F
 ClientSampleId :
 COMP-1

Tgt Ion: 82 Resp: 281264
 Ion Ratio Lower Upper
 82 100
 128 47.5 37.7 56.5
 54 56.9 45.7 68.5

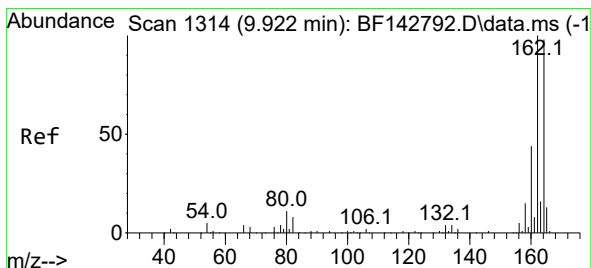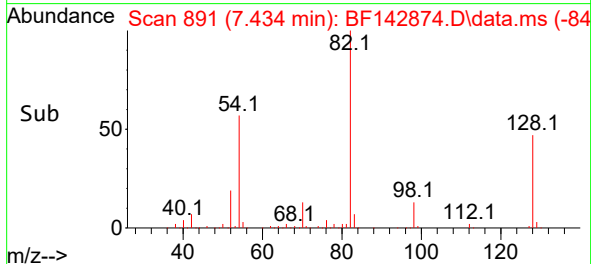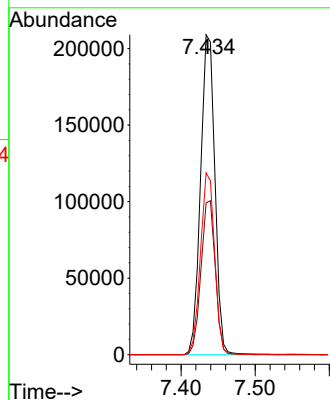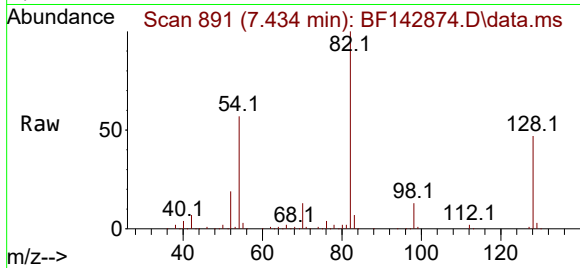

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.916 min Scan# 1313
 Delta R.T. -0.006 min
 Lab File: BF142874.D
 Acq: 26 Jun 2025 18:05

Tgt Ion:164 Resp: 163617
 Ion Ratio Lower Upper
 164 100
 162 101.1 81.8 122.8
 160 45.0 36.0 54.0

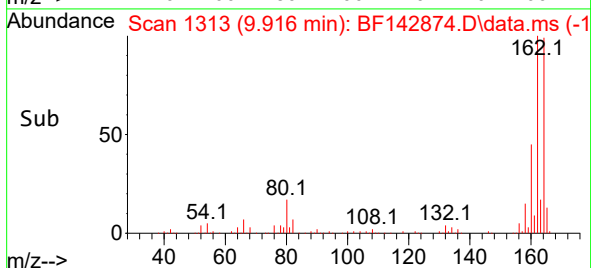
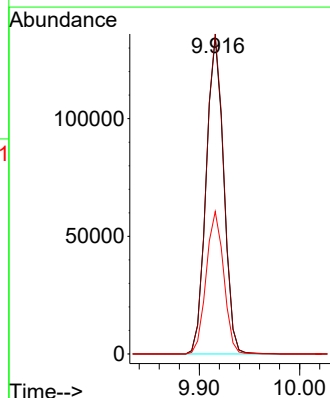
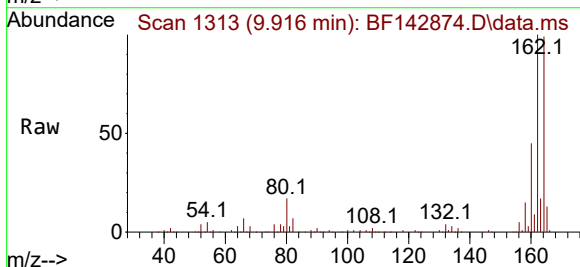




#42
2,4,6-Tribromophenol
Concen: 49.340 ng
RT: 10.704 min Scan# 1447
Delta R.T. -0.012 min
Lab File: BF142874.D
Acq: 26 Jun 2025 18:05




Instrument :
BNA_F
ClientSampleId :
COMP-1

Tgt Ion: 330 Resp: 83075
Ion Ratio Lower Upper
330 100
332 94.5 75.0 112.6
141 31.9 25.3 37.9

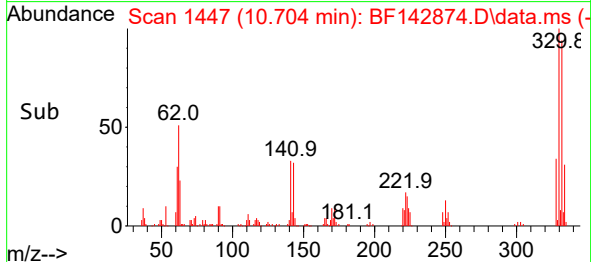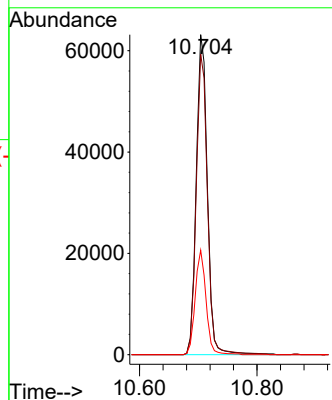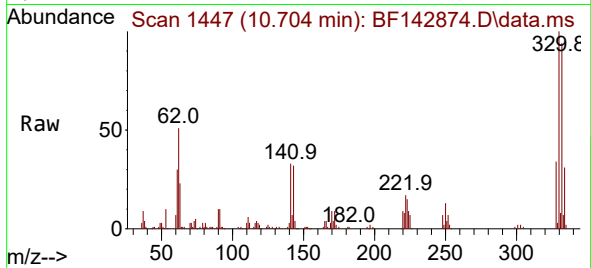

#45
2-Fluorobiphenyl
Concen: 51.125 ng
RT: 9.234 min Scan# 1197
Delta R.T. -0.011 min
Lab File: BF142874.D
Acq: 26 Jun 2025 18:05

Tgt Ion: 172 Resp: 636753
Ion Ratio Lower Upper
172 100
171 34.9 28.2 42.4
170 23.1 18.5 27.7


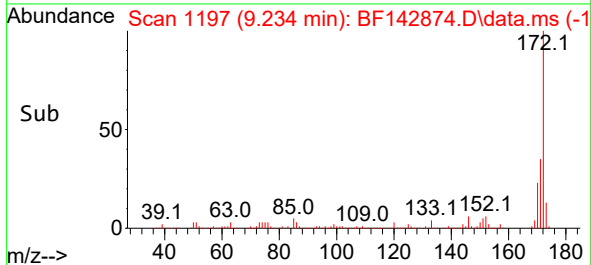
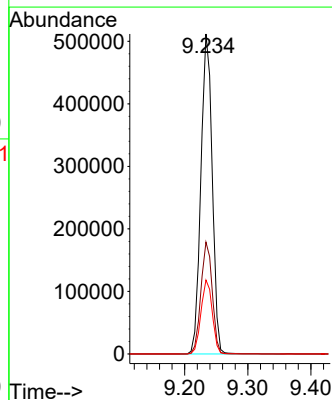
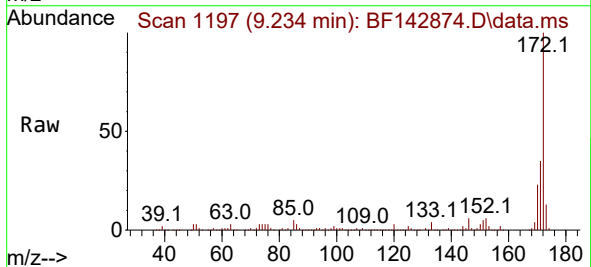




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.404 min Scan# 1
Delta R.T. -0.006 min
Lab File: BF142874.D
Acq: 26 Jun 2025 18:05




Instrument :
BNA_F
ClientSampleId :
COMP-1

Tgt Ion:188 Resp: 266840
Ion Ratio Lower Upper
188 100
94 7.8 6.7 10.1
80 8.3 6.9 10.3

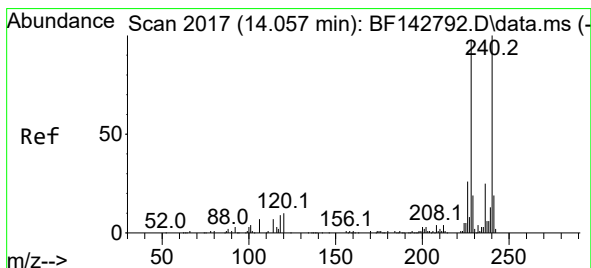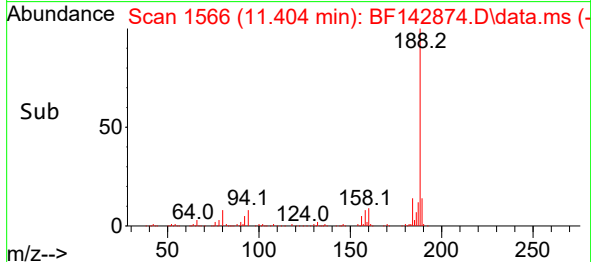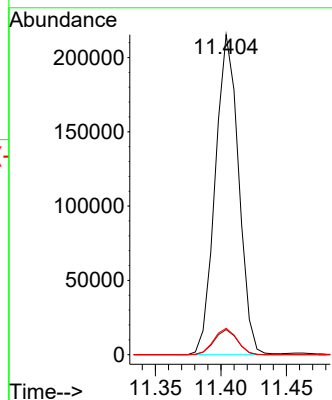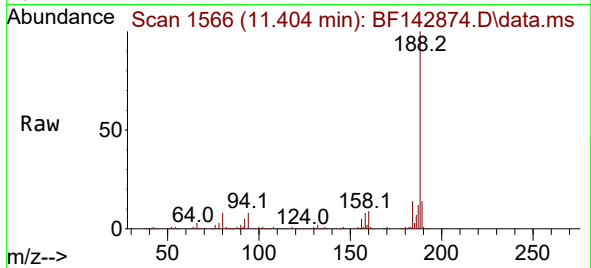

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.051 min Scan# 2016
Delta R.T. -0.006 min
Lab File: BF142874.D
Acq: 26 Jun 2025 18:05

Tgt Ion:240 Resp: 136110
Ion Ratio Lower Upper
240 100
120 9.4 8.2 12.2
236 24.1 19.8 29.8


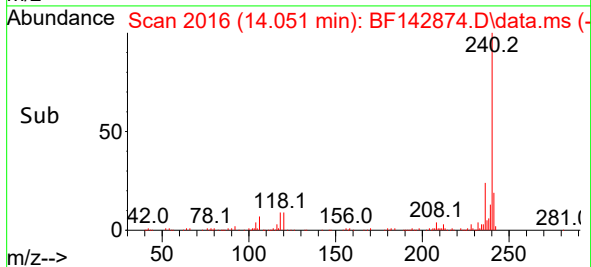
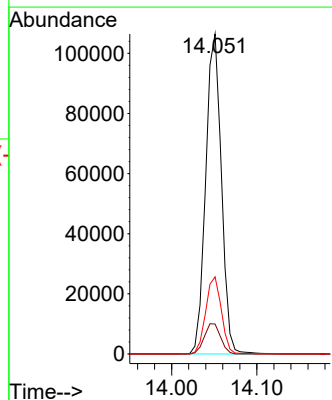
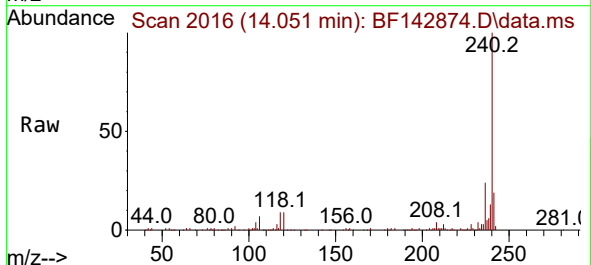




#79
 Terphenyl-d14
 Concen: 50.447 ng
 RT: 12.992 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF142874.D
 Acq: 26 Jun 2025 18:05

Instrument :
 BNA_F
 ClientSampleId :
 COMP-1

Tgt Ion:244 Resp: 496947
 Ion Ratio Lower Upper
 244 100
 212 6.5 5.4 8.0
 122 10.1 8.2 12.2

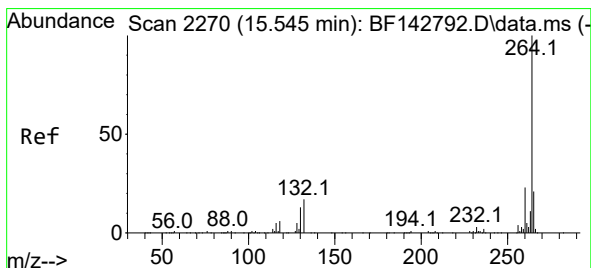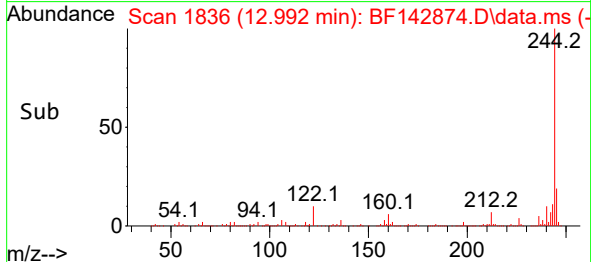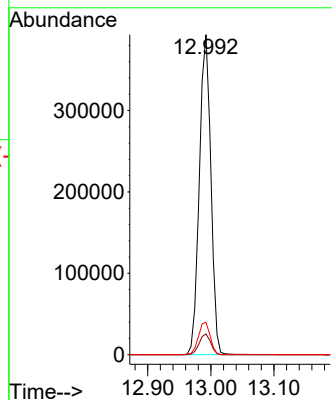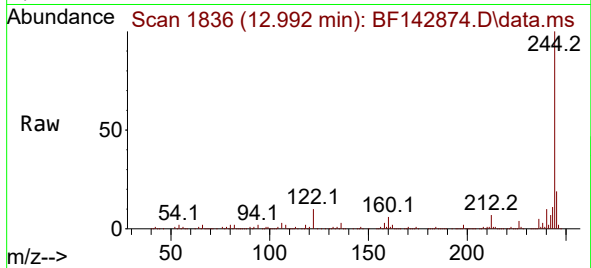

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.539 min Scan# 2269
 Delta R.T. -0.006 min
 Lab File: BF142874.D
 Acq: 26 Jun 2025 18:05

Tgt Ion:264 Resp: 163547
 Ion Ratio Lower Upper
 264 100
 260 22.5 18.1 27.1
 265 21.2 16.6 25.0

