


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062625\
Data File : BF142856.D
Acq On : 26 Jun 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 24 05:28:21 2025

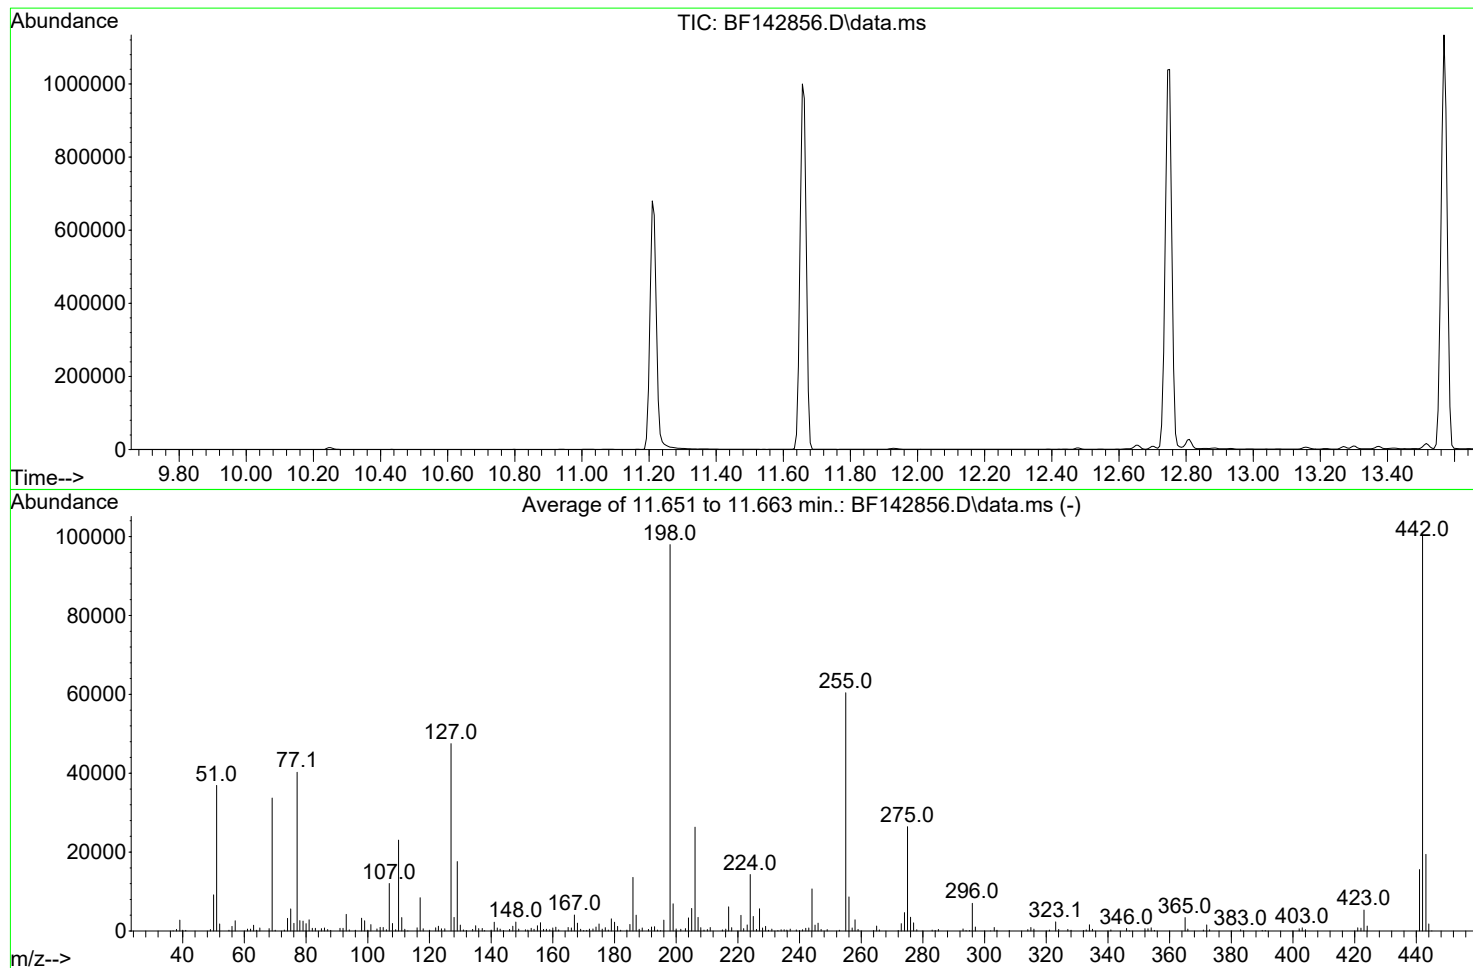

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	602	PASS
69	69	100	100	100.0	33723	PASS
70	69	0.00	2	0.6	189	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	97987	PASS
199	198	5	9	7.0	6886	PASS
365	198	1	100	3.5	3393	PASS
441	443	0.01	150	80.1	15571	PASS
442	442	100	100	100.0	100104	PASS
443	442	15	24	19.4	19440	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/26/2025	BNA_F	<u>BF142856.D</u>
Compound Name	Response	Retention Time
DDT	291948	13.568
DDD	5615	13.298
DDE	466	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6081	298029	2.04

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062625\
Data File : BF142856.D
Acq On : 26 Jun 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 26 11:10:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

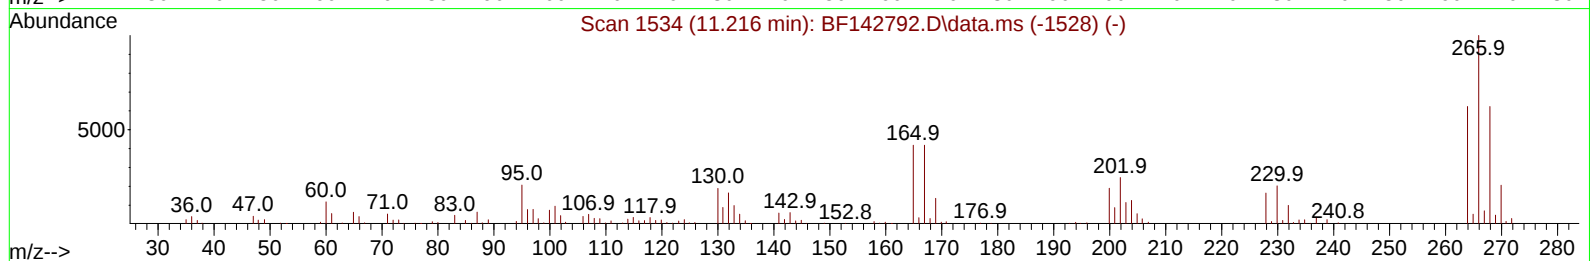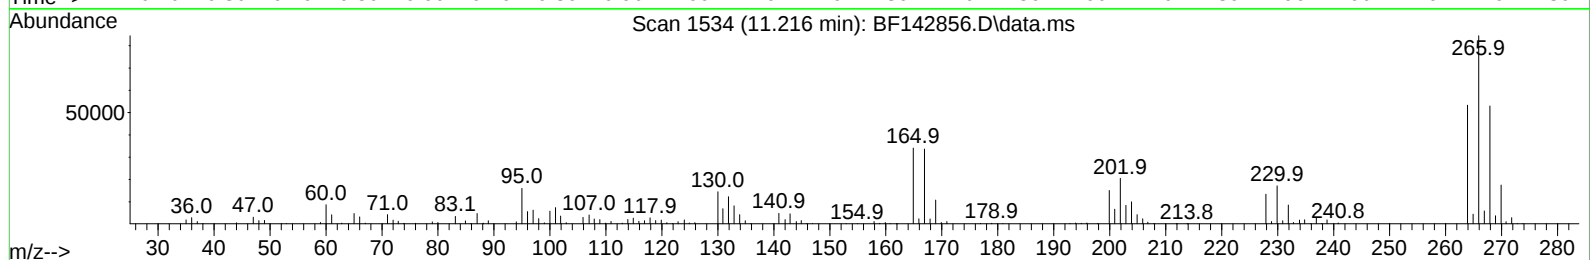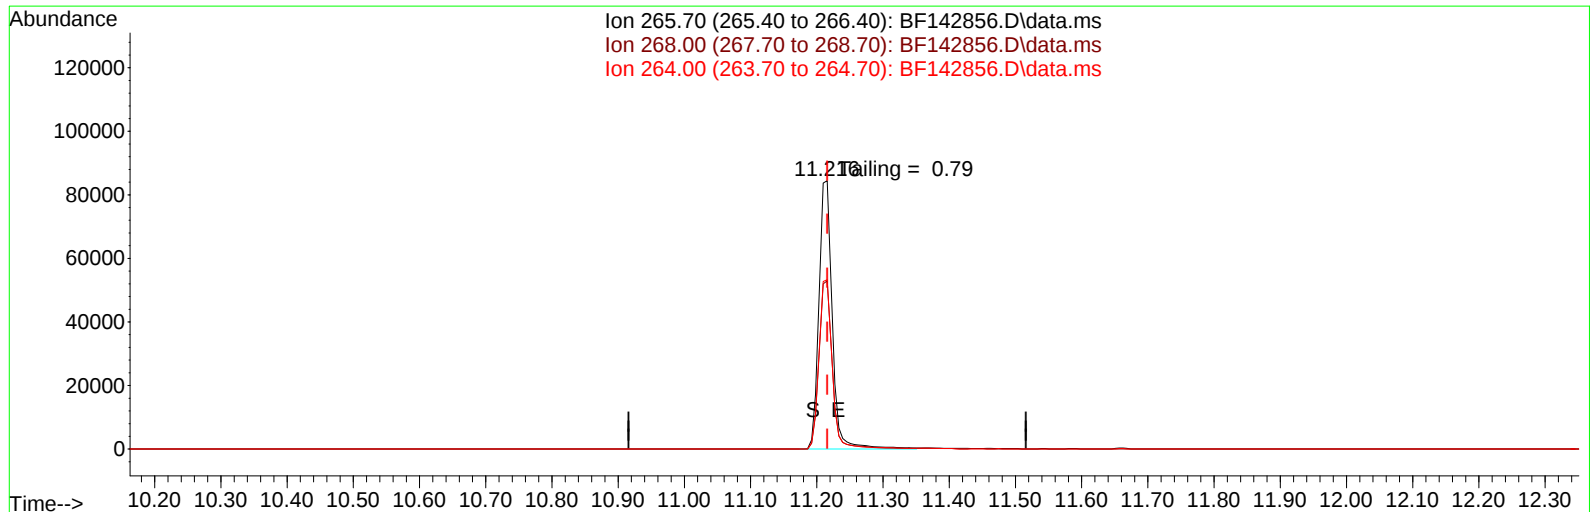

TIC: BF142856.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.000) 32945.90 ng




response 118961

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.68
264.00	62.40	63.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062625\
Data File : BF142856.D
Acq On : 26 Jun 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 26 11:10:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

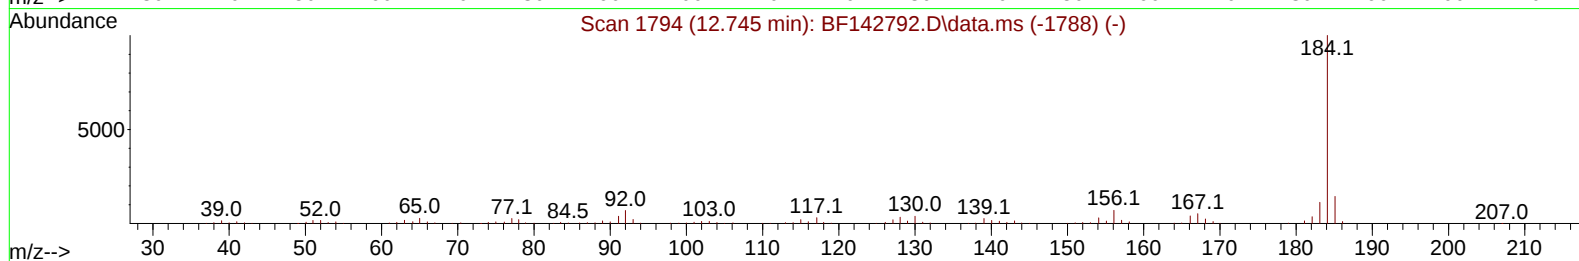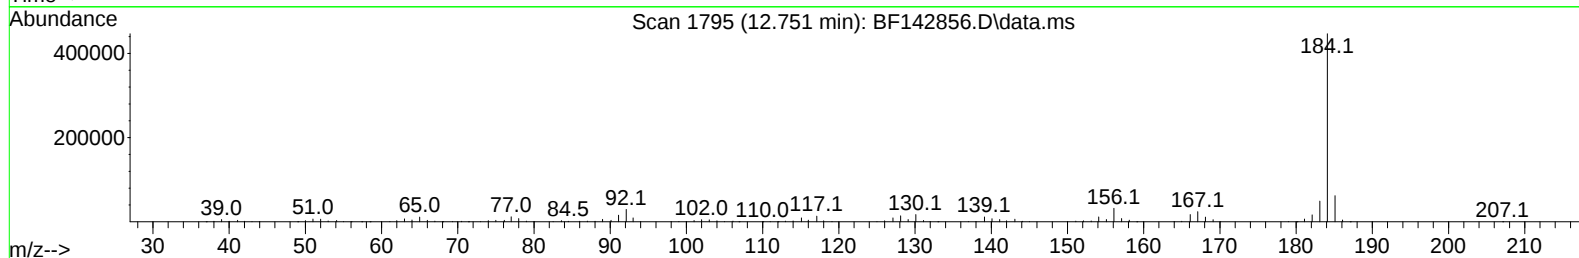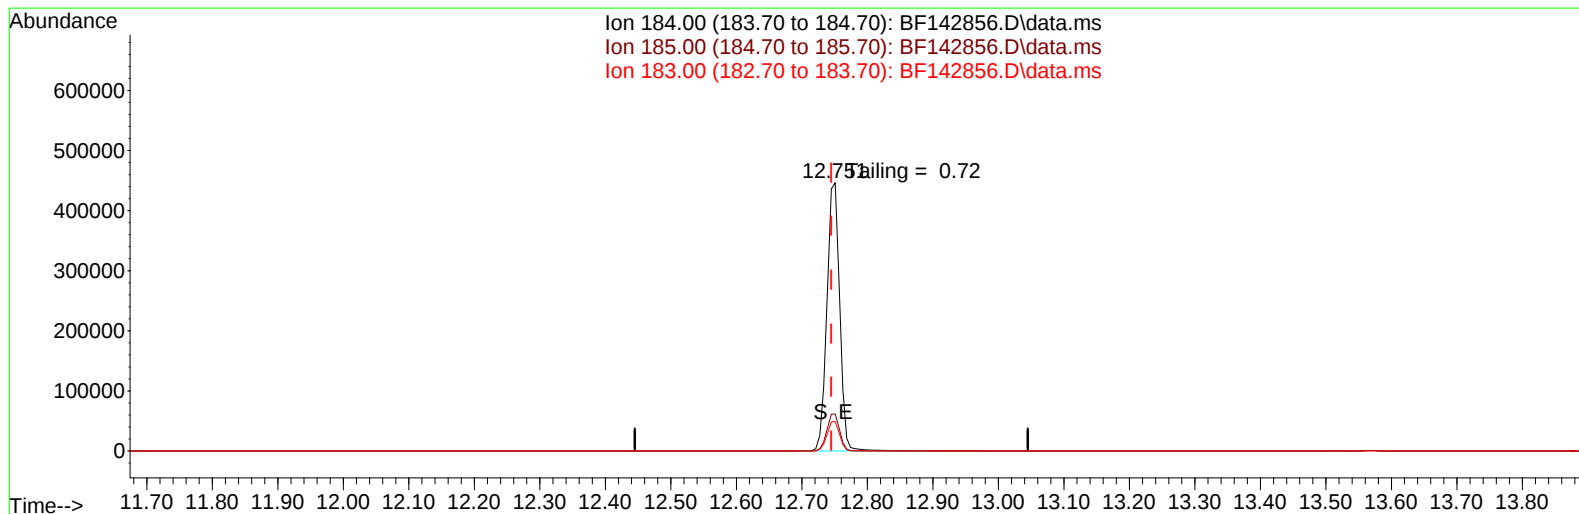

TIC: BF142856.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 0.00 ng

response 609276

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.87
183.00	11.20	11.04
0.00	0.00	0.00