

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062716\
 Data File : BF088462.D
 Acq On : 27 Jun 2016 20:25
 Operator : UM/SJ
 Sample : H3701-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TEC-COMP-B2B

Quant Time: Jun 28 06:27:51 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 19:14:18 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.54	152	71368	20.00	ng	-0.01
21) Naphthalene-d8	7.83	136	266547	20.00	ng	-0.01
38) Acenaphthene-d10	9.56	164	117805	20.00	ng	-0.02
63) Phenanthrene-d10	11.05	188	200598	20.00	ng	-0.01
75) Chrysene-d12	13.68	240	137460	20.00	ng	-0.01
86) Perylene-d12	15.03	264	149658	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.12	112	531225	127.25	ng	-0.01
7) Phenol-d6	6.20	99	646354	127.75	ng	-0.03
23) Nitrobenzene-d5	7.12	82	435855	95.49	ng	-0.02
41) 2,4,6-Tribromophenol	10.36	330	144055	115.81	ng	-0.01
44) 2-Fluorobiphenyl	8.90	172	680646	91.17	ng	-0.02
78) Terphenyl-d14	12.63	244	451669	74.77	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.31	163	179825	21.07	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062716\
Data File : BF088462.D
Acq On : 27 Jun 2016 20:25
Operator : UM/SJ
Sample : H3701-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEC-COMP-B2B

Quant Time: Jun 28 06:27:51 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 19:14:18 2016
Response via : Initial Calibration

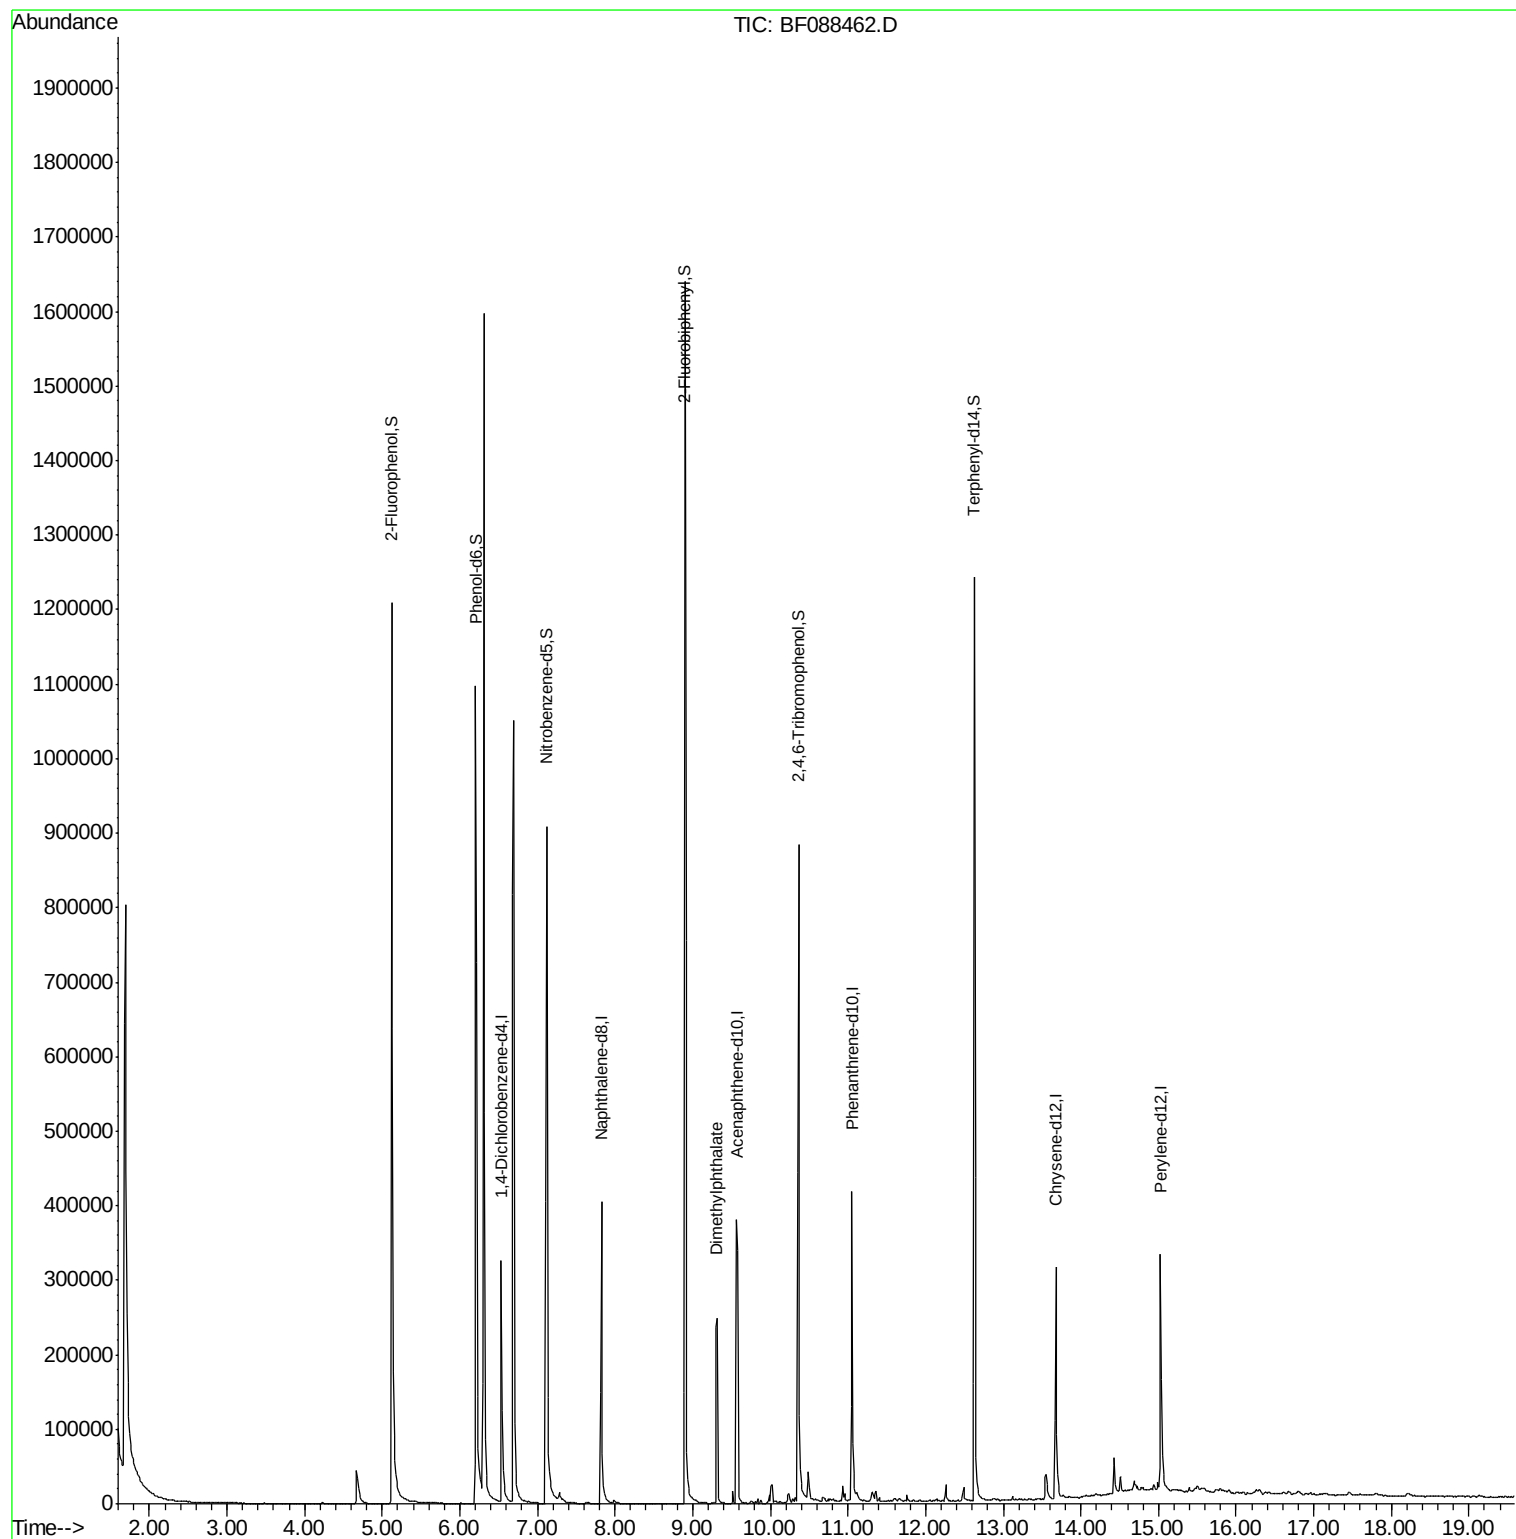

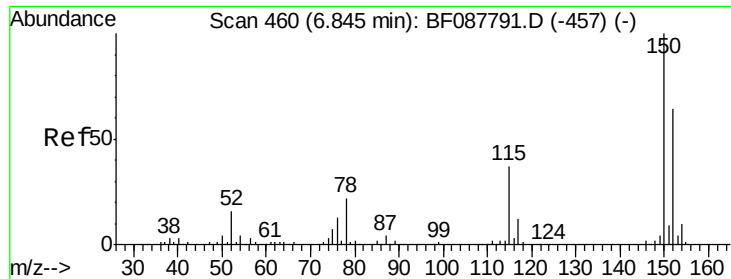


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.54 min Scan# 433
Delta R.T. -0.01 min
Lab File: BF088462.D
Acq: 27 Jun 2016 20:25

Instrument :
BNA_F
ClientSampleId :
TEC-COMP-B2B

Tot Ion:152 Resp: 71368
Ion Ratio Lower Upper
152 100
150 158.9 123.8 185.6
115 63.2 39.6 59.4#

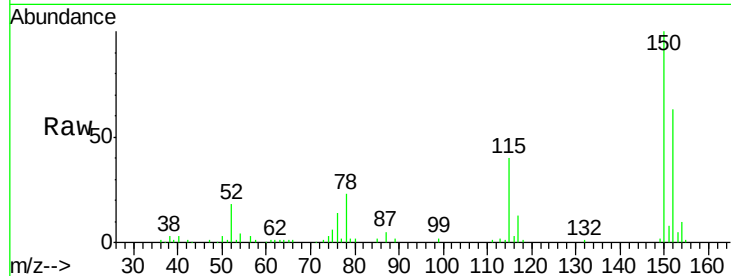


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

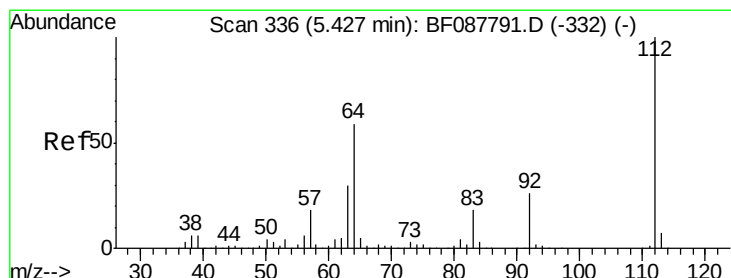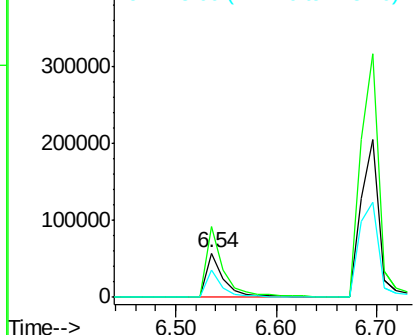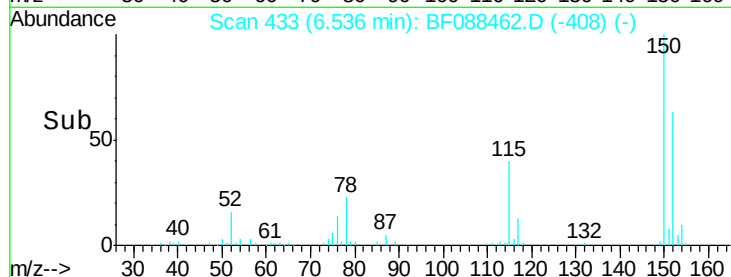



#5


2-Fluorophenol
Concen: 127.25 ng
RT: 5.12 min Scan# 309
Delta R.T. -0.01 min
Lab File: BF088462.D
Acq: 27 Jun 2016 20:25

Tgt Ion:112 Resp: 531225
Ion Ratio Lower Upper
112 100
64 56.1 42.2 63.2
63 29.3 21.8 32.8

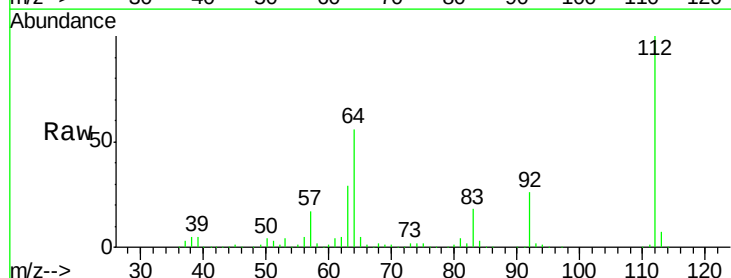

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

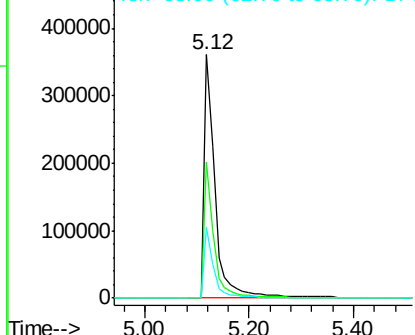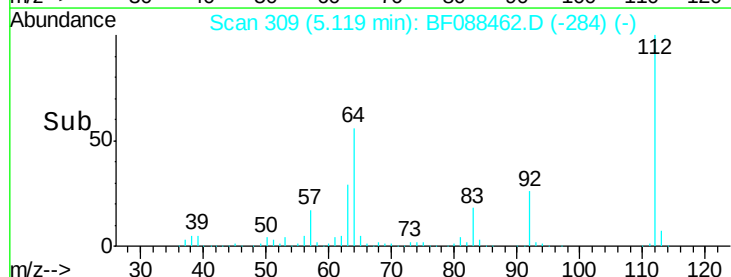

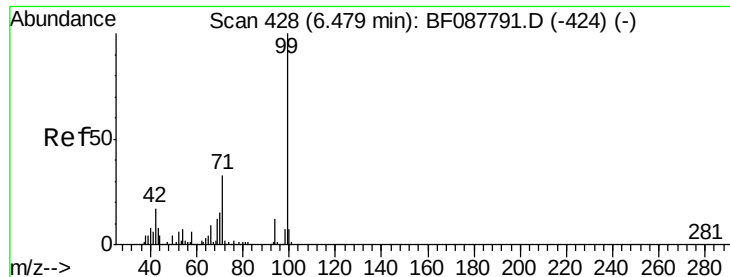

#7

Phenol-d6

Concen: 127.75 ng

RT: 6.20 min Scan# 404

Delta R.T. -0.03 min

Lab File: BF088462.D

Acq: 27 Jun 2016 20:25

Instrument :

BNA_F

ClientSampleId :

TEC-COMP-B2B


Tot Ion: 99 Resp: 646354

Ion Ratio Lower Upper

99 100

42 15.2 12.2 18.2




71 34.5 23.4 35.0

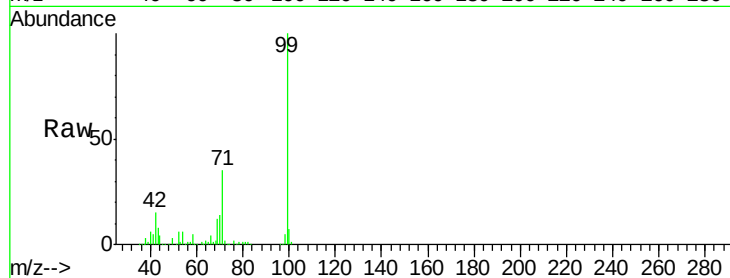

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

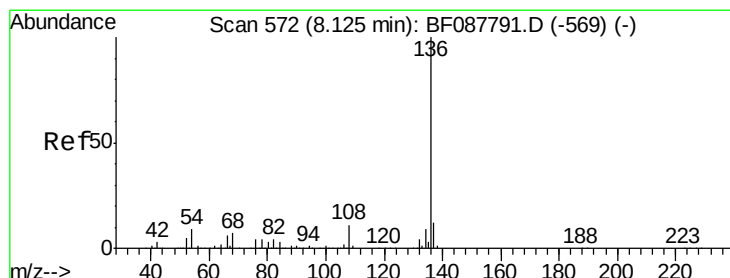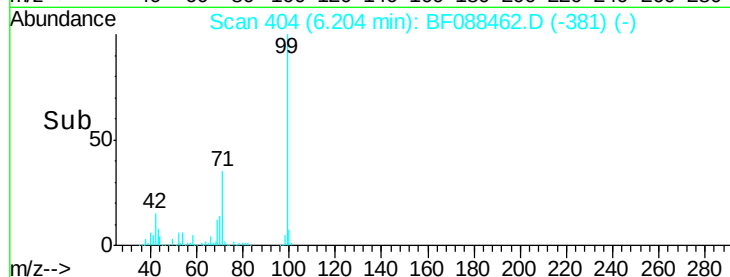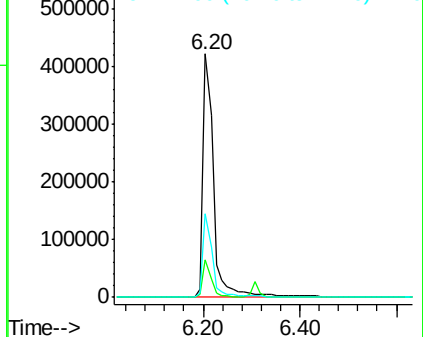

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.83 min Scan# 546

Delta R.T. -0.01 min

Lab File: BF088462.D

Acq: 27 Jun 2016 20:25

Tgt Ion: 136 Resp: 266547


Ion Ratio Lower Upper

136 100

137 10.4 9.1 13.7

54 5.1 6.6 10.0#

68 4.5 5.1 7.7#


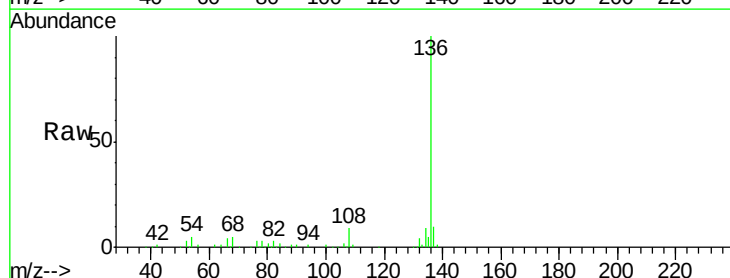



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

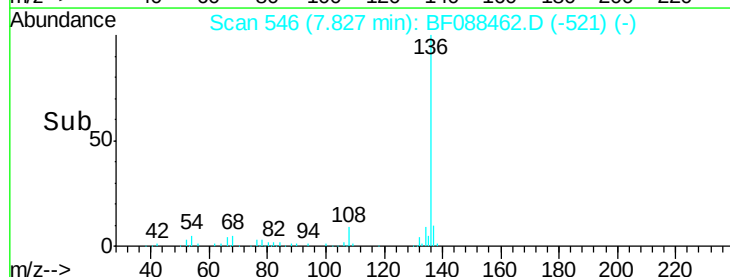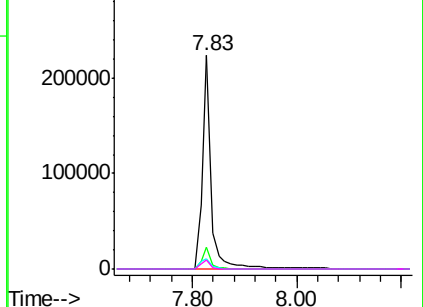


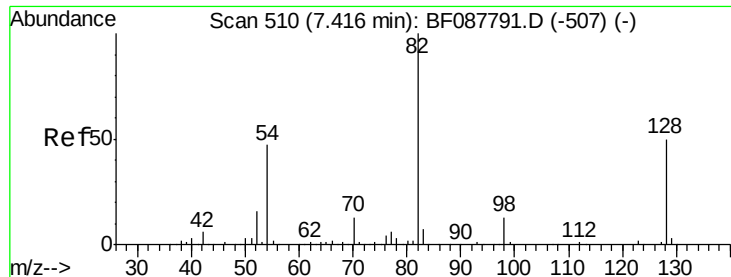




#23
Nitrobenzene-d5
Concen: 95.49 ng
RT: 7.12 min Scan# 484
Delta R.T. -0.02 min
Lab File: BF088462.D
Acq: 27 Jun 2016 20:25

Instrument :
BNA_F
ClientSampleId :
TEC-COMP-B2B

Tot Ion: 82 Resp: 435855
Ion Ratio Lower Upper
82 100
128 51.5 35.9 53.9
54 41.4 40.9 61.3

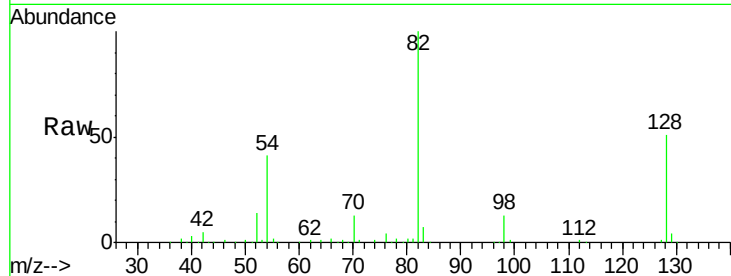


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

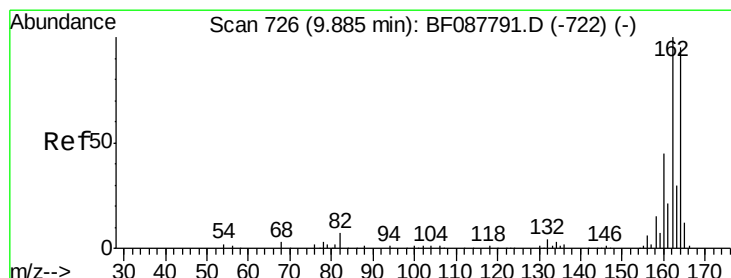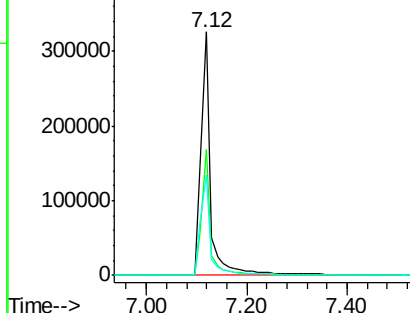
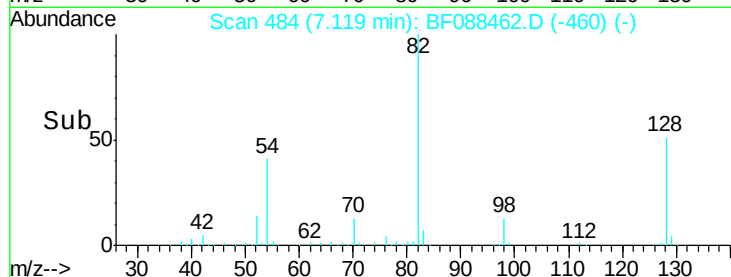



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.56 min Scan# 698
Delta R.T. -0.02 min
Lab File: BF088462.D
Acq: 27 Jun 2016 20:25

Tgt Ion:164 Resp: 117805
Ion Ratio Lower Upper
164 100
162 103.7 85.4 128.2
160 46.1 39.5 59.3

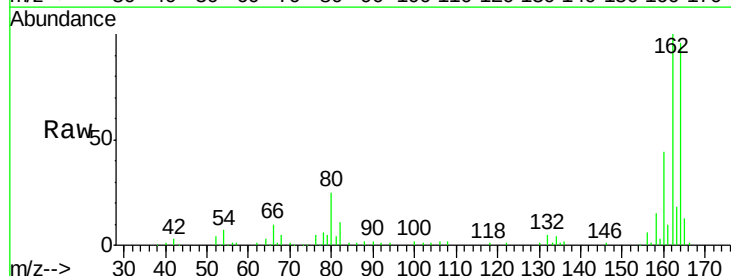

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

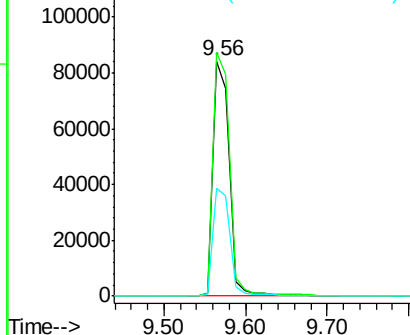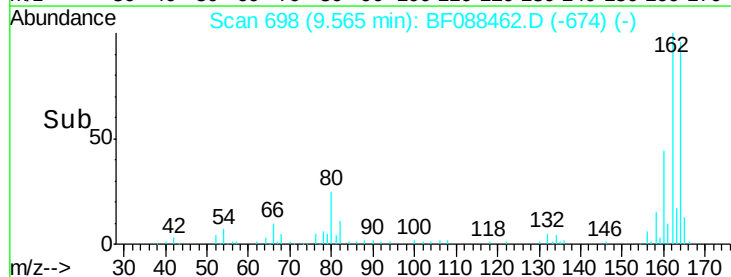


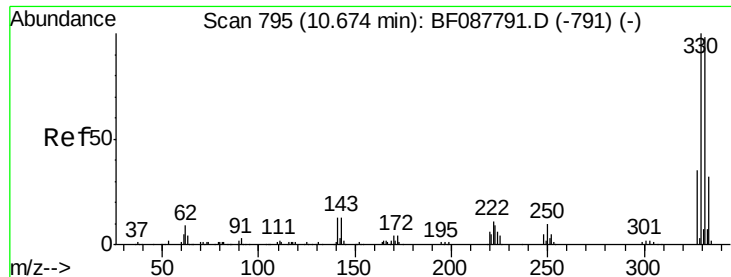




#41
 2,4,6-Tribromophenol
 Concen: 115.81 ng
 RT: 10.36 min Scan# 768
 Delta R.T. -0.01 min
 Lab File: BF088462.D
 Acq: 27 Jun 2016 20:25

Instrument :
 BNA_F
 ClientSampleId :
 TEC-COMP-B2B

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.1	0.0	0.0#
141	37.4	0.0	0.0#

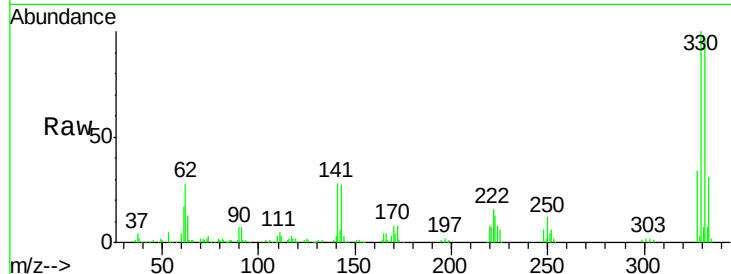


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

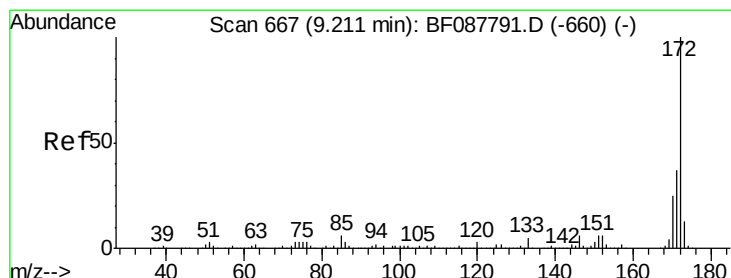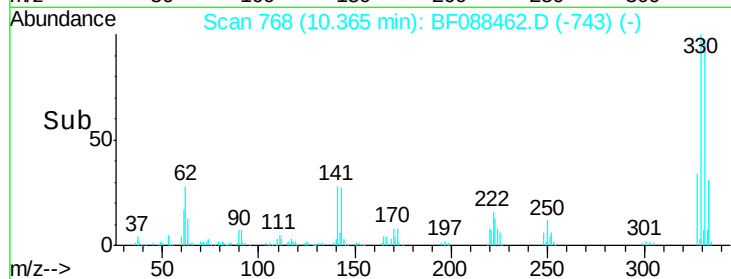
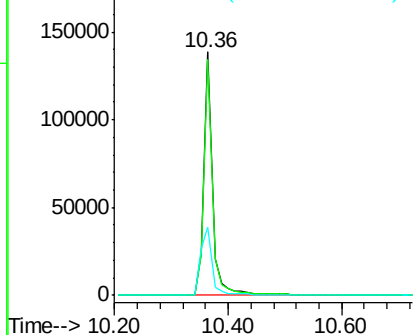



#44
 2-Fluorobiphenyl
 Concen: 91.17 ng
 RT: 8.90 min Scan# 640
 Delta R.T. -0.02 min
 Lab File: BF088462.D
 Acq: 27 Jun 2016 20:25

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.1	28.6	43.0
170	23.8	19.2	28.8

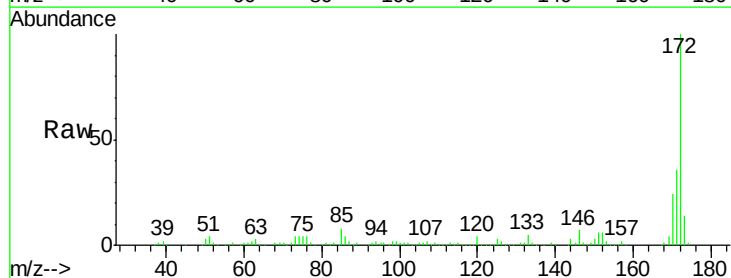

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

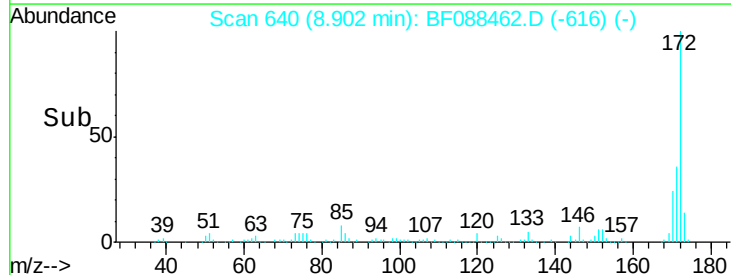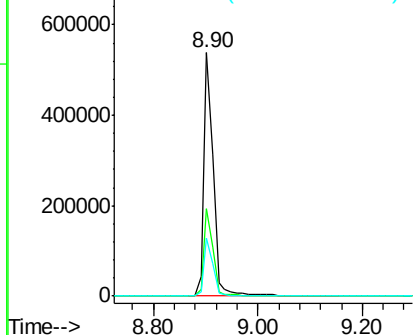

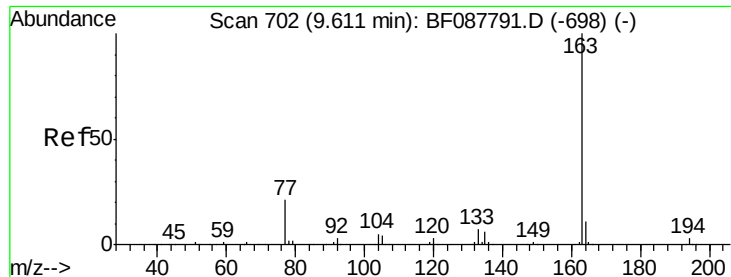

#49

Dimethylphthalate

Concen: 21.07 ng

RT: 9.31 min Scan# 676

Delta R.T. -0.02 min

Lab File: BF088462.D

Acq: 27 Jun 2016 20:25

Instrument :

BNA_F

ClientSampleId :

TEC-COMP-B2B


Tot Ion:163 Resp: 179825

Ion Ratio Lower Upper

163 100

194 3.7 2.8 4.2




164 9.4 8.3 12.5

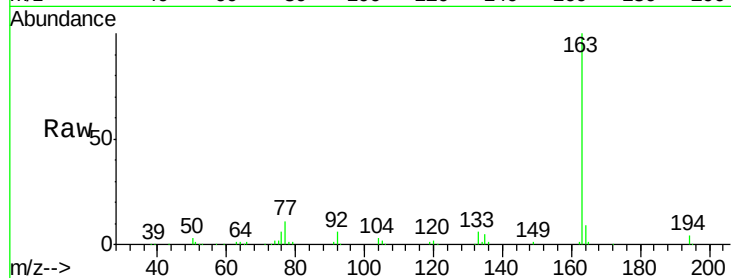

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

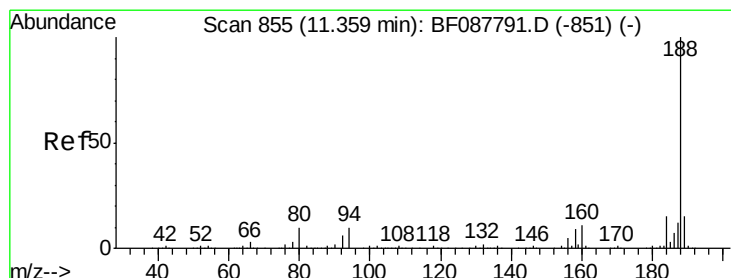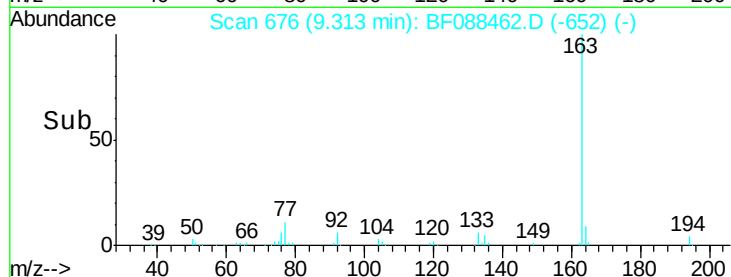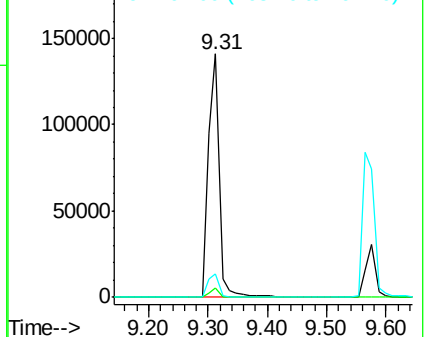

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.05 min Scan# 828

Delta R.T. -0.01 min

Lab File: BF088462.D

Acq: 27 Jun 2016 20:25


Tgt Ion:188 Resp: 200598

Ion Ratio Lower Upper

188 100

94 8.3 9.0 13.6#



80 8.6 10.0 15.0#

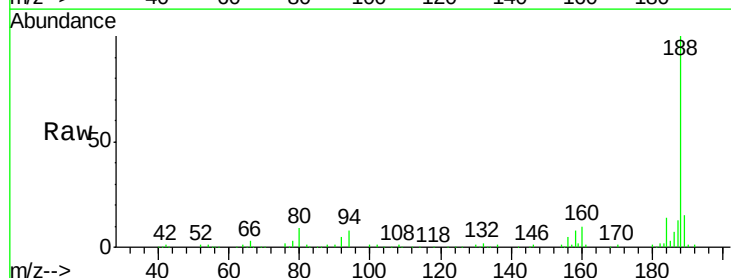


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

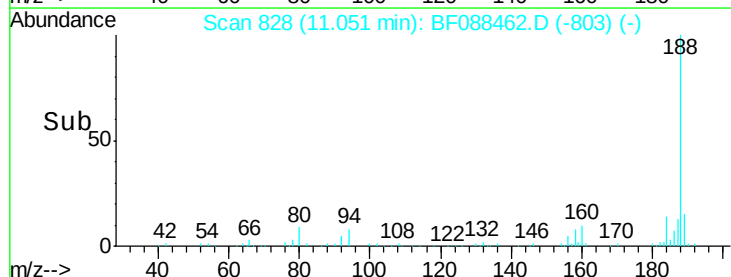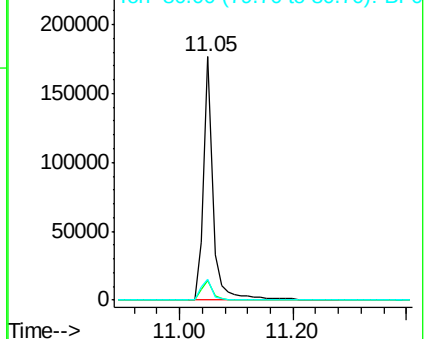

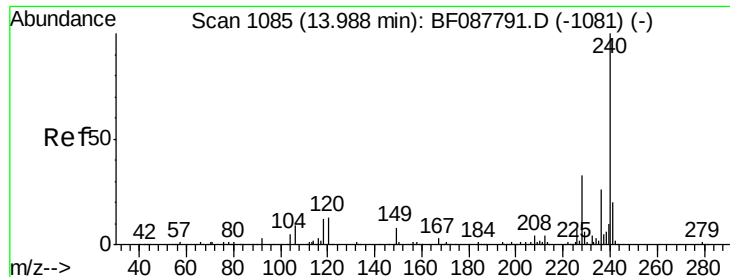

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.68 min Scan# 1058

Delta R.T. -0.01 min

Lab File: BF088462.D

Acq: 27 Jun 2016 20:25

Instrument :

BNA_F

ClientSampleId :

TEC-COMP-B2B


Tot Ion:240 Resp: 137460

Ion Ratio Lower Upper

240 100

120 11.0 6.8 10.2#




236 25.5 20.2 30.2

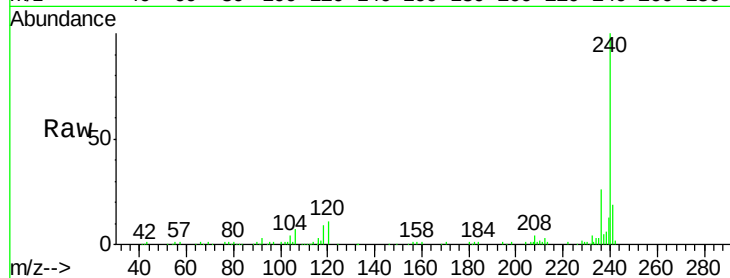

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

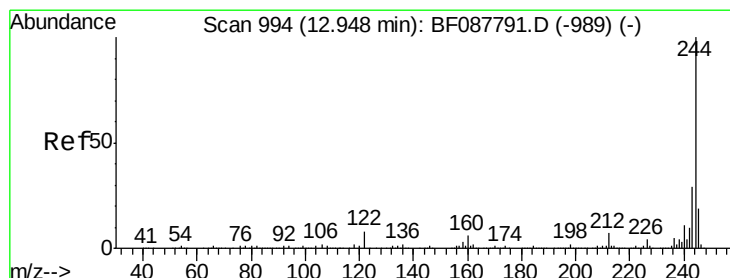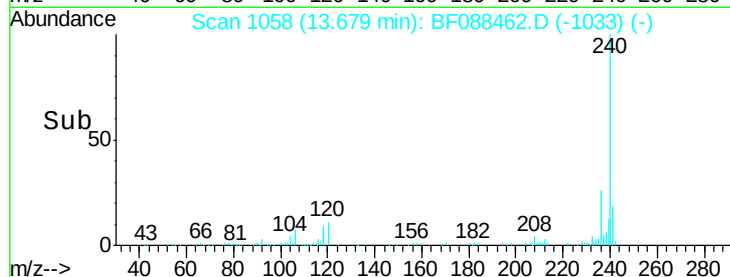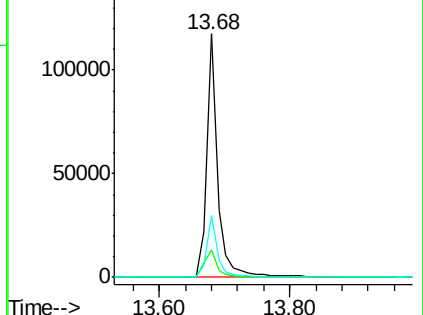

#78

Terphenyl-d14

Concen: 74.77 ng

RT: 12.63 min Scan# 966

Delta R.T. -0.01 min

Lab File: BF088462.D

Acq: 27 Jun 2016 20:25


Tgt Ion:244 Resp: 451669

Ion Ratio Lower Upper

244 100

212 7.7 6.0 9.0



122 15.4 11.2 16.8

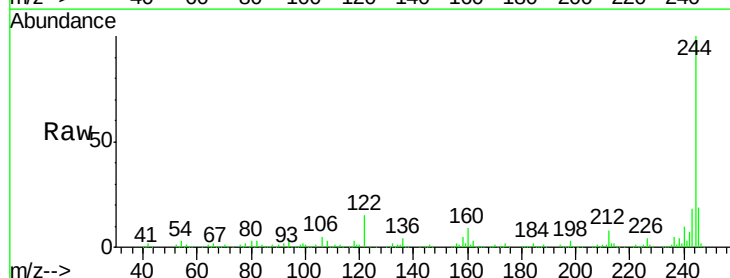


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

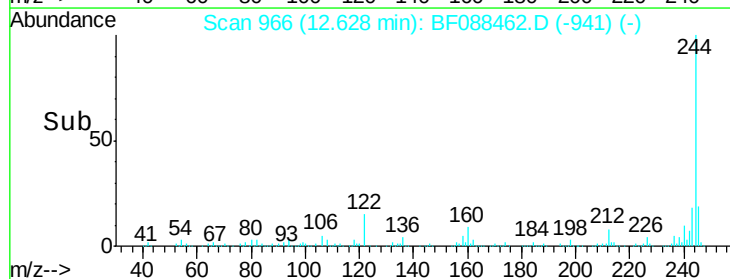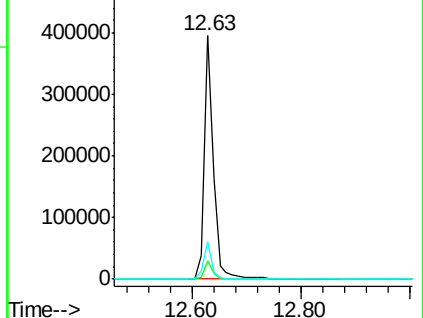


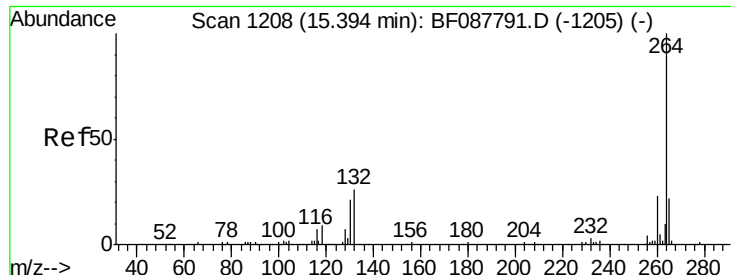

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.03 min Scan# 1176
 Delta R.T. -0.01 min
 Lab File: BF088462.D
 Acq: 27 Jun 2016 20:25

Instrument :
 BNA_F
 ClientSampleId :
 TEC-COMP-B2B

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.0	19.2	28.8
265	21.6	16.9	25.3

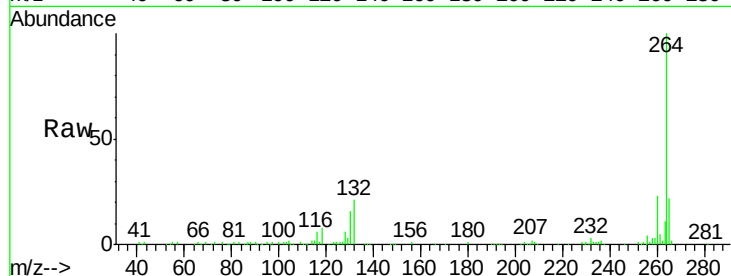

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

