


Data Path : Z:\HPCHEM1\BNA F\DATA\BF062716\
 Data File : BF088455.D
 Acq On : 27 Jun 2016 15:14
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 28 05:25:55 2016

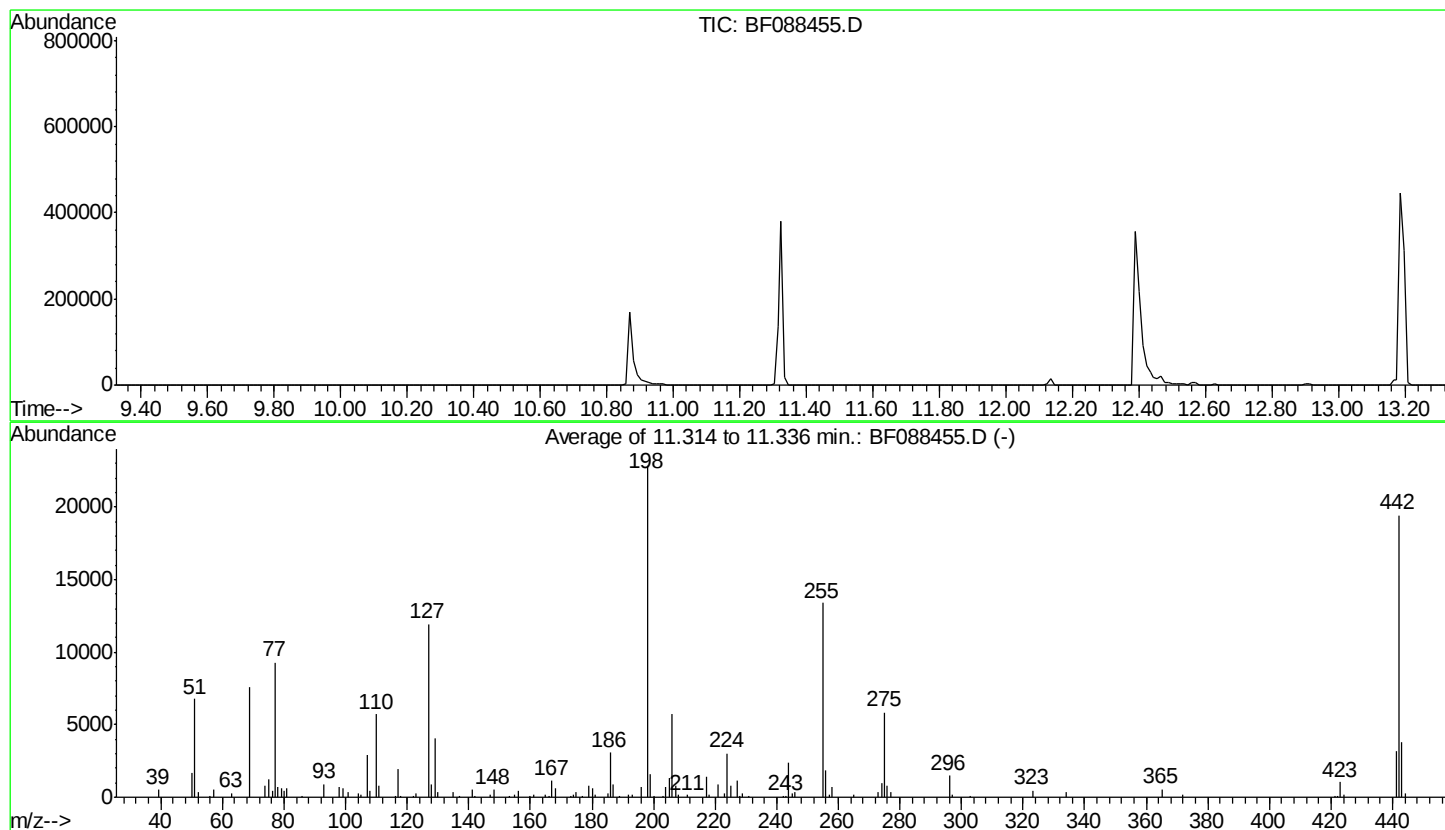

AutoFind: Scans 851, 852, 853; Background Corrected with Scan 847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	6794	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.1	7565	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.2	11925	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22857	PASS
199	198	5	9	6.8	1551	PASS
275	198	10	60	25.7	5869	PASS
365	198	1	100	2.5	576	PASS
441	442	0.01	24	16.3	3162	PASS
442	198	50	100	85.1	19453	PASS
443	442	15	24	19.7	3825	PASS