


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062716\
 Data File : BF088475.D
 Acq On : 28 Jun 2016 3:56
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 28 05:25:55 2016

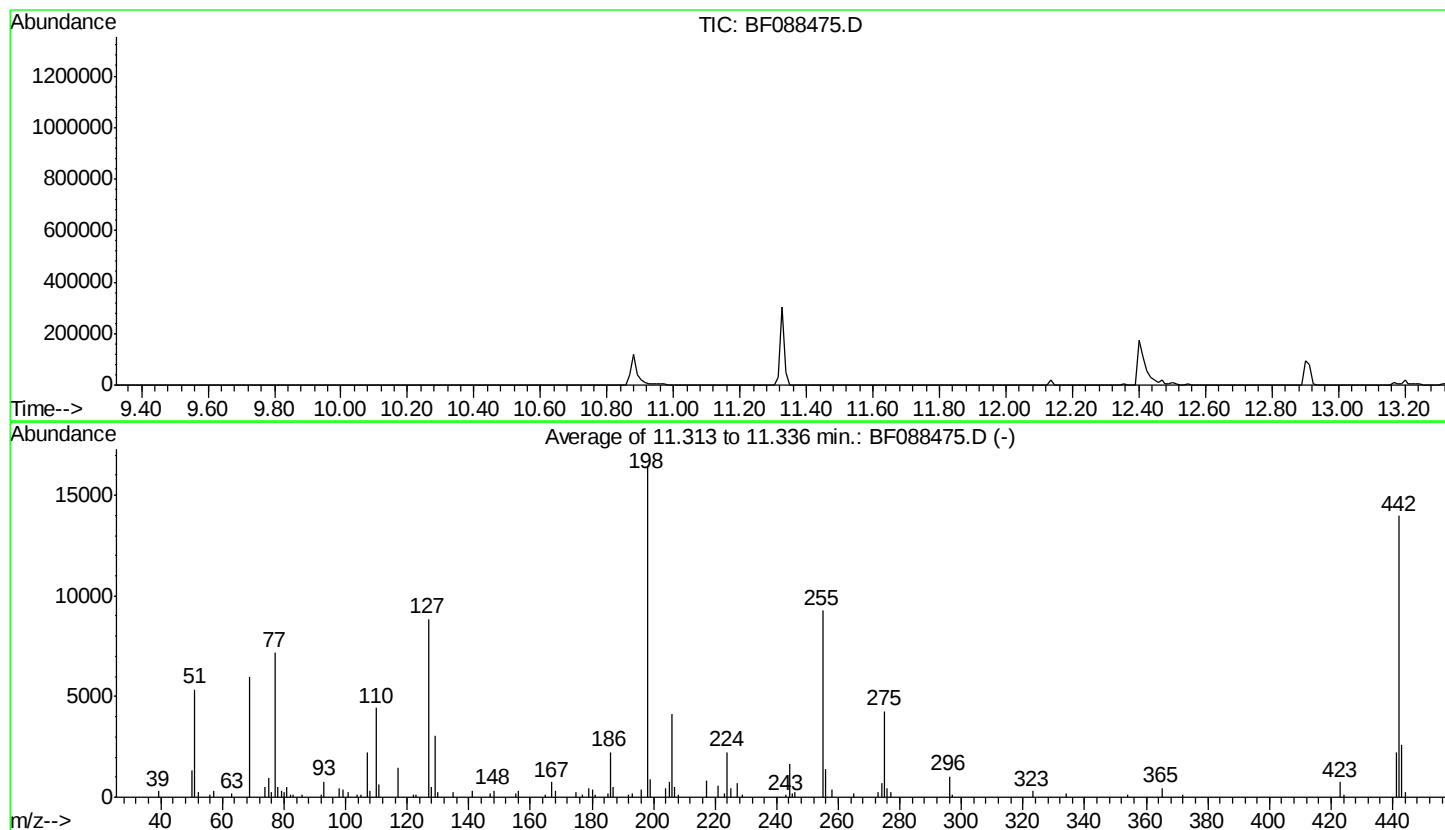

AutoFind: Scans 851, 852, 853; Background Corrected with Scan 848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	5373	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.2	5965	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.8	8861	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16471	PASS
199	198	5	9	5.5	912	PASS
275	198	10	60	26.0	4280	PASS
365	198	1	100	2.9	475	PASS
441	442	0.01	24	16.0	2231	PASS
442	198	50	100	84.8	13971	PASS
443	442	15	24	18.7	2608	PASS