

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062717\
 Data File : BF096240.D
 Acq On : 28 Jun 2017 2:20
 Operator : SJ/MA
 Sample : I3870-02DL 100X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jun 28 04:12:12 2017
 Quant Method : Z:\HPCHEM1\BNA F\Methods\8270-BF062717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 27 15:17:15 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.78	152	154836	20.00	ng	0.00
21) Naphthalene-d8	8.06	136	579545	20.00	ng	0.00
38) Acenaphthene-d10	9.82	164	207139	20.00	ng	0.00
63) Phenanthrene-d10	11.29	188	334232	20.00	ng	0.00
75) Chrysene-d12	13.92	240	285716	20.00	ng	0.00
86) Perylene-d12	15.34	264	197194	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.39	112	1073	0.10	ng	0.00
7) Phenol-d6	6.40	99	2164	0.17	ng	0.00
23) Nitrobenzene-d5	7.33	82	7289	0.87	ng	-0.02
41) 2,4,6-Tribromophenol	10.59	330	290	0.18	ng	0.00
44) 2-Fluorobiphenyl	9.13	172	14417	1.27	ng	-0.02
78) Terphenyl-d14	12.87	244	10255	0.90	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	6.31	77	2326	Below Cal		# 1
27) 2,4-Dimethylphenol	7.72	122	51346	5.98	ng	92
31) Naphthalene	8.09	128	1388679	49.72	ng	100
32) Benzoic acid	7.91	122	5830	9.57	ng	# 14
33) 4-Chloroaniline	8.09	127	183796	15.90	ng	# 32
37) 2-Methylnaphthalene	8.77	142	70842	3.90	ng	95
50) 2,6-Dinitrotoluene	9.82	165	25488	8.27	ng	# 34
56) 2,4-Dinitrotoluene	9.82	165	25488	6.56	ng	# 33
70) Phenanthrene	11.32	178	15277	Below Cal		97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062717\
Data File : BF096240.D
Acq On : 28 Jun 2017 2:20
Operator : SJ/MA
Sample : I3870-02DL 100X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jun 28 04:12:12 2017
Quant Method : Z:\HPCHEM1\BNA F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 27 15:17:15 2017
Response via : Initial Calibration

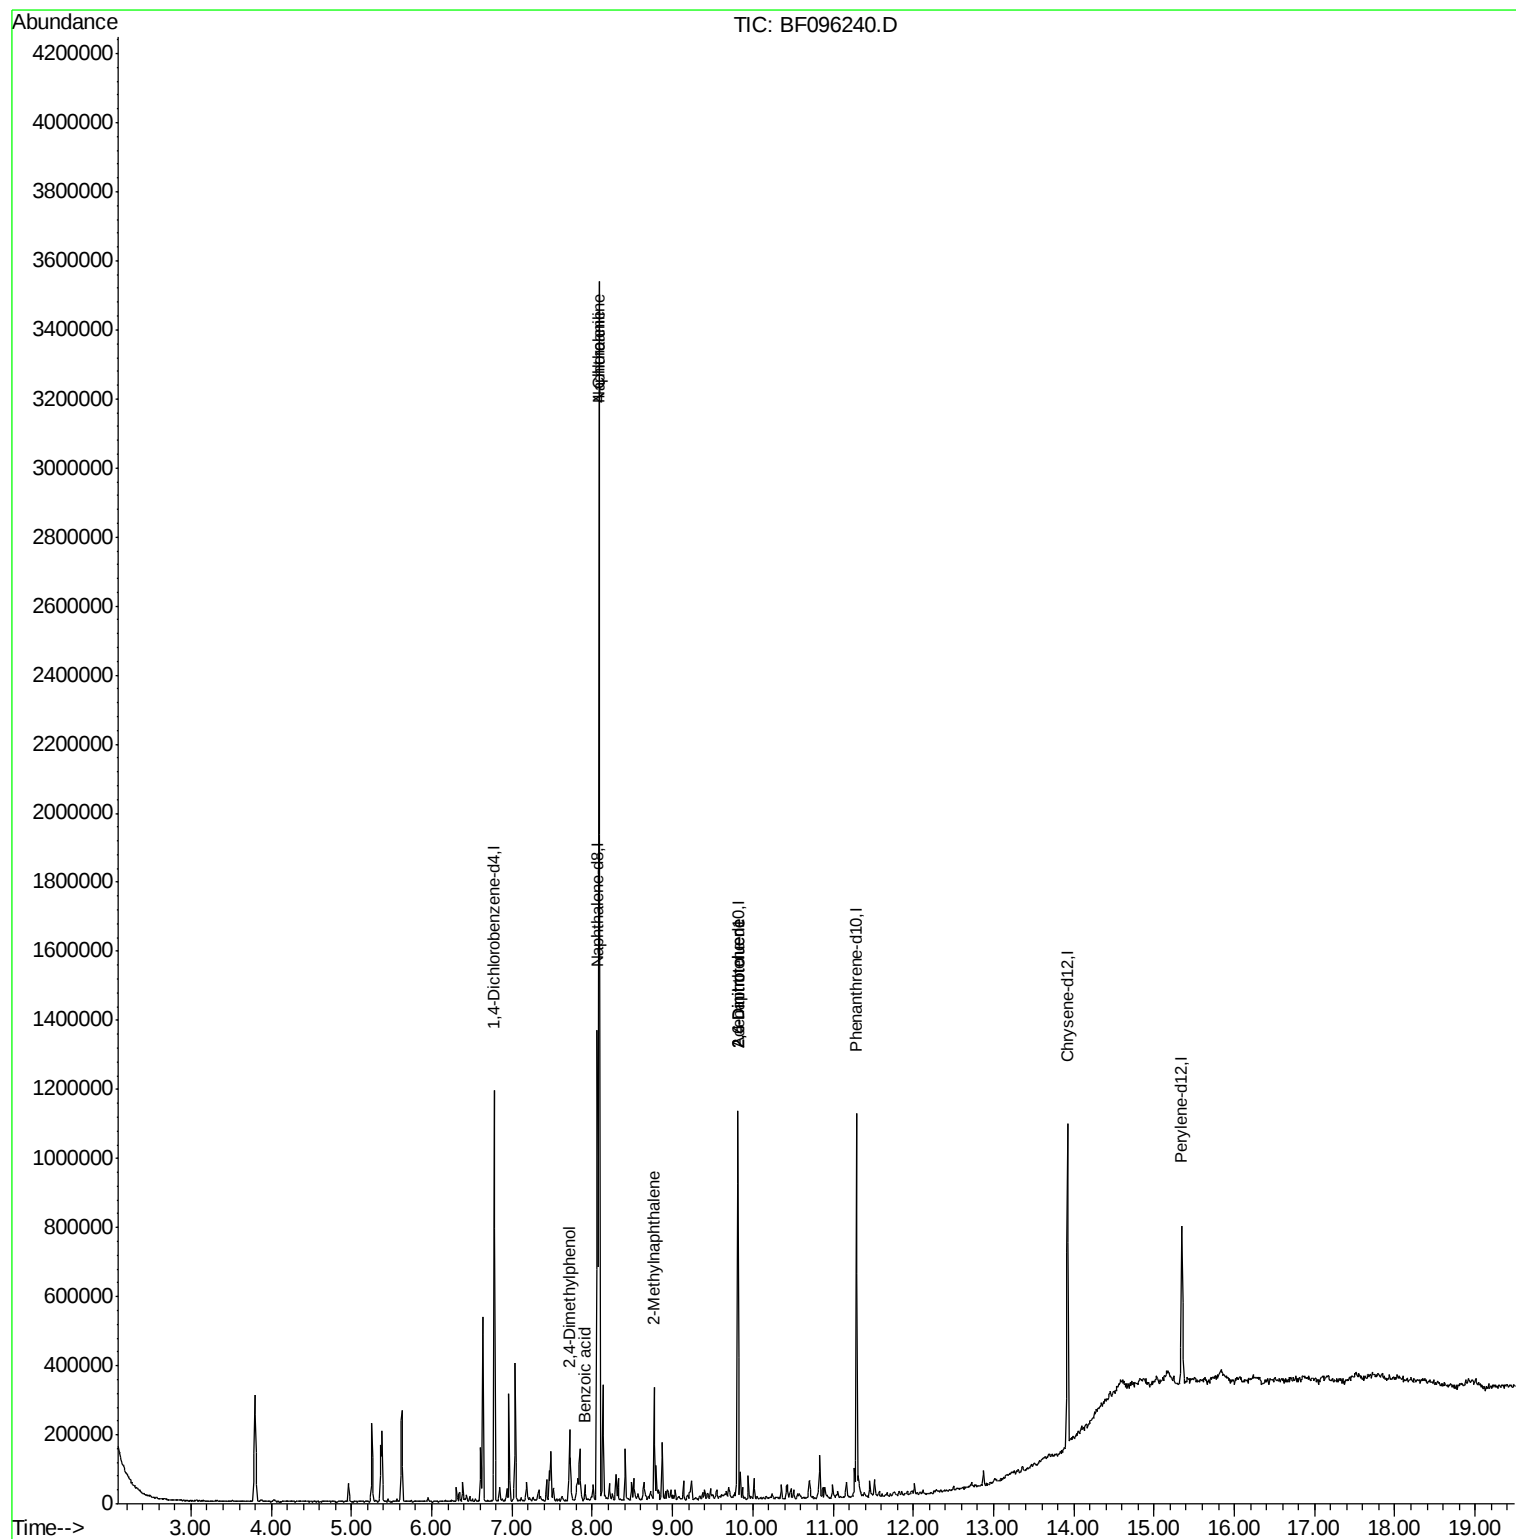

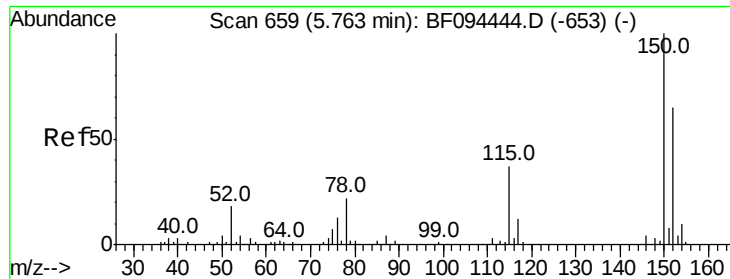


#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.78 min Scan# 798
Delta R.T. -0.00 min
Lab File: BF096240.D
Acq: 28 Jun 2017 2:20

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 154836
Ion Ratio Lower Upper
152 100
150 157.3 126.2 189.2
115 66.4 52.2 78.2

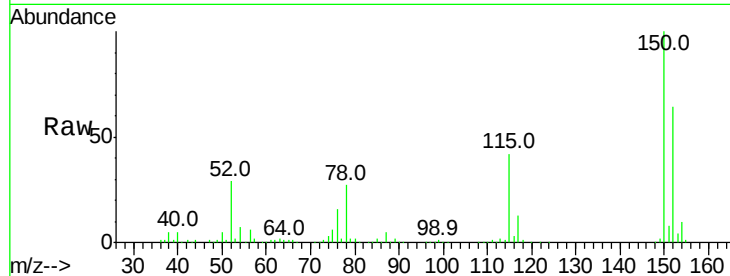


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

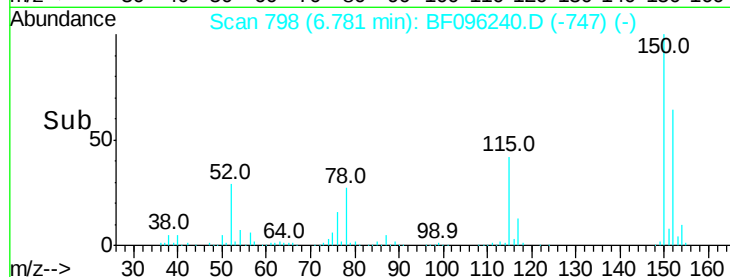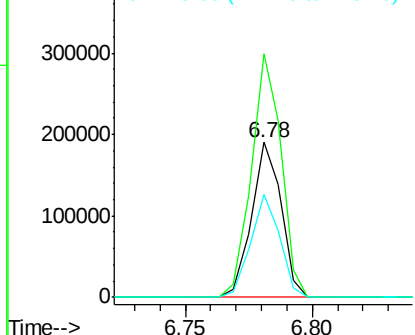



#5


2-Fluorophenol
Concen: 0.10 ng
RT: 5.39 min Scan# 561
Delta R.T. 0.01 min
Lab File: BF096240.D
Acq: 28 Jun 2017 2:20

Tgt Ion:112 Resp: 1073
Ion Ratio Lower Upper
112 100
64 101.7 46.0 69.0#
63 254.4 23.4 35.0#

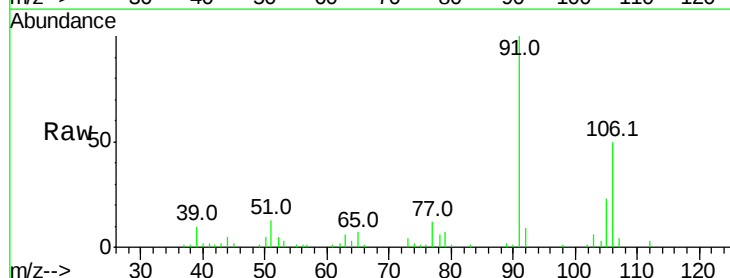

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

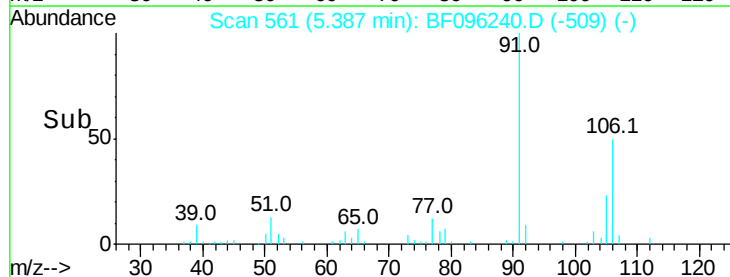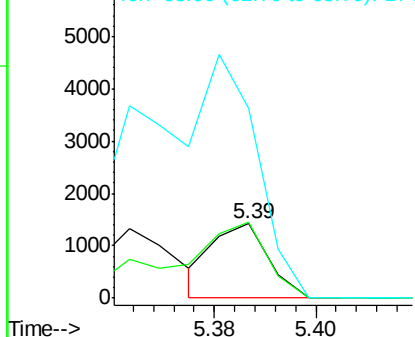

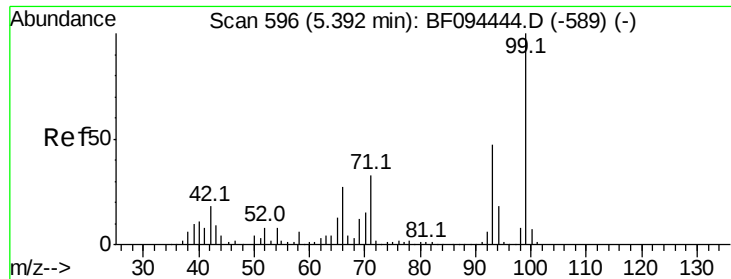

#7

Phenol-d6

Concen: 0.17 ng

RT: 6.40 min Scan# 733

Delta R.T. 0.01 min

Lab File: BF096240.D

Acq: 28 Jun 2017 2:20

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 2164

Ion Ratio Lower Upper

99 100

42 25.6 13.5 20.3#




71 38.6 24.5 36.7#



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

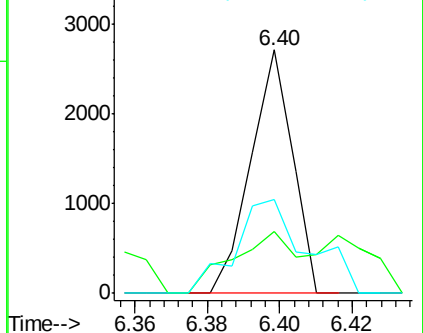

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.06 min Scan# 1016

Delta R.T. 0.01 min

Lab File: BF096240.D

Acq: 28 Jun 2017 2:20

Tgt Ion: 136 Resp: 579545


Ion Ratio Lower Upper

136 100

137 11.1 8.5 12.7

54 11.2 4.9 7.3#

68 7.1 4.1 6.1#





Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0




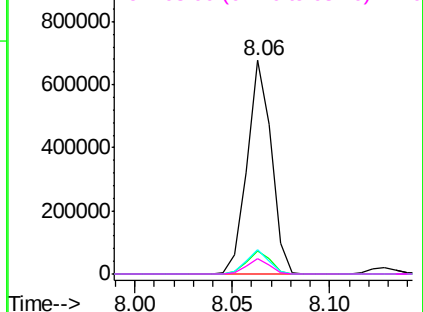




#23
Nitrobenzene-d5
Concen: 0.87 ng
RT: 7.33 min Scan# 892
Delta R.T. -0.02 min
Lab File: BF096240.D
Acq: 28 Jun 2017 2:20




Instrument :
BNA_F
ClientSampleId :


Tot Ion	82	Resp	7289
Ion Ratio	100	Lower	Upper
128	36.0	34.0	51.0
54	65.6	42.2	63.2#

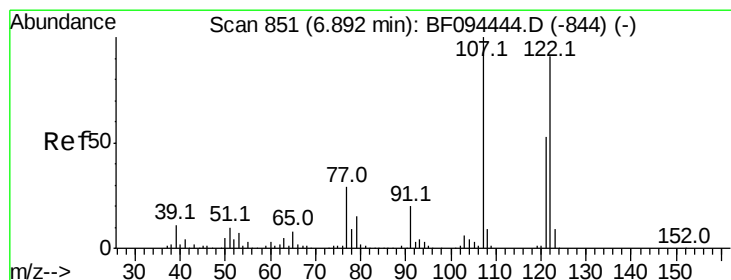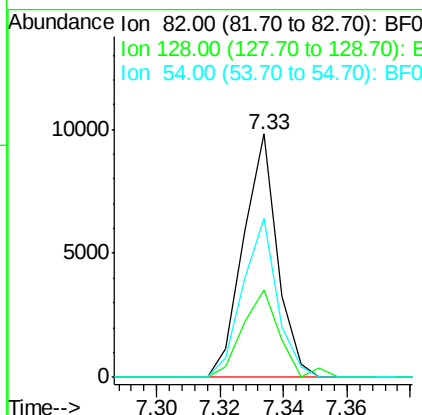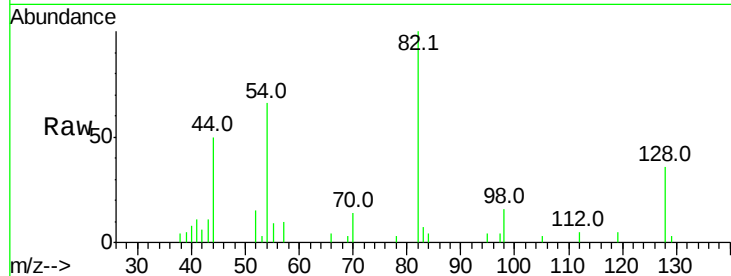

#27
2,4-Dimethylphenol
Concen: 5.98 ng
RT: 7.72 min Scan# 957
Delta R.T. 0.01 min
Lab File: BF096240.D
Acq: 28 Jun 2017 2:20

Tgt Ion	122	Resp	51346
Ion Ratio <td>100</td> <td>Lower</td> <td>Upper</td>	100	Lower	Upper
107	99.6	89.2	133.8
121	58.3	45.2	67.8

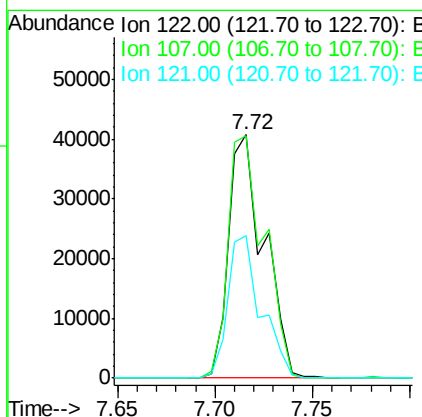

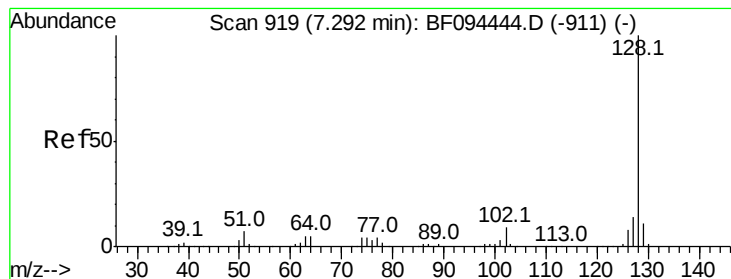

#31

Naphthalene

Concen: 49.72 ng

RT: 8.09 min Scan# 1020

Delta R.T. 0.01 min

Lab File: BF096240.D

Acq: 28 Jun 2017 2:20

Instrument :

BNA_F

ClientSampleId :


Tot Ion:128 Resp: 1388679

Ion Ratio Lower Upper

128 100

129 11.1 9.0 13.6




127 13.3 10.8 16.2



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

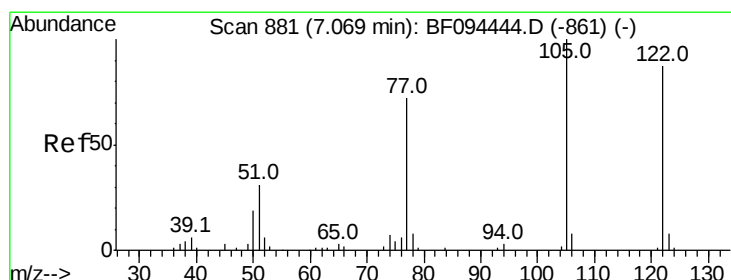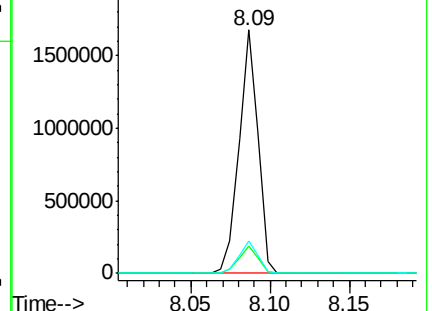

#32

Benzoic acid

Concen: 9.57 ng

RT: 7.91 min Scan# 990

Delta R.T. 0.02 min

Lab File: BF096240.D

Acq: 28 Jun 2017 2:20


Tgt Ion:122 Resp: 5830

Ion Ratio Lower Upper

122 100

105 6.1 103.3 143.3#



77 33.9 73.7 113.7#




Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BF0



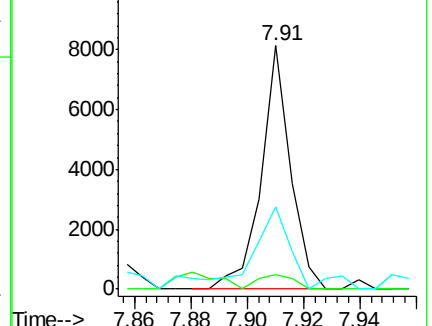



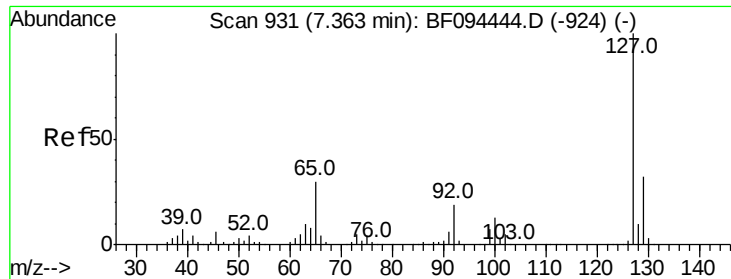

#33
4-Chloroaniline
Concen: 15.90 ng
RT: 8.09 min Scan# 1020
Delta R.T. -0.04 min
Lab File: BF096240.D
Acq: 28 Jun 2017 2:20




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
127	100		
129	83.7	26.2	39.2#
65	0.0	27.8	41.8#
92	0.2	16.8	25.2#

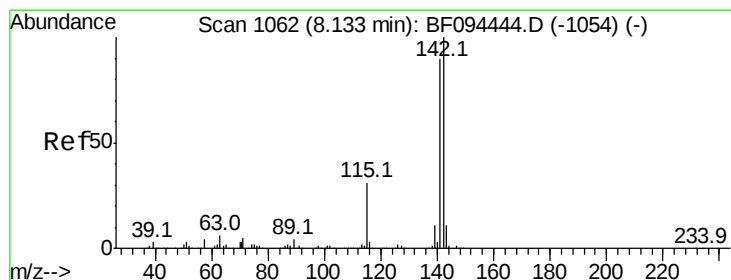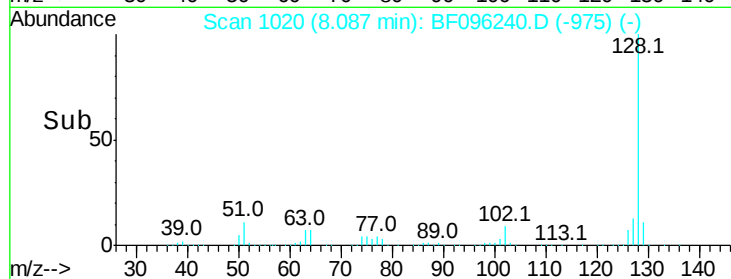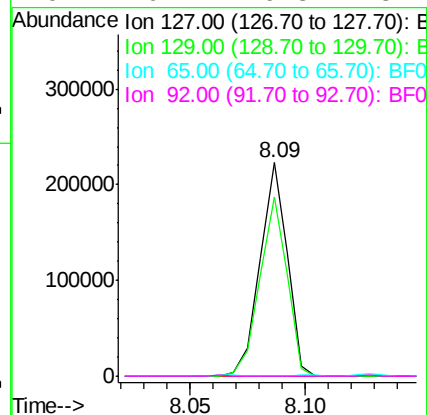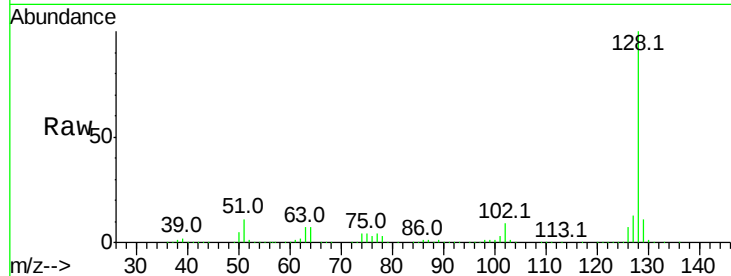

#37
2-Methylnaphthalene
Concen: 3.90 ng
RT: 8.77 min Scan# 1137
Delta R.T. 0.01 min
Lab File: BF096240.D
Acq: 28 Jun 2017 2:20

Tgt Ion	Ratio	Lower	Upper
142	100		
141	86.1	71.3	106.9
115	28.4	27.1	40.7

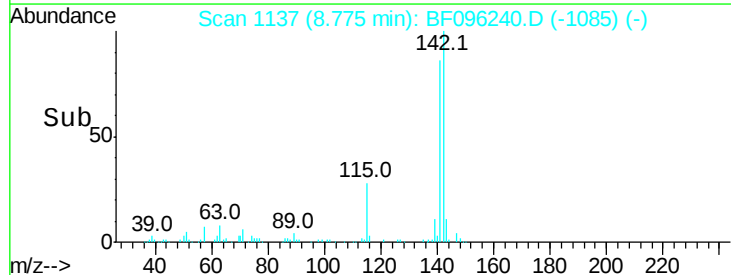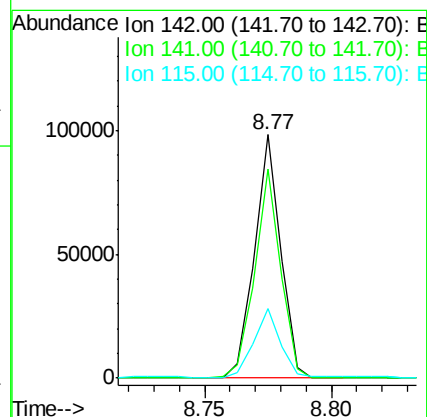

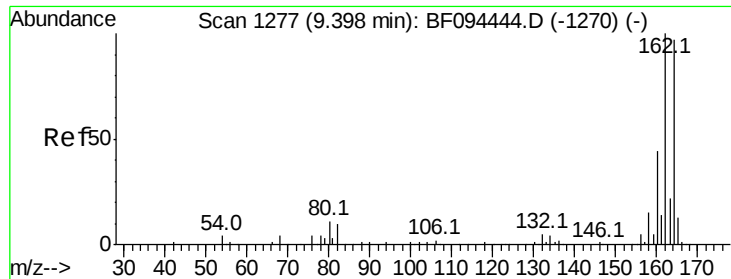

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.82 min Scan# 1314

Delta R.T. 0.01 min

Lab File: BF096240.D

Acq: 28 Jun 2017 2:20

Instrument :

BNA_F

ClientSampleId :


Tot Ion:164 Resp: 207139

Ion Ratio Lower Upper

164 100

162 103.7 82.6 123.8




160 44.9 36.2 54.2



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

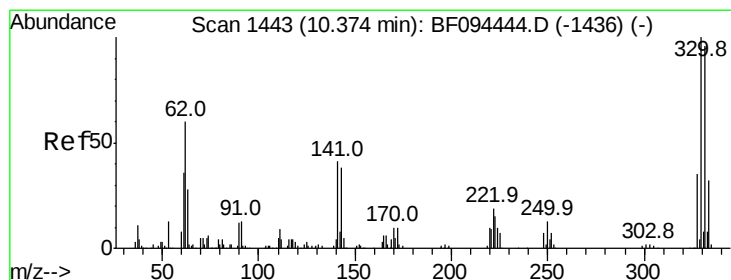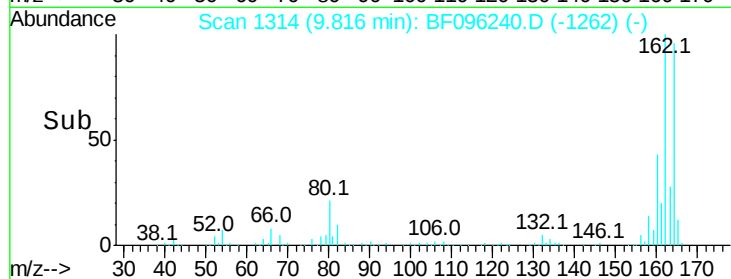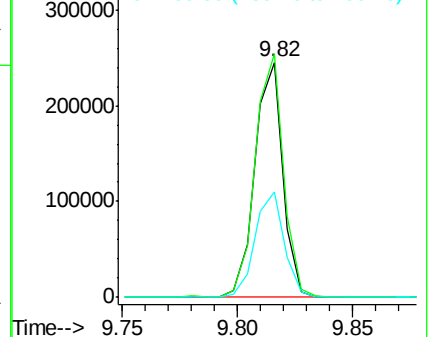

#41

2,4,6-Tribromophenol

Concen: 0.18 ng

RT: 10.59 min Scan# 1446

Delta R.T. -0.00 min

Lab File: BF096240.D

Acq: 28 Jun 2017 2:20


Tgt Ion:330 Resp: 290

Ion Ratio Lower Upper

330 100

332 74.1 76.6 115.0#



141 0.0 31.4 47.2#

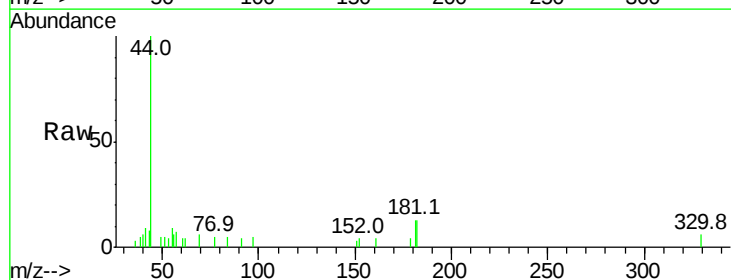


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

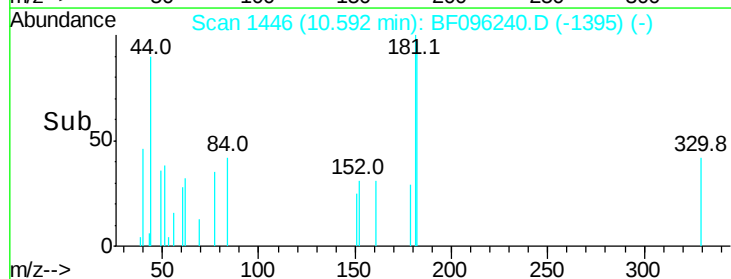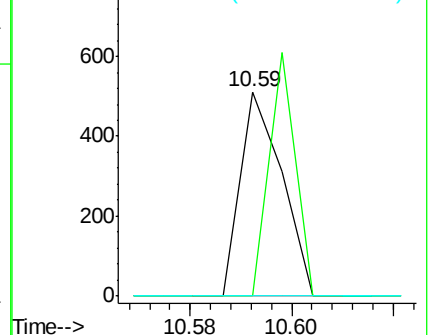







#44
2-Fluorobiphenyl
Concen: 1.27 ng
RT: 9.13 min Scan# 1198
Delta R.T. -0.02 min
Lab File: BF096240.D
Acq: 28 Jun 2017 2:20

Instrument :
BNA_F
ClientSampleId :

Tot Ion:172 Resp: 14417
Ion Ratio Lower Upper
172 100
171 33.2 29.6 44.4
170 26.7 19.8 29.8

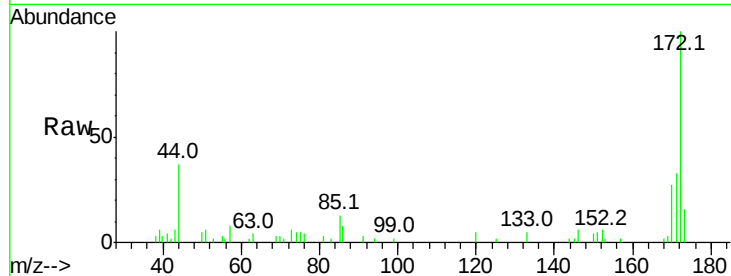


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E


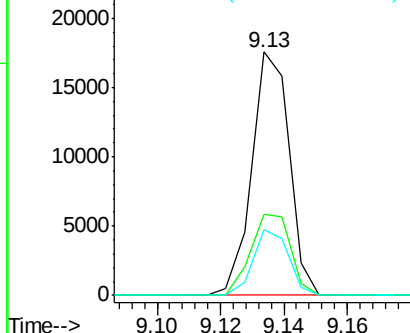



#50
2,6-Dinitrotoluene
Concen: 8.27 ng
RT: 9.82 min Scan# 1314
Delta R.T. 0.21 min
Lab File: BF096240.D
Acq: 28 Jun 2017 2:20

Tgt Ion:165 Resp: 25488
Ion Ratio Lower Upper
165 100
63 1.1 34.3 51.5#
89 2.2 37.1 55.7#

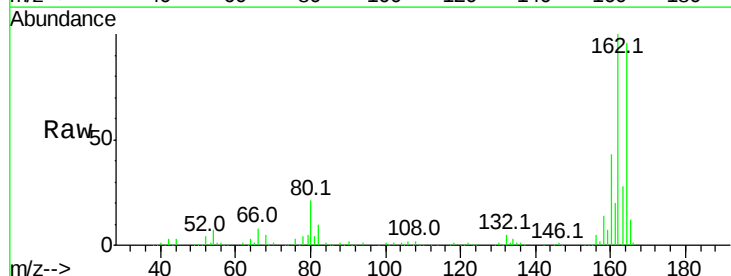

Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF0
Ion 89.00 (88.70 to 89.70): BF0




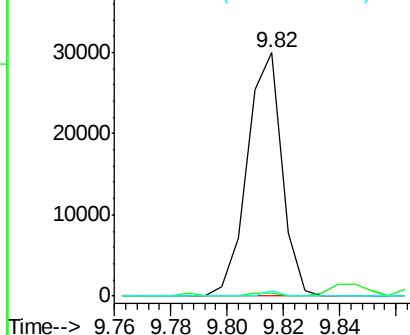


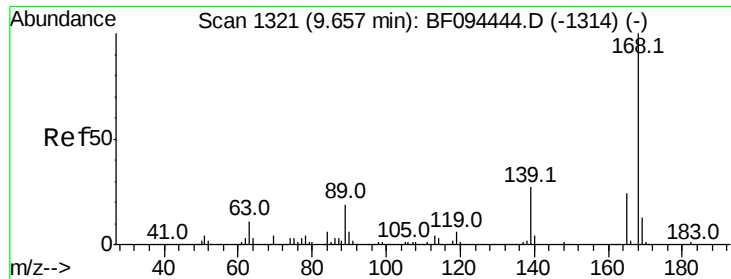

#56
 2,4-Dinitrotoluene
 Concen: 6.56 ng
 RT: 9.82 min Scan# 1314
 Delta R.T. -0.19 min
 Lab File: BF096240.D
 Acq: 28 Jun 2017 2:20




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
165	100		
63	1.1	25.4	38.0#
89	2.2	46.4	69.6#
182	0.0	1.8	2.6#

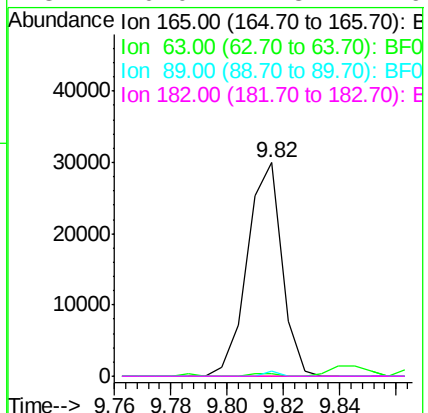

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.29 min Scan# 1565
 Delta R.T. 0.01 min
 Lab File: BF096240.D
 Acq: 28 Jun 2017 2:20

Tgt Ion	Ratio	Lower	Upper
188	100		
94	14.7	9.4	14.2#
80	15.1	10.2	15.2



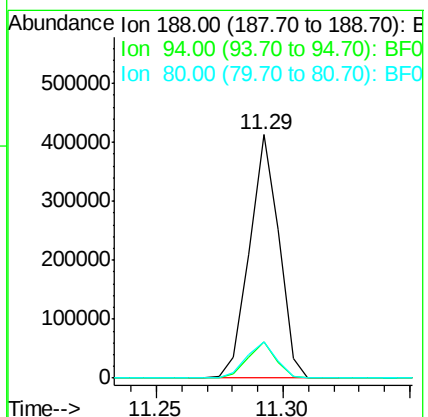





#70
Phenanthrene
Concen: Below Cal
RT: 11.32 min Scan# 1569
Delta R.T. -0.01 min
Lab File: BF096240.D
Acq: 28 Jun 2017 2:20




Instrument :
BNA_F
ClientSampled :


Tot Ion:178 Resp: 15277
Ion Ratio Lower Upper
178 100
176 19.5 16.2 24.4
179 17.7 12.6 19.0

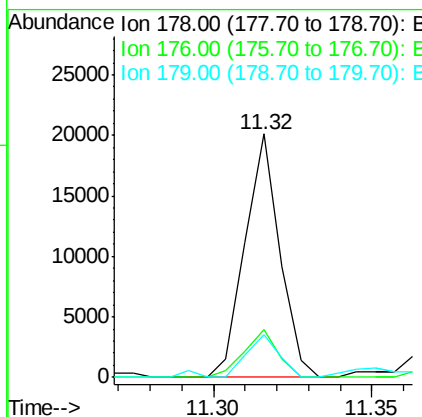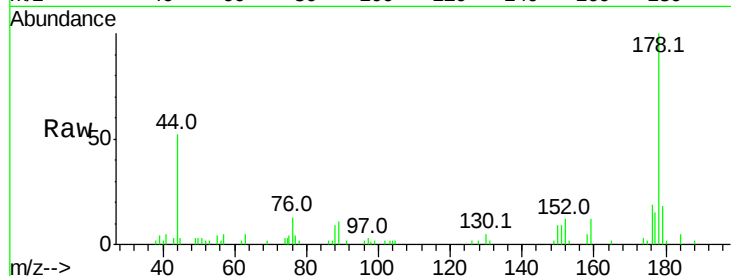

#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.92 min Scan# 2012
Delta R.T. 0.01 min
Lab File: BF096240.D
Acq: 28 Jun 2017 2:20

Tgt Ion:240 Resp: 285716
Ion Ratio Lower Upper
240 100
120 18.4 5.8 8.8#
236 26.2 20.5 30.7

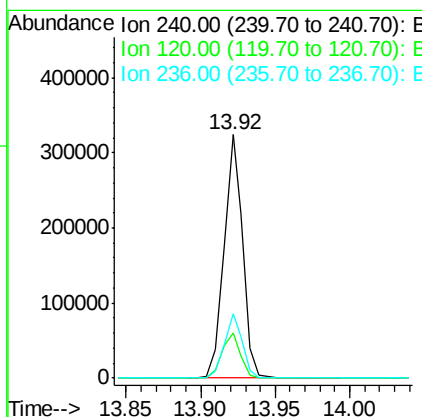


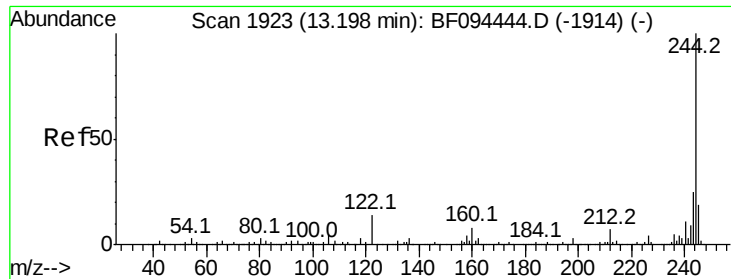




#78
 Terphenyl-d14
 Concen: 0.90 ng
 RT: 12.87 min Scan# 1834
 Delta R.T. 0.01 min
 Lab File: BF096240.D
 Acq: 28 Jun 2017 2:20

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:244 Resp: 10255
 Ion Ratio Lower Upper
 244 100
 212 6.2 6.0 9.0
 122 21.0 10.3 15.5#




Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

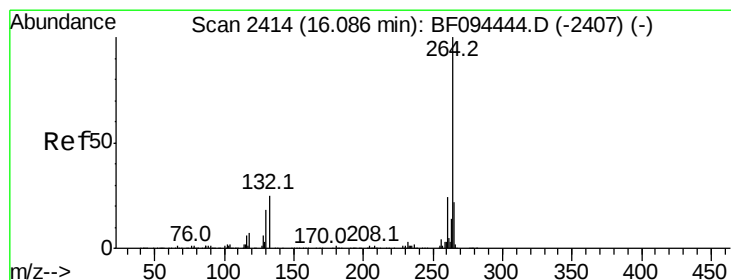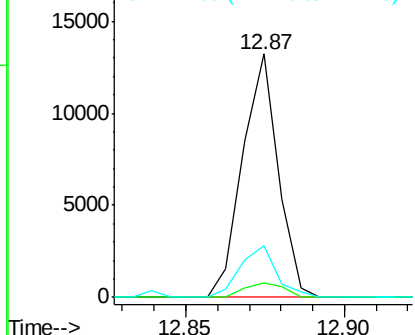

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.34 min Scan# 2254
 Delta R.T. 0.01 min
 Lab File: BF096240.D
 Acq: 28 Jun 2017 2:20

Tgt Ion:264 Resp: 197194
 Ion Ratio Lower Upper
 264 100
 260 22.4 19.5 29.3
 265 21.1 17.2 25.8

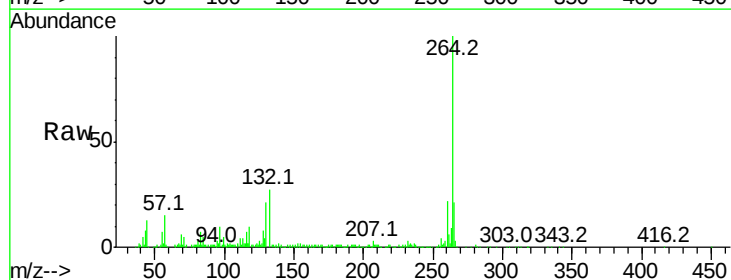

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

