




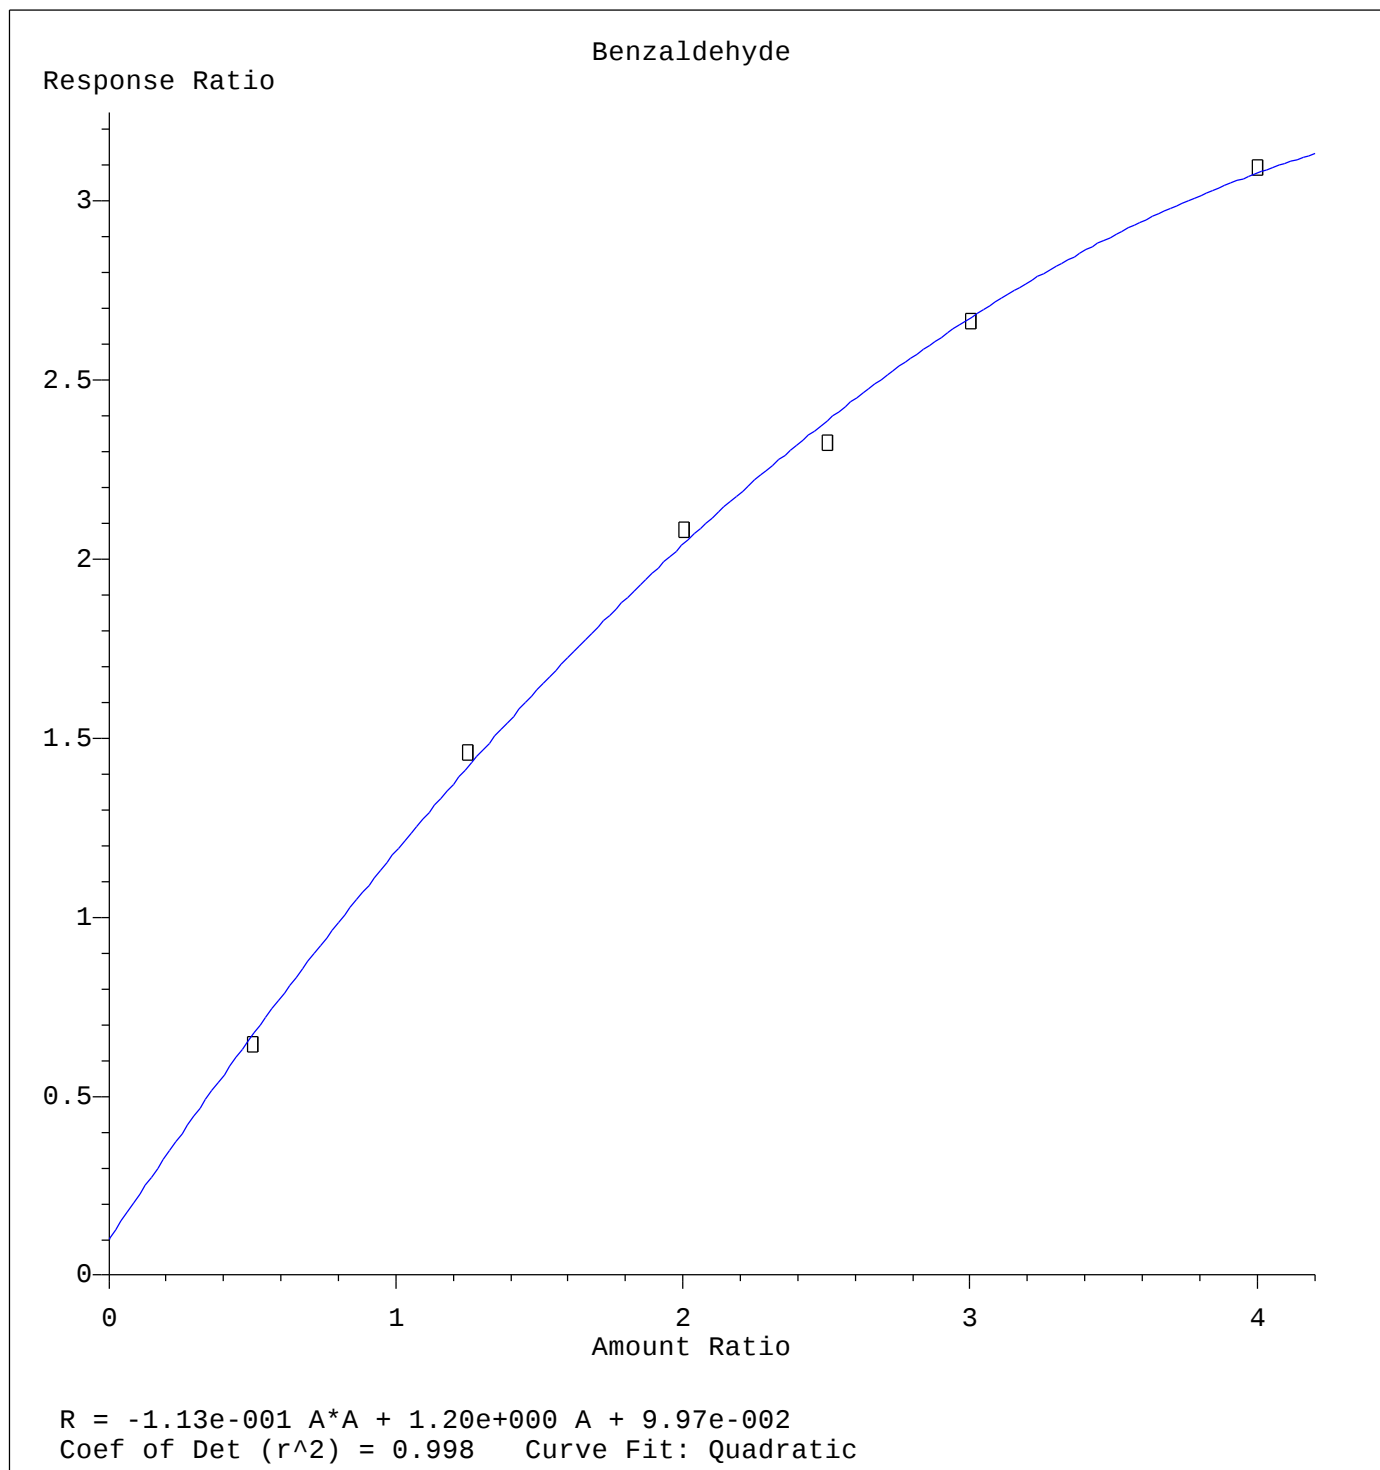


Method Name: Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Calibration Table Last Updated: Wed Jun 28 15:41:49 2017

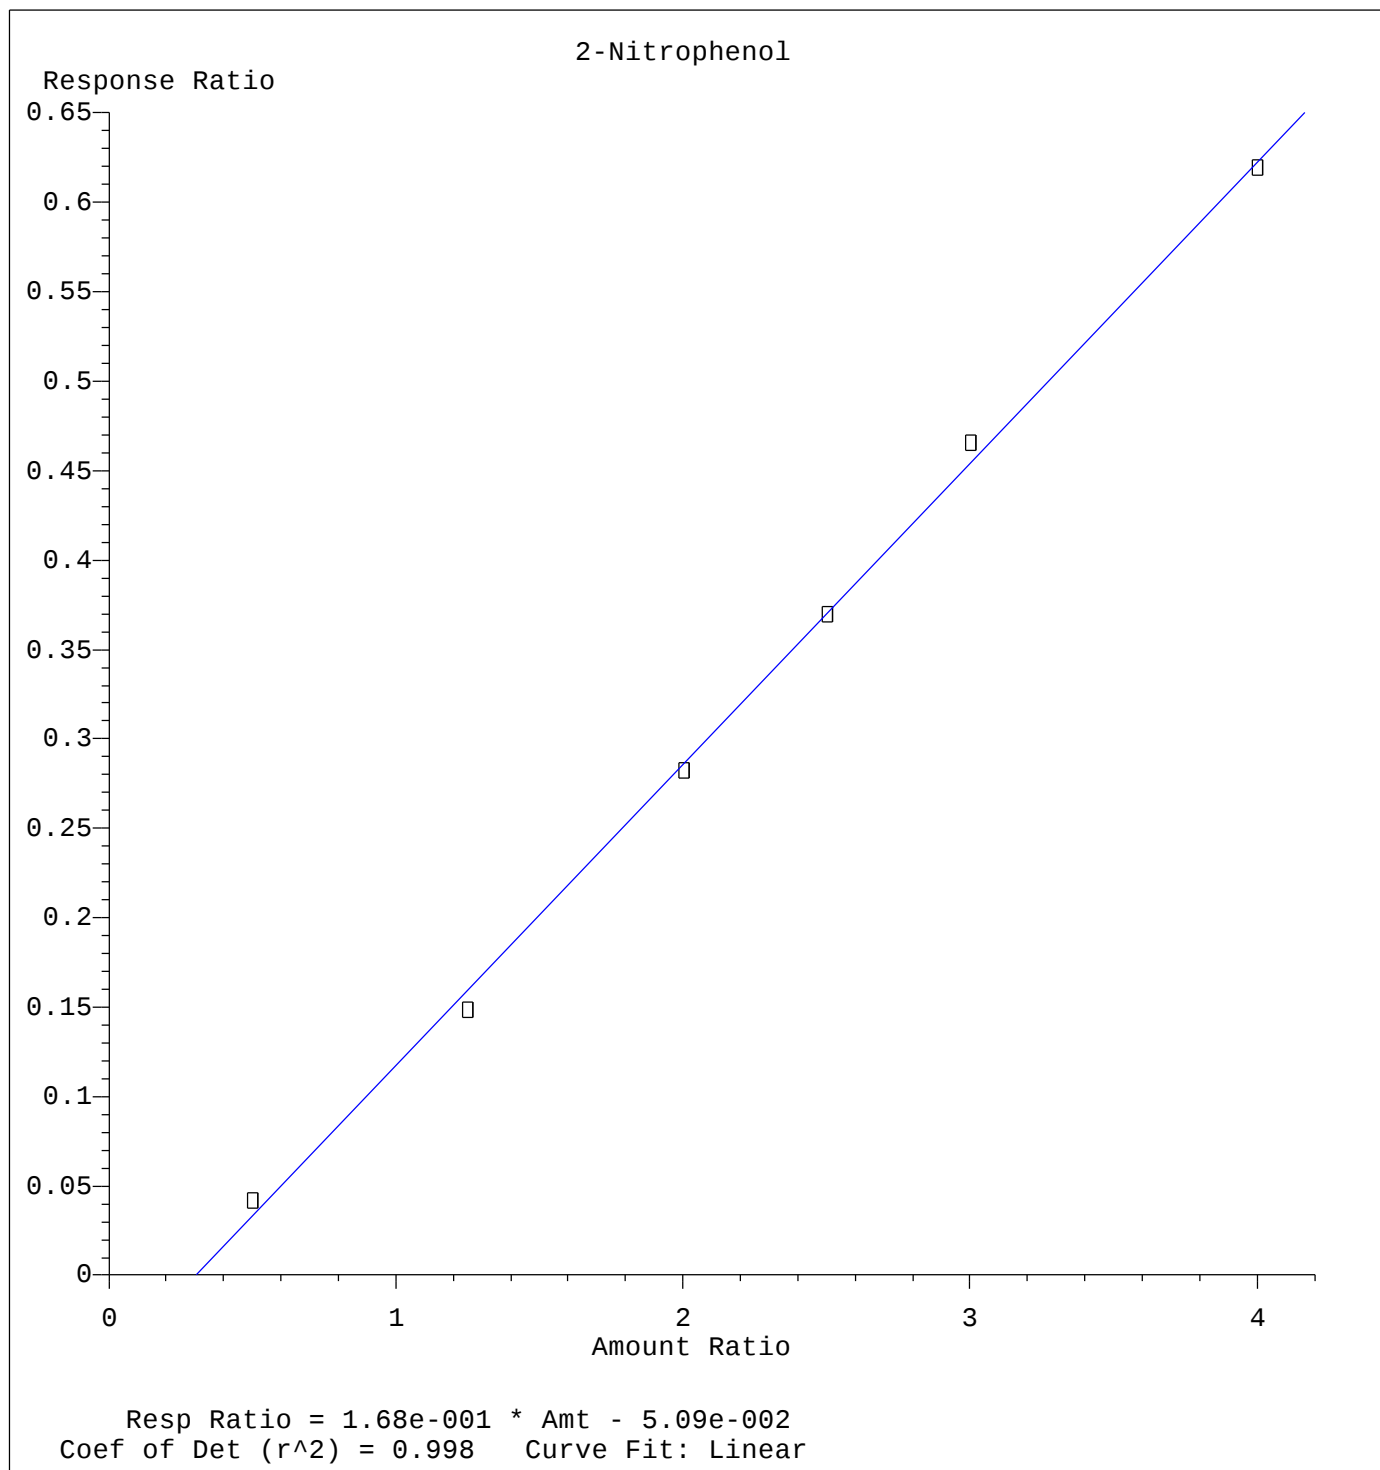


Method Name: Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Calibration Table Last Updated: Wed Jun 28 15:41:49 2017

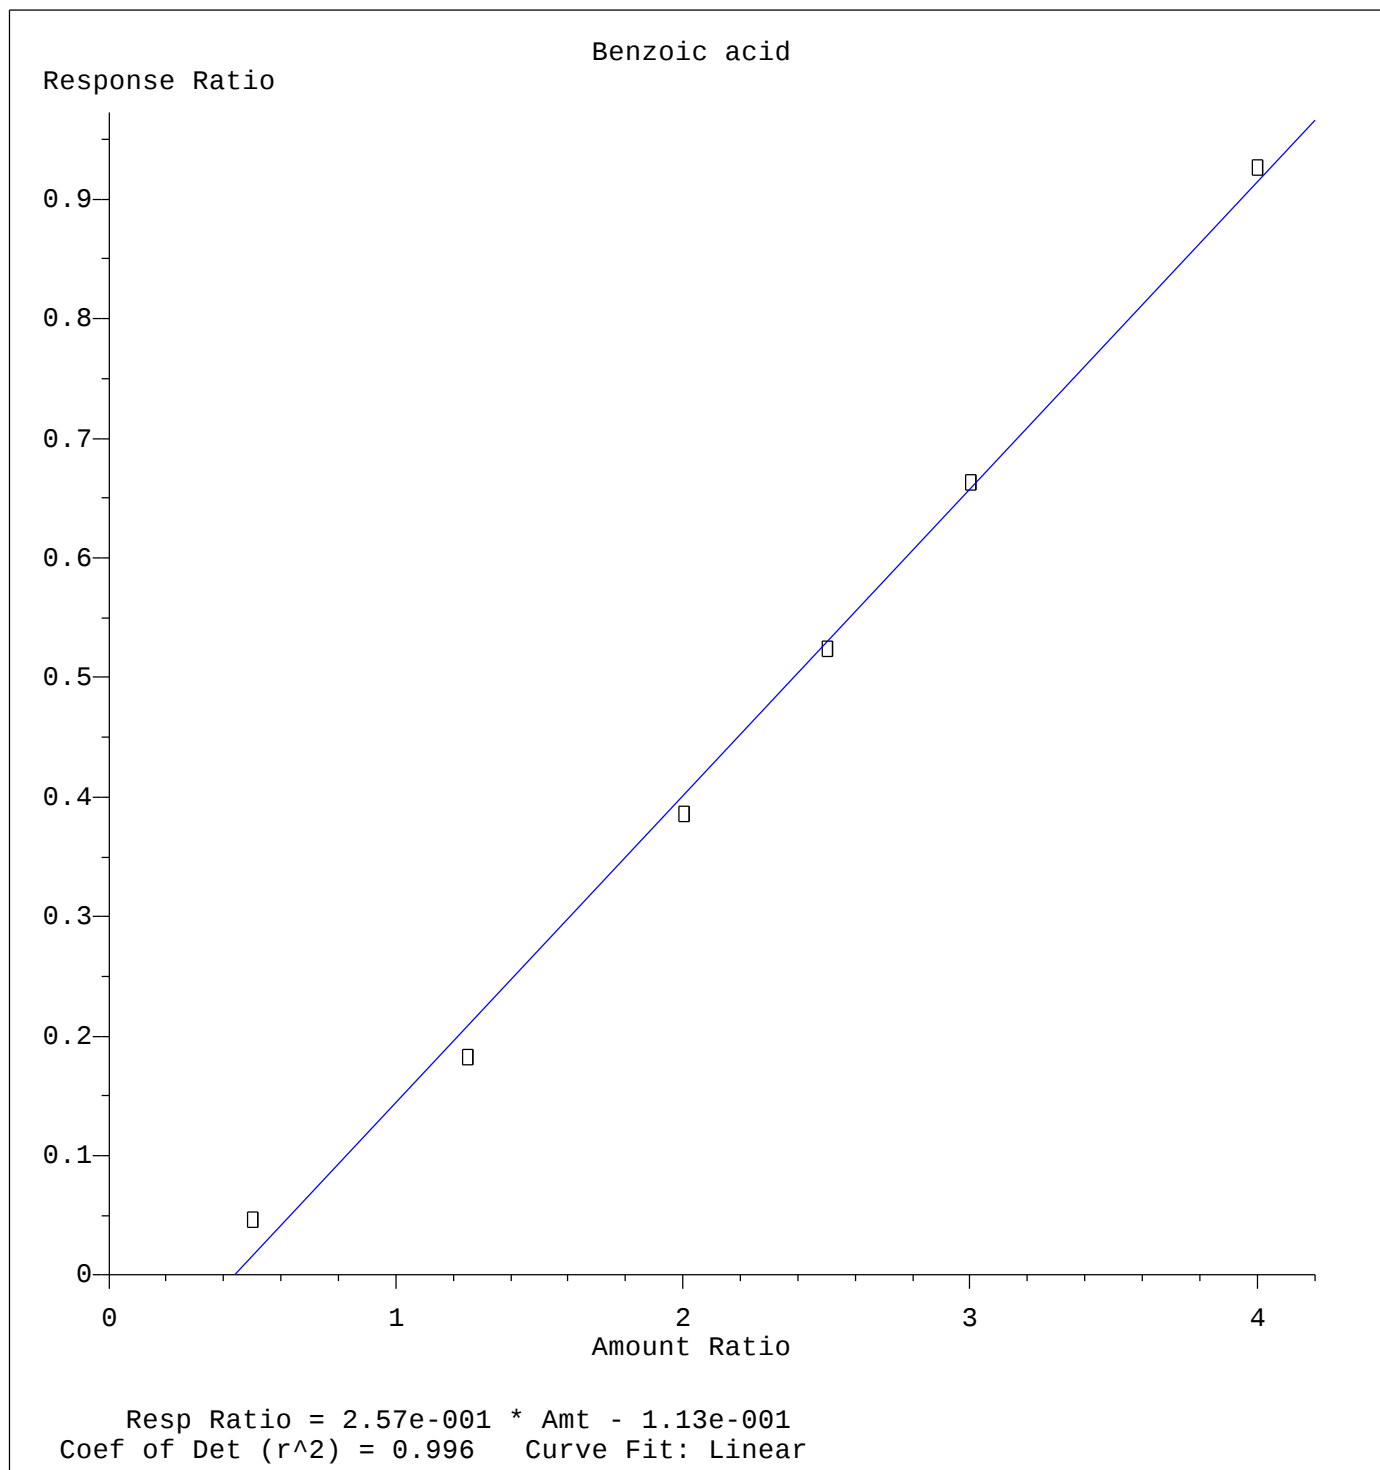

Method Name: Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Calibration Table Last Updated: Wed Jun 28 15:41:49 2017

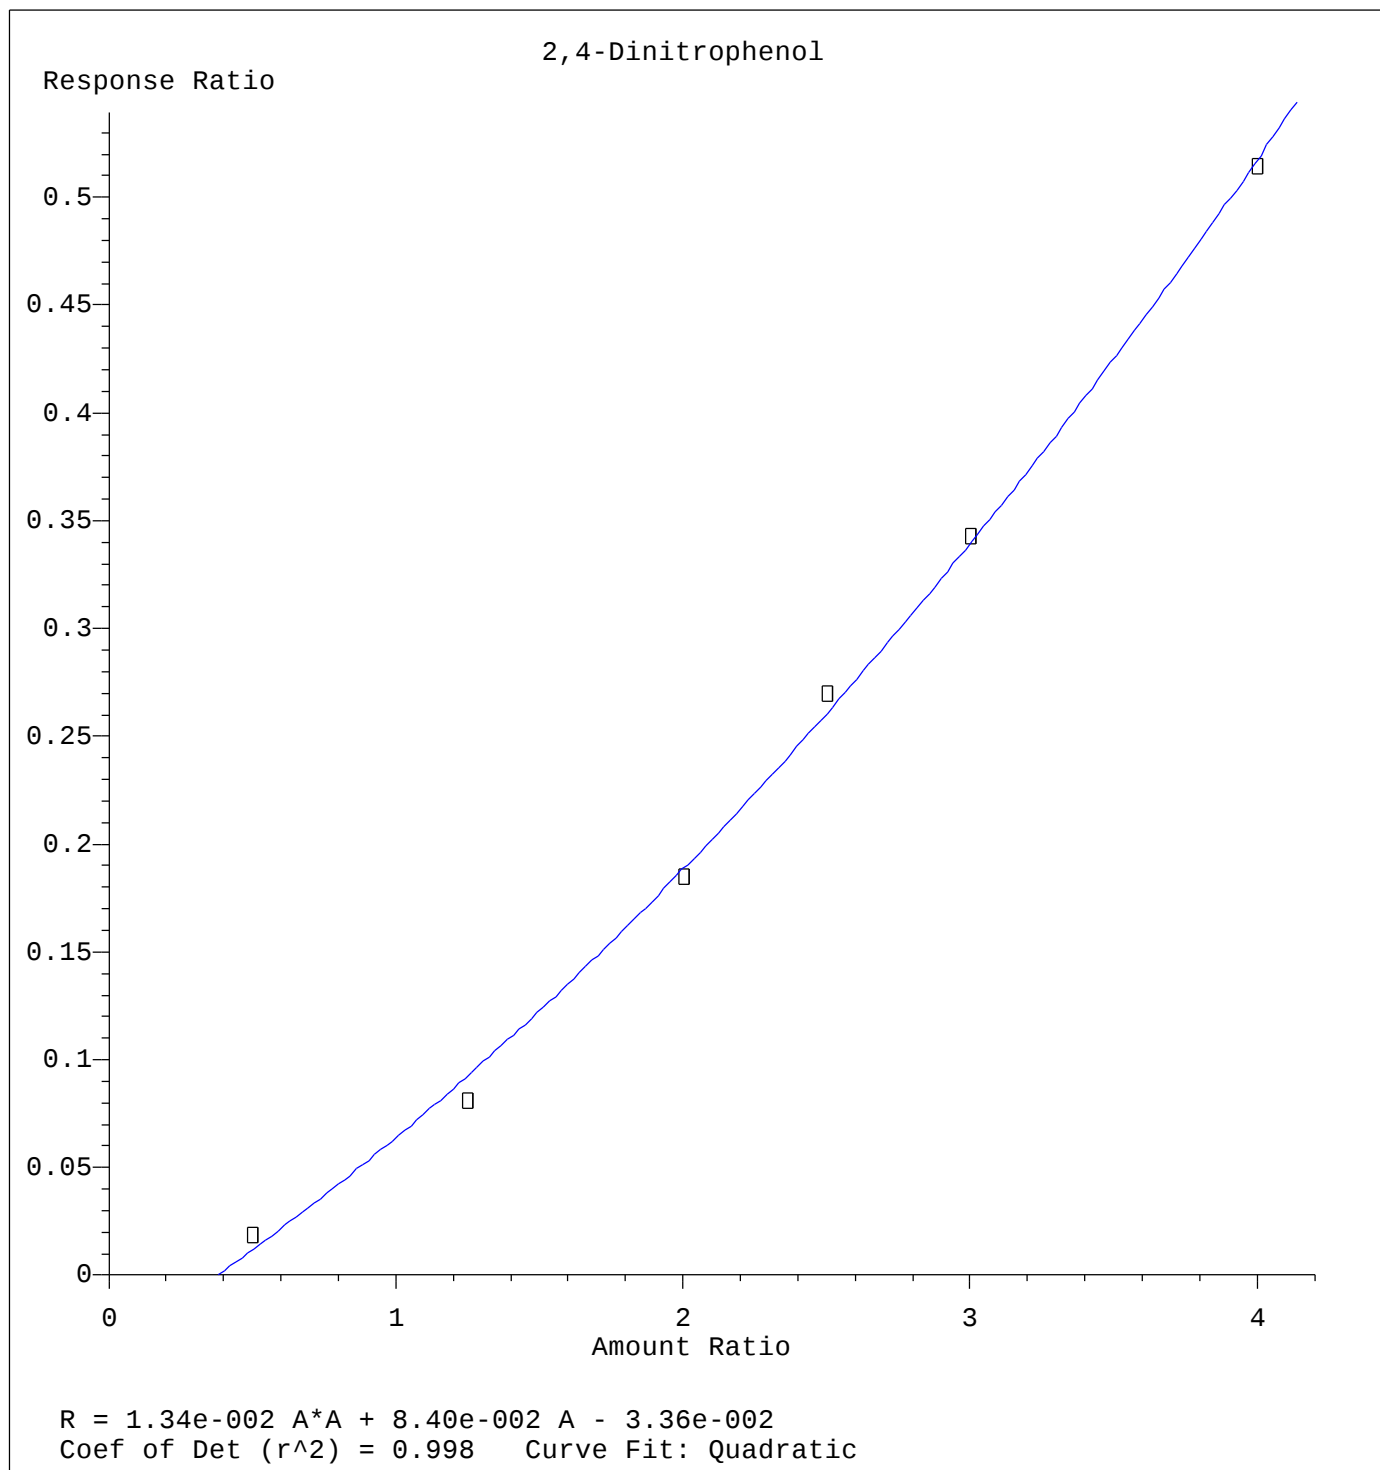


Method Name: Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Calibration Table Last Updated: Wed Jun 28 15:41:49 2017

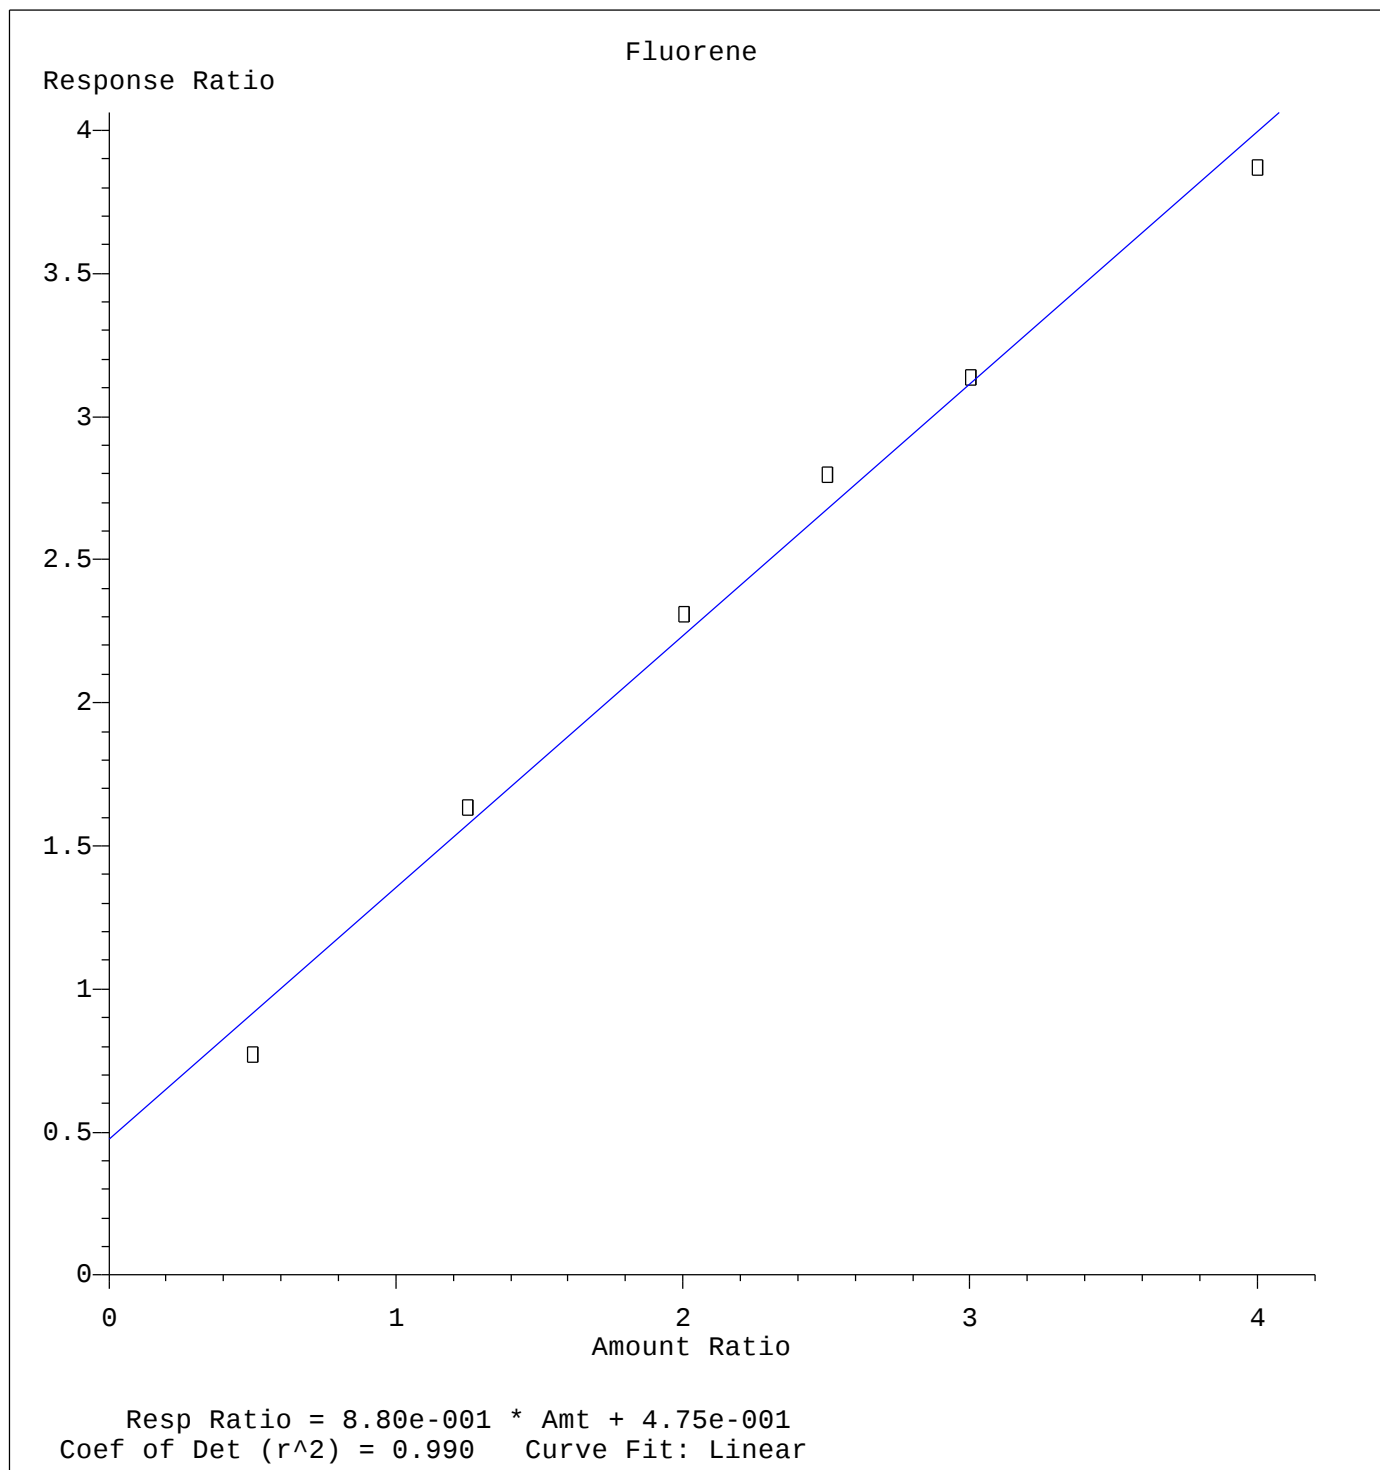

Method Name: Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Calibration Table Last Updated: Wed Jun 28 15:41:49 2017

4-Chlorophenyl-phenylether


Response Ratio

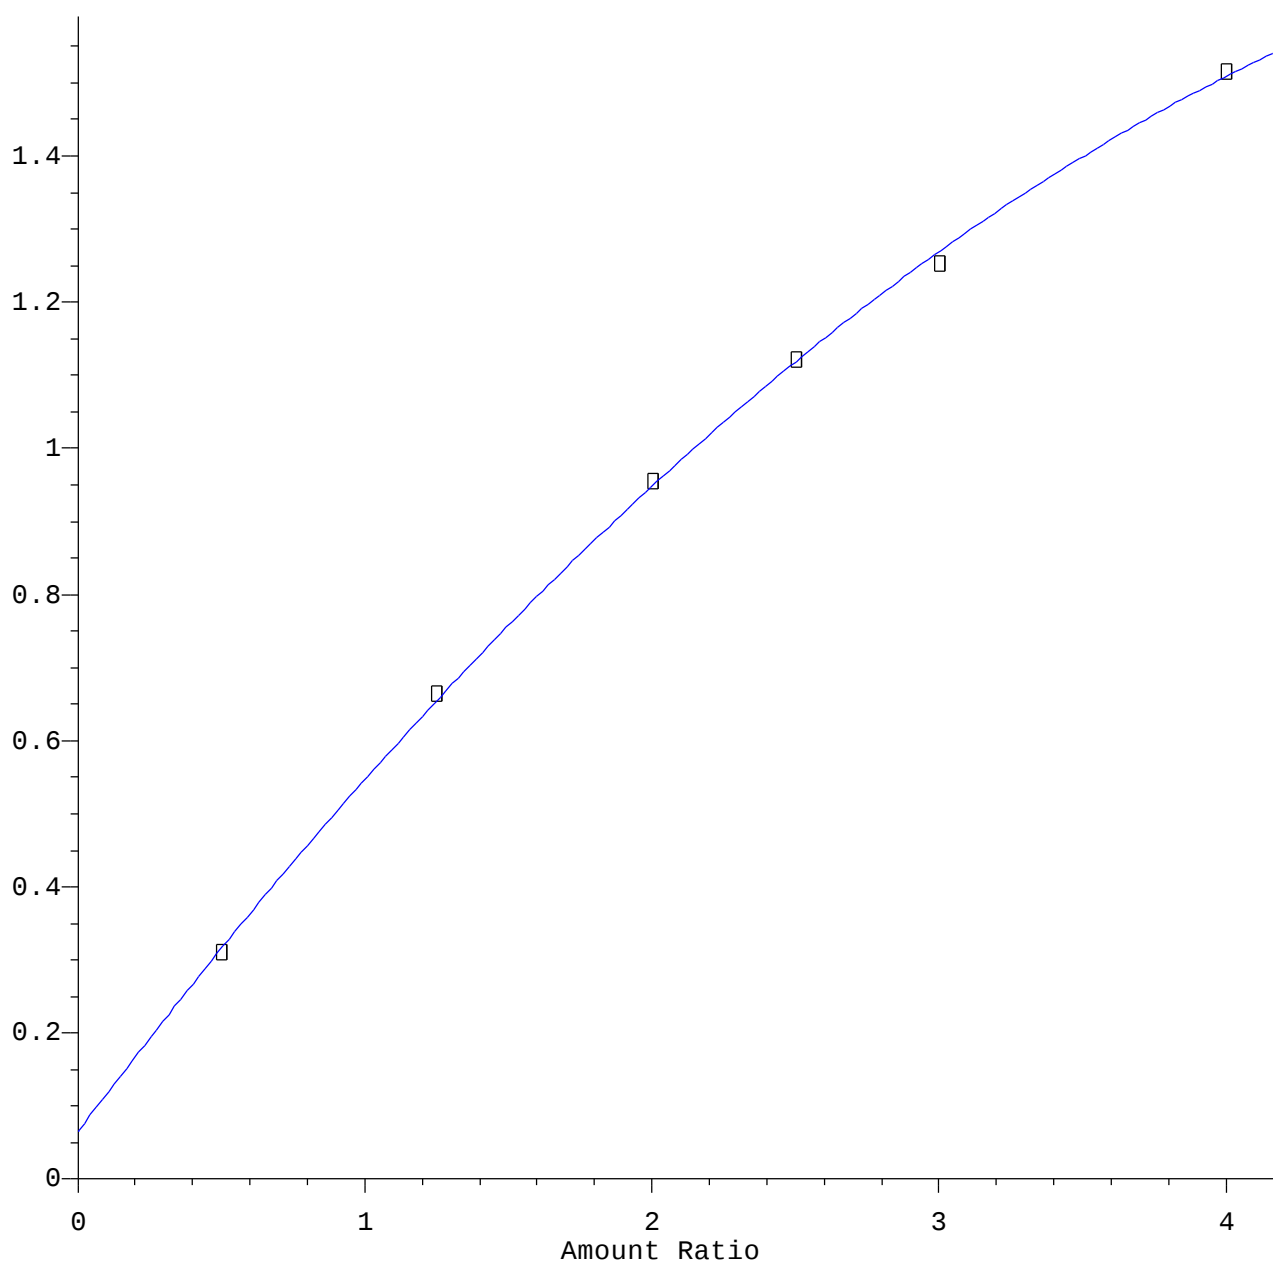

$R = -4.04e-002 A^2 + 5.23e-001 A + 6.48e-002$
Coef of Det (r^2) = 0.999 Curve Fit: Quadratic


Method Name: Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Calibration Table Last Updated: Wed Jun 28 15:41:49 2017

4,6-Dinitro-2-methylphenol

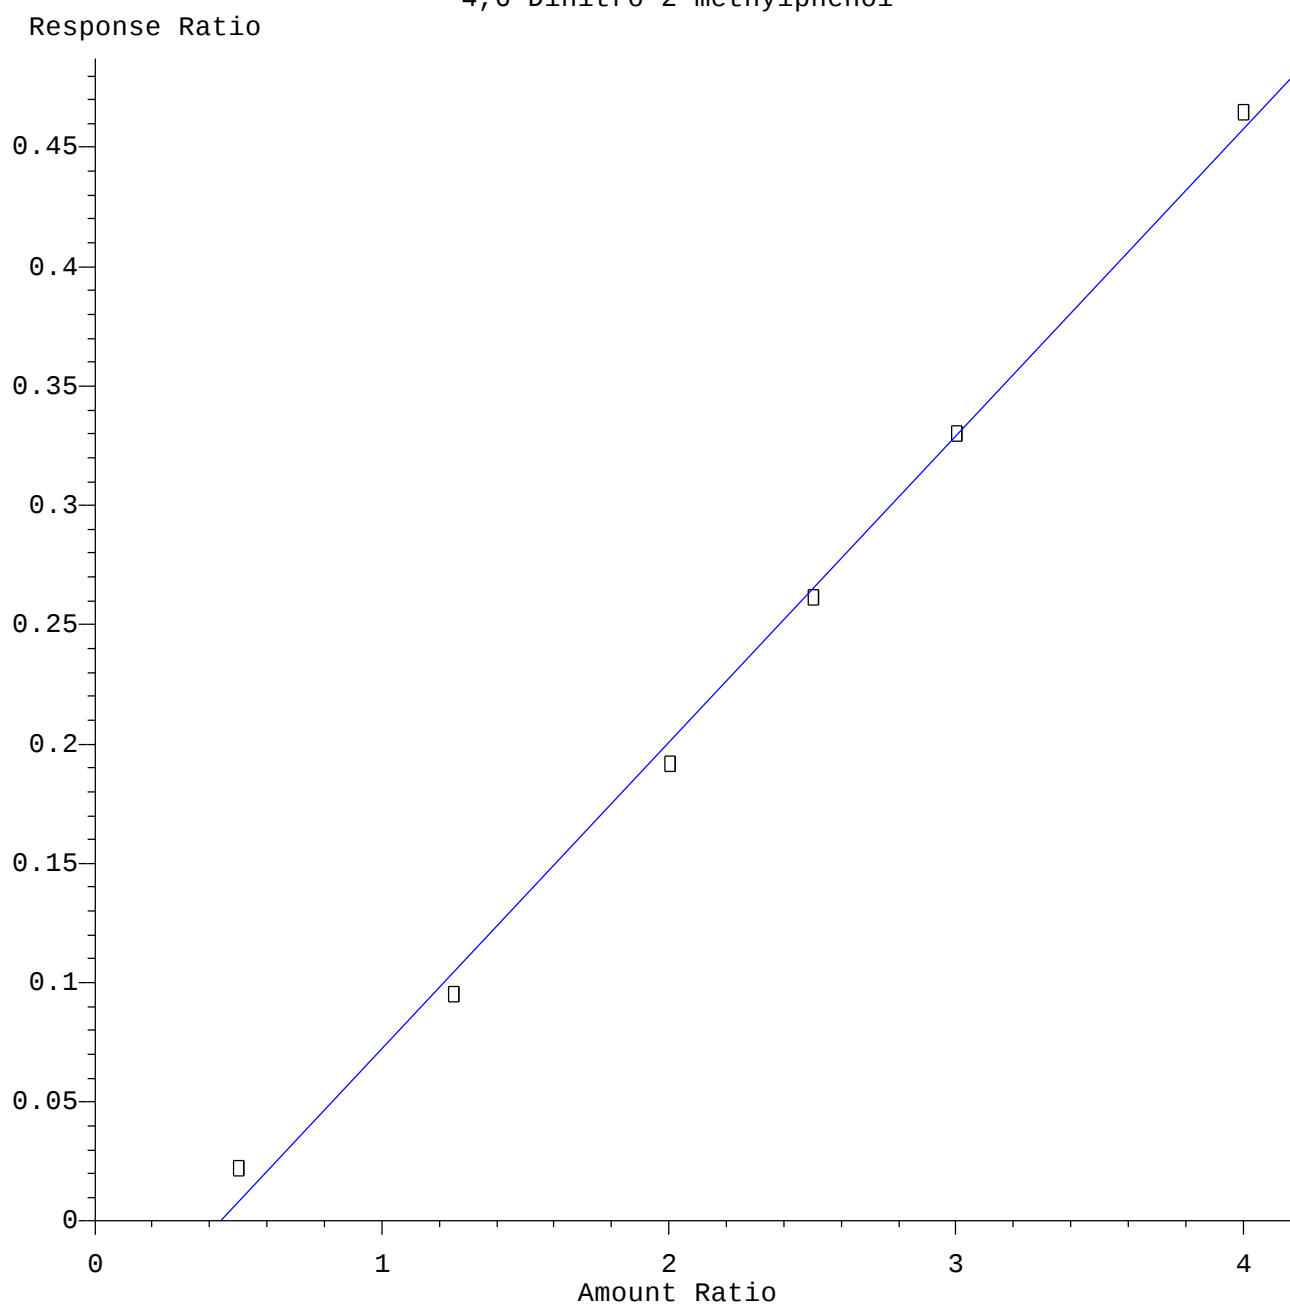

Resp Ratio = $1.28 \times 10^{-1} \times \text{Amt} - 5.62 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Calibration Table Last Updated: Wed Jun 28 15:41:49 2017

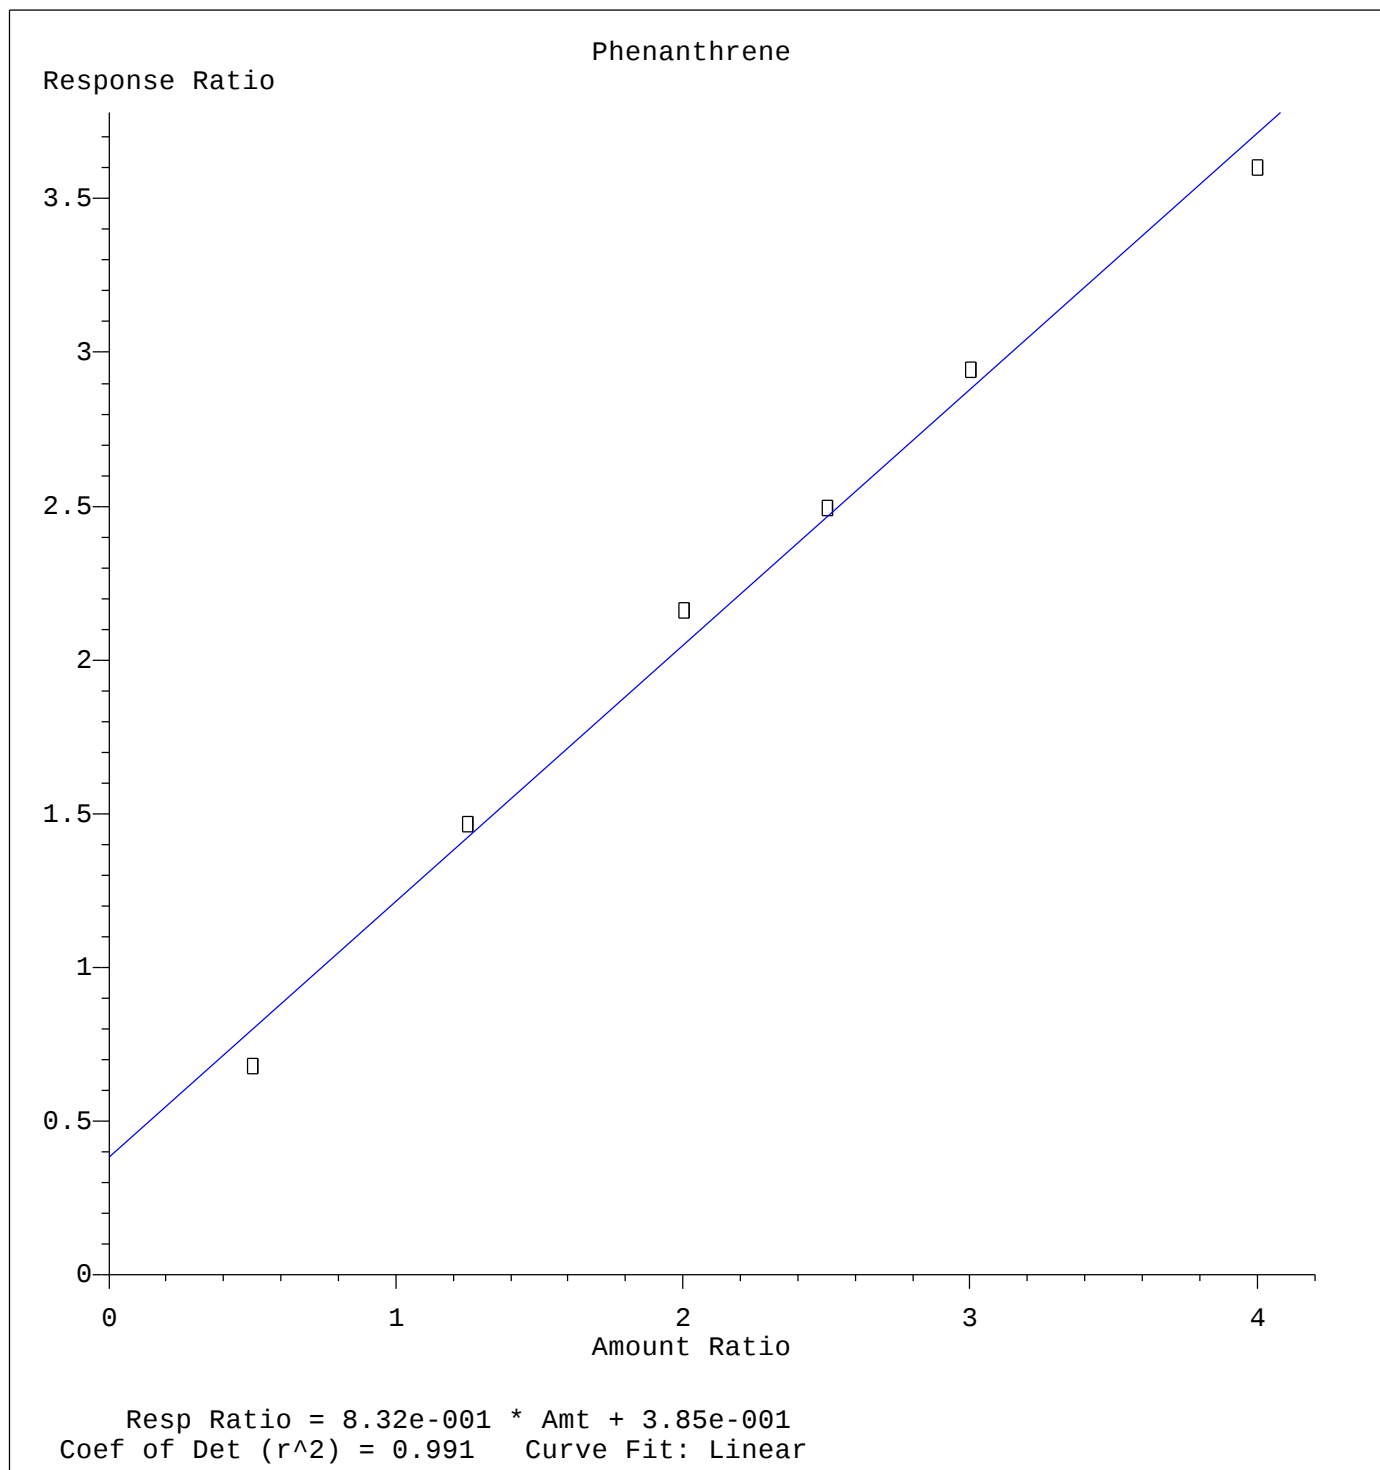

Method Name: Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Calibration Table Last Updated: Wed Jun 28 15:41:49 2017