

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
 Data File : BF096222.D
 Acq On : 27 Jun 2017 18:02
 Operator : SJ/MA
 Sample : I3868-04 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-062217-B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.963	485	489	496	rVB	183199	185531	12.13%	1.218%
2	5.381	556	560	564	rBV	1345117	1128084	73.75%	7.406%
3	6.398	729	733	736	rBV	1291337	1112307	72.72%	7.302%
4	6.539	753	757	761	rVB	1300683	1115492	72.93%	7.323%
5	6.781	794	798	801	rBV	1297787	1133805	74.13%	7.443%
6	6.934	820	824	827	rBV	1039456	814243	53.23%	5.345%
7	7.333	888	892	895	rBV	708877	633679	41.43%	4.160%
8	7.416	903	906	914	rVB2	19155	20316	1.33%	0.133%
9	8.057	1011	1015	1019	rBV	1751820	1529573	100.00%	10.042%
10	9.133	1194	1198	1201	rVB	1391603	1074843	70.27%	7.056%
11	9.527	1261	1265	1268	rBV	224325	188764	12.34%	1.239%
12	9.645	1276	1285	1290	rBV7	18834	40681	2.66%	0.267%
13	9.704	1291	1295	1302	rVB2	21627	30219	1.98%	0.198%
14	9.810	1309	1313	1317	rBV2	1679058	1402178	91.67%	9.205%
15	10.222	1380	1383	1386	rBV2	23110	27051	1.77%	0.178%
16	10.257	1386	1389	1392	rVB	28634	26673	1.74%	0.175%
17	10.586	1442	1445	1449	rVB	527887	472432	30.89%	3.102%
18	10.727	1466	1469	1471	rBV	36267	35318	2.31%	0.232%
19	11.169	1542	1544	1547	rBV2	23219	21430	1.40%	0.141%
20	11.286	1560	1564	1568	rBV	1235535	1063744	69.55%	6.983%
21	11.521	1601	1604	1610	rBV2	29261	28862	1.89%	0.189%
22	11.821	1652	1655	1659	rBV	69292	73278	4.79%	0.481%
23	12.339	1740	1743	1751	rBV2	102787	92792	6.07%	0.609%
24	12.492	1765	1769	1771	rBV3	23524	22623	1.48%	0.149%
25	12.610	1784	1789	1795	rBV2	92712	129828	8.49%	0.852%
26	12.721	1806	1808	1811	rVB2	20668	17669	1.16%	0.116%
27	12.868	1829	1833	1837	rBV	764081	635304	41.53%	4.171%
28	13.327	1908	1911	1915	rBV4	17376	22727	1.49%	0.149%
29	13.774	1984	1987	1992	rVB3	68934	85089	5.56%	0.559%
30	13.915	2007	2011	2015	rBV	1176393	1016043	66.43%	6.670%
31	14.409	2092	2095	2100	rBV3	50470	59945	3.92%	0.394%
32	15.339	2248	2253	2260	rBV	772588	991820	64.84%	6.511%

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096222.D
Acq On : 27 Jun 2017 18:02
Operator : SJ/MA
Sample : I3868-04 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-062217-B

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 15232343

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096222.D
Acq On : 27 Jun 2017 18:02
Operator : SJ/MA
Sample : I3868-04 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-062217-B

Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

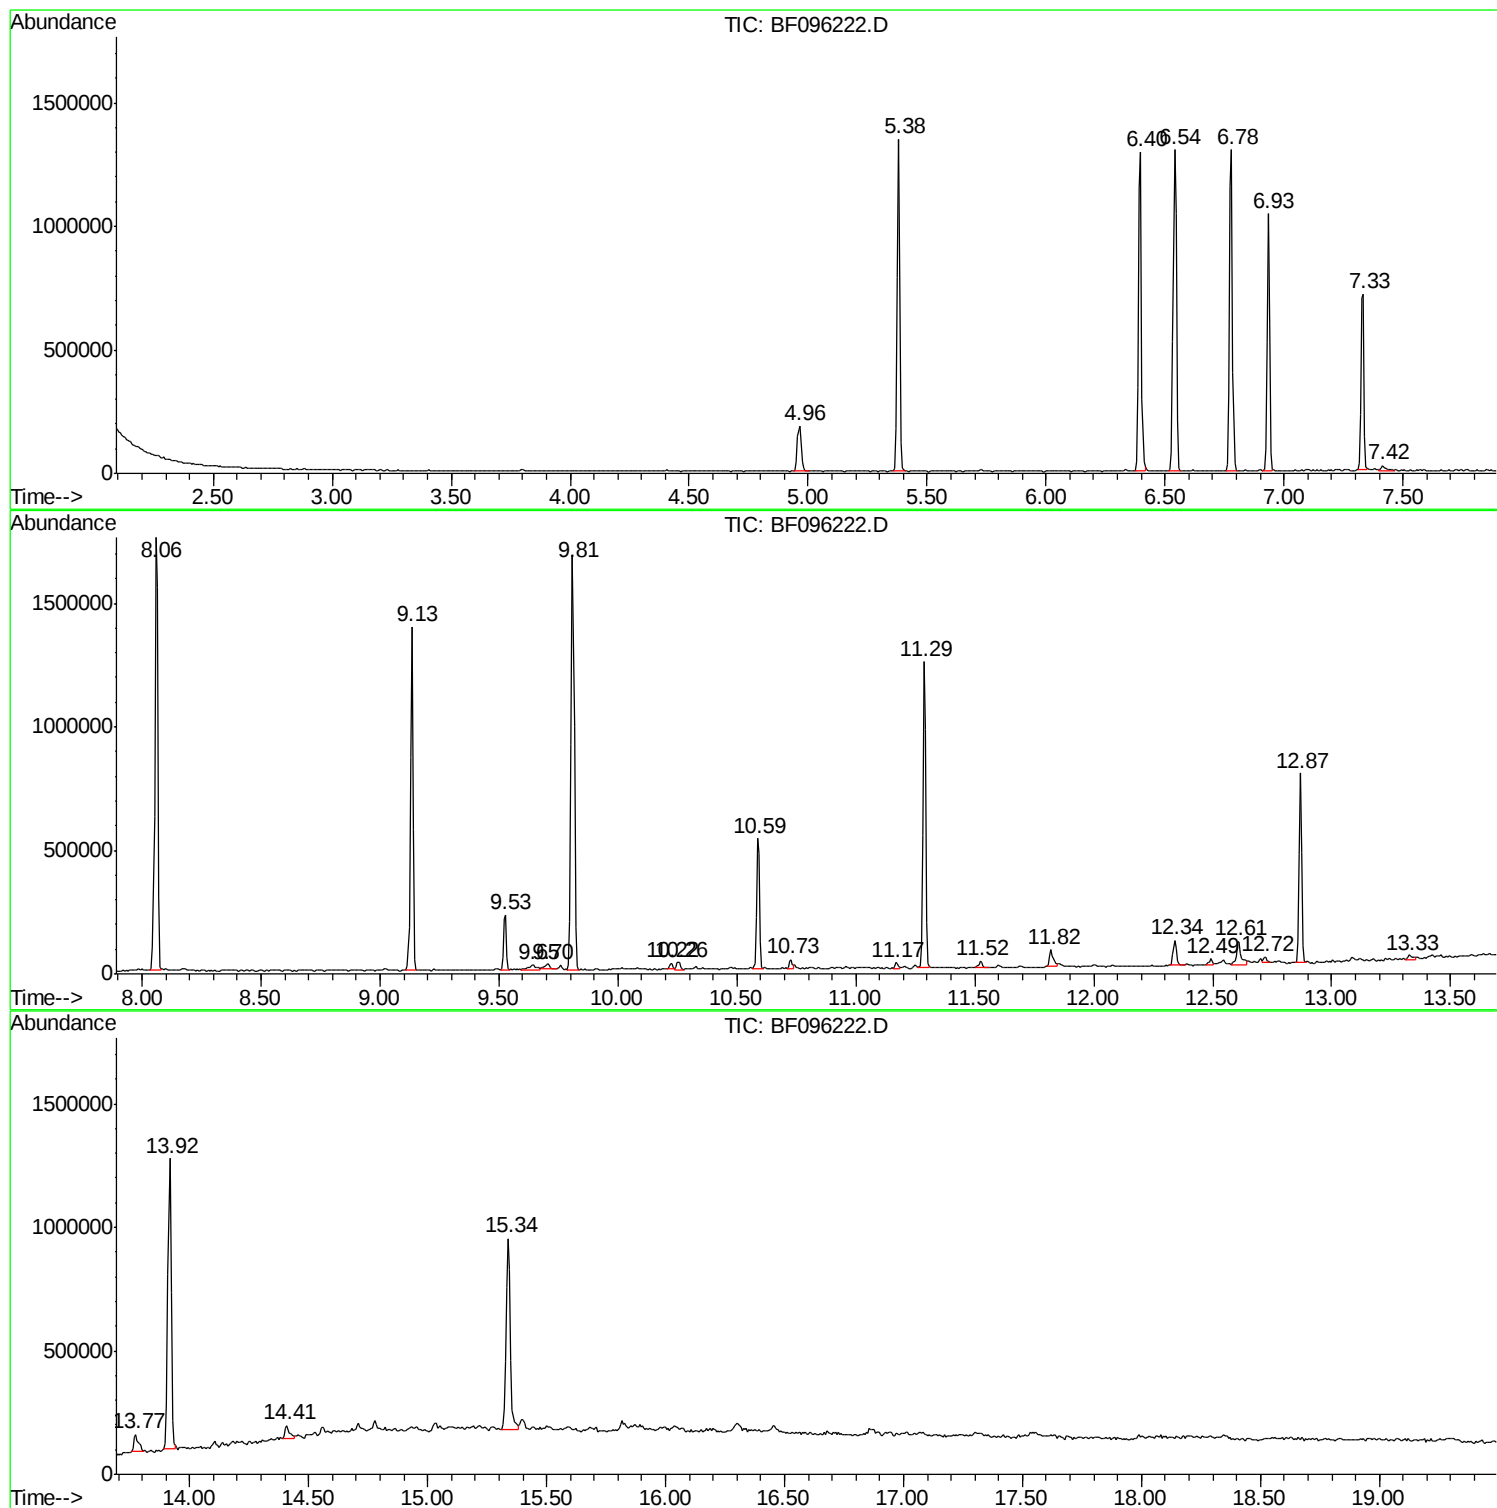

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096222.D
Acq On : 27 Jun 2017 18:02
Operator : SJ/MA
Sample : I3868-04 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-062217-B










Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.96	3.27 ng	185531	1,4-Dichlorobenzene-d4	6.78

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	36
3			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
4			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	33
5			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25

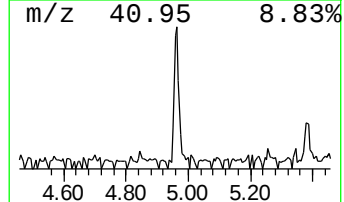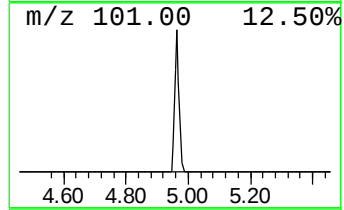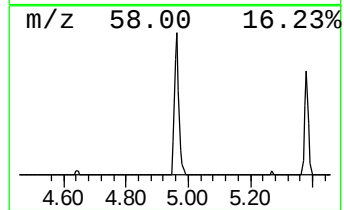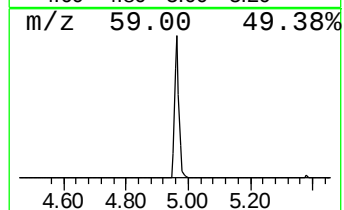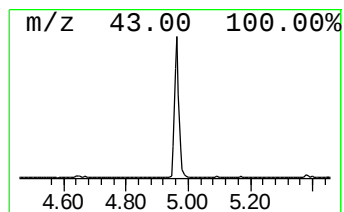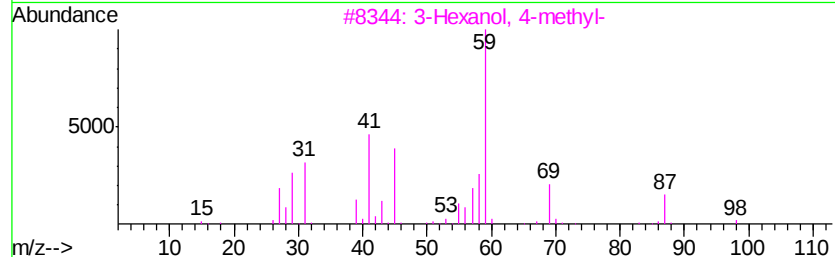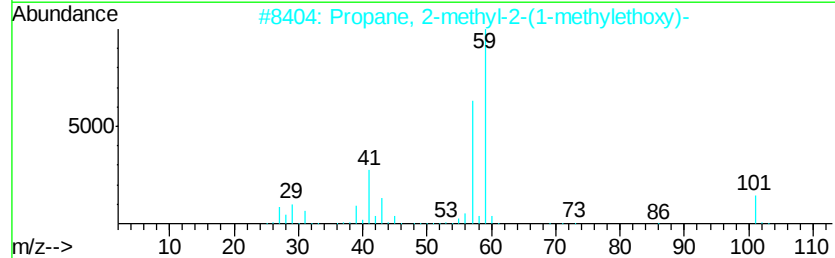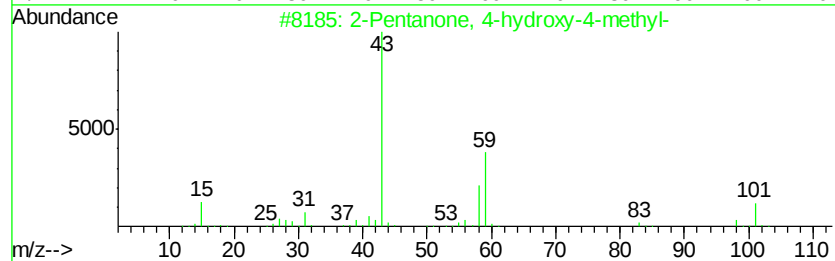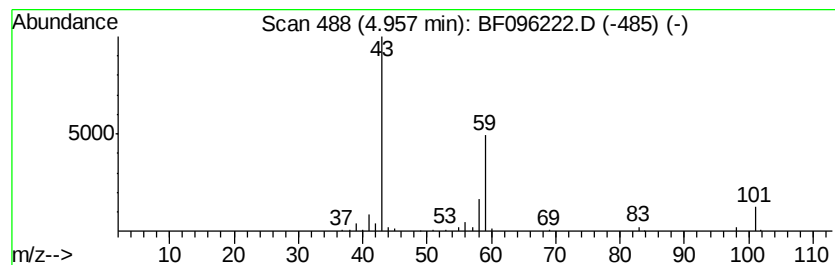

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096222.D
Acq On : 27 Jun 2017 18:02
Operator : SJ/MA
Sample : I3868-04 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-062217-B










Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.54 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.54	19.68 ng	1115490	1,4-Dichlorobenzene-d4	6.78

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		Amphetaminil	250	C17H18N2	017590-01-1	10

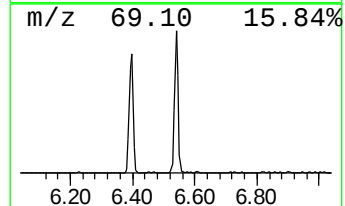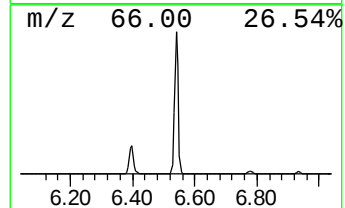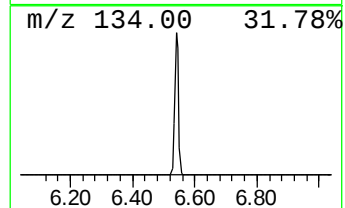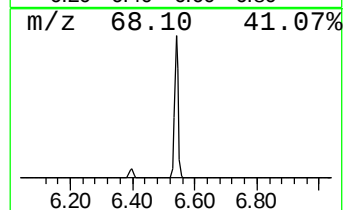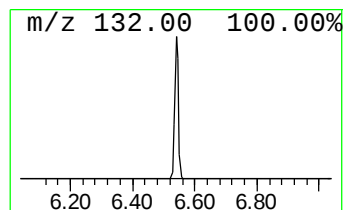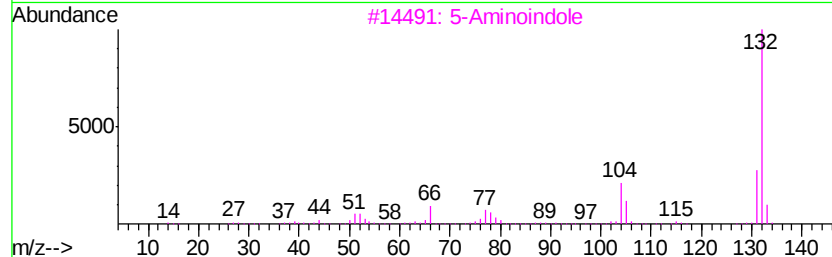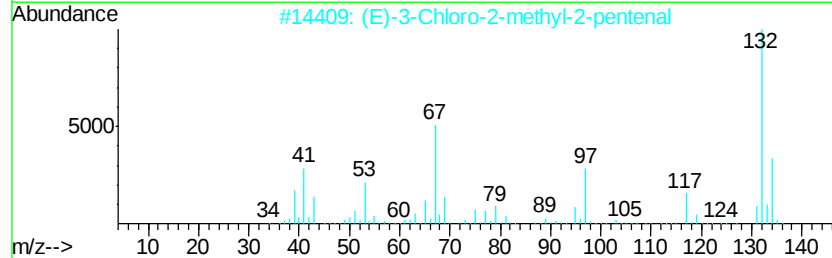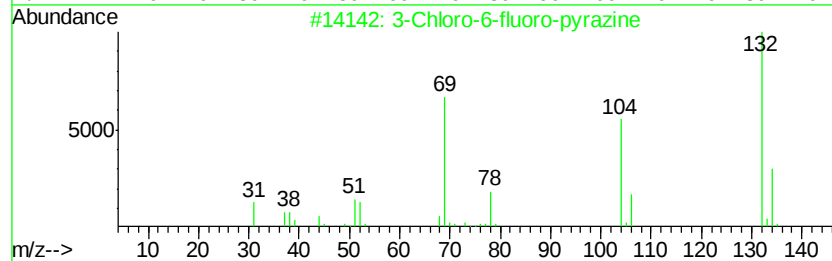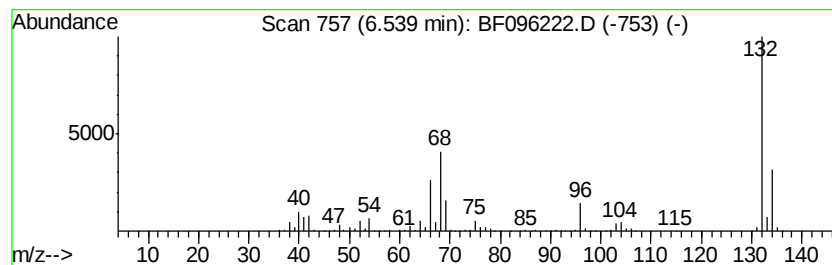

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096222.D
Acq On : 27 Jun 2017 18:02
Operator : SJ/MA
Sample : I3868-04 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
CL-01-062217-B

Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Octadecanoic acid Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.	
12.61	2.56 ng	129828	Chrysene-d12	13.92	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Octadecanoic acid	284	C18H36O2	000057-11-4	95
2	Decanoic acid, silver(1+) salt	278	C10H19AgO2	013126-67-5	62
3	Pentadecanoic acid	242	C15H30O2	001002-84-2	52
4	Alpha-d-xylopyranose	150	C5H10O5	006763-34-4	27
5	Sulfurous acid, 2-propyl tetra...	320	C17H36O3S	1000309-12-5	25

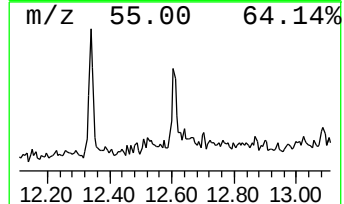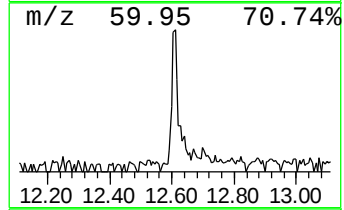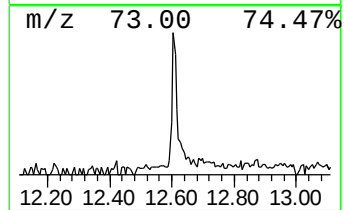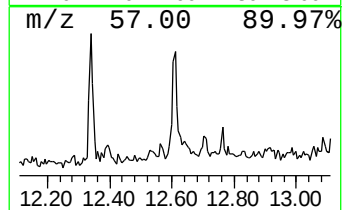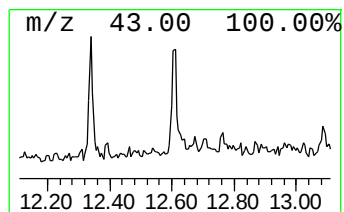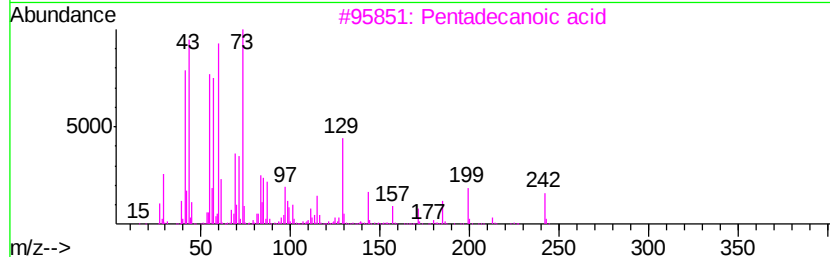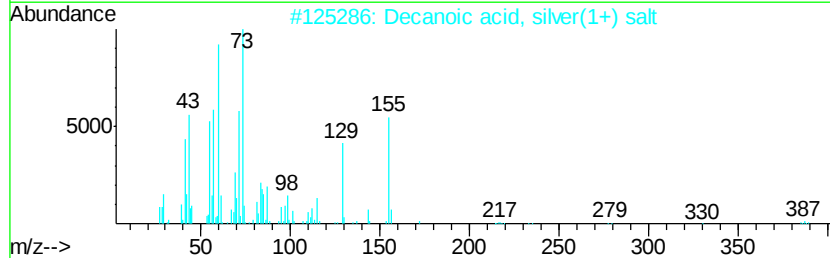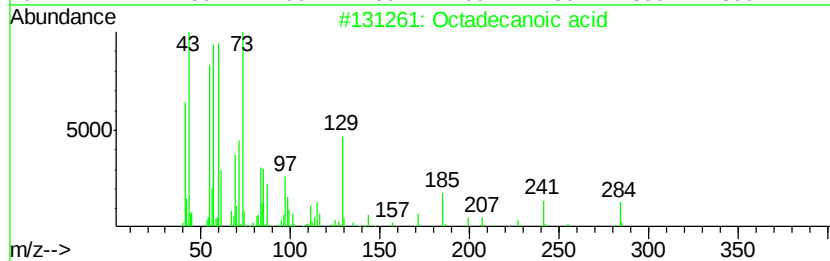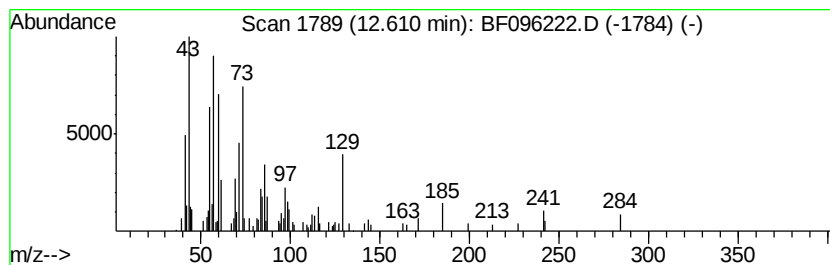

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096222.D
Acq On : 27 Jun 2017 18:02
Operator : SJ/MA
Sample : I3868-04 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-062217-B

Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.96	3.3	ng	185531	1	6.78	1133810	20.0
unknown6.54	6.54	19.7	ng	1115490	1	6.78	1133810	20.0
Octadecanoic acid	12.61	2.6	ng	129828	5	13.92	1016040	20.0