

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
 Data File : BF096223.D
 Acq On : 27 Jun 2017 18:30
 Operator : SJ/MA
 Sample : I3868-07 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-062217-C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.963	485	489	495	rVB	186997	189634	11.36%	0.884%
2	5.381	556	560	564	rBV	1306495	1100790	65.97%	5.132%
3	6.398	728	733	736	rBV	1212379	1098396	65.82%	5.120%
4	6.540	753	757	761	rBV	1282708	1090564	65.35%	5.084%
5	6.781	794	798	801	rBV	1328208	1182292	70.85%	5.512%
6	6.934	820	824	828	rVB	1032603	803886	48.17%	3.747%
7	7.328	886	891	894	rBV	721695	644255	38.61%	3.003%
8	7.392	899	902	904	rVB	39458	33347	2.00%	0.155%
9	7.422	904	907	909	rBV3	20504	28051	1.68%	0.131%
10	7.592	931	936	940	rVB6	27746	31521	1.89%	0.147%
11	7.710	954	956	962	rVB3	17544	21578	1.29%	0.101%
12	7.792	967	970	974	rBV5	18700	27248	1.63%	0.127%
13	7.828	974	976	980	rVB3	20966	25812	1.55%	0.120%
14	7.975	997	1001	1003	rBV4	15982	21997	1.32%	0.103%
15	8.057	1011	1015	1019	rBV	1835798	1668681	100.00%	7.779%
16	8.139	1027	1029	1031	rVB	31631	23872	1.43%	0.111%
17	8.163	1031	1033	1037	rBV5	15780	21524	1.29%	0.100%
18	8.239	1043	1046	1049	rBV4	24992	29026	1.74%	0.135%
19	8.363	1062	1067	1070	rBV4	49276	68276	4.09%	0.318%
20	8.386	1070	1071	1074	rVB3	26894	22137	1.33%	0.103%
21	8.416	1074	1076	1079	rBV3	37595	33203	1.99%	0.155%
22	8.451	1079	1082	1086	rBV4	47044	51289	3.07%	0.239%
23	8.498	1086	1090	1094	rVV4	61712	92250	5.53%	0.430%
24	8.569	1099	1102	1105	rVV4	37622	39866	2.39%	0.186%
25	8.663	1115	1118	1121	rBV	172455	148487	8.90%	0.692%
26	8.763	1132	1135	1138	rVB3	43236	49766	2.98%	0.232%
27	8.822	1141	1145	1147	rBV4	25724	42702	2.56%	0.199%
28	8.886	1150	1156	1158	rBV4	51956	64928	3.89%	0.303%
29	8.945	1164	1166	1169	rBV3	40782	38156	2.29%	0.178%
30	9.028	1178	1180	1183	rVB	53357	37931	2.27%	0.177%
31	9.069	1185	1187	1189	rVV3	28991	27748	1.66%	0.129%
32	9.098	1189	1192	1194	rVV2	87163	81064	4.86%	0.378%
33	9.133	1194	1198	1201	rVV	1352817	1045808	62.67%	4.875%
34	9.181	1204	1206	1208	rBV3	26244	21691	1.30%	0.101%

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
 Data File : BF096223.D
 Acq On : 27 Jun 2017 18:30
 Operator : SJ/MA
 Sample : I3868-07 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-062217-C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	9.228	1211	1214	1218	rVV	263154	234903	14.08%	1.095%
36	9.286	1221	1224	1226	rVV3	62016	77493	4.64%	0.361%
37	9.310	1226	1228	1231	rVB4	31892	25026	1.50%	0.117%
38	9.392	1239	1242	1245	rBV5	35826	33431	2.00%	0.156%
39	9.457	1249	1253	1254	rBV3	49520	59083	3.54%	0.275%
40	9.528	1262	1265	1267	rBV	240605	228955	13.72%	1.067%
41	9.551	1267	1269	1270	rVV	94033	70499	4.22%	0.329%
42	9.569	1270	1272	1275	rVB3	68098	53893	3.23%	0.251%
43	9.604	1275	1278	1281	rVB2	52039	50692	3.04%	0.236%
44	9.639	1281	1284	1286	rBV3	24165	30306	1.82%	0.141%
45	9.698	1292	1294	1297	rVB4	24814	22602	1.35%	0.105%
46	9.757	1301	1304	1307	rVB	368427	263625	15.80%	1.229%
47	9.810	1308	1313	1317	rBV2	1671917	1479203	88.65%	6.896%
48	9.992	1340	1344	1346	rBV3	55779	95113	5.70%	0.443%
49	10.016	1346	1348	1351	rVV3	61978	60822	3.64%	0.284%
50	10.045	1351	1353	1356	rVV2	37139	30337	1.82%	0.141%
51	10.080	1356	1359	1363	rVB3	88519	87588	5.25%	0.408%
52	10.116	1363	1365	1366	rBV	37531	23164	1.39%	0.108%
53	10.257	1385	1389	1391	rVB	391323	329249	19.73%	1.535%
54	10.380	1407	1410	1415	rVV7	35073	52340	3.14%	0.244%
55	10.416	1415	1416	1419	rVB2	40262	33145	1.99%	0.155%
56	10.475	1422	1426	1429	rVV	151717	191041	11.45%	0.891%
57	10.527	1432	1435	1438	rVB	51308	44504	2.67%	0.207%
58	10.557	1438	1440	1442	rBV2	61123	54589	3.27%	0.254%
59	10.586	1442	1445	1449	rVB2	523002	477102	28.59%	2.224%
60	10.727	1466	1469	1478	rBV	475360	510993	30.62%	2.382%
61	10.922	1499	1502	1506	rBV2	58860	96297	5.77%	0.449%
62	10.957	1506	1508	1510	rVB	55645	42440	2.54%	0.198%
63	10.986	1510	1513	1515	rVB	45194	36656	2.20%	0.171%
64	11.016	1515	1518	1520	rBV	44110	40661	2.44%	0.190%
65	11.051	1522	1524	1528	rVB3	56978	53410	3.20%	0.249%
66	11.175	1542	1545	1548	rBV	483739	376958	22.59%	1.757%
67	11.204	1548	1550	1556	rVB	135425	139686	8.37%	0.651%
68	11.286	1561	1564	1567	rVV	1185983	1045499	62.65%	4.874%
69	11.310	1567	1568	1572	rVB2	71042	53540	3.21%	0.250%
70	11.445	1589	1591	1594	rVB2	39834	32685	1.96%	0.152%
71	11.486	1595	1598	1600	rVV2	41166	37644	2.26%	0.175%

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
 Data File : BF096223.D
 Acq On : 27 Jun 2017 18:30
 Operator : SJ/MA
 Sample : I3868-07 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-062217-C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	11.522	1601	1604	1607	rVV3	52700	62489	3.74%	0.291%
73	11.557	1608	1610	1613	rVV3	35315	29433	1.76%	0.137%
74	11.598	1614	1617	1623	rVB	332695	284340	17.04%	1.326%
75	11.692	1631	1633	1638	rVB2	48375	51841	3.11%	0.242%
76	11.763	1642	1645	1647	rBV3	34911	39811	2.39%	0.186%
77	11.822	1652	1655	1659	rVV4	91139	104080	6.24%	0.485%
78	11.857	1659	1661	1664	rVB4	30934	29319	1.76%	0.137%
79	11.898	1665	1668	1671	rBV5	41534	47245	2.83%	0.220%
80	12.004	1684	1686	1690	rVB	267170	210567	12.62%	0.982%
81	12.157	1710	1712	1714	rBV2	20455	21302	1.28%	0.099%
82	12.286	1732	1734	1737	rVB3	35566	31838	1.91%	0.148%
83	12.339	1740	1743	1746	rBV3	42349	46339	2.78%	0.216%
84	12.380	1746	1750	1751	rBV2	170110	164284	9.85%	0.766%
85	12.392	1751	1752	1756	rVB2	239319	210275	12.60%	0.980%
86	12.492	1766	1769	1773	rBV	138656	155308	9.31%	0.724%
87	12.533	1773	1776	1783	rVV5	75753	113410	6.80%	0.529%
88	12.610	1786	1789	1796	rVV3	90673	111100	6.66%	0.518%
89	12.721	1803	1808	1813	rBV	148577	166531	9.98%	0.776%
90	12.763	1813	1815	1818	rVB	126808	105882	6.35%	0.494%
91	12.869	1830	1833	1837	rBV	704431	596179	35.73%	2.779%
92	13.027	1857	1860	1861	rBV3	29531	30852	1.85%	0.144%
93	13.121	1873	1876	1879	rVB	111215	104493	6.26%	0.487%
94	13.151	1879	1881	1888	rBV5	35518	69471	4.16%	0.324%
95	13.245	1895	1897	1900	rVB3	43473	35078	2.10%	0.164%
96	13.463	1931	1934	1938	rVB	70147	75283	4.51%	0.351%
97	13.774	1984	1987	1988	rBV	82903	67753	4.06%	0.316%
98	13.916	2007	2011	2014	rBV	1080377	1040863	62.38%	4.852%
99	15.339	2249	2253	2258	rBV	603670	735254	44.06%	3.428%
100	16.039	2369	2372	2380	rVB4	121662	227781	13.65%	1.062%


Sum of corrected areas: 21451351

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096223.D
Acq On : 27 Jun 2017 18:30
Operator : SJ/MA
Sample : I3868-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-062217-C

Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

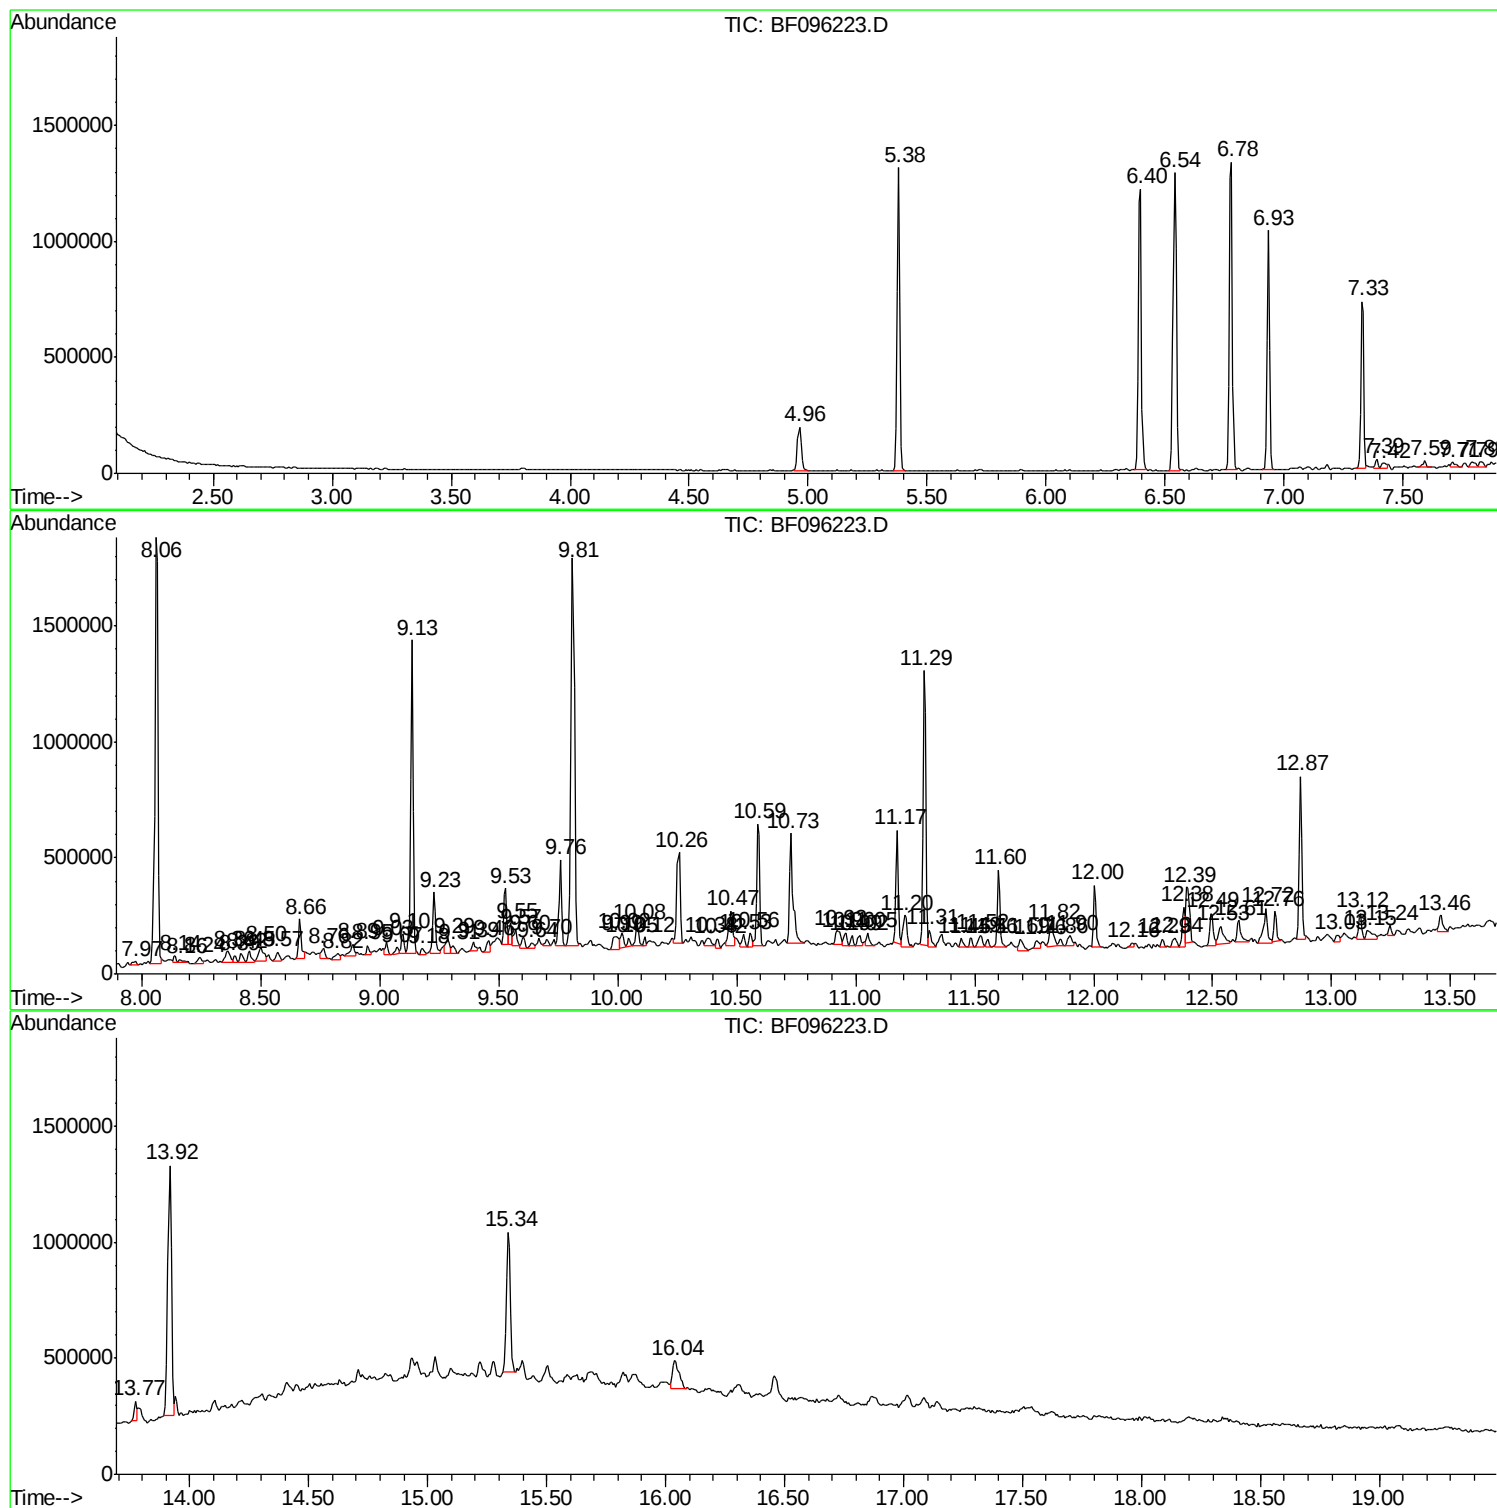

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096223.D
Acq On : 27 Jun 2017 18:30
Operator : SJ/MA
Sample : I3868-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-062217-C










Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 11

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.96	3.21 ng	189634	1,4-Dichlorobenzene-d4	6.78

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	40
3			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	36
4			2-Pentanol, 2,4-dimethyl-	116	C7H16O	000625-06-9	36
5			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9

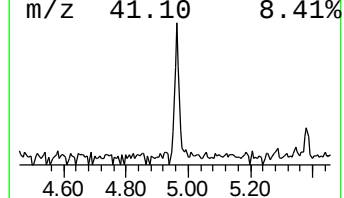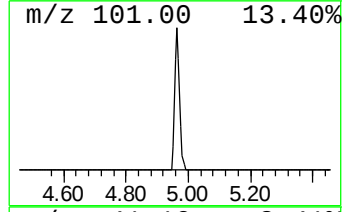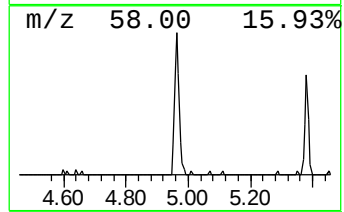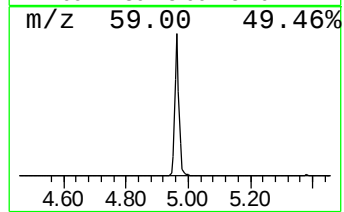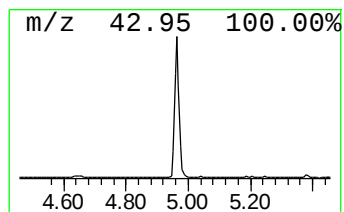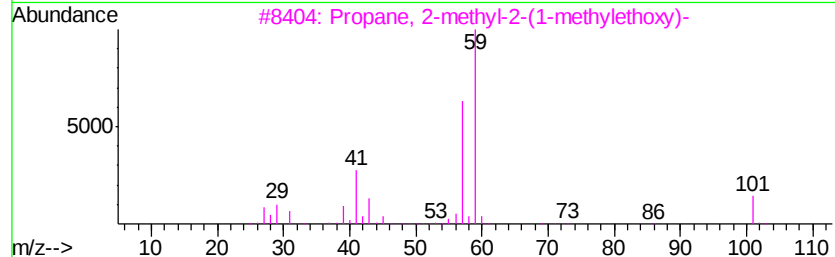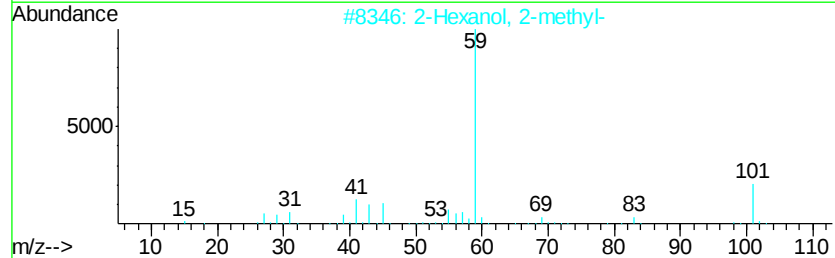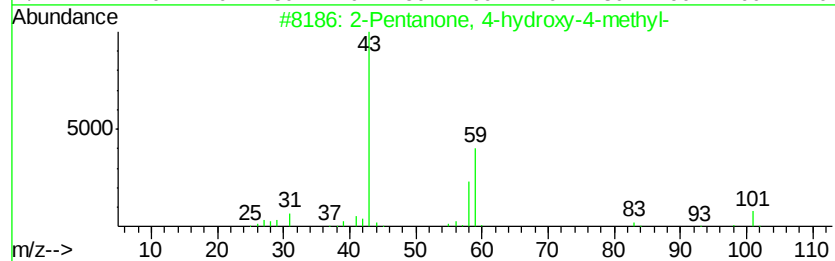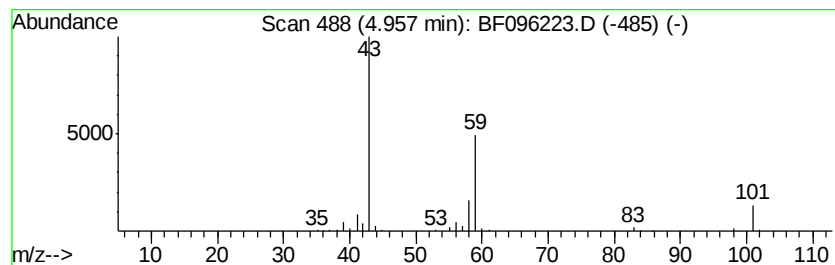

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096223.D
Acq On : 27 Jun 2017 18:30
Operator : SJ/MA
Sample : I3868-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-062217-C










Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.54 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.54	18.45 ng	1090560	1,4-Dichlorobenzene-d4	6.78

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			5-Aminoindole	132	C8H8N2	005192-03-0	12
3			Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
4			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
5			1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

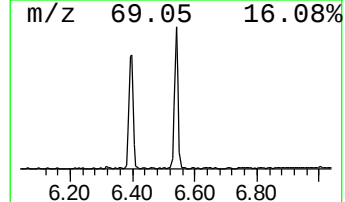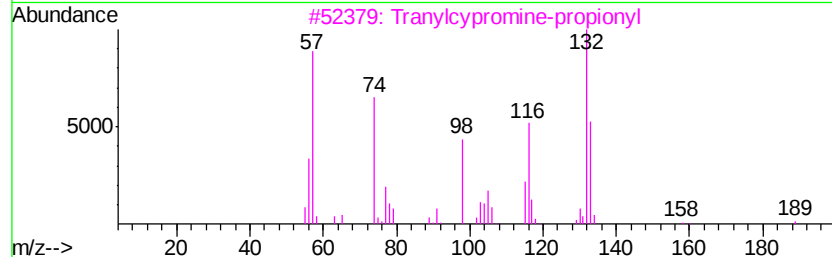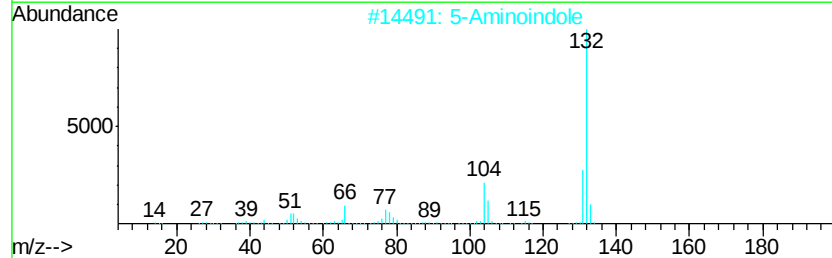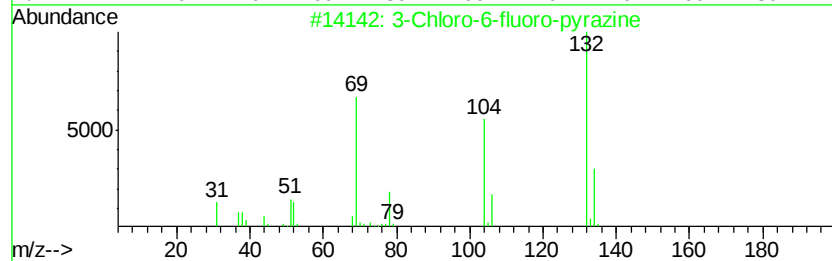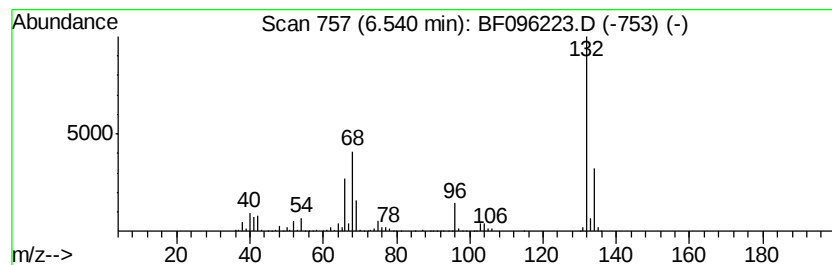

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
 Data File : BF096223.D
 Acq On : 27 Jun 2017 18:30
 Operator : SJ/MA
 Sample : I3868-07 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-062217-C










Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
 TIC Integration Parameters: LSCINT.P

 Peak Number 5 Tridecane Concentration Rank 10

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.76	3.56 ng	263625	Acenaphthene-d10	9.81

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Tridecane		184	C13H28	000629-50-5	90
2	Tetradecane		198	C14H30	000629-59-4	83
3	Hexadecane		226	C16H34	000544-76-3	80
4	Octane, 3,5-dimethyl-		142	C10H22	015869-93-9	74
5	Dodecane, 3-methyl-		184	C13H28	017312-57-1	72

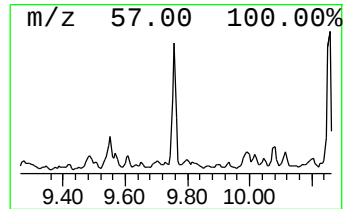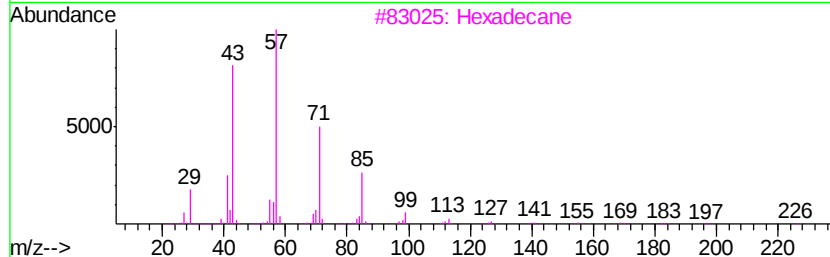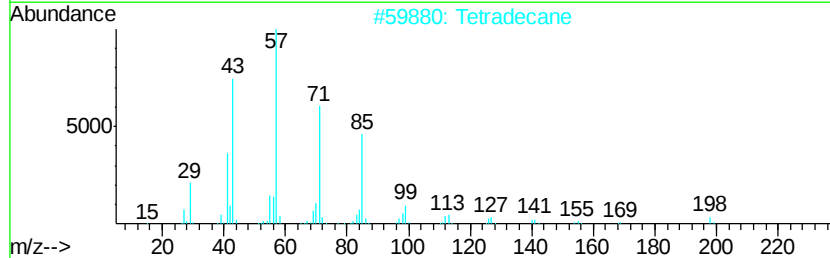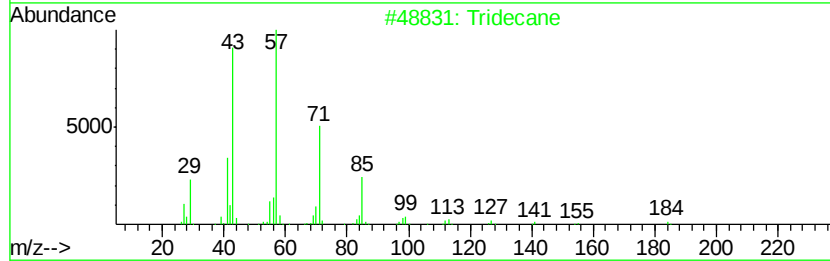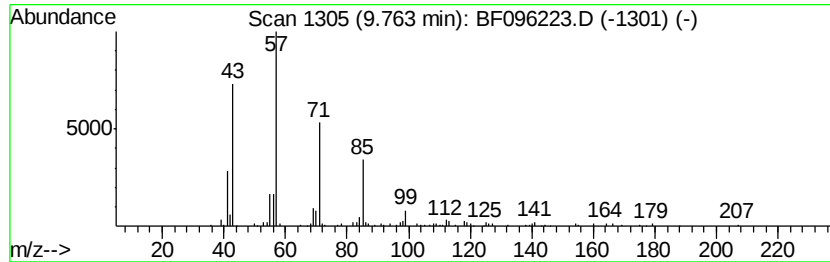

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096223.D
Acq On : 27 Jun 2017 18:30
Operator : SJ/MA
Sample : I3868-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
CL-01-062217-C

Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 7 Decane, 2,6,8-trimethyl- Concentration Rank 15

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.47	2.58 ng	191041	Acenaphthene-d10	9.81
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1	Decane, 2,6,8-trimethyl-	184 C13H28	062108-26-3	94
2	Undecane, 3,6-dimethyl-	184 C13H28	017301-28-9	80
3	Undecane, 3,5-dimethyl-	184 C13H28	017312-81-1	78
4	Dodecane, 6-methyl-	184 C13H28	006044-71-9	72
5	Undecane, 2,5-dimethyl-	184 C13H28	017301-22-3	62

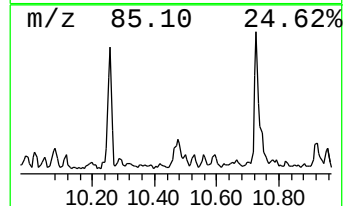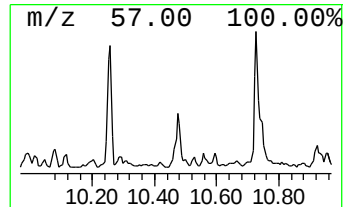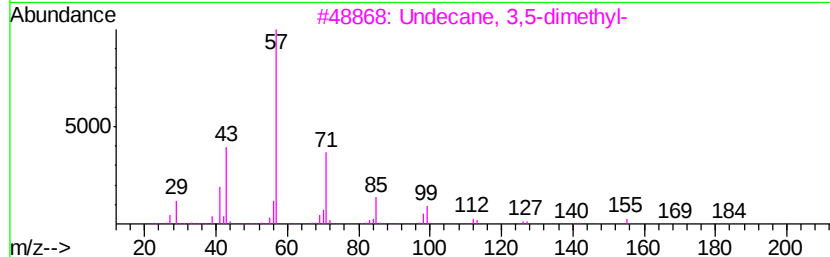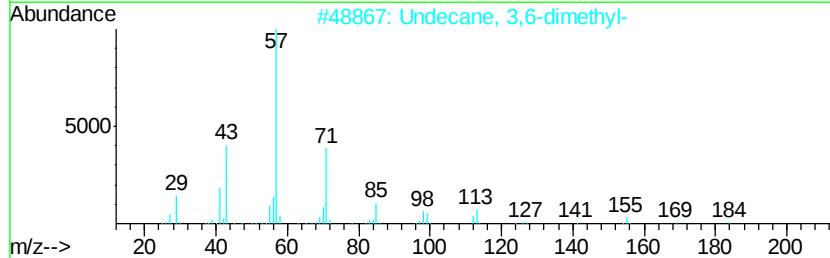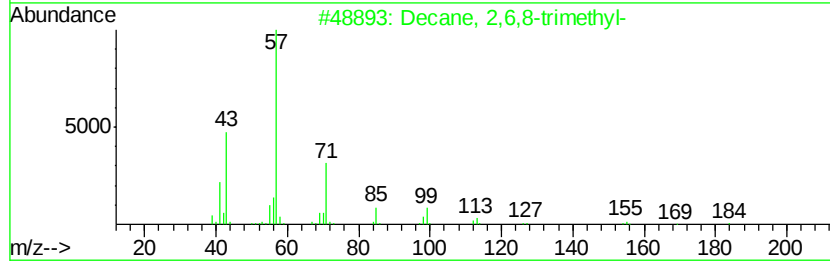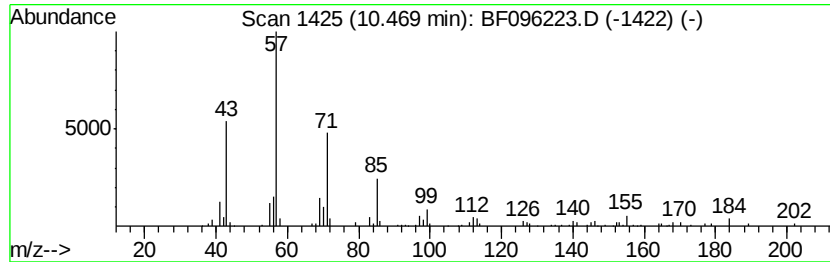

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096223.D
Acq On : 27 Jun 2017 18:30
Operator : SJ/MA
Sample : I3868-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
CL-01-062217-C

Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 9 Dodecane, 4-methyl- Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD		R.T.	
11.17	7.21 ng	376958	Phenanthrene-d10		11.29	
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Dodecane, 4-methyl-		184	C13H28	006117-97-1	87
2	Hexadecane		226	C16H34	000544-76-3	86
3	Heneicosane		296	C21H44	000629-94-7	86
4	Undecane, 3,5-dimethyl-		184	C13H28	017312-81-1	83
5	Sulfurous acid, 2-propyl tetradec...		320	C17H36O3S	1000309-12-5	72

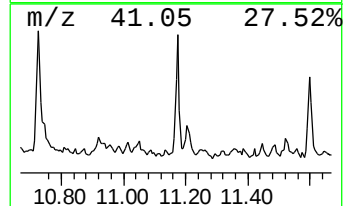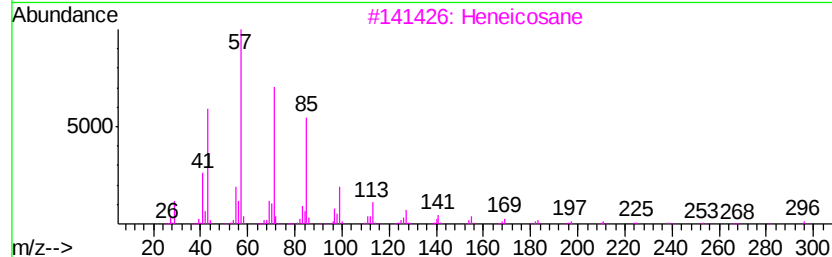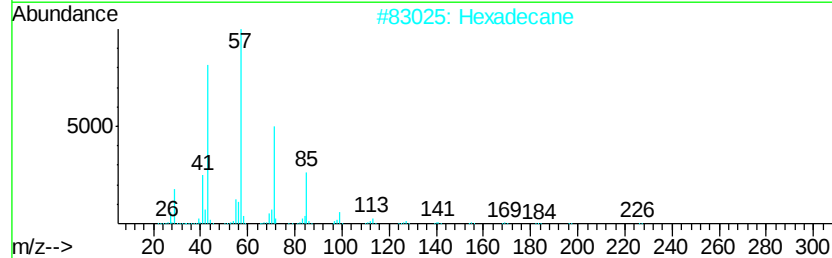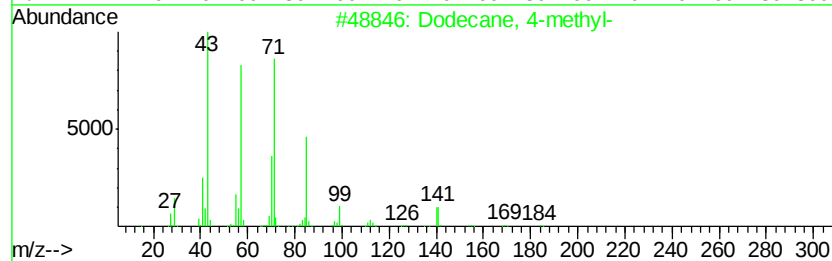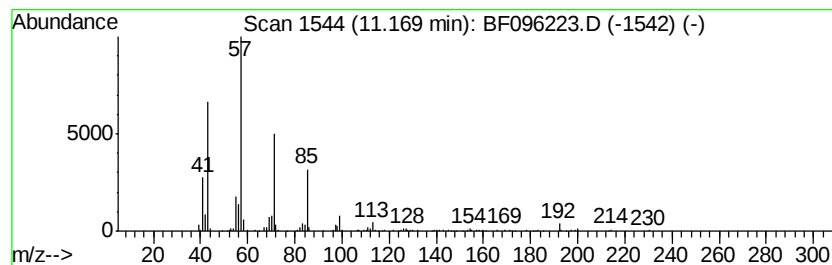

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096223.D
Acq On : 27 Jun 2017 18:30
Operator : SJ/MA
Sample : I3868-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
CL-01-062217-C

Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 11 Hexadecane Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.		
11.60	5.44 ng	284340	Phenanthrene-d10	11.29		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Hexadecane		226	C16H34	000544-76-3	90
2	Tridecane, 1-iodo-		310	C13H27I	035599-77-0	83
3	Tetracosane		338	C24H50	000646-31-1	83
4	Tetradecane, 1-iodo-		324	C14H29I	019218-94-1	80
5	Sulfurous acid, 2-ethylhexyl hex...		278	C14H30O3S	1000309-20-2	80

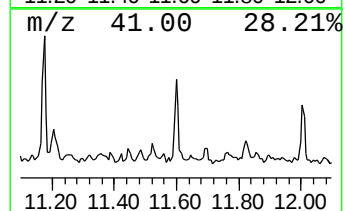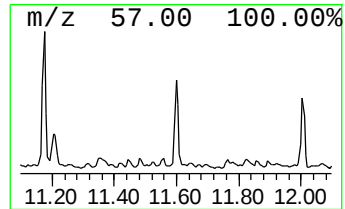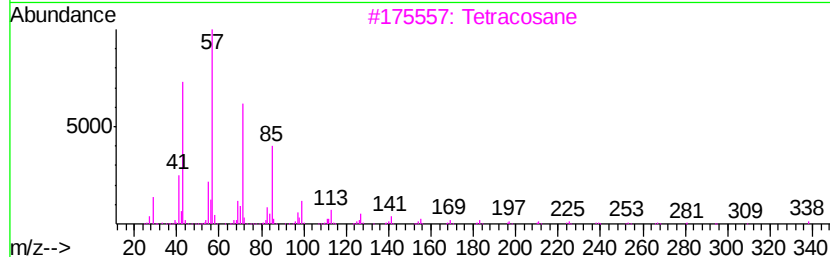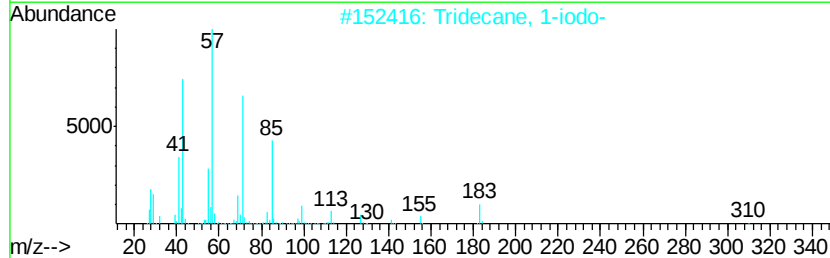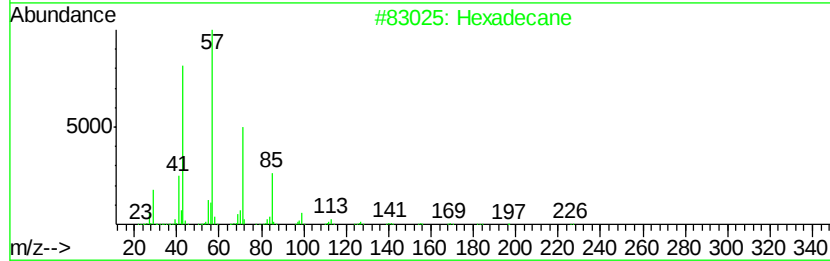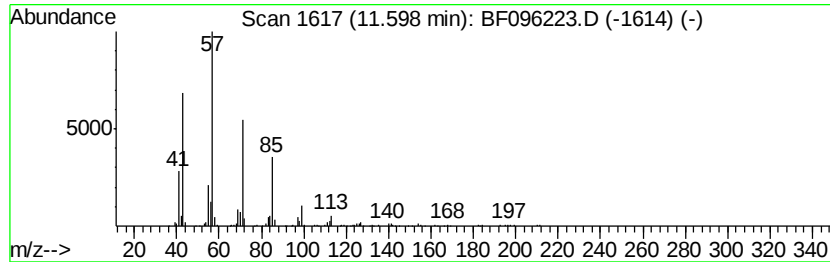

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096223.D
Acq On : 27 Jun 2017 18:30
Operator : SJ/MA
Sample : I3868-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-062217-C










Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 12 Heptacosane Concentration Rank 8

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.00	4.03 ng	210567	Phenanthrene-d10	11.29

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Heptacosane	380	C27H56	000593-49-7	86
2		Dodecane, 2-methyl-6-propyl-	226	C16H34	055045-08-4	86
3		Hexadecane	226	C16H34	000544-76-3	78
4		Heptadecane	240	C17H36	000629-78-7	76
5		Decane, 3-methyl-	156	C11H24	013151-34-3	74

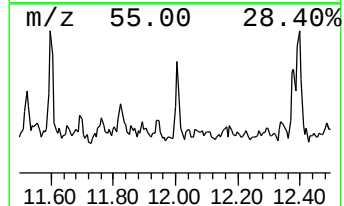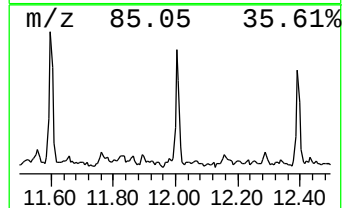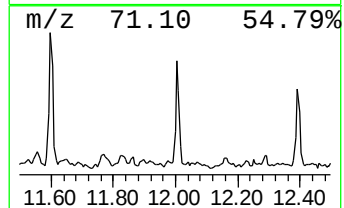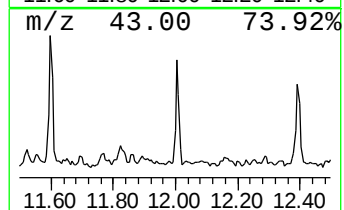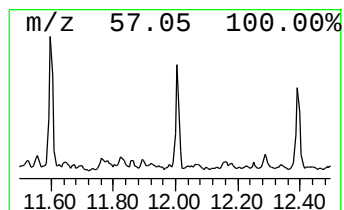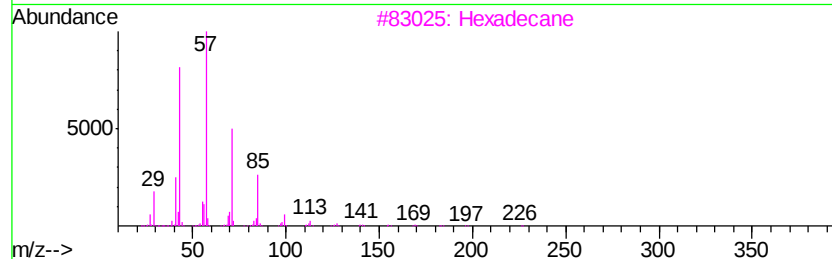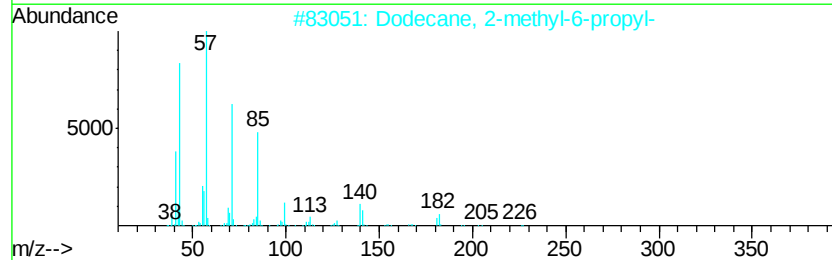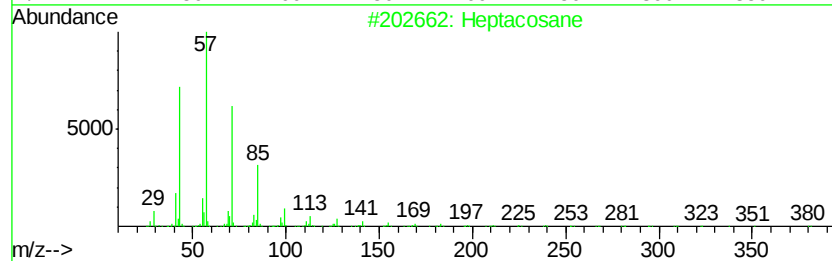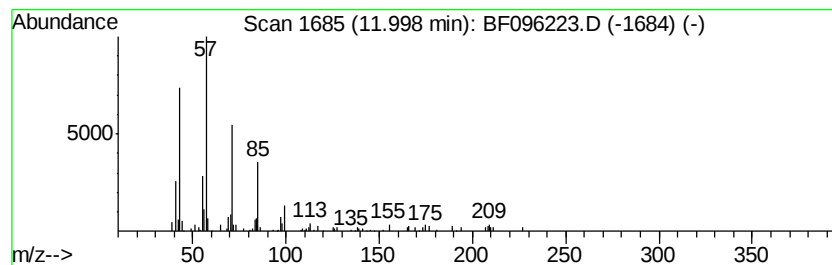

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096223.D
Acq On : 27 Jun 2017 18:30
Operator : SJ/MA
Sample : I3868-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-062217-C










Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 13 2-Chloroethyl linoleate Concentration Rank 13

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.38	3.14 ng	164284	Phenanthrene-d10	11.29

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Chloroethyl linoleate	342	C20H35ClO2	025525-76-2	86
2		Bicyclo[2.2.2]octane, 2-methyl-	124	C9H16	000766-53-0	80
3		4,5-Nonadiene, 2-methyl-	138	C10H18	055956-32-6	74
4		9,12-Octadecadienoic acid, methy...	294	C19H34O2	002566-97-4	70
5		(Z)6,(Z)9-Pentadecadien-1-ol	224	C15H28O	077899-11-7	64

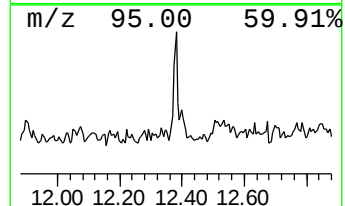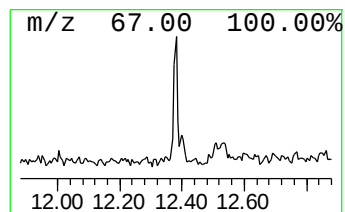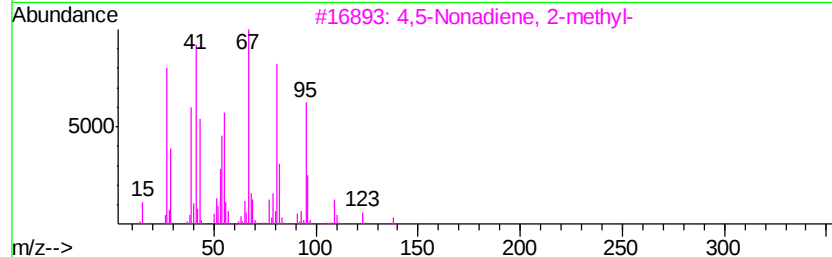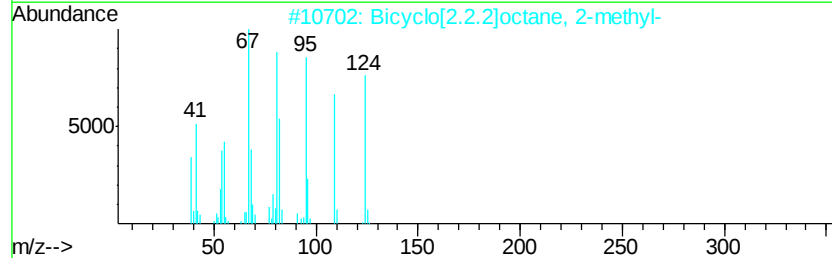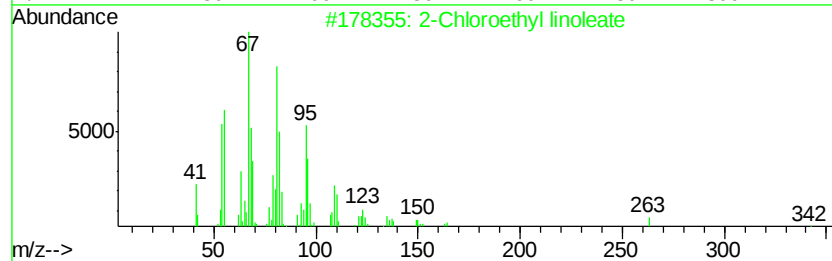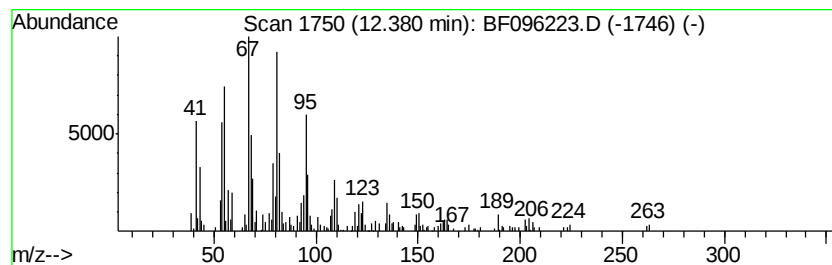

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096223.D
Acq On : 27 Jun 2017 18:30
Operator : SJ/MA
Sample : I3868-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
CL-01-062217-C

Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 14 Heneicosane Concentration Rank 9

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.39	4.02 ng	210275	Phenanthrene-d10	11.29
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1	Heneicosane		296 C21H44	000629-94-7 78
2	Sulfurous acid, 2-propyl tetradec...		320 C17H36O3S	1000309-12-5 72
3	Heptadecane		240 C17H36	000629-78-7 72
4	Octacosane		394 C28H58	000630-02-4 64
5	Decane, 2,3,6-trimethyl-		184 C13H28	062238-12-4 59

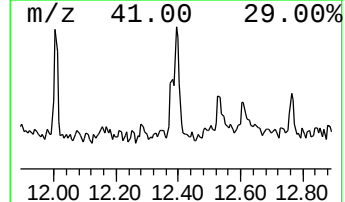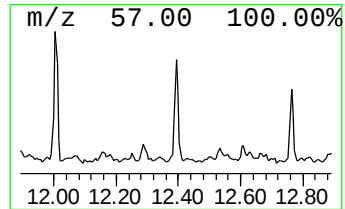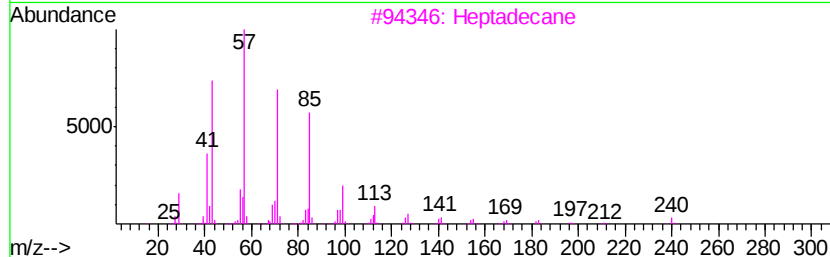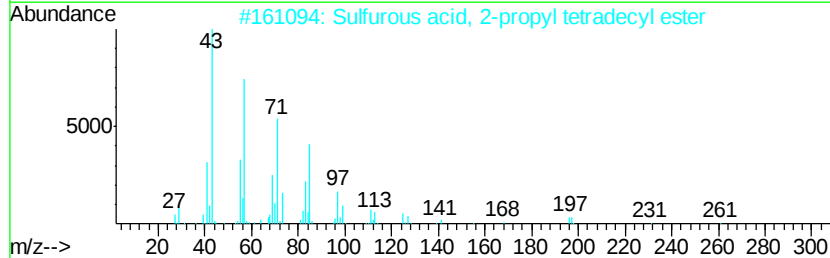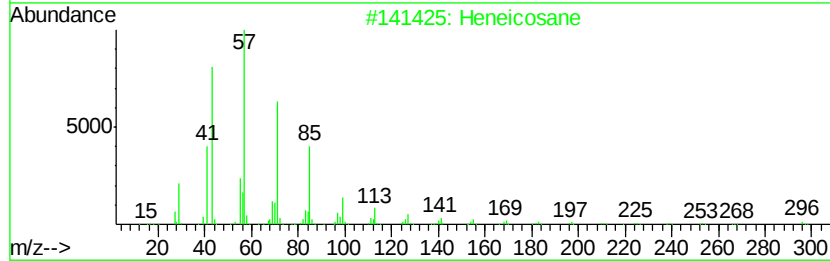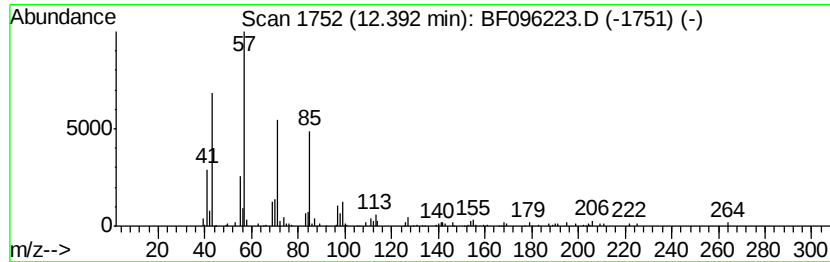

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096223.D
Acq On : 27 Jun 2017 18:30
Operator : SJ/MA
Sample : I3868-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
CL-01-062217-C

Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 15 unknown12.61 Concentration Rank 16

R.T.	EstConc	Area	Relative to ISTD	R.T.	
12.61	2.13 ng	111100	Chrysene-d12	13.92	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Undecanoic acid	186	C11H22O2	000112-37-8	46
2	n-Decanoic acid	172	C10H20O2	000334-48-5	30
3	Oxalic acid, propyl tetradecyl e...	328	C19H36O4	1000309-26-7	30
4	1-Octadecanesulphonyl chloride	352	C18H37ClO2S	1000342-70-4	30
5	Hydroxylamine, O-decyl-	173	C10H23NO	029812-79-1	30

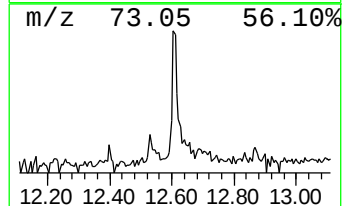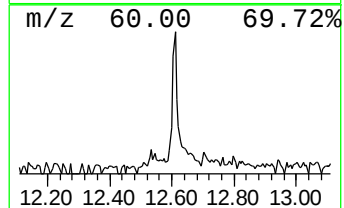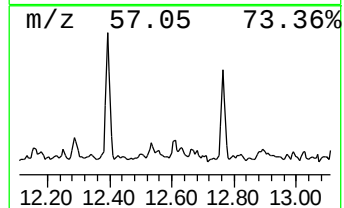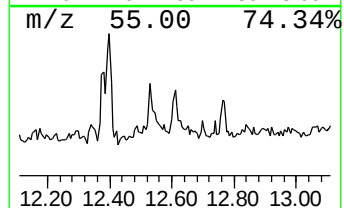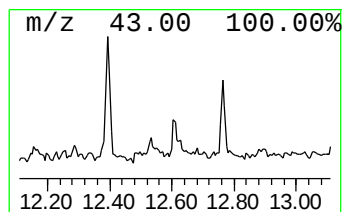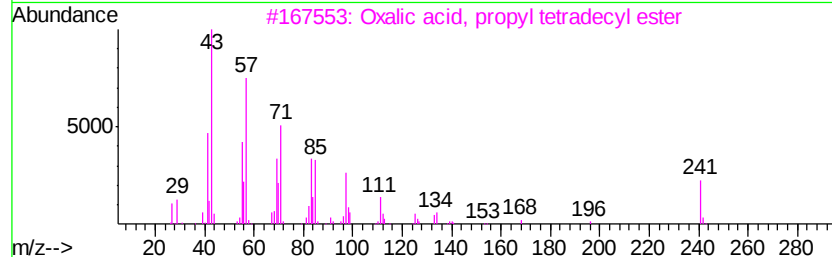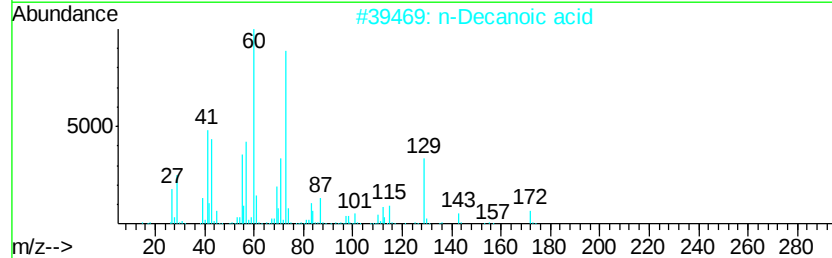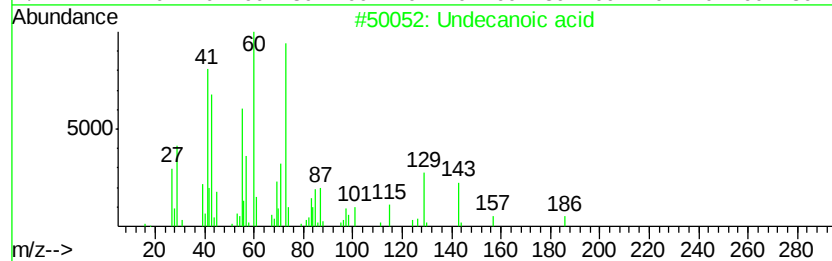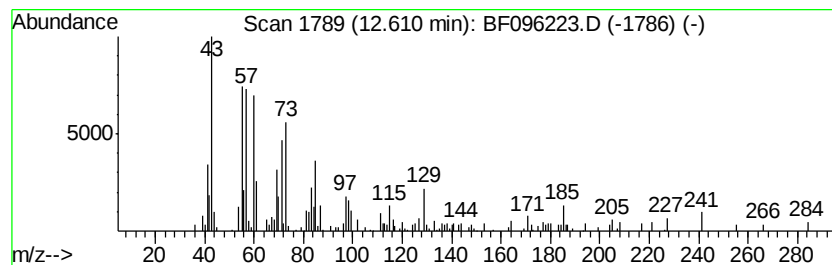

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096223.D
Acq On : 27 Jun 2017 18:30
Operator : SJ/MA
Sample : I3868-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
CL-01-062217-C

Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 16 Heptadecane Concentration Rank 17

R.T.	EstConc	Area	Relative to ISTD	R.T.	
13.12	2.01 ng	104493	Chrysene-d12	13.92	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Heptadecane	240	C17H36	000629-78-7	86
2	Heptacosane	380	C27H56	000593-49-7	68
3	Heptadecane, 9-octyl-	352	C25H52	007225-64-1	62
4	Heptadecane, 2-methyl-	254	C18H38	001560-89-0	59
5	Hexadecane, 3-methyl-	240	C17H36	006418-43-5	59

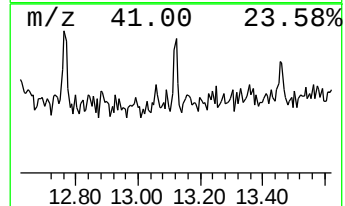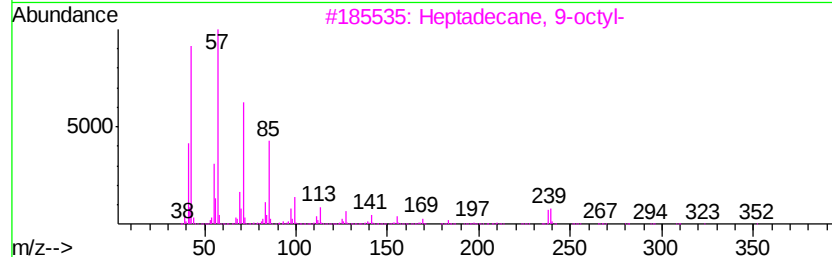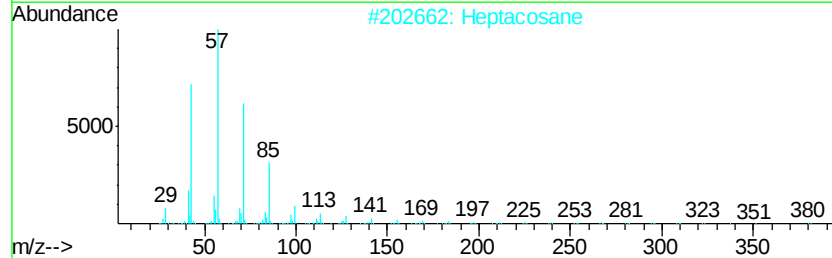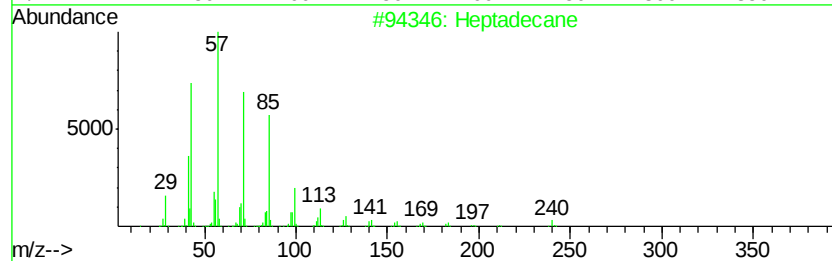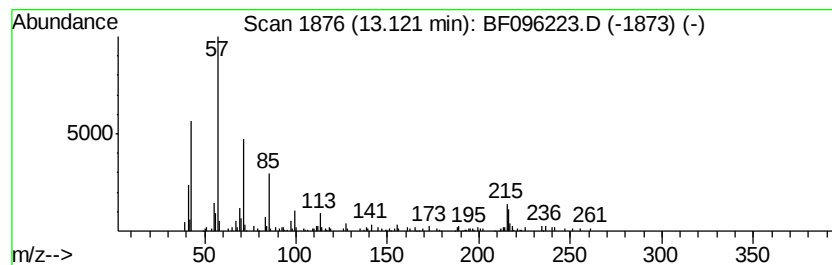

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096223.D
Acq On : 27 Jun 2017 18:30
Operator : SJ/MA
Sample : I3868-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
CL-01-062217-C

Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 17 28-Nor-17.beta.(H)-hopane Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.04	6.20 ng	227781	Perylene-d12	15.34
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1	28-Nor-17.beta.(H)-hopane	398	C29H50	036728-72-0 78
2	2H-1,2,3-Triazole-4-carboxaldehy...	191	C9H6FN3O	051306-43-5 38
3	Propenoic acid, 3-(3,4-dimethoxy...	344	C19H24N2O4	1000259-51-5 30
4	4-Fluoro-2-trifluoromethylbenzoi...	318	C14H7ClF4O2	1000357-66-5 22
5	2,3-Dimethyl-6-(3-methyl-buteryl...	248	C15H20O3	071940-30-2 22

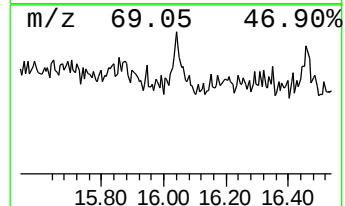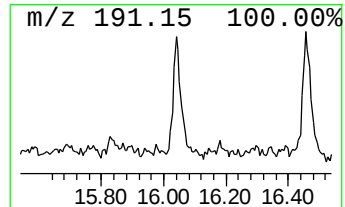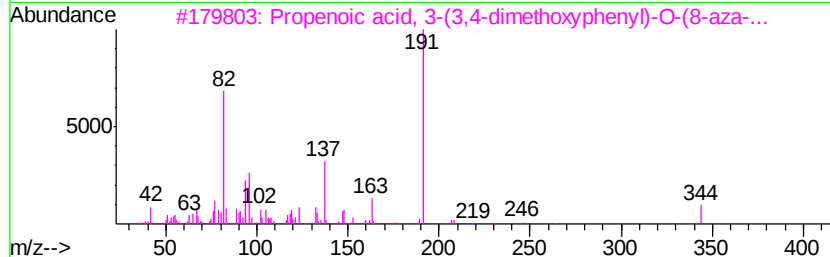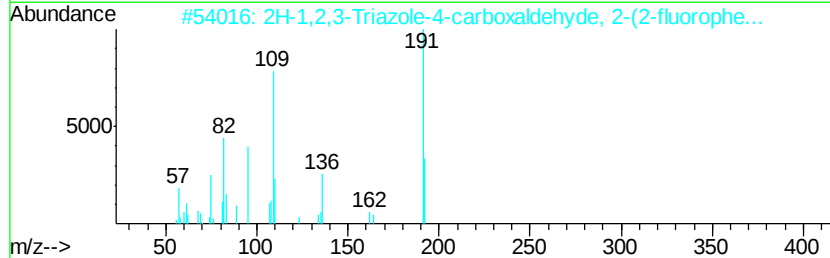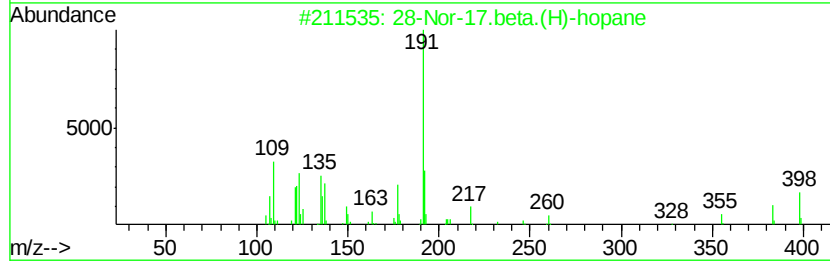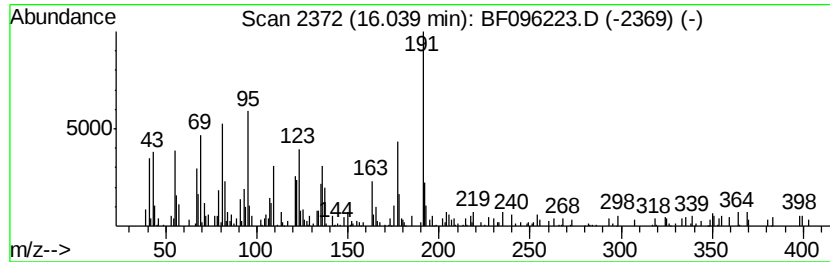

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062717\
Data File : BF096223.D
Acq On : 27 Jun 2017 18:30
Operator : SJ/MA
Sample : I3868-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-062217-C

Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.96	3.2	ng	189634	1	6.78	1182290	20.0
unknown6.54	6.54	18.4	ng	1090560	1	6.78	1182290	20.0
Tridecane	9.76	3.6	ng	263625	3	9.81	1479200	20.0
Decane, 2,6,8-tri...	10.47	2.6	ng	191041	3	9.81	1479200	20.0
Dodecane, 4-methyl-	11.17	7.2	ng	376958	4	11.29	1045500	20.0
Hexadecane	11.60	5.4	ng	284340	4	11.29	1045500	20.0
Heptacosane	12.00	4.0	ng	210567	4	11.29	1045500	20.0
2-Chloroethyl lin...	12.38	3.1	ng	164284	4	11.29	1045500	20.0
Heneicosane	12.39	4.0	ng	210275	4	11.29	1045500	20.0
unknown12.61	12.61	2.1	ng	111100	5	13.92	1040860	20.0
Heptadecane	13.12	2.0	ng	104493	5	13.92	1040860	20.0
28-Nor-17.beta.(H...	16.04	6.2	ng	227781	6	15.34	735254	20.0