


Data Path : Z:\HPCHEM1\BNA F\Data\BF062717\
 Data File : BF096207.D
 Acq On : 27 Jun 2017 9:56
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 28 15:41:49 2017

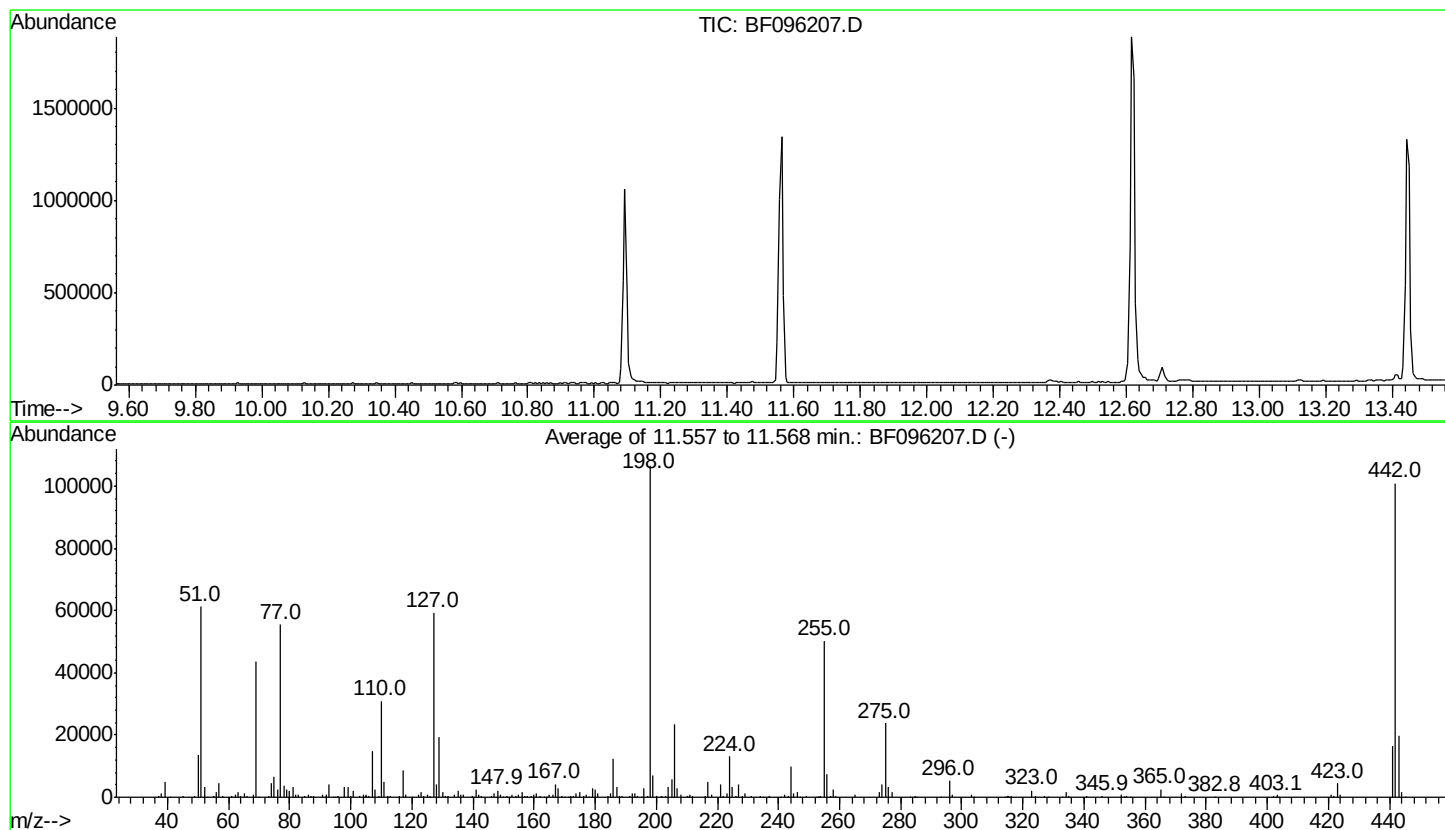

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.4	61127	PASS
68	69	0.00	2	1.4	633	PASS
69	198	0.00	100	41.1	43803	PASS
70	69	0.00	2	0.3	145	PASS
127	198	10	80	55.6	59298	PASS
197	198	0.00	2	0.5	577	PASS
198	198	100	100	100.0	106557	PASS
199	198	5	9	6.5	6956	PASS
275	198	10	60	22.4	23819	PASS
365	198	1	100	2.4	2603	PASS
441	442	0.01	24	16.2	16337	PASS
442	198	50	100	94.6	100856	PASS
443	442	15	24	19.7	19915	PASS