


Data Path : Z:\HPCHEM1\BNA F\Data\BF062717\
 Data File : BF096216.D
 Acq On : 27 Jun 2017 15:13
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF062717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 28 15:41:49 2017

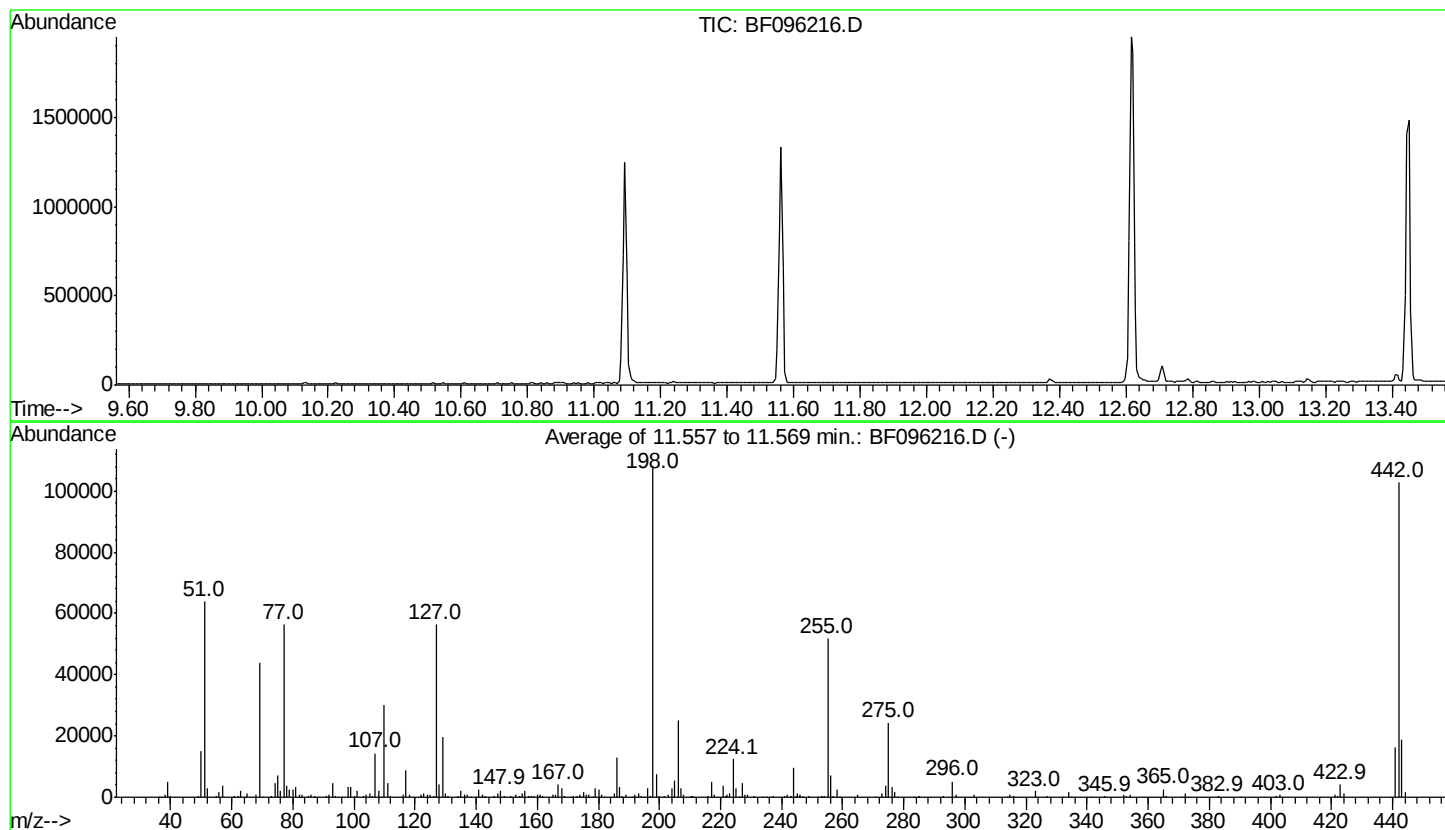

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.1	63930	PASS
68	69	0.00	2	1.9	825	PASS
69	198	0.00	100	40.6	43976	PASS
70	69	0.00	2	0.4	155	PASS
127	198	10	80	52.1	56349	PASS
197	198	0.00	2	0.3	330	PASS
198	198	100	100	100.0	108240	PASS
199	198	5	9	7.1	7686	PASS
275	198	10	60	22.5	24365	PASS
365	198	1	100	2.4	2596	PASS
441	442	0.01	24	15.9	16286	PASS
442	198	50	100	94.9	102728	PASS
443	442	15	24	18.3	18764	PASS