
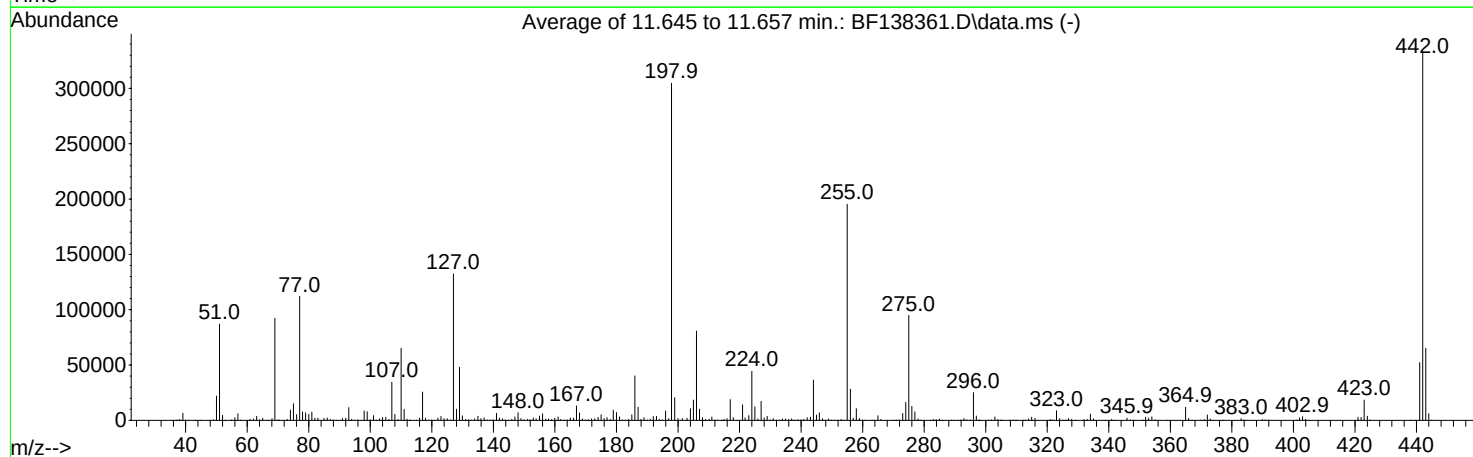


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF062724\  
Data File : BF138361.D  
Acq On : 27 Jun 2024 12:18  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF061224.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Jun 13 01:52:47 2024

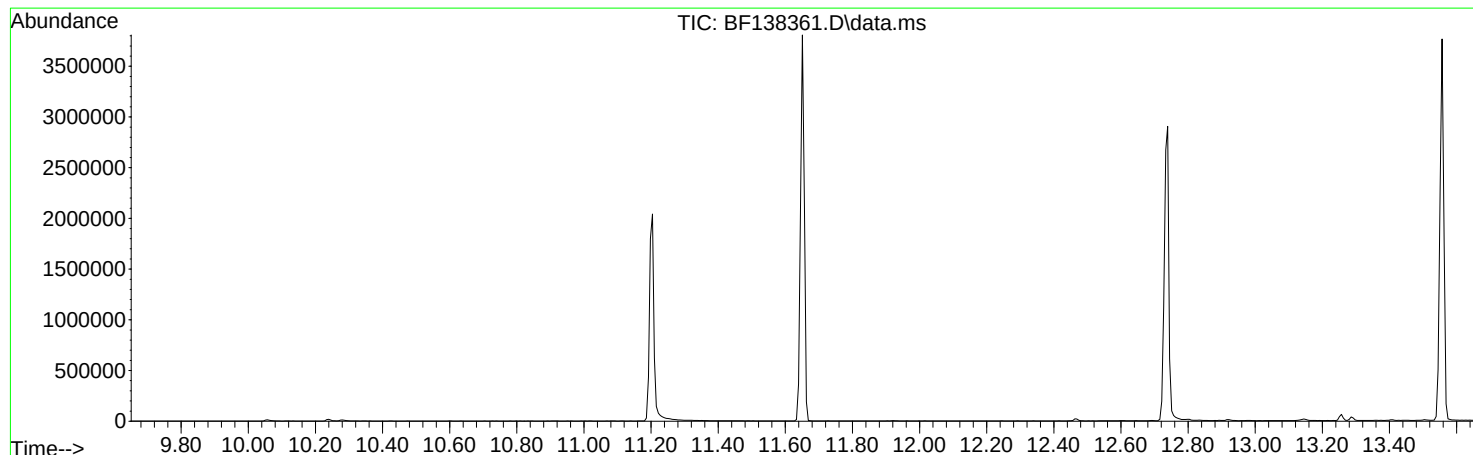




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 28.6         | 87112      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 1567       | PASS                |
| 69             | 198             | 0.00            | 100             | 30.3         | 92203      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 459        | PASS                |
| 127            | 198             | 10              | 80              | 43.4         | 132272     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 1614       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 304597     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 20498      | PASS                |
| 275            | 198             | 10              | 60              | 31.1         | 94795      | PASS                |
| 365            | 198             | 1               | 100             | 3.9          | 11814      | PASS                |
| 441            | 198             | 0.01            | 100             | 17.1         | 52163      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 332416     | PASS                |
| 443            | 442             | 15              | 24              | 19.6         | 65219      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF062724\  
Data File : BF138361.D  
Acq On : 27 Jun 2024 12:18  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jun 27 12:49:32 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF061224.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jun 13 01:52:47 2024  
Response via : Initial Calibration

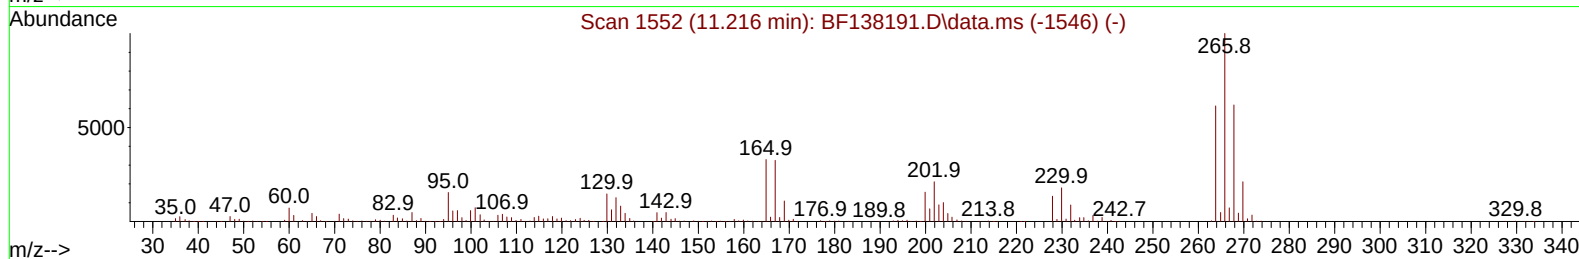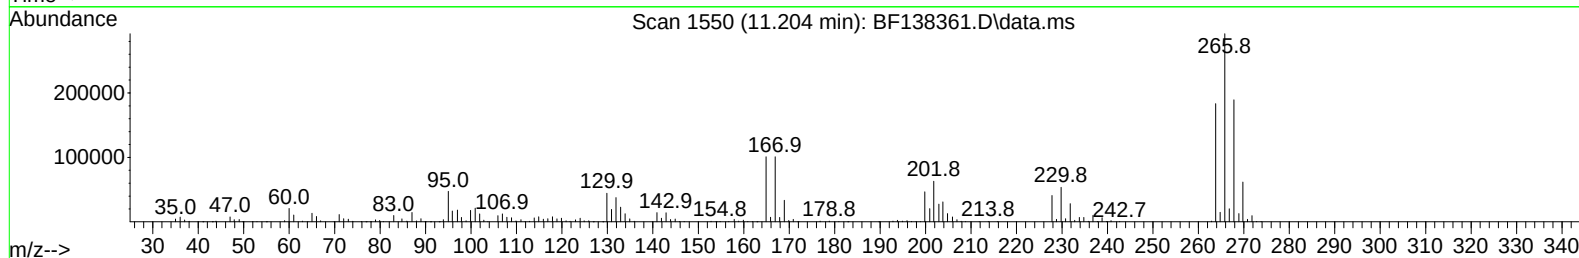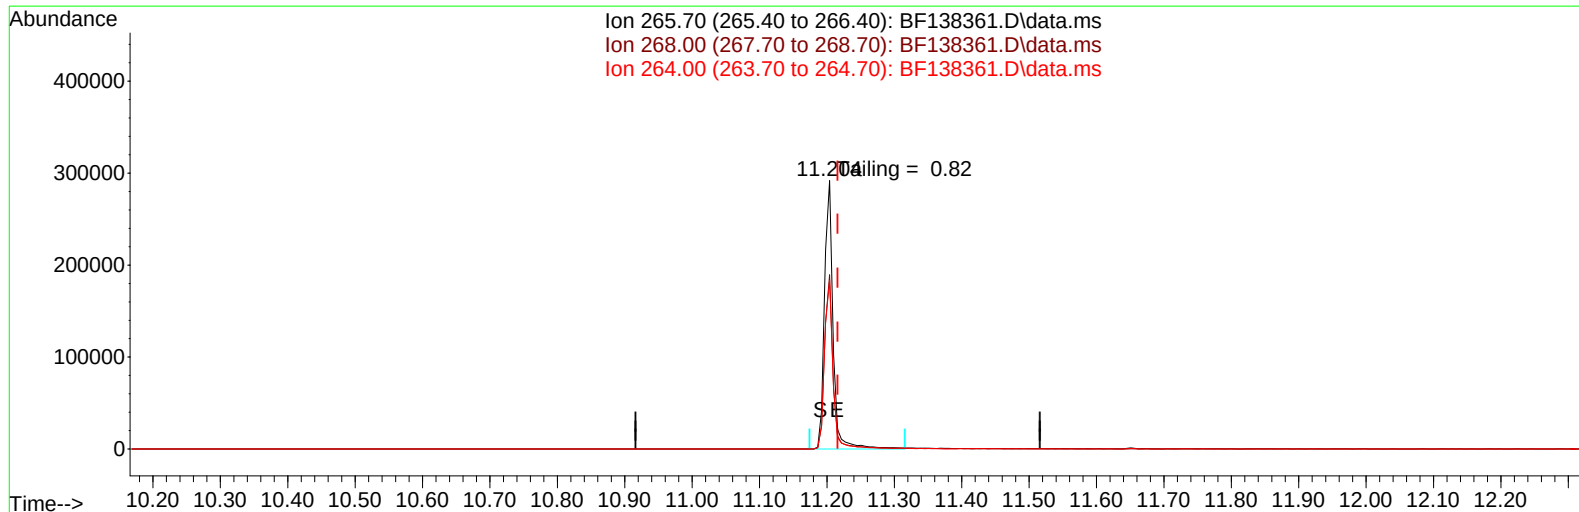

TIC: BF138361.D\data.ms

**(70) Pentachlorophenol (C)**

11.204min (-0.012) 27973.48 ng




response 258300

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.90  | 64.91  |
| 264.00 | 61.50  | 62.85  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF062724\  
Data File : BF138361.D  
Acq On : 27 Jun 2024 12:18  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jun 27 12:49:32 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF061224.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jun 13 01:52:47 2024  
Response via : Initial Calibration

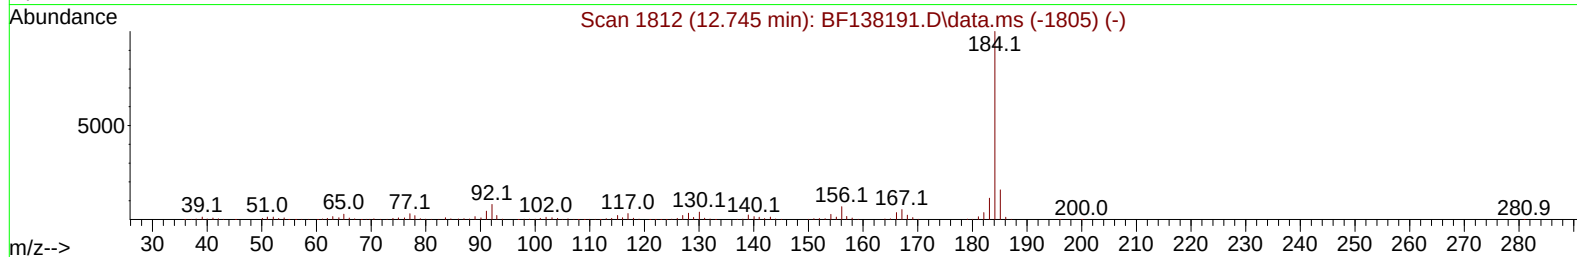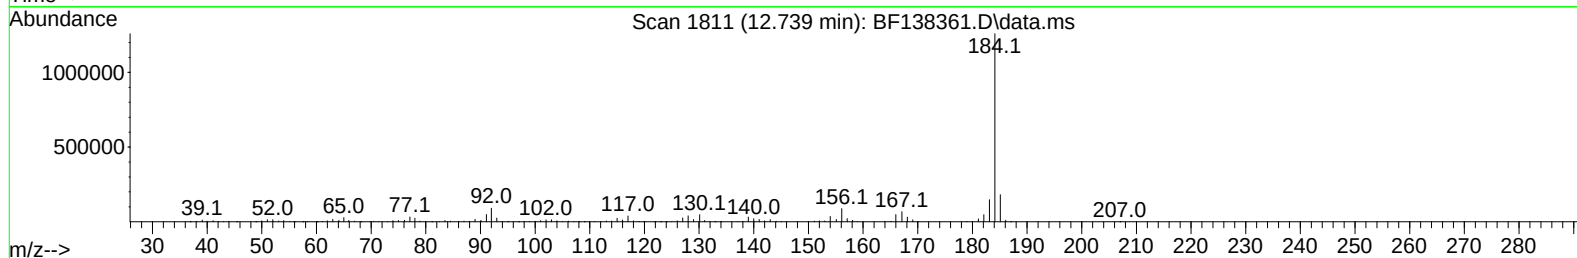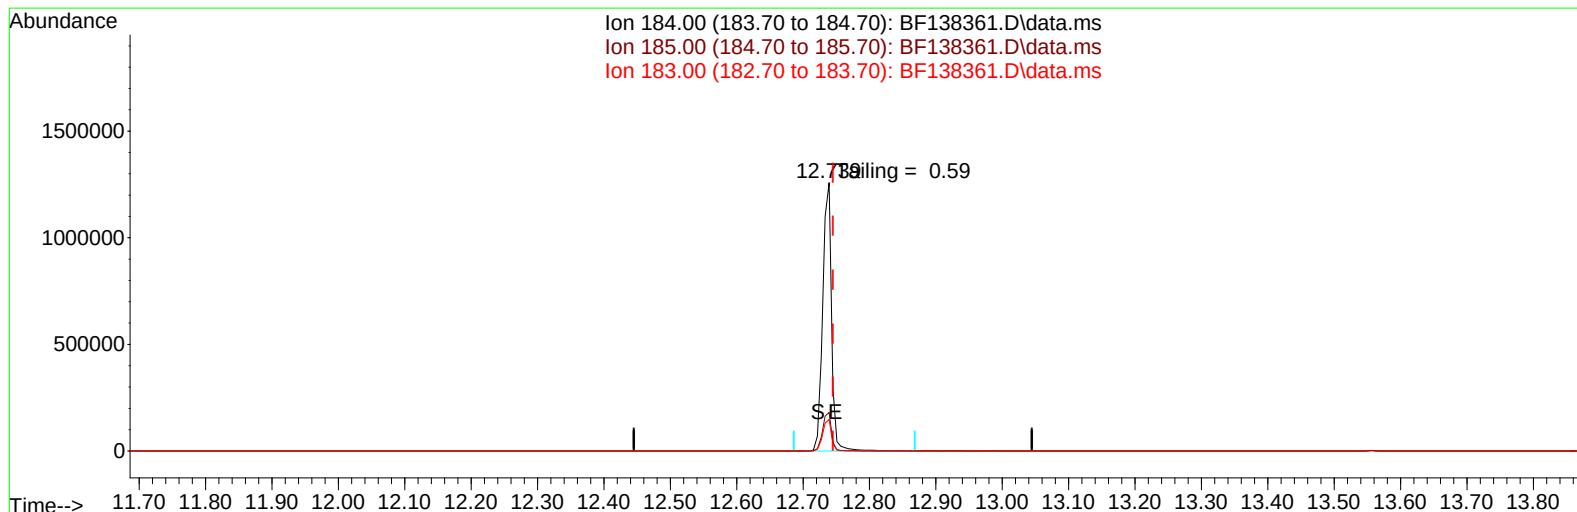

TIC: BF138361.D\data.ms

**(77) Benzidine**

12.739min (-0.006) 0.00 ng

response 1168480

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.80  | 14.38  |
| 183.00 | 11.30  | 11.78  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 6/27/2024     | BNA_F            | <u>BF138361.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 620347           | 13.557             |
| DDD           | 15965            | 13.257             |
| DDE           | 1699             | 12.921             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 17664         | 638011           | 2.77               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP