

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062725\
 Data File : BF142886.D
 Acq On : 27 Jun 2025 11:52
 Operator : RC/JU
 Sample : Q2413-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-73

Quant Time: Jun 27 12:24:11 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 24 05:28:21 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	71511	20.000	ng	0.00
21) Naphthalene-d8	8.157	136	269771	20.000	ng	-0.01
39) Acenaphthene-d10	9.916	164	131916	20.000	ng	0.00
64) Phenanthrene-d10	11.404	188	195199	20.000	ng	0.00
76) Chrysene-d12	14.051	240	151359	20.000	ng	0.00
86) Perylene-d12	15.545	264	151859	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.499	112	340790	79.343	ng	0.00
7) Phenol-d6	6.504	99	410766	81.060	ng	0.00
23) Nitrobenzene-d5	7.440	82	247380	50.298	ng	0.00
42) 2,4,6-Tribromophenol	10.710	330	104194	76.754	ng	0.00
45) 2-Fluorobiphenyl	9.234	172	520514	51.835	ng	-0.01
79) Terphenyl-d14	12.992	244	377407	34.452	ng	0.00
Target Compounds						
60) Diethylphthalate	10.328	149	24407	2.915	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062725\
Data File : BF142886.D
Acq On : 27 Jun 2025 11:52
Operator : RC/JU
Sample : Q2413-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-73

Quant Time: Jun 27 12:24:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration




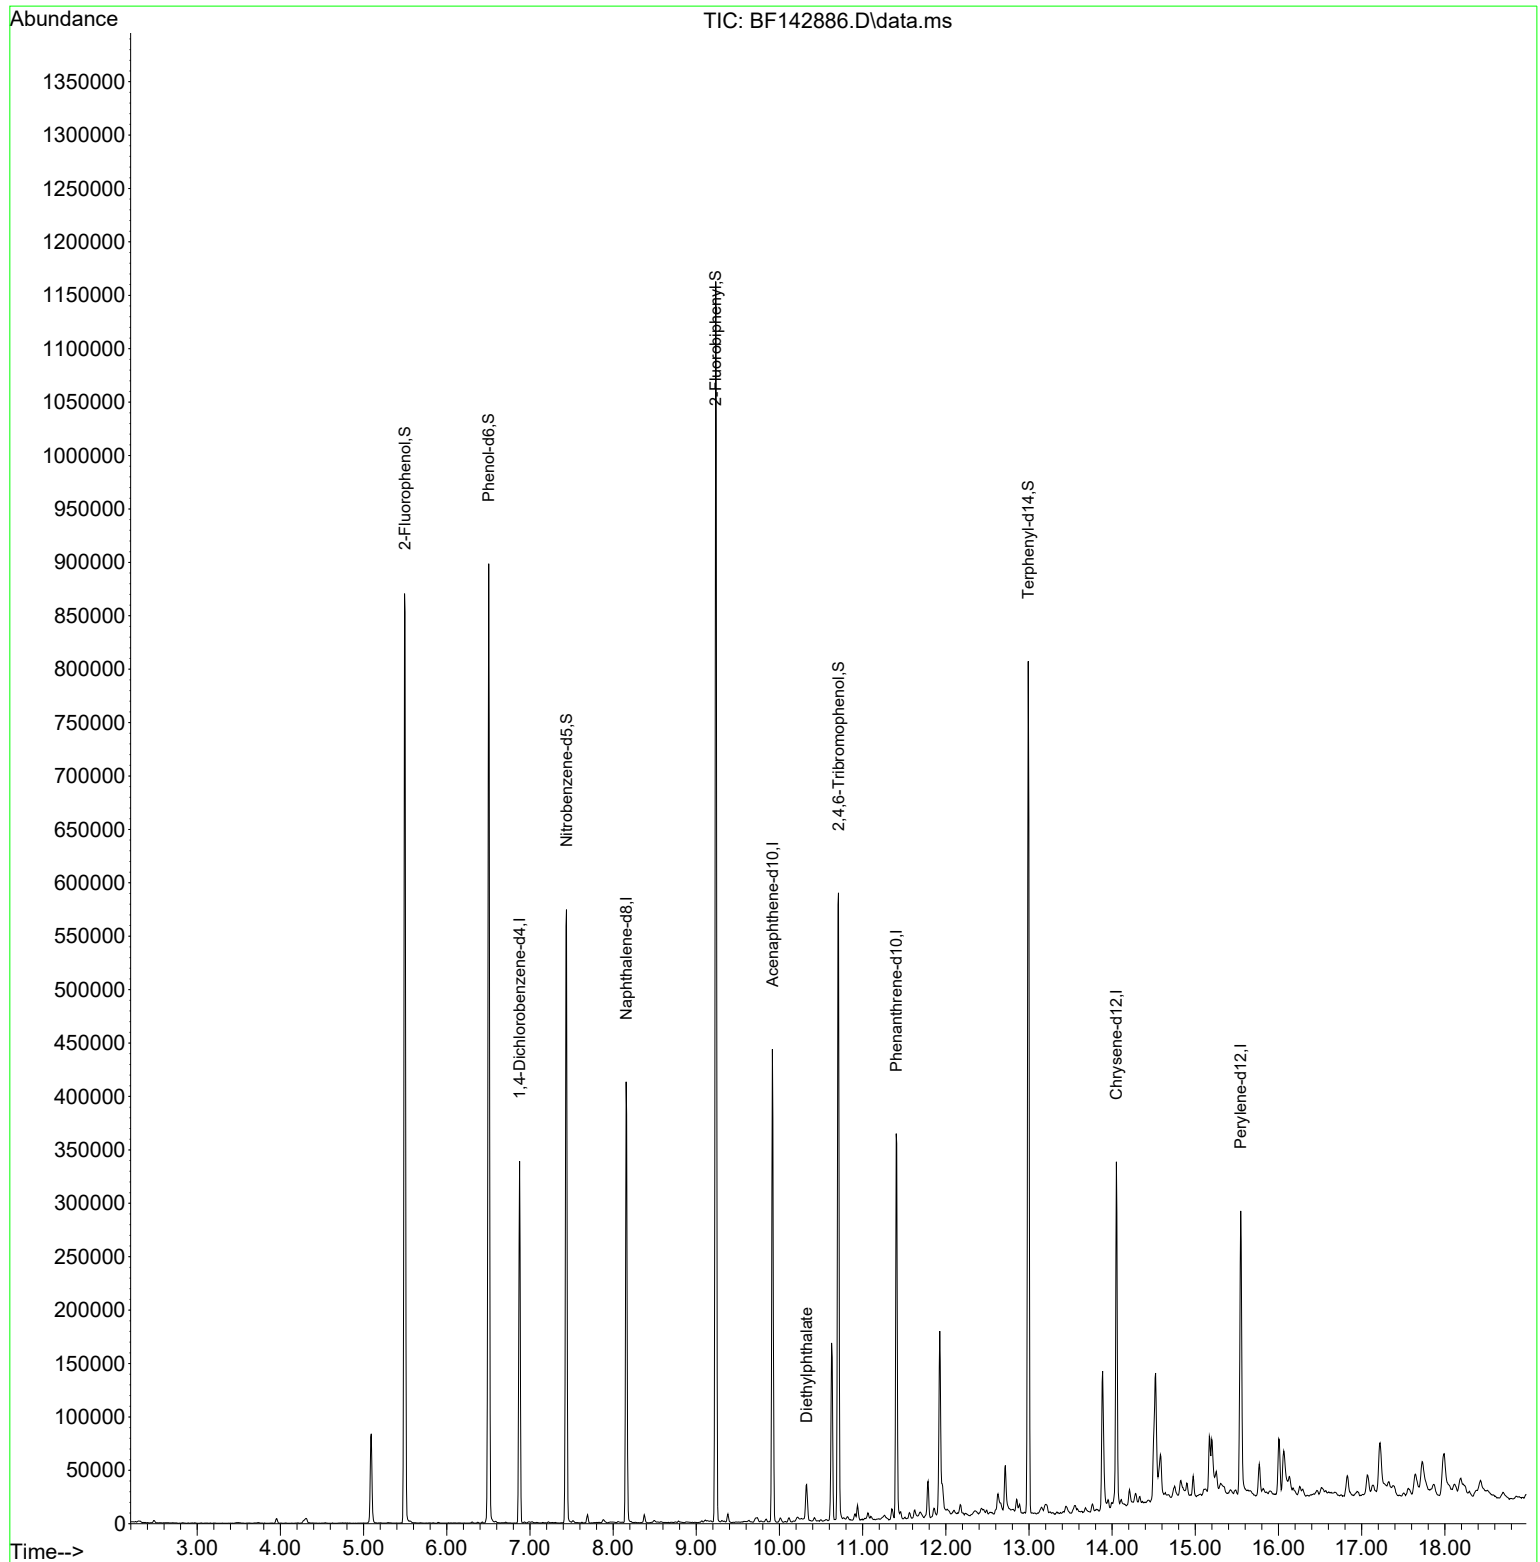




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.875 min Scan# 797
 Delta R.T. -0.006 min
 Lab File: BF142886.D
 Acq: 27 Jun 2025 11:52




Instrument :
 BNA_F
 ClientSampleId :
 TP-73


Tgt Ion:152 Resp: 71511
 Ion Ratio Lower Upper
 152 100
 150 158.4 127.2 190.8
 115 59.3 46.6 69.8

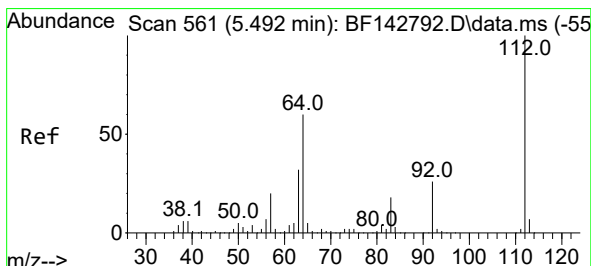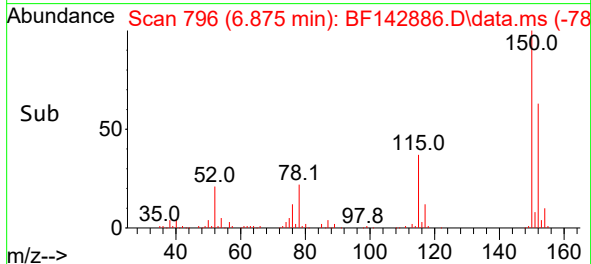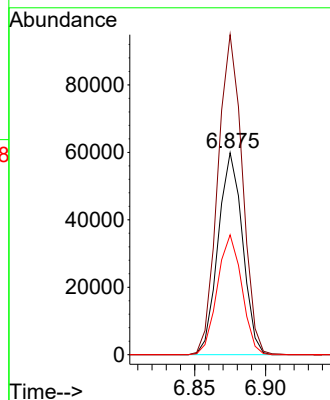

#5
 2-Fluorophenol
 Concen: 79.343 ng
 RT: 5.499 min Scan# 562
 Delta R.T. 0.007 min
 Lab File: BF142886.D
 Acq: 27 Jun 2025 11:52

Tgt Ion:112 Resp: 340790
 Ion Ratio Lower Upper
 112 100
 64 56.1 48.2 72.2
 63 29.8 25.7 38.5


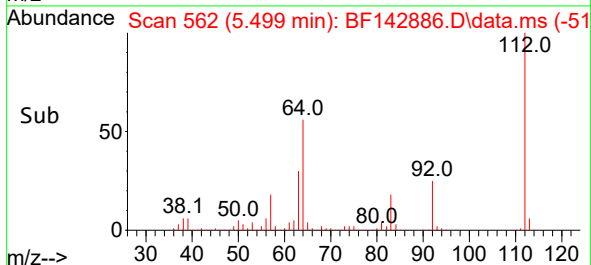
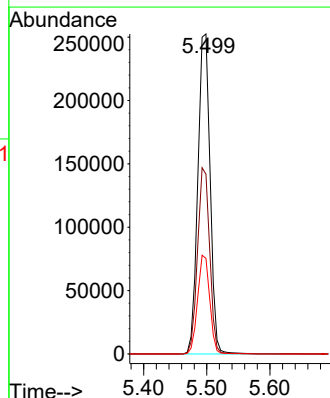
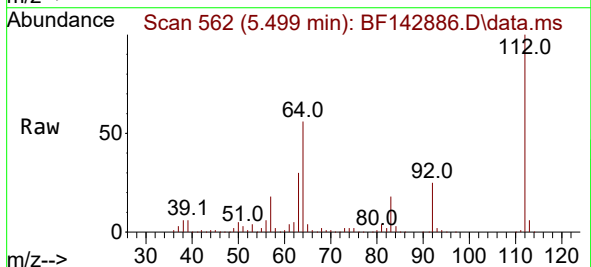


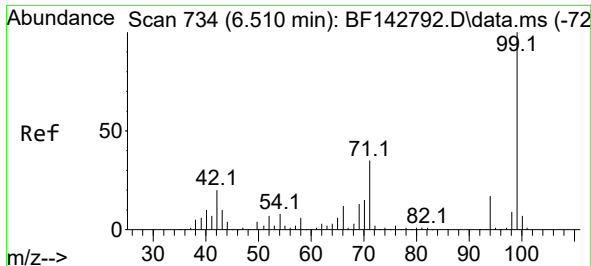

#7
Phenol-d6
Concen: 81.060 ng
RT: 6.504 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF142886.D
Acq: 27 Jun 2025 11:52




Instrument :
BNA_F
ClientSampleId :
TP-73


Tgt Ion: 99 Resp: 410766
Ion Ratio Lower Upper
99 100
42 19.6 15.9 23.9
71 35.0 27.8 41.8

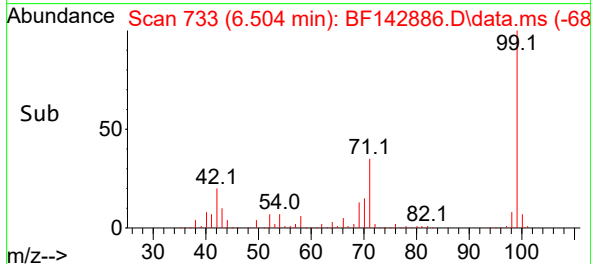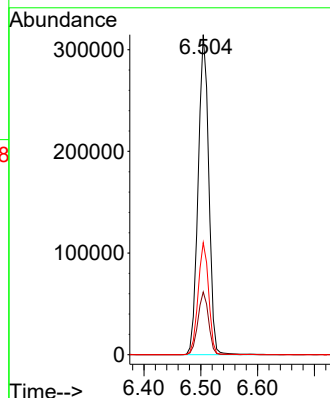

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.157 min Scan# 1014
Delta R.T. -0.012 min
Lab File: BF142886.D
Acq: 27 Jun 2025 11:52

Tgt Ion: 136 Resp: 269771
Ion Ratio Lower Upper
136 100
137 10.9 8.4 12.6
54 7.8 6.3 9.5
68 4.4 3.7 5.5

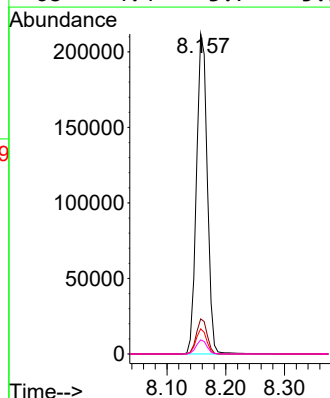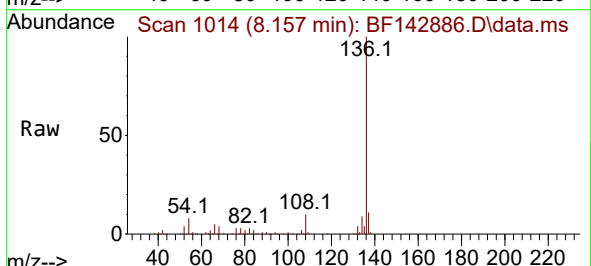

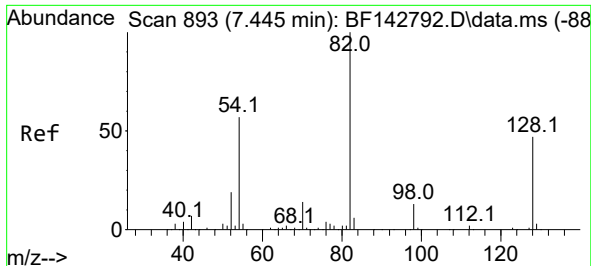

#23

Nitrobenzene-d5

Concen: 50.298 ng

RT: 7.440 min Scan# 89

Delta R.T. -0.005 min

Lab File: BF142886.D

Acq: 27 Jun 2025 11:52

Instrument :

BNA_F

ClientSampleId :

TP-73





Tgt Ion: 82 Resp: 247380

Ion Ratio Lower Upper

82 100

128 49.1 37.7 56.5

54 55.6 45.7 68.5

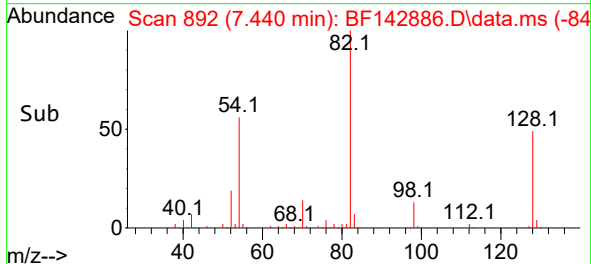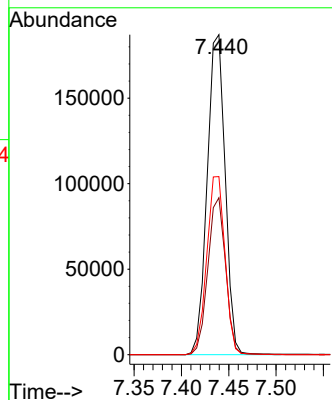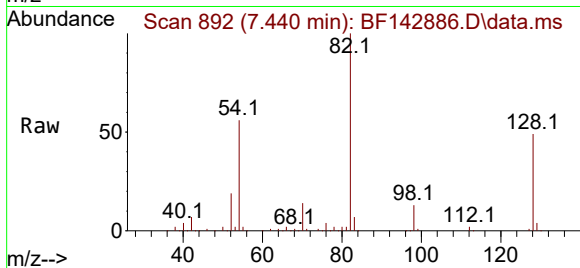

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.916 min Scan# 1313

Delta R.T. -0.006 min

Lab File: BF142886.D

Acq: 27 Jun 2025 11:52




Tgt Ion:164 Resp: 131916


Ion Ratio Lower Upper

164 100

162 99.2 81.8 122.8

160 44.2 36.0 54.0


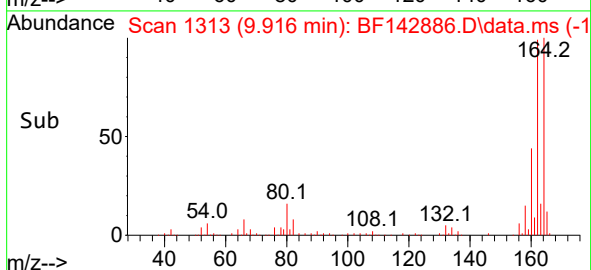
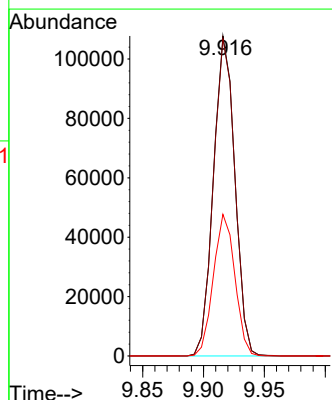
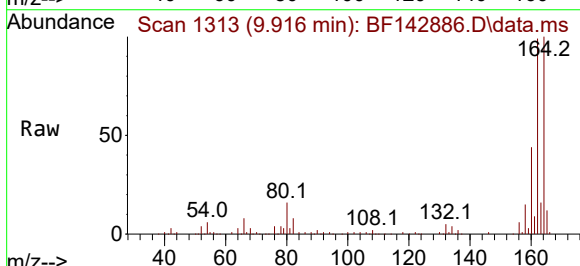


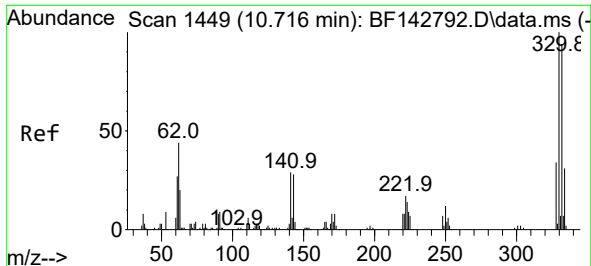

#42
2,4,6-Tribromophenol
Concen: 76.754 ng
RT: 10.710 min Scan# 1448
Delta R.T. -0.006 min
Lab File: BF142886.D
Acq: 27 Jun 2025 11:52




Instrument :
BNA_F
ClientSampleId :
TP-73


Tgt Ion:330 Resp: 104194
Ion Ratio Lower Upper
330 100
332 95.3 75.0 112.6
141 32.4 25.3 37.9

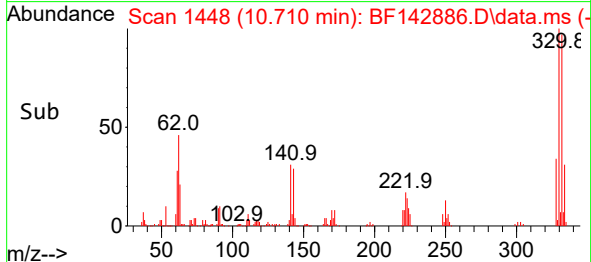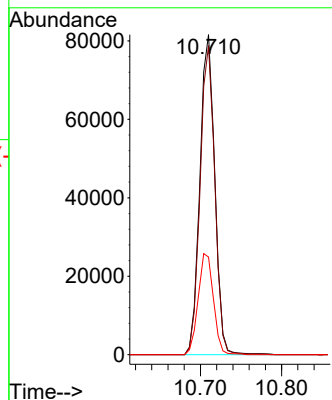

#45
2-Fluorobiphenyl
Concen: 51.835 ng
RT: 9.234 min Scan# 1197
Delta R.T. -0.011 min
Lab File: BF142886.D
Acq: 27 Jun 2025 11:52

Tgt Ion:172 Resp: 520514
Ion Ratio Lower Upper
172 100
171 34.7 28.2 42.4
170 22.6 18.5 27.7


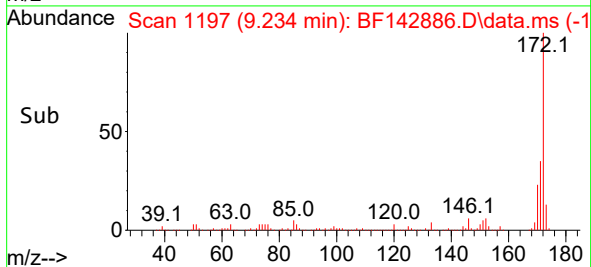
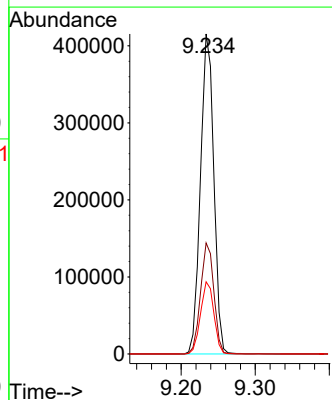
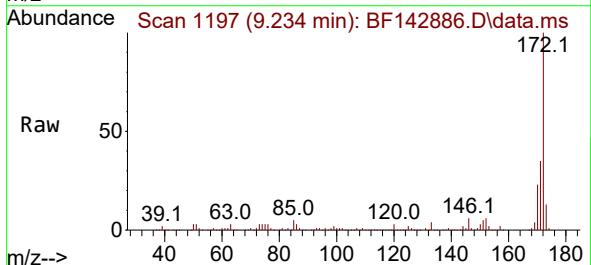


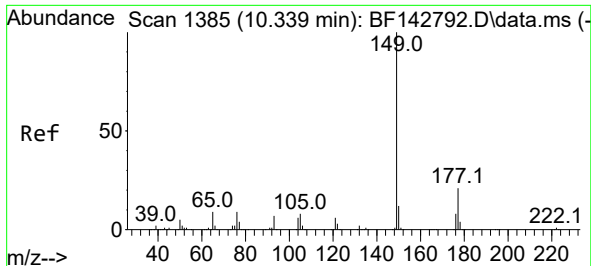

#60
Diethylphthalate
Concen: 2.915 ng
RT: 10.328 min Scan# 11
Delta R.T. -0.012 min
Lab File: BF142886.D
Acq: 27 Jun 2025 11:52




Instrument :
BNA_F
ClientSampleId :
TP-73


Tgt Ion:149 Resp: 24407
Ion Ratio Lower Upper
149 100
177 21.8 17.0 25.6
150 13.2 9.8 14.6

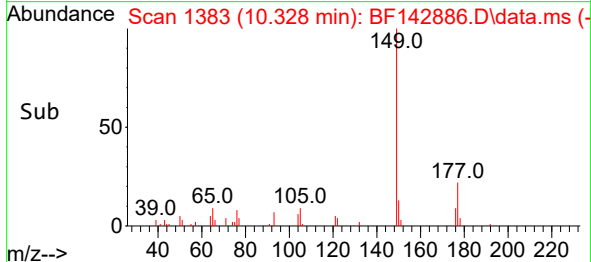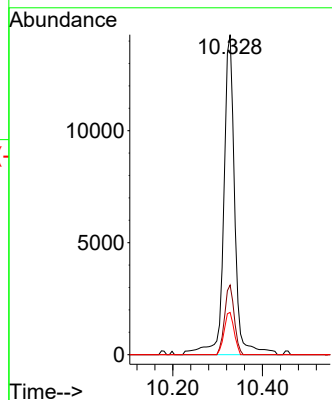

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.404 min Scan# 1566
Delta R.T. -0.006 min
Lab File: BF142886.D
Acq: 27 Jun 2025 11:52

Tgt Ion:188 Resp: 195199
Ion Ratio Lower Upper
188 100
94 8.4 6.7 10.1
80 8.7 6.9 10.3

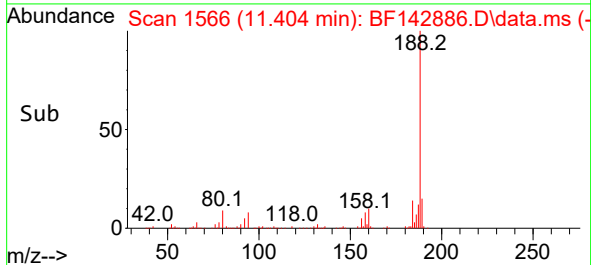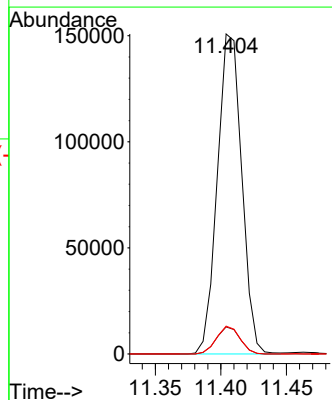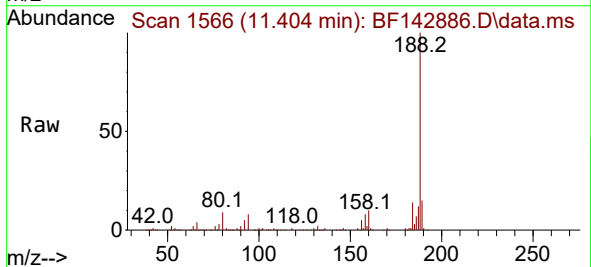



#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.051 min Scan# 20

Delta R.T. -0.006 min

Lab File: BF142886.D

Acq: 27 Jun 2025 11:52

Instrument :

BNA_F

ClientSampleId :

TP-73





Tgt Ion:240 Resp: 151359

Ion Ratio Lower Upper

240 100

120 10.2 8.2 12.2

236 25.5 19.8 29.8

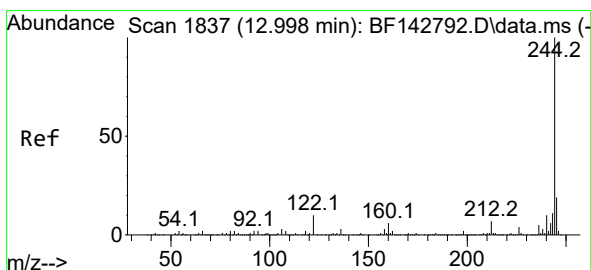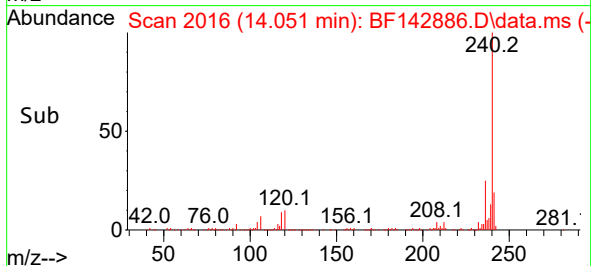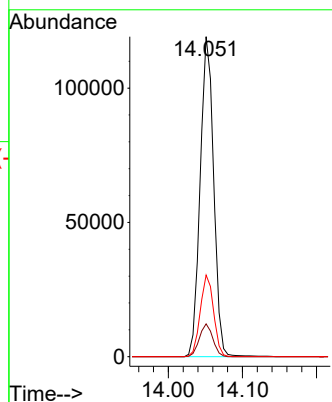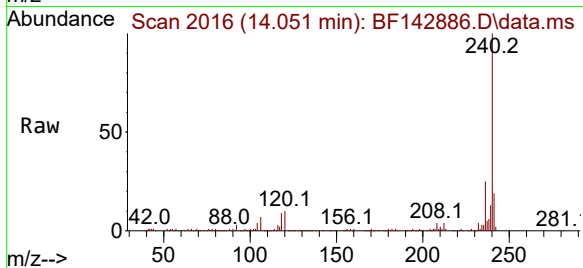

#79

Terphenyl-d14

Concen: 34.452 ng

RT: 12.992 min Scan# 1836

Delta R.T. -0.006 min

Lab File: BF142886.D

Acq: 27 Jun 2025 11:52




Tgt Ion:244 Resp: 377407


Ion Ratio Lower Upper

244 100

212 6.5 5.4 8.0


122 10.0 8.2 12.2

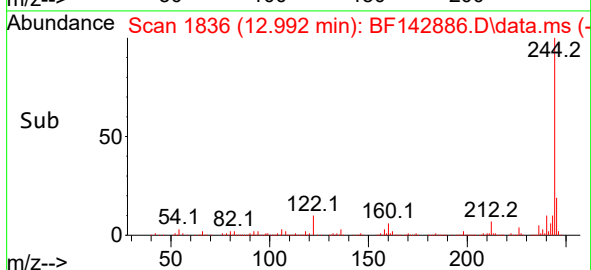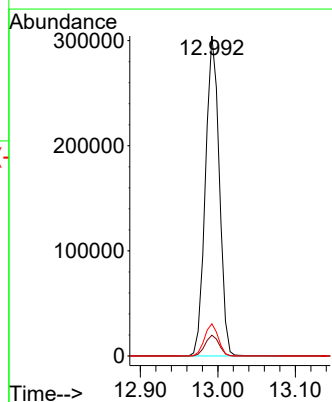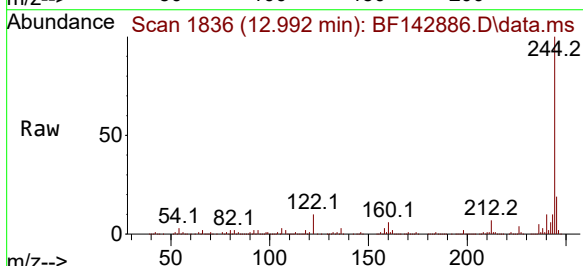



#86
Perylene-d12
Concen: 20.000 ng
RT: 15.545 min Scan# 21
Delta R.T. 0.000 min
Lab File: BF142886.D
Acq: 27 Jun 2025 11:52

Instrument :
BNA_F
ClientSampleId :
TP-73

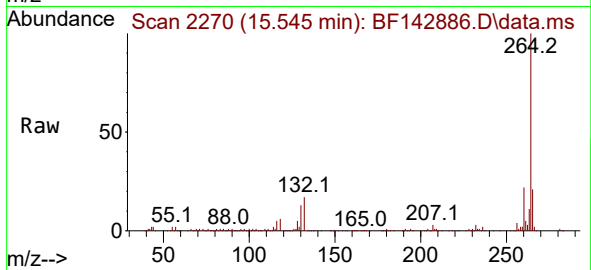

Tgt Ion:264 Resp: 151859

Ion	Ratio	Lower	Upper
264	100		
260	22.3	18.1	27.1
265	21.2	16.6	25.0

