

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062725\
 Data File : BF142889.D
 Acq On : 27 Jun 2025 13:19
 Operator : RC/JU
 Sample : Q2413-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-35

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 06/30/2025
 Supervised By :Jagrut Upadhyay 06/30/2025

Quant Time: Jun 27 13:49:37 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 24 05:28:21 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	69777	20.000	ng	0.00
21) Naphthalene-d8	8.157	136	263920	20.000	ng	-0.01
39) Acenaphthene-d10	9.916	164	134370	20.000	ng	0.00
64) Phenanthrene-d10	11.404	188	199779	20.000	ng	0.00
76) Chrysene-d12	14.051	240	149012	20.000	ng	0.00
86) Perylene-d12	15.545	264	152863	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.492	112	340387	81.219	ng	0.00
7) Phenol-d6	6.504	99	409015	82.720	ng	0.00
23) Nitrobenzene-d5	7.439	82	251521	52.274	ng	0.00
42) 2,4,6-Tribromophenol	10.710	330	105823	76.530	ng	0.00
45) 2-Fluorobiphenyl	9.233	172	528561	51.675	ng	-0.01
79) Terphenyl-d14	12.992	244	417524	38.715	ng	0.00
Target Compounds						Qvalue
71) Phenanthrene	11.427	178	46316	4.280	ng	99
75) Fluoranthene	12.621	202	121010	11.782	ng	99
78) Pyrene	12.851	202	94631	6.775	ng	99
81) Benzo(a)anthracene	14.045	228	68261m	6.790	ng	
83) Chrysene	14.080	228	51723	5.766	ng	98
87) Indeno(1,2,3-cd)pyrene	17.051	276	25850	2.220	ng	96
88) Benzo(b)fluoranthene	15.109	252	75991m	8.591	ng	
89) Benzo(k)fluoranthene	15.121	252	29658m	3.584	ng	
90) Benzo(a)pyrene	15.480	252	49698	5.816	ng	99
92) Benzo(g,h,i)perylene	17.503	276	21403	2.269	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062725\
Data File : BF142889.D
Acq On : 27 Jun 2025 13:19
Operator : RC/JU
Sample : Q2413-01
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
TP-35

Quant Time: Jun 27 13:49:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 06/30/2025
Supervised By :Jagrut Upadhyay 06/30/2025

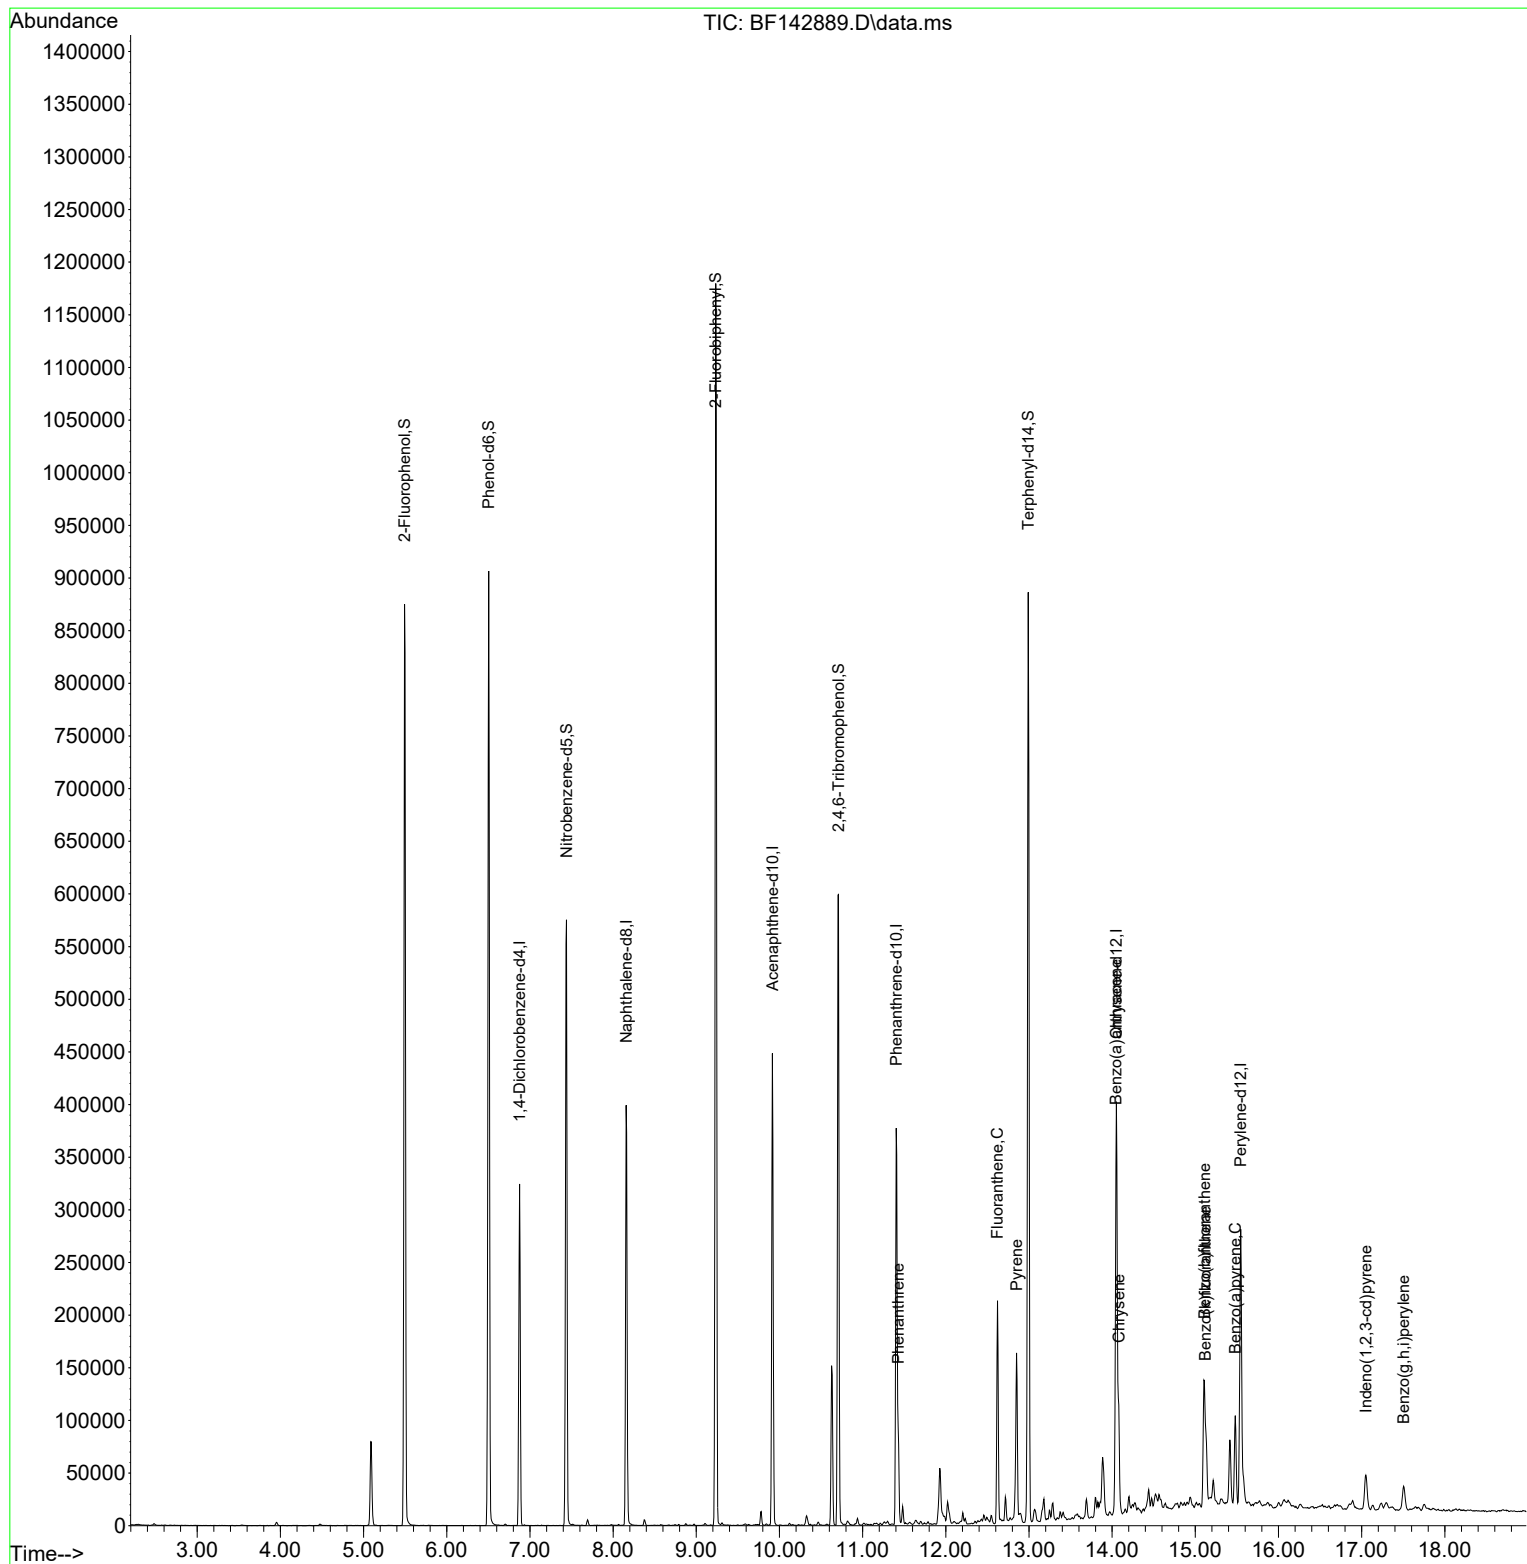



#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.875 min Scan# 797
Delta R.T. -0.006 min
Lab File: BF142889.D
Acq: 27 Jun 2025 13:19




Instrument :
BNA_F
ClientSampleId :
TP-35



Tgt Ion:152 Resp: 6977
Ion Ratio Lower Upper
152 100
150 157.8 127.2 190.8
115 59.0 46.6 69.8




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 06/30/2025
Supervised By :Jagrut Upadhyay 06/30/2025

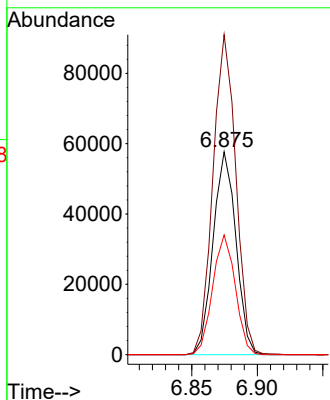

#5
2-Fluorophenol
Concen: 81.219 ng
RT: 5.492 min Scan# 561
Delta R.T. 0.000 min
Lab File: BF142889.D
Acq: 27 Jun 2025 13:19


Tgt Ion:112 Resp: 340387
Ion Ratio Lower Upper
112 100
64 58.2 48.2 72.2
63 31.4 25.7 38.5

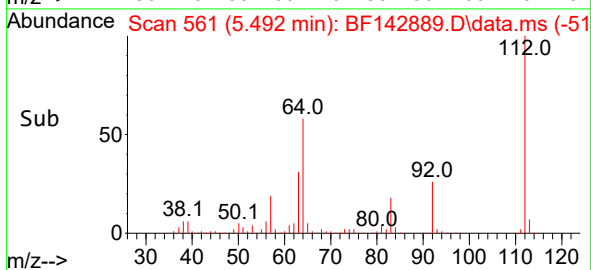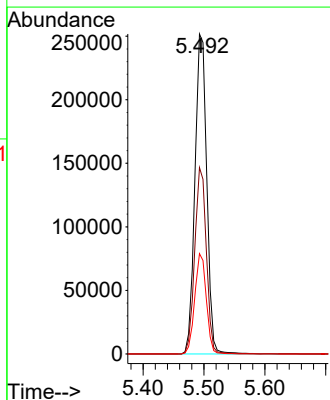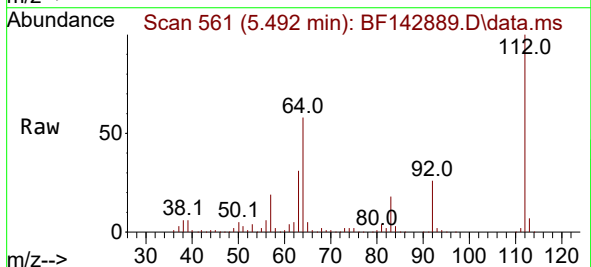



#7
Phenol-d6
Concen: 82.720 ng
RT: 6.504 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF142889.D
Acq: 27 Jun 2025 13:19




Instrument :
BNA_F
ClientSampleId :
TP-35




Tgt Ion: 99 Resp: 409015
Ion Ratio Lower Upper
99 100
42 19.7 15.9 23.9
71 35.2 27.8 41.8

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 06/30/2025
Supervised By :Jagrut Upadhyay 06/30/2025

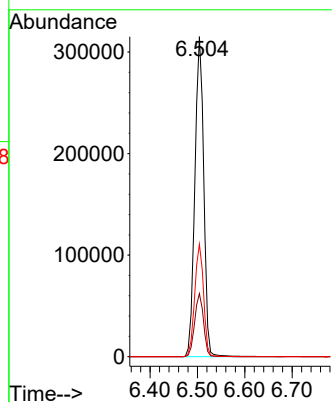


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.157 min Scan# 1014
Delta R.T. -0.012 min
Lab File: BF142889.D
Acq: 27 Jun 2025 13:19



Tgt Ion:136 Resp: 263920
Ion Ratio Lower Upper
136 100
137 11.2 8.4 12.6
54 7.9 6.3 9.5
68 4.4 3.7 5.5

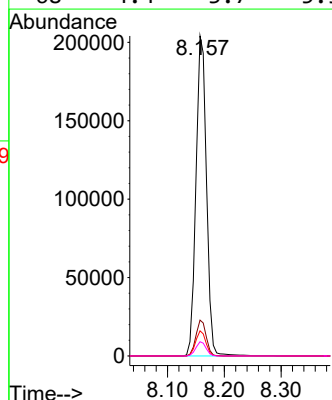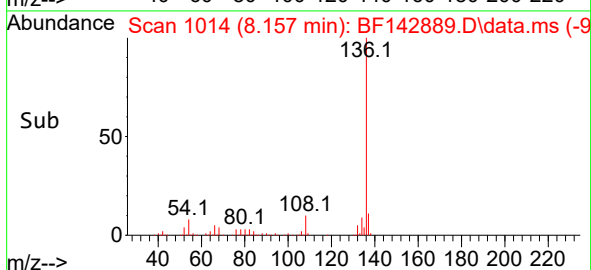



#23

Nitrobenzene-d5

Concen: 52.274 ng

RT: 7.439 min Scan# 89

Delta R.T. -0.006 min

Lab File: BF142889.D

Acq: 27 Jun 2025 13:19

Instrument :

BNA_F

ClientSampleId :

TP-35

Tgt Ion: 82 Resp: 25152





Ion	Ratio	Lower	Upper
82	100		
128	48.5	37.7	56.5
54	54.8	45.7	68.5

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 06/30/2025

Supervised By :Jagrut Upadhyay 06/30/2025

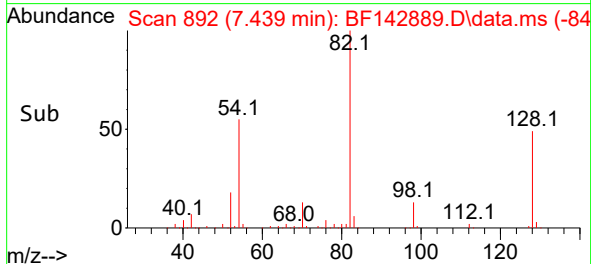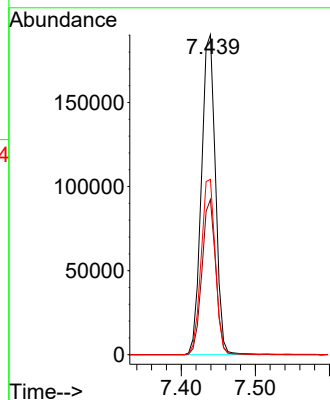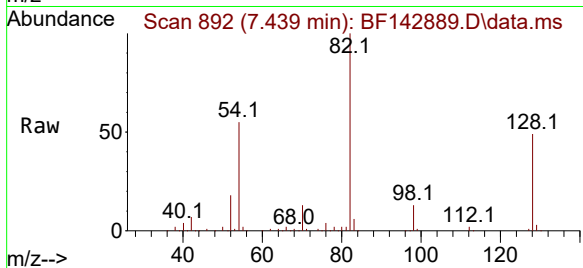

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.916 min Scan# 1313




Delta R.T. -0.006 min


Lab File: BF142889.D

Acq: 27 Jun 2025 13:19

Tgt Ion:164 Resp: 134370


Ion	Ratio	Lower	Upper
164	100		
162	100.1	81.8	122.8
160	43.9	36.0	54.0

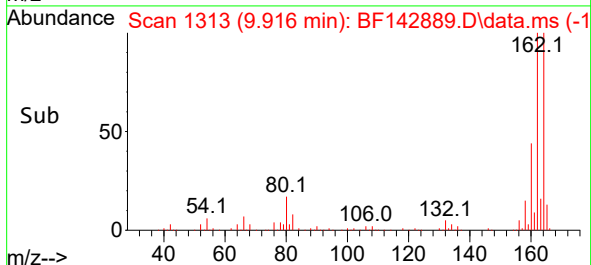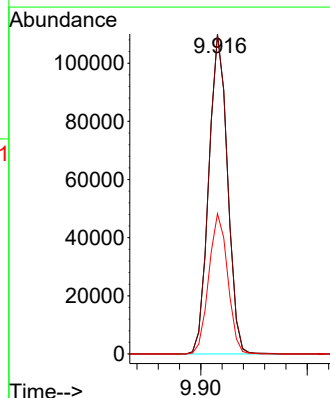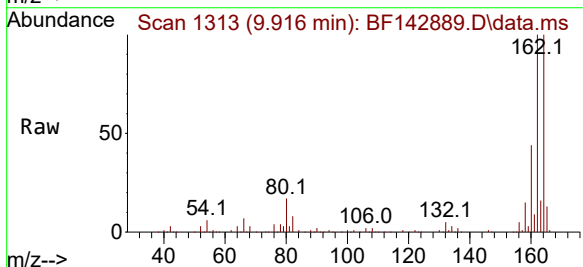



#42
2,4,6-Tribromophenol
Concen: 76.530 ng
RT: 10.710 min Scan# 1449
Delta R.T. -0.006 min
Lab File: BF142889.D
Acq: 27 Jun 2025 13:19




Instrument :
BNA_F
ClientSampleId :
TP-35

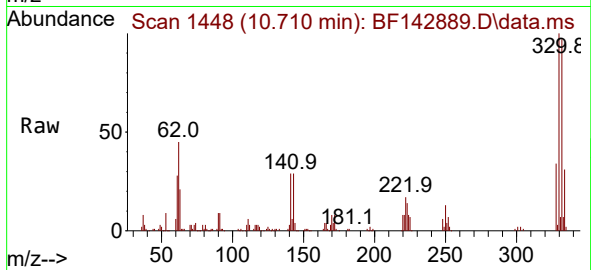


Tgt Ion: 330 Resp: 105823
Ion Ratio Lower Upper
330 100
332 97.0 75.0 112.6
141 31.8 25.3 37.9

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 06/30/2025
Supervised By :Jagrut Upadhyay 06/30/2025

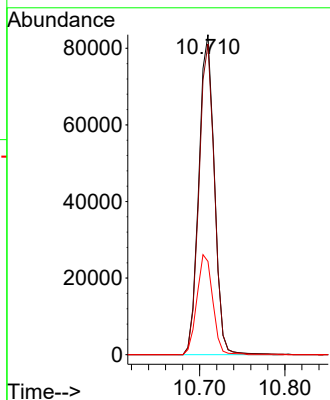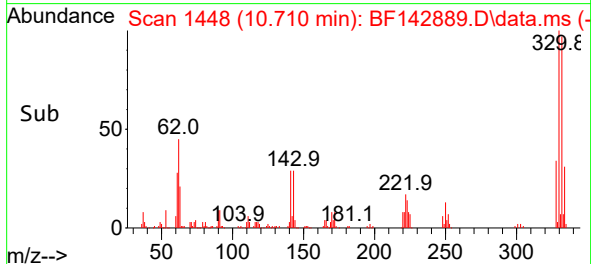


#45
2-Fluorobiphenyl
Concen: 51.675 ng
RT: 9.233 min Scan# 1197
Delta R.T. -0.012 min
Lab File: BF142889.D
Acq: 27 Jun 2025 13:19

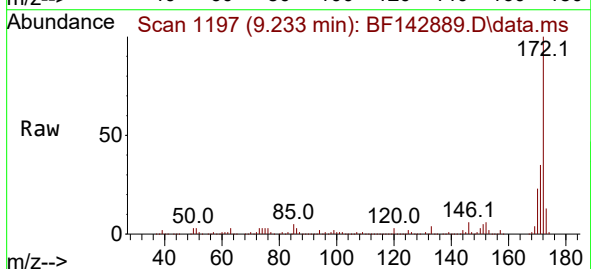


Tgt Ion: 172 Resp: 528561
Ion Ratio Lower Upper
172 100
171 35.0 28.2 42.4
170 22.7 18.5 27.7

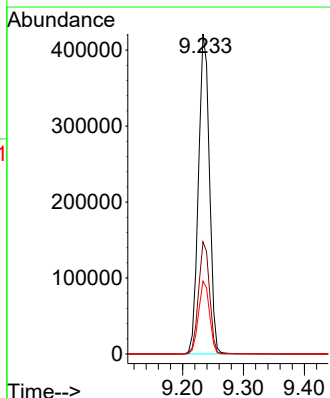

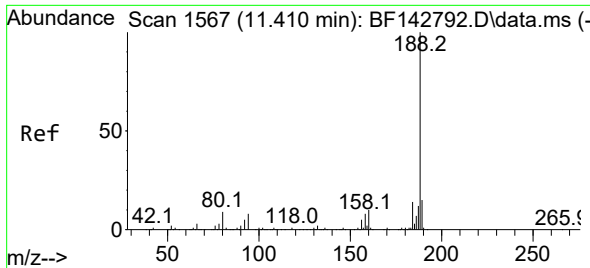

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.404 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF142889.D
Acq: 27 Jun 2025 13:19




Instrument :
BNA_F
ClientSampleId :
TP-35

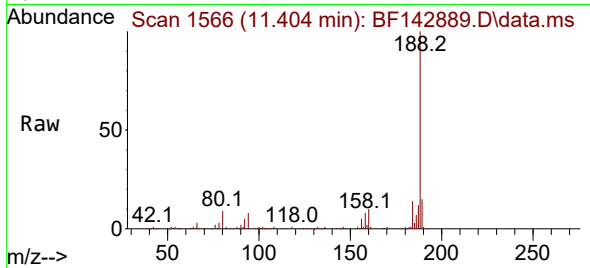

Tgt Ion:188 Resp: 199779
Ion Ratio Lower Upper
188 100
94 8.0 6.7 10.1
80 8.7 6.9 10.3




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 06/30/2025
Supervised By :Jagrut Upadhyay 06/30/2025

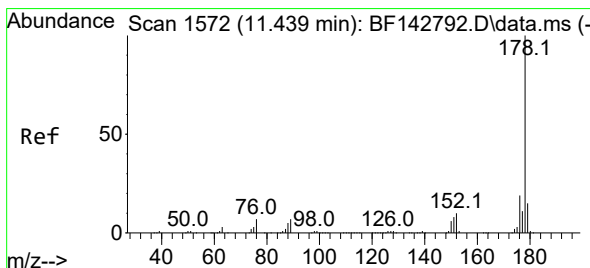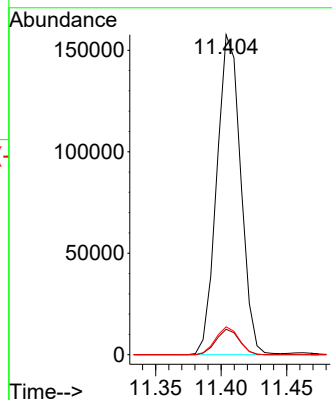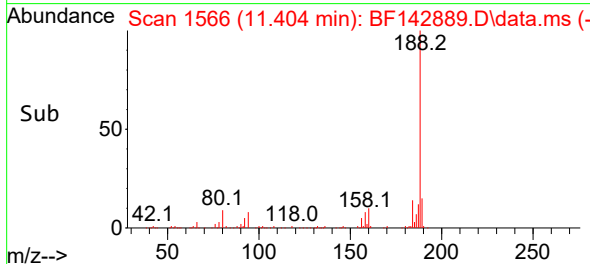

#71
Phenanthrene
Concen: 4.280 ng
RT: 11.427 min Scan# 1570
Delta R.T. -0.012 min
Lab File: BF142889.D
Acq: 27 Jun 2025 13:19

Tgt Ion:178 Resp: 46316
Ion Ratio Lower Upper
178 100
176 18.9 15.1 22.7
179 15.6 12.0 18.0

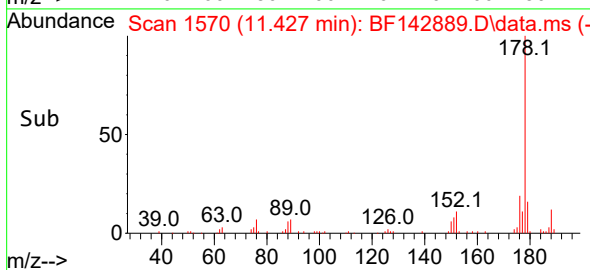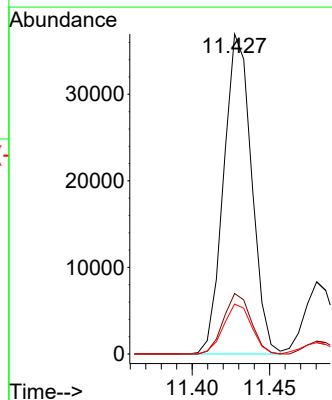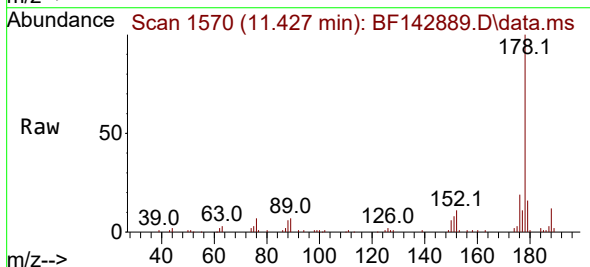

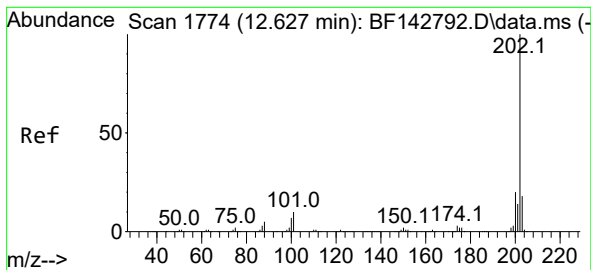

#75

Fluoranthene

Concen: 11.782 ng

RT: 12.621 min Scan# 11

Delta R.T. -0.006 min

Lab File: BF142889.D

Acq: 27 Jun 2025 13:19

Instrument :

BNA_F

ClientSampleId :

TP-35

Tgt Ion:202 Resp: 121010

Ion Ratio Lower Upper

202 100

101 9.5 0.0 29.7





203 16.7 0.0 37.5

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 06/30/2025

Supervised By :Jagrut Upadhyay 06/30/2025

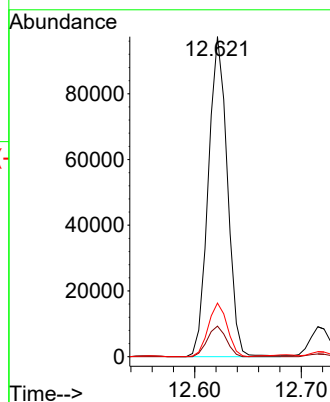

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.051 min Scan# 2016

Delta R.T. -0.006 min

Lab File: BF142889.D

Acq: 27 Jun 2025 13:19




Tgt Ion:240 Resp: 149012


Ion Ratio Lower Upper

240 100

120 10.4 8.2 12.2

236 24.7 19.8 29.8

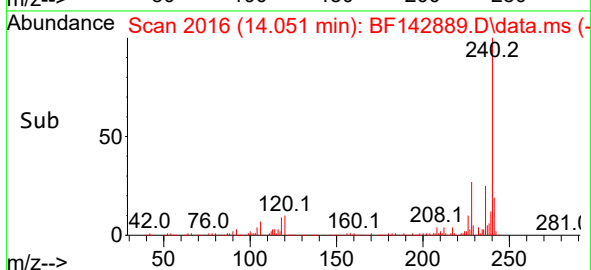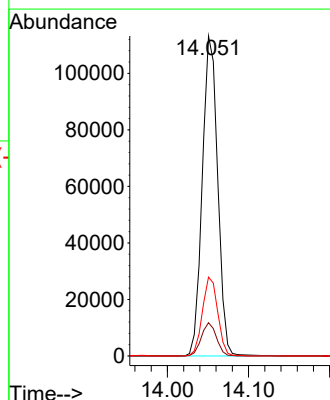



#78

Pyrene

Concen: 6.775 ng

RT: 12.851 min Scan# 1812

Delta R.T. -0.006 min

Lab File: BF142889.D

Acq: 27 Jun 2025 13:19

Instrument :

BNA_F

ClientSampleId :

TP-35

Tgt Ion:202 Resp: 9463

Ion Ratio Lower Upper

202 100

200 18.9 15.7 23.5





203 17.5 13.8 20.6

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 06/30/2025

Supervised By :Jagrut Upadhyay 06/30/2025

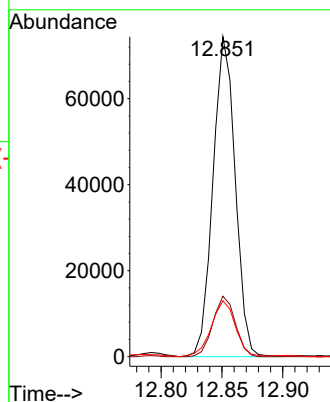

#79

Terphenyl-d14

Concen: 38.715 ng

RT: 12.992 min Scan# 1836

Delta R.T. -0.006 min

Lab File: BF142889.D

Acq: 27 Jun 2025 13:19




Tgt Ion:244 Resp: 417524


Ion Ratio Lower Upper

244 100

212 6.8 5.4 8.0


122 10.3 8.2 12.2

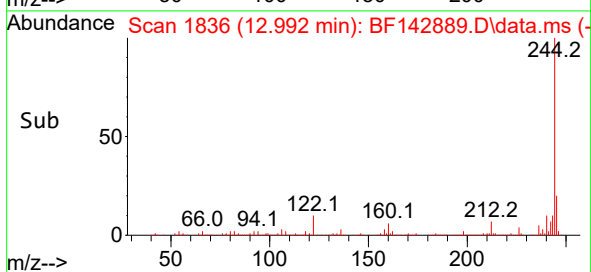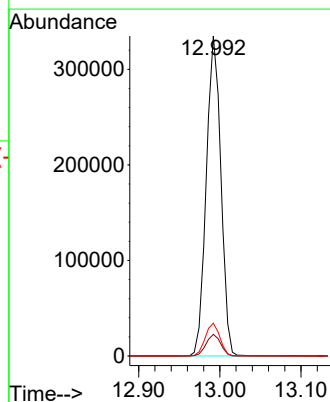

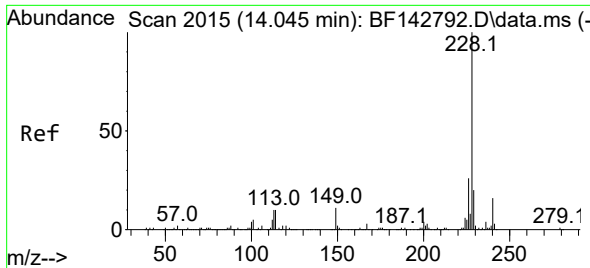

#81
Benzo(a)anthracene
Concen: 6.790 ng m
RT: 14.045 min Scan# 2015
Delta R.T. -0.000 min
Lab File: BF142889.D
Acq: 27 Jun 2025 13:19




Instrument :
BNA_F
ClientSampleId :
TP-35

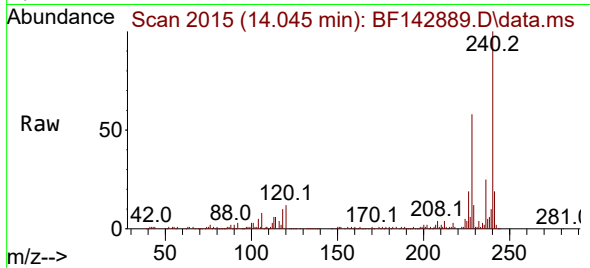

Tgt Ion:228 Resp: 6826
Ion Ratio Lower Upper
228 100
226 33.7 21.2 31.8
229 20.2 15.6 23.4




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 06/30/2025
Supervised By :Jagrut Upadhyay 06/30/2025

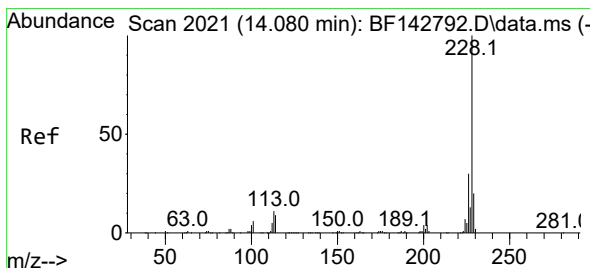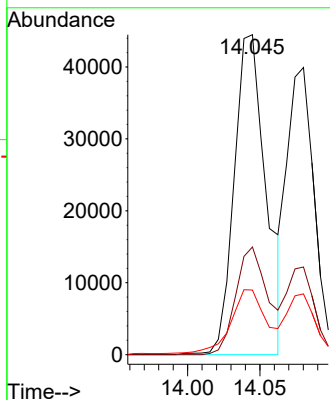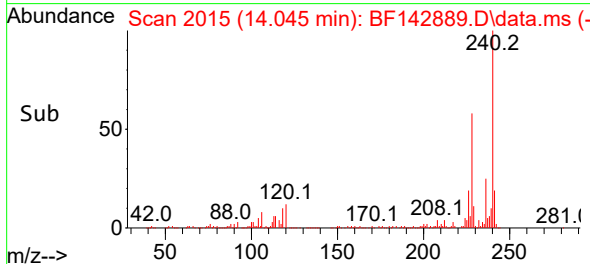

#83
Chrysene
Concen: 5.766 ng
RT: 14.080 min Scan# 2021
Delta R.T. -0.000 min
Lab File: BF142889.D
Acq: 27 Jun 2025 13:19


Tgt Ion:228 Resp: 51723
Ion Ratio Lower Upper
228 100
226 30.5 23.7 35.5
229 21.2 15.7 23.5

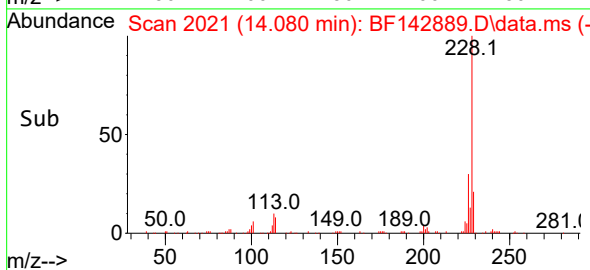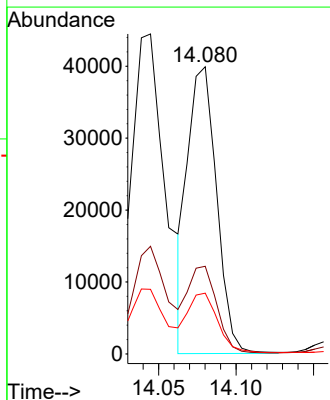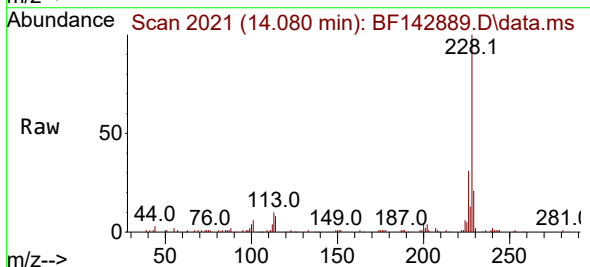



#86
Perylene-d12
Concen: 20.000 ng
RT: 15.545 min Scan# 21
Delta R.T. -0.000 min
Lab File: BF142889.D
Acq: 27 Jun 2025 13:19




Instrument :
BNA_F
ClientSampleId :
TP-35




Tgt Ion:264 Resp: 15286
Ion Ratio Lower Upper
264 100
260 22.3 18.1 27.1
265 21.5 16.6 25.0

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 06/30/2025
Supervised By :Jagrut Upadhyay 06/30/2025

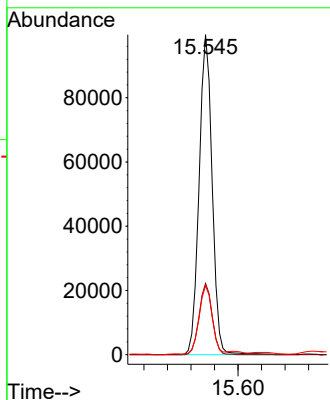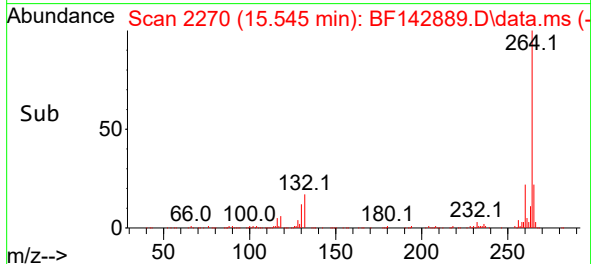


#87
Indeno(1,2,3-cd)pyrene
Concen: 2.220 ng
RT: 17.051 min Scan# 2526
Delta R.T. -0.012 min
Lab File: BF142889.D
Acq: 27 Jun 2025 13:19

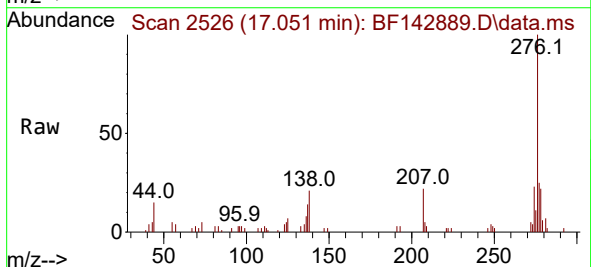


Tgt Ion:276 Resp: 25850
Ion Ratio Lower Upper
276 100
138 22.0 20.2 30.4
277 25.3 19.8 29.6

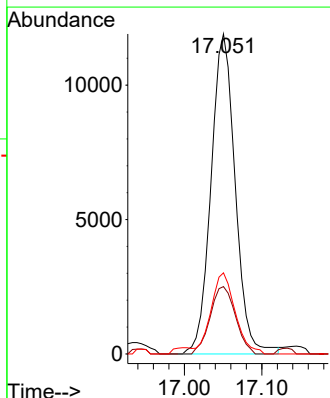



#88
Benzo(b)fluoranthene
Concen: 8.591 ng m
RT: 15.109 min Scan# 2196
Delta R.T. -0.000 min
Lab File: BF142889.D
Acq: 27 Jun 2025 13:19




Instrument :
BNA_F
ClientSampleId :
TP-35




Tgt Ion:252 Resp: 7599
Ion Ratio Lower Upper
252 100
253 22.5 17.5 26.3
125 10.8 7.4 11.0

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 06/30/2025
Supervised By :Jagrut Upadhyay 06/30/2025

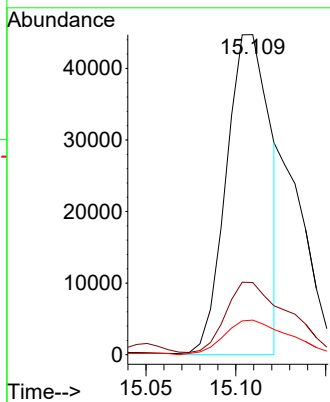


#89
Benzo(k)fluoranthene
Concen: 3.584 ng m
RT: 15.121 min Scan# 2198
Delta R.T. -0.018 min
Lab File: BF142889.D
Acq: 27 Jun 2025 13:19

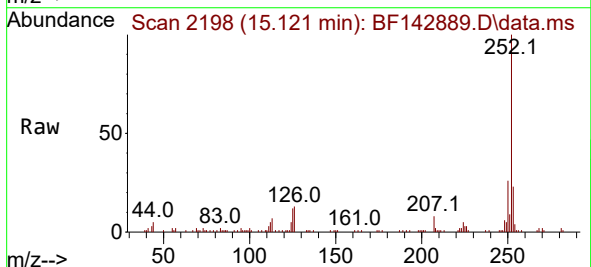

Tgt Ion:252 Resp: 29658
Ion Ratio Lower Upper
252 100
253 23.0 17.2 25.8
125 11.9 7.4 11.2#

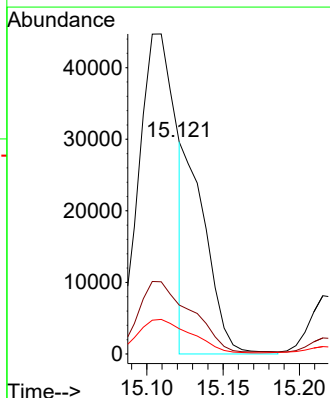



#90
Benzo(a)pyrene
Concen: 5.816 ng
RT: 15.480 min Scan# 21
Delta R.T. -0.006 min
Lab File: BF142889.D
Acq: 27 Jun 2025 13:19

Instrument :

BNA_F

ClientSampleId :





TP-35

Tgt Ion:252 Resp: 49698
Ion Ratio Lower Upper
252 100
253 22.9 17.5 26.3
125 10.6 8.6 12.8

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 06/30/2025
Supervised By :Jagrut Upadhyay 06/30/2025

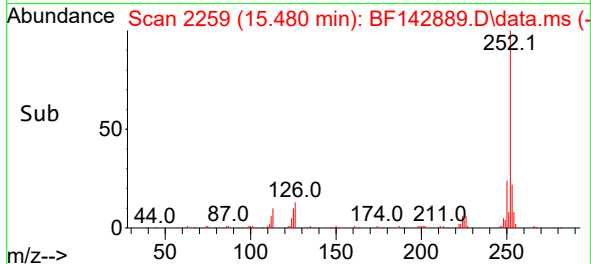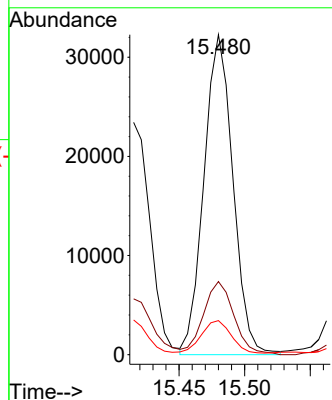

#92
Benzo(g,h,i)perylene
Concen: 2.269 ng
RT: 17.503 min Scan# 2603
Delta R.T. -0.012 min
Lab File: BF142889.D
Acq: 27 Jun 2025 13:19

Tgt Ion:276 Resp: 21403
Ion Ratio Lower Upper
276 100
277 23.0 18.8 28.2
138 21.7 17.6 26.4

