

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062725\
 Data File : BF142884.D
 Acq On : 27 Jun 2025 10:49
 Operator : RC/JU
 Sample : PB168625BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB168625BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142884.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	490	496	514	rBV	118912	206123	7.68%	1.327%
2	5.504	557	563	569	rBV	1478776	2022550	75.35%	13.023%
3	6.504	727	733	739	rBV	1385764	1981056	73.80%	12.756%
4	6.875	791	796	801	rBV	354750	429736	16.01%	2.767%
5	7.440	885	892	897	rBV	925259	1324980	49.36%	8.532%
6	8.157	1008	1014	1033	rBV	440837	567380	21.14%	3.653%
7	9.234	1190	1197	1202	rBV	1993353	2684291	100.00%	17.284%
8	9.916	1307	1313	1324	rBV	524426	655033	24.40%	4.218%
9	10.710	1442	1448	1468	rBV	1230008	1635610	60.93%	10.532%
10	11.404	1561	1566	1574	rBV	538238	671844	25.03%	4.326%
11	12.992	1830	1836	1842	rBV	1839949	2515390	93.71%	16.197%
12	14.051	2011	2016	2024	rBV	336078	428928	15.98%	2.762%
13	15.539	2263	2269	2279	rBV	249111	407184	15.17%	2.622%




Sum of corrected areas: 15530105

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062725\
Data File : BF142884.D
Acq On : 27 Jun 2025 10:49
Operator : RC/JU
Sample : PB168625BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168625BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

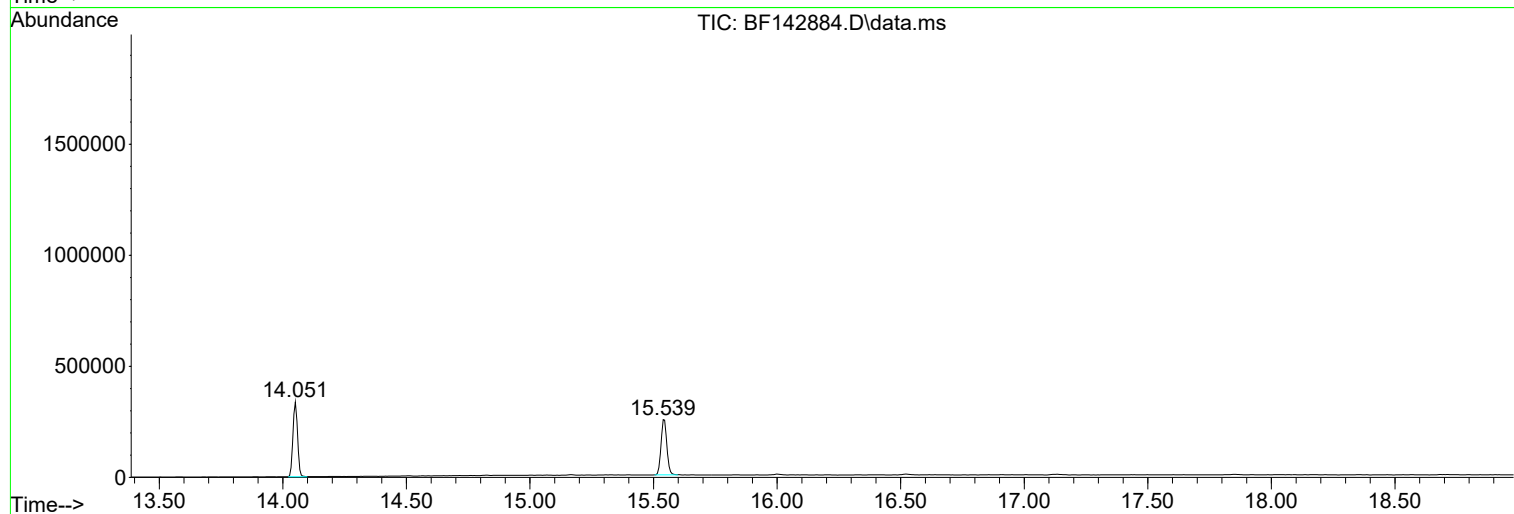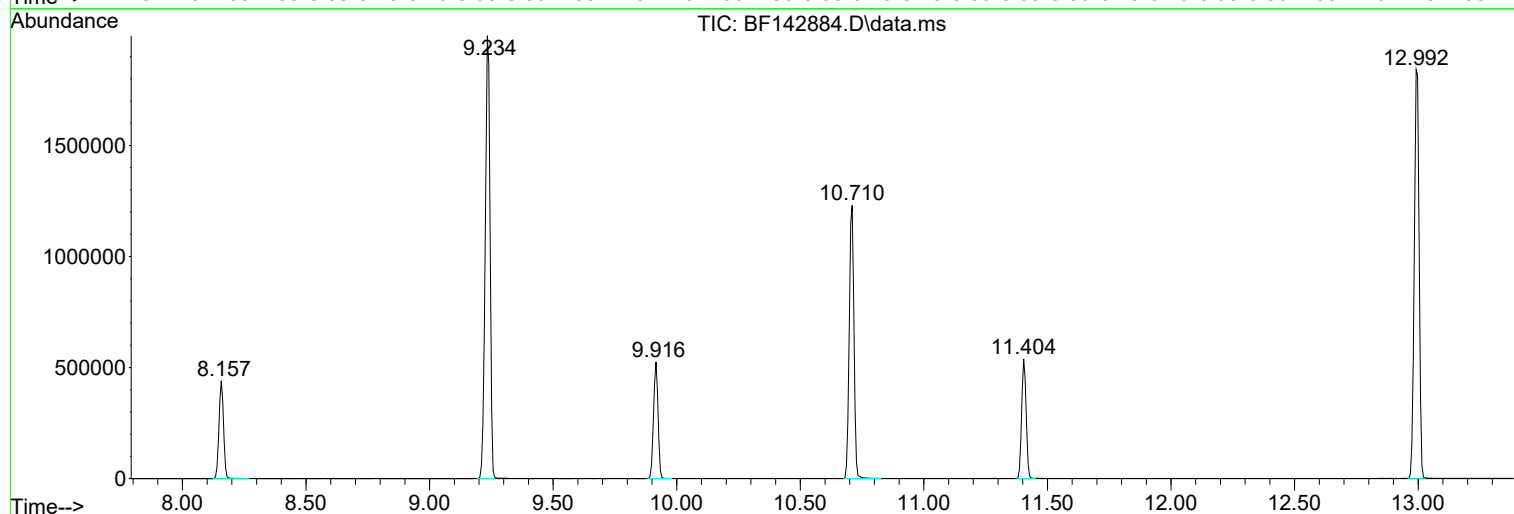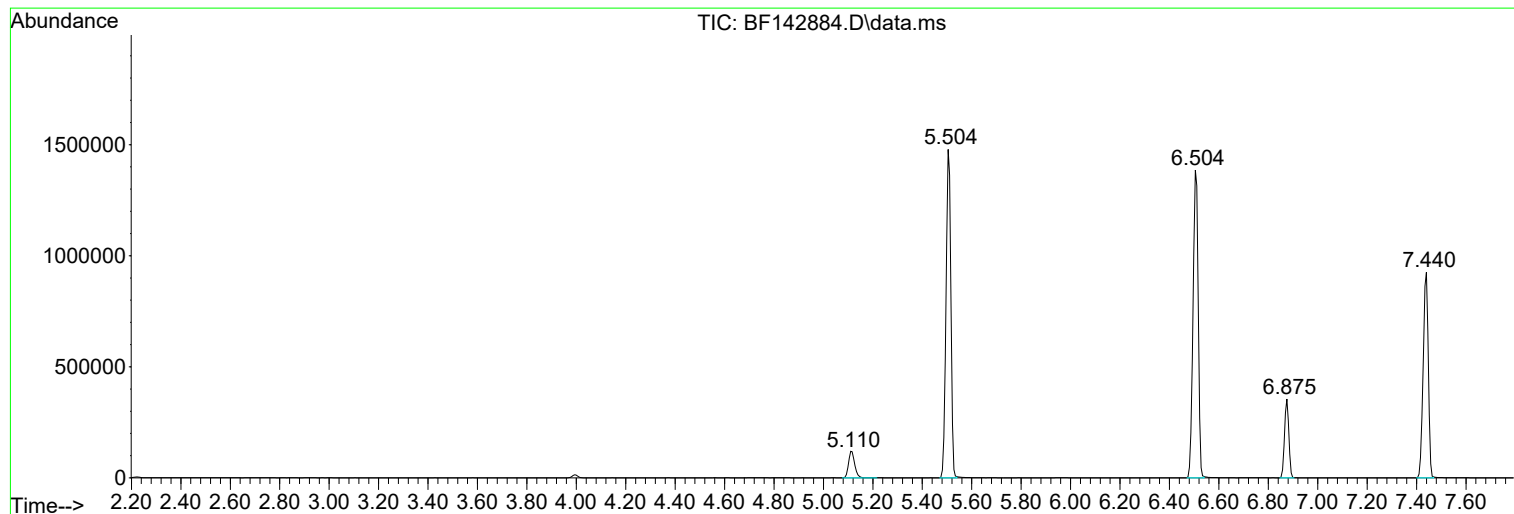

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062725\
Data File : BF142884.D
Acq On : 27 Jun 2025 10:49
Operator : RC/JU
Sample : PB168625BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168625BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062725\
Data File : BF142884.D
Acq On : 27 Jun 2025 10:49
Operator : RC/JU
Sample : PB168625BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168625BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------