


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062725\
Data File : BF142881.D
Acq On : 27 Jun 2025 09:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 24 05:28:21 2025

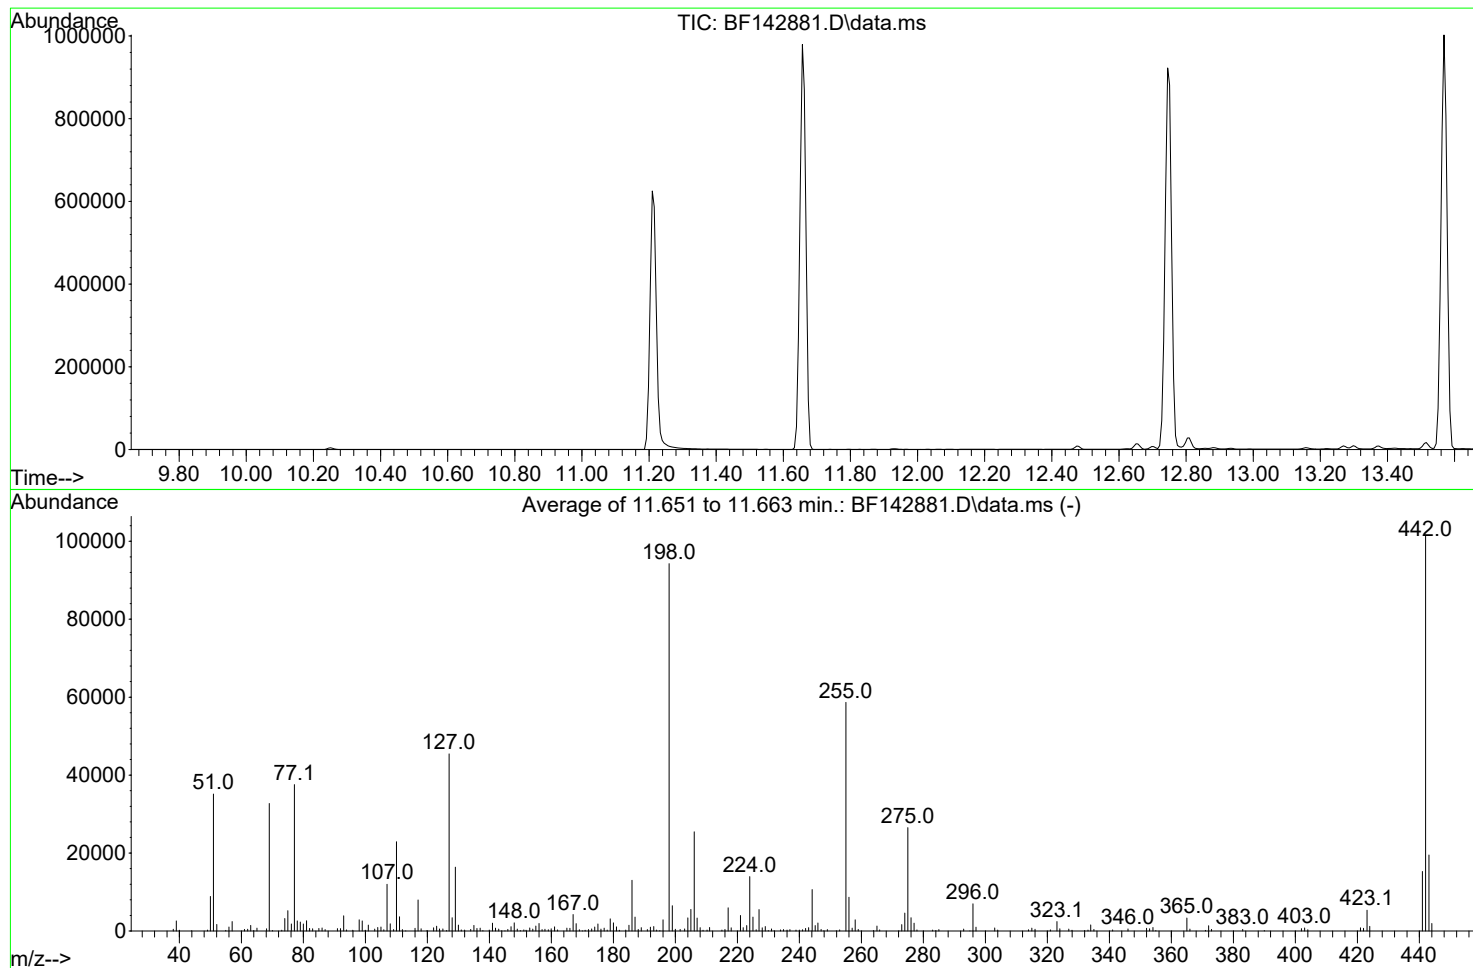

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	593	PASS
69	69	100	100	100.0	32725	PASS
70	69	0.00	2	0.4	117	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	94272	PASS
199	198	5	9	6.9	6501	PASS
365	198	1	100	3.5	3336	PASS
441	443	0.01	150	78.5	15290	PASS
442	442	100	100	100.0	101312	PASS
443	442	15	24	19.2	19487	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/27/2025	BNA_F	<u>BF142881.D</u>
Compound Name	Response	Retention Time
DDT	257142	13.568
DDD	5962	13.268
DDE	683	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6645	263787	2.52

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062725\
Data File : BF142881.D
Acq On : 27 Jun 2025 09:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 27 11:46:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

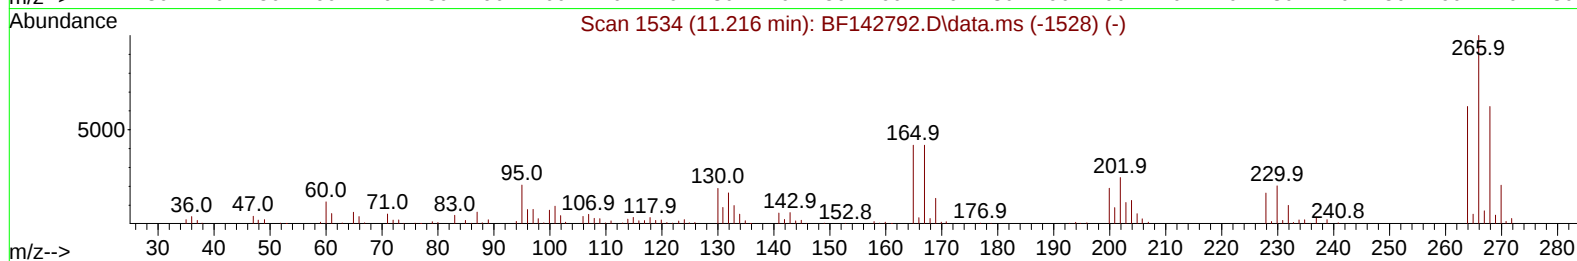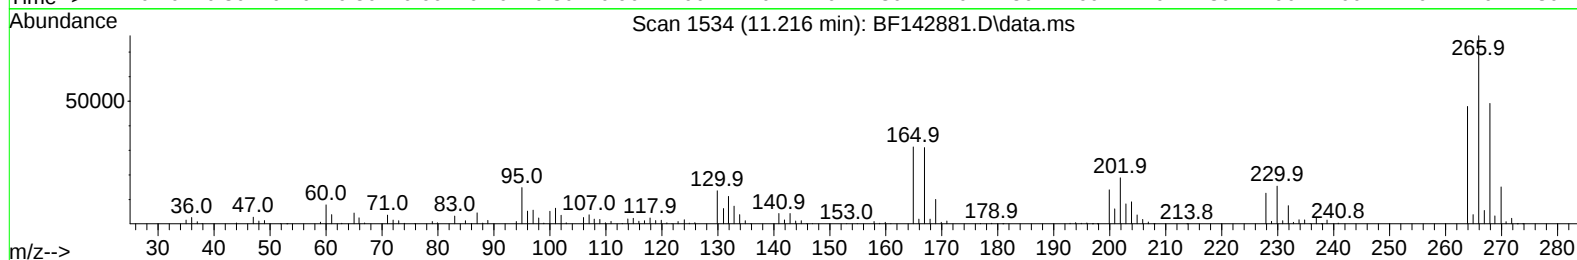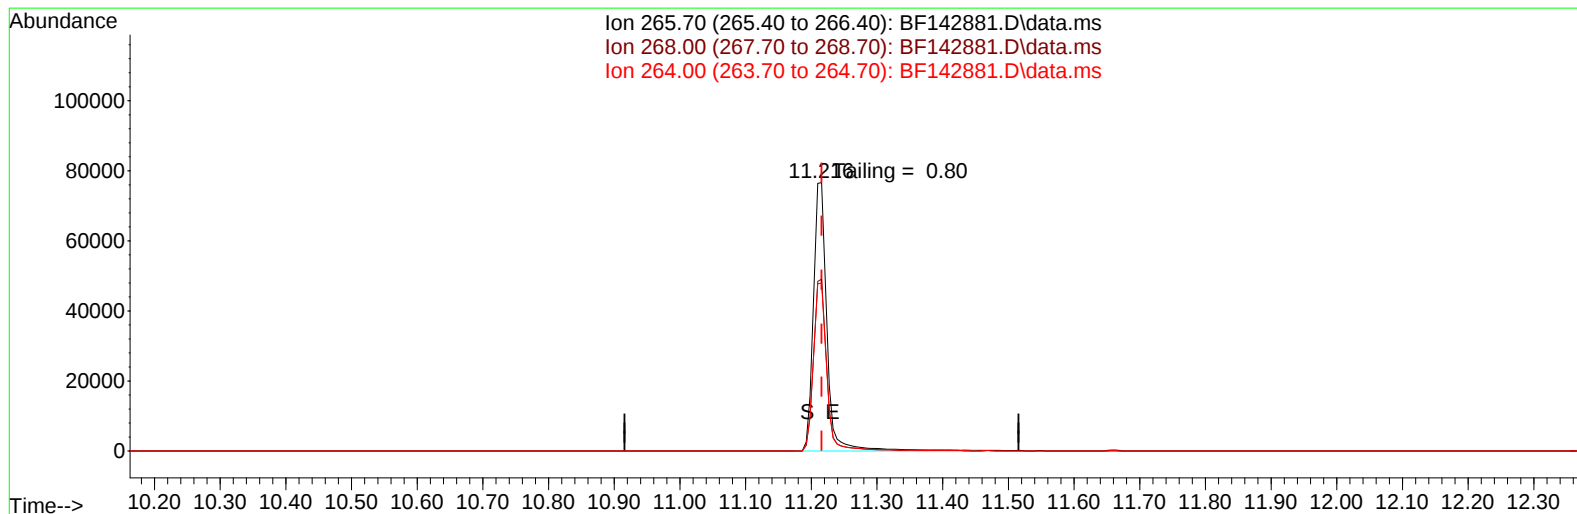

TIC: BF142881.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.000) 30391.06 ng




response 110119

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.06
264.00	62.40	62.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062725\
Data File : BF142881.D
Acq On : 27 Jun 2025 09:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 27 11:46:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

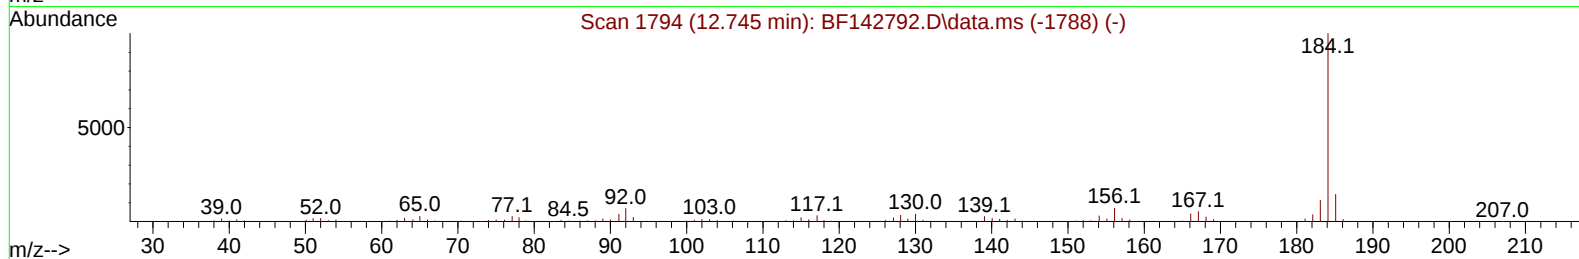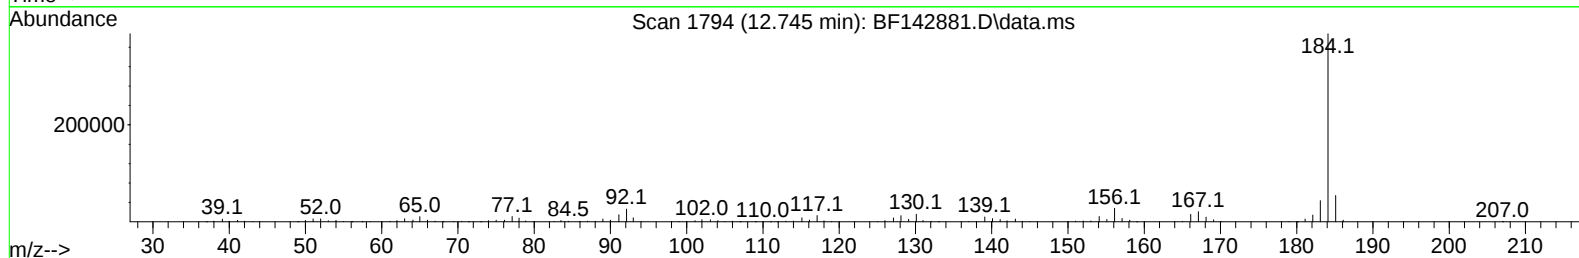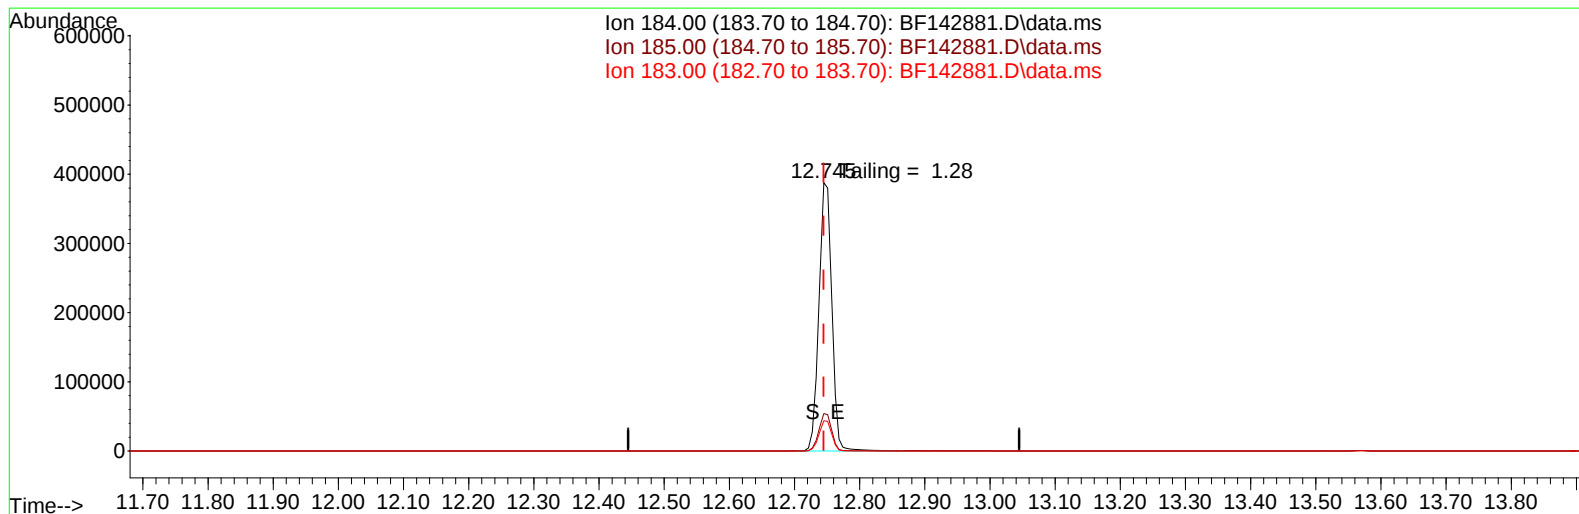

TIC: BF142881.D\data.ms

(77) Benzidine

12.745min (0.000) 0.00 ng

response 535637

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.98
183.00	11.20	11.30
0.00	0.00	0.00