


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062816\
Data File : BF088484.D
Acq On : 28 Jun 2016 17:34
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 28 05:25:55 2016

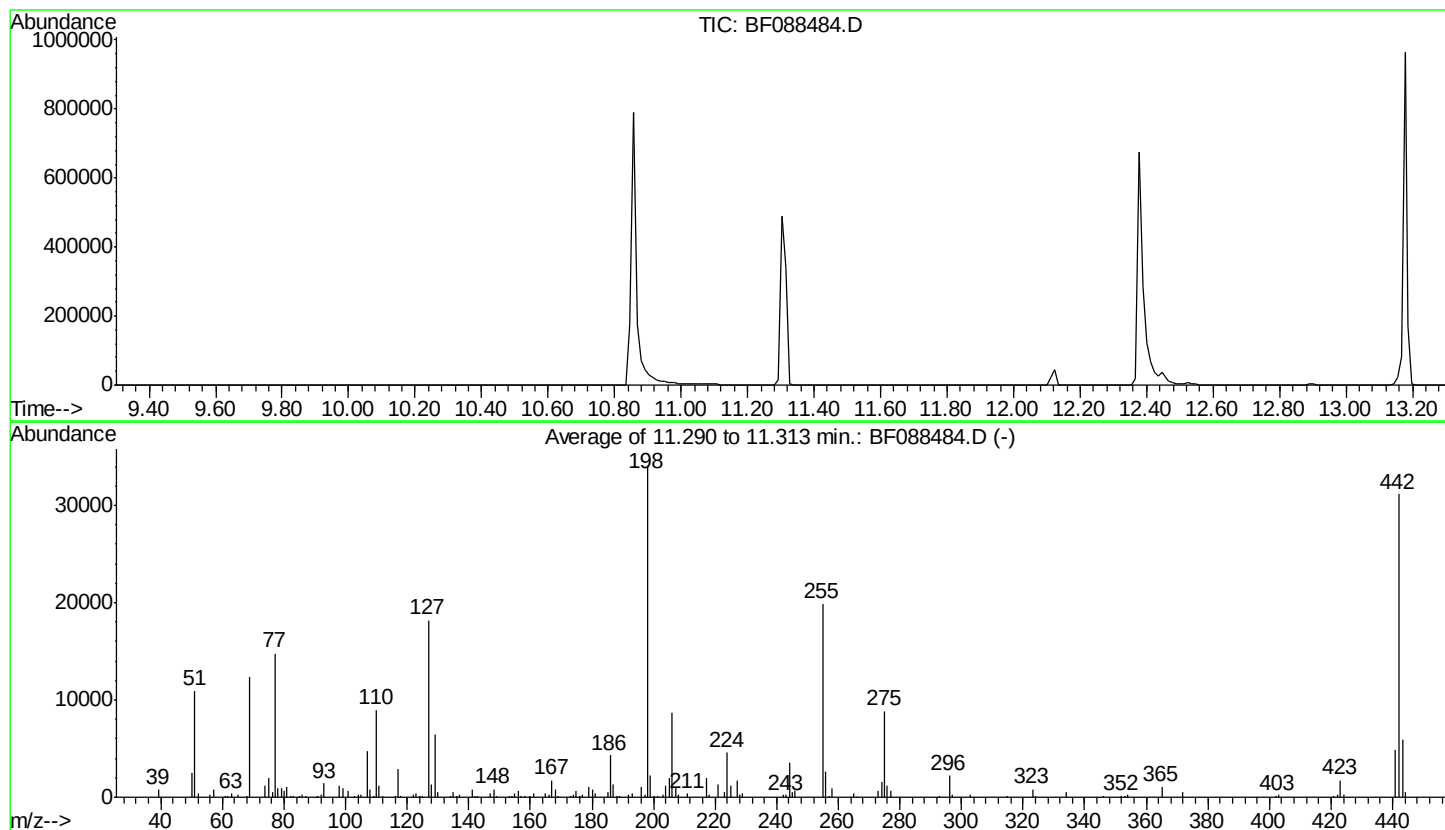

AutoFind: Scans 849, 850, 851; Background Corrected with Scan 846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	10986	PASS
68	69	0.00	2	1.5	189	PASS
69	198	0.00	100	36.3	12370	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.5	18228	PASS
197	198	0.00	2	0.6	210	PASS
198	198	100	100	100.0	34094	PASS
199	198	5	9	6.5	2215	PASS
275	198	10	60	26.0	8864	PASS
365	198	1	100	3.1	1057	PASS
441	442	0.01	24	15.7	4899	PASS
442	198	50	100	91.4	31162	PASS
443	442	15	24	19.2	5978	PASS