

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062817\
 Data File : BF096254.D
 Acq On : 28 Jun 2017 17:29
 Operator : SJ/MA
 Sample : I3852-05 20X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-31-0-1.5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.334	377	382	388	rVB2	19815	26956	2.15%	0.360%
2	4.963	486	489	495	rVB	58541	57941	4.62%	0.775%
3	5.381	554	560	565	rBV	124135	117208	9.35%	1.567%
4	6.398	729	733	739	rVB	169294	129539	10.33%	1.732%
5	6.545	754	758	761	rVB	149140	121930	9.72%	1.631%
6	6.781	794	798	802	rBV	1172394	932061	74.34%	12.464%
7	6.939	821	825	828	rBV	114601	103900	8.29%	1.389%
8	7.334	888	892	895	rBV	94866	71896	5.73%	0.961%
9	8.063	1012	1016	1019	rBV	1602666	1253855	100.00%	16.767%
10	8.498	1087	1090	1095	rBV2	15133	17257	1.38%	0.231%
11	9.098	1189	1192	1194	rVB	21701	19018	1.52%	0.254%
12	9.133	1195	1198	1202	rVV	169141	135434	10.80%	1.811%
13	9.228	1209	1214	1220	rBV6	13622	23946	1.91%	0.320%
14	9.528	1262	1265	1268	rBV	39354	38333	3.06%	0.513%
15	9.551	1268	1269	1273	rVB	25328	16159	1.29%	0.216%
16	9.816	1310	1314	1318	rBV	1322232	1142283	91.10%	15.275%
17	10.480	1424	1427	1429	rVB	24464	23225	1.85%	0.311%
18	10.592	1443	1446	1451	rVB3	45931	39806	3.17%	0.532%
19	10.745	1467	1472	1478	rVB	59591	63066	5.03%	0.843%
20	11.210	1548	1551	1556	rVB	52706	53460	4.26%	0.715%
21	11.292	1562	1565	1568	rBV	1205362	986392	78.67%	13.190%
22	11.351	1572	1575	1581	rVB8	10436	17094	1.36%	0.229%
23	11.557	1608	1610	1616	rBV7	15889	16775	1.34%	0.224%
24	11.804	1648	1652	1653	rBV4	11639	17319	1.38%	0.232%
25	11.822	1653	1655	1660	rVB6	17287	17958	1.43%	0.240%
26	11.904	1666	1669	1672	rBV5	16315	16718	1.33%	0.224%
27	12.221	1721	1723	1726	rBV3	16620	17090	1.36%	0.229%
28	12.286	1732	1734	1739	rVB6	21106	23665	1.89%	0.316%
29	12.345	1741	1744	1746	rBV4	23849	23397	1.87%	0.313%
30	12.504	1768	1771	1774	rBV3	31409	35491	2.83%	0.475%
31	12.874	1831	1834	1840	rBV	137307	129751	10.35%	1.735%
32	13.921	2009	2012	2016	rBV	1093405	971780	77.50%	12.995%
33	15.351	2251	2255	2260	rVB	689703	817352	65.19%	10.930%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062817\
Data File : BF096254.D
Acq On : 28 Jun 2017 17:29
Operator : SJ/MA
Sample : I3852-05 20X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-31-0-1.5

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 7478055

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062817\
Data File : BF096254.D
Acq On : 28 Jun 2017 17:29
Operator : SJ/MA
Sample : I3852-05 20X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-31-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

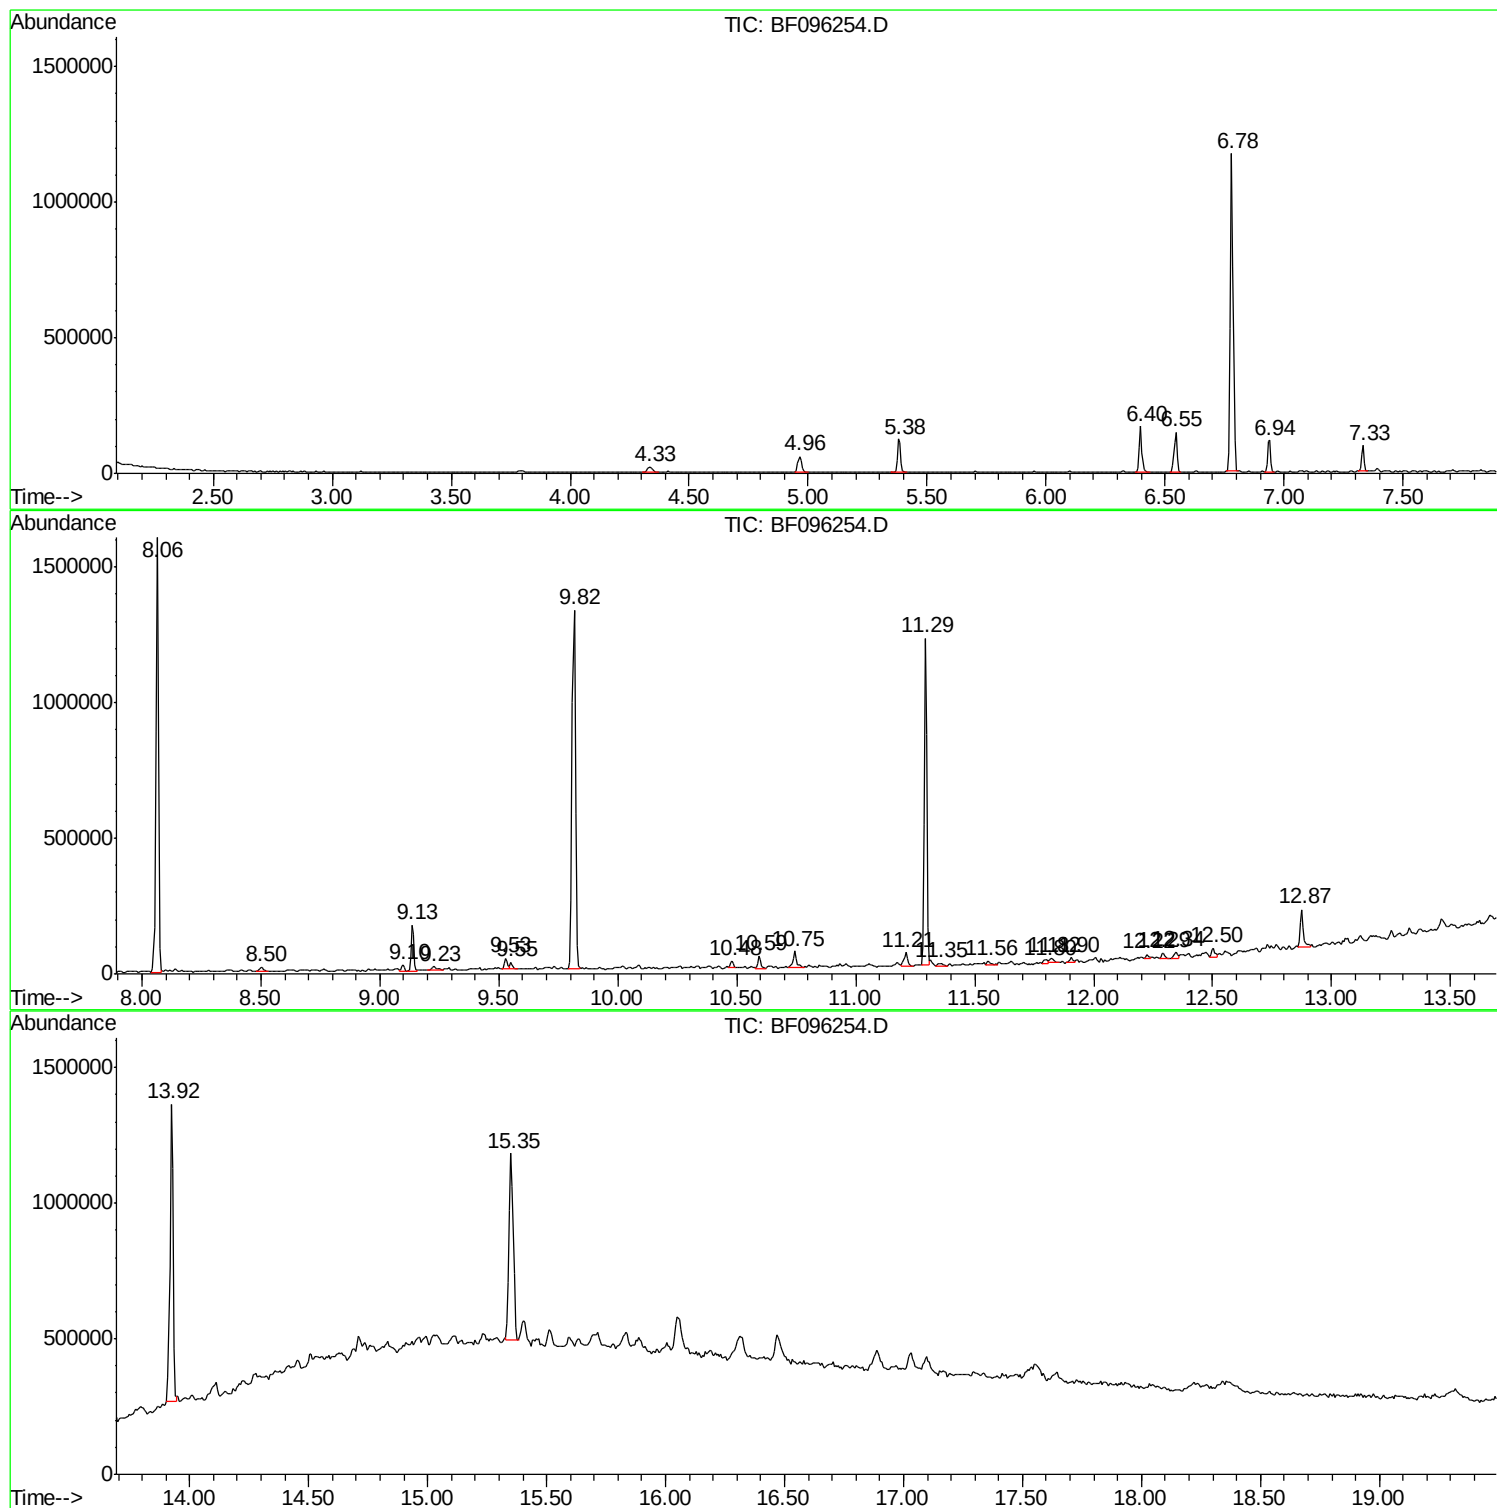

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062817\
Data File : BF096254.D
Acq On : 28 Jun 2017 17:29
Operator : SJ/MA
Sample : I3852-05 20X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-31-0-1.5










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.55 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.55	2.62 ng	121930	1,4-Dichlorobenzene-d4	6.78

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	38
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
3		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	9
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

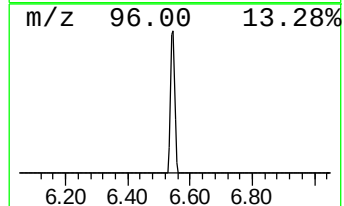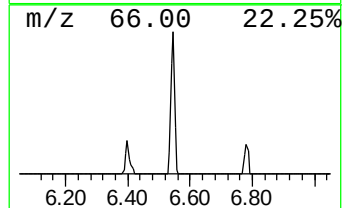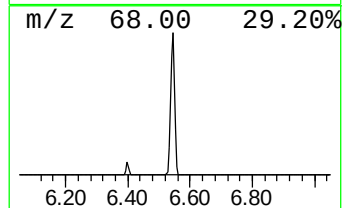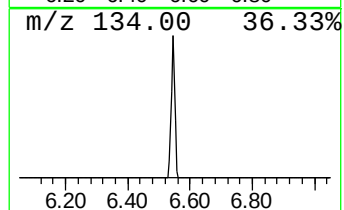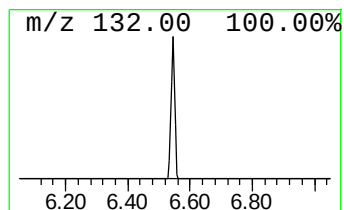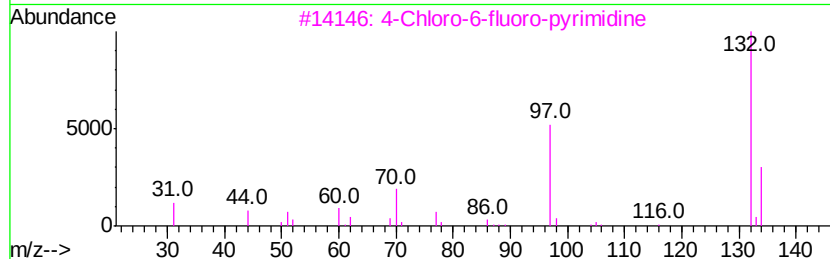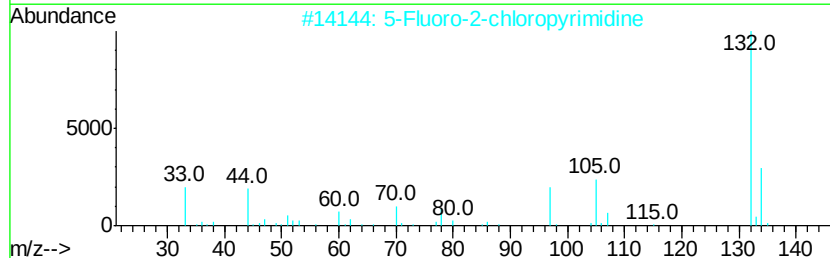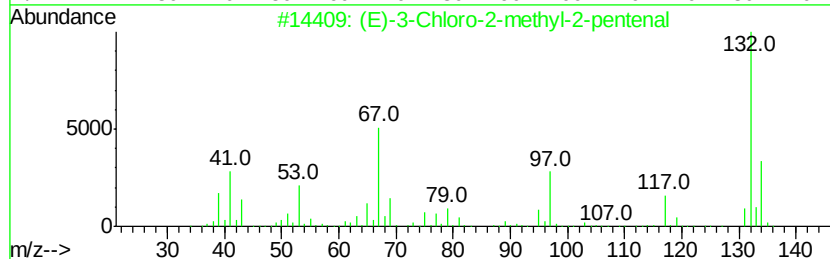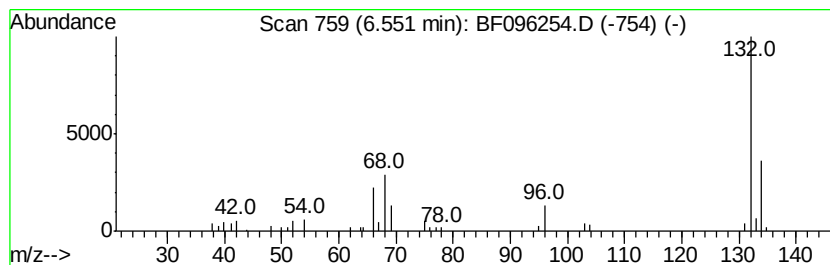

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062817\
Data File : BF096254.D
Acq On : 28 Jun 2017 17:29
Operator : SJ/MA
Sample : I3852-05 20X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-31-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.55	6.55	2.6	ng	121930	1	6.78	932061	20.0