

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062817\
 Data File : BF096274.D
 Acq On : 29 Jun 2017 3:41
 Operator : SJ/MA
 Sample : I3852-18 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-50-1.5-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF062717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.963	486	489	498	rBV	80939	78840	7.16%	0.916%
2	5.387	557	561	566	rBV	484118	422547	38.36%	4.910%
3	6.404	730	734	744	rVB	519010	444513	40.36%	5.165%
4	6.545	755	758	762	rBV	517647	416585	37.82%	4.841%
5	6.781	795	798	802	rBV	997323	851405	77.30%	9.893%
6	6.939	821	825	828	rVB	388413	310775	28.22%	3.611%
7	7.334	889	892	896	rBV	301635	228921	20.78%	2.660%
8	7.751	959	963	967	rBV2	11143	13760	1.25%	0.160%
9	8.063	1013	1016	1020	rBV	1335102	1101387	100.00%	12.798%
10	9.139	1195	1199	1202	rBV	504421	414087	37.60%	4.811%
11	9.228	1211	1214	1217	rBV4	11244	13253	1.20%	0.154%
12	9.528	1262	1265	1268	rBV	42152	35739	3.24%	0.415%
13	9.816	1310	1314	1318	rBV	1246939	1035145	93.99%	12.028%
14	10.257	1386	1389	1392	rVB	14008	14443	1.31%	0.168%
15	10.480	1422	1427	1430	rBV3	17570	24092	2.19%	0.280%
16	10.598	1443	1447	1450	rBV	167054	148086	13.45%	1.721%
17	10.698	1461	1464	1467	rBV	34480	30160	2.74%	0.350%
18	10.727	1467	1469	1471	rVV	17553	18717	1.70%	0.217%
19	10.745	1471	1472	1476	rVB2	24788	17277	1.57%	0.201%
20	11.174	1538	1545	1548	rBV4	18451	30954	2.81%	0.360%
21	11.210	1548	1551	1554	rVB3	14673	16397	1.49%	0.191%
22	11.292	1562	1565	1569	rBV	1058403	957317	86.92%	11.124%
23	11.692	1629	1633	1639	rBV9	6876	15437	1.40%	0.179%
24	11.822	1653	1655	1659	rBV4	19466	21217	1.93%	0.247%
25	11.863	1659	1662	1664	rBV	18967	15731	1.43%	0.183%
26	12.504	1768	1771	1774	rVB	63835	56392	5.12%	0.655%
27	12.727	1807	1809	1812	rVB	42029	35732	3.24%	0.415%
28	12.874	1831	1834	1838	rBV	421931	358190	32.52%	4.162%
29	13.927	2009	2013	2016	rBV	910432	893584	81.13%	10.383%
30	15.357	2252	2256	2260	rVB	506015	585516	53.16%	6.803%




Sum of corrected areas: 8606199

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062817\
 Data File : BF096274.D
 Acq On : 29 Jun 2017 3:41
 Operator : SJ/MA
 Sample : I3852-18 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 Client Sampled :
 G-50-1.5-3

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF062717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
 TIC Integration Parameters: LSCINT.P

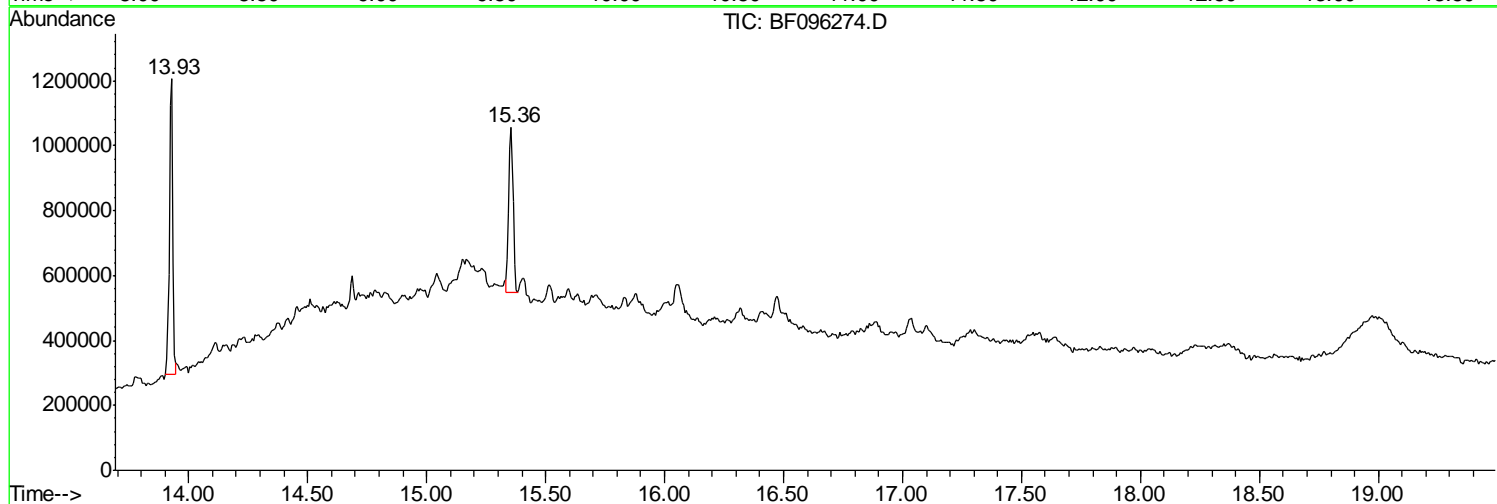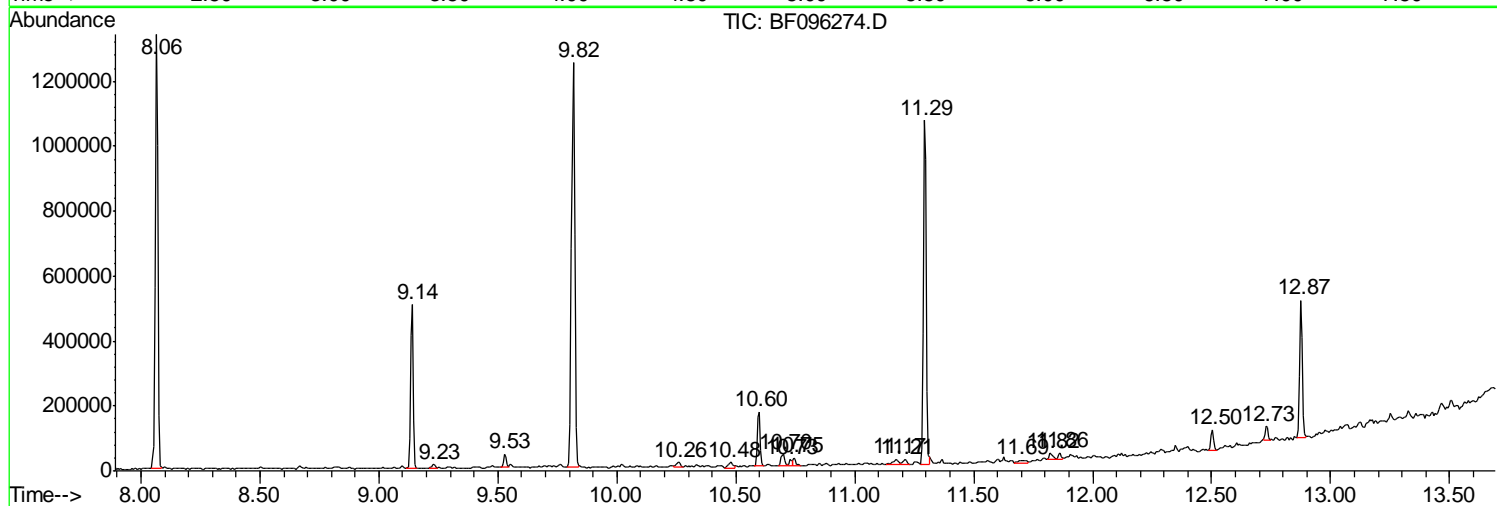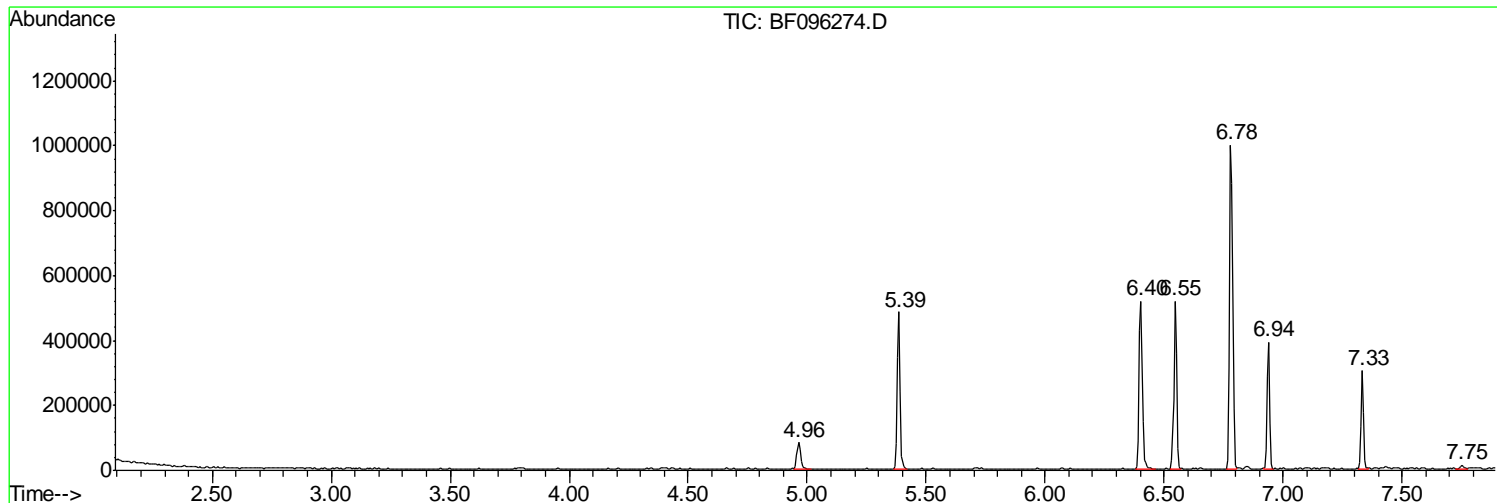

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062817\
 Data File : BF096274.D
 Acq On : 29 Jun 2017 3:41
 Operator : SJ/MA
 Sample : I3852-18 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampled :
 G-50-1.5-3










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF062717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
 TIC Integration Parameters: LSCINT.P

 Peak Number 1 unknown6.55 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.55	9.79 ng	416585	1,4-Dichlorobenzene-d4	6.78

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Tranlycypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
4		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

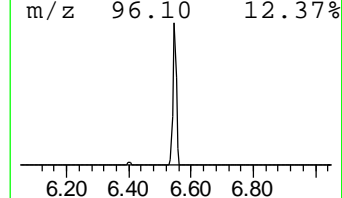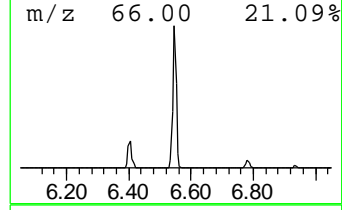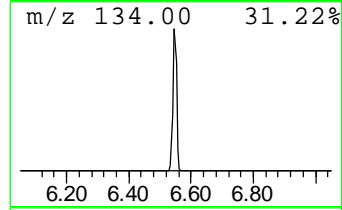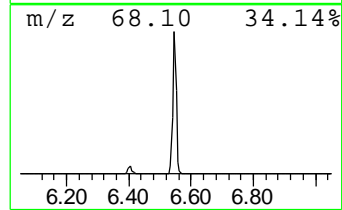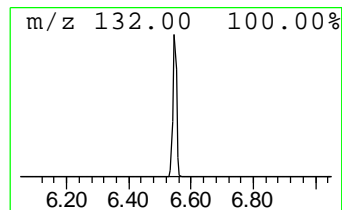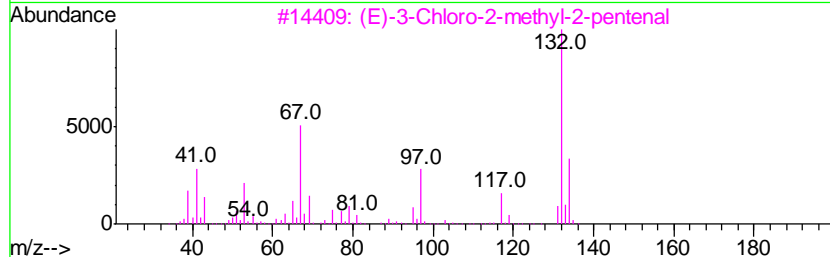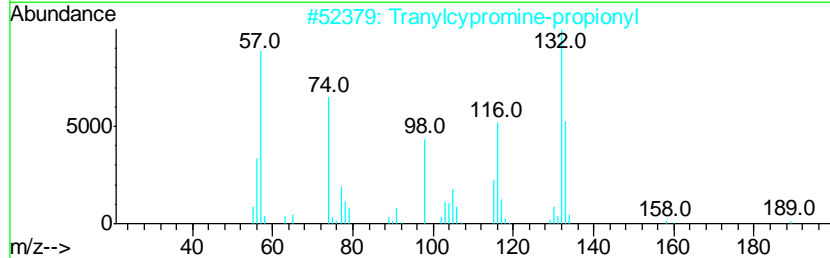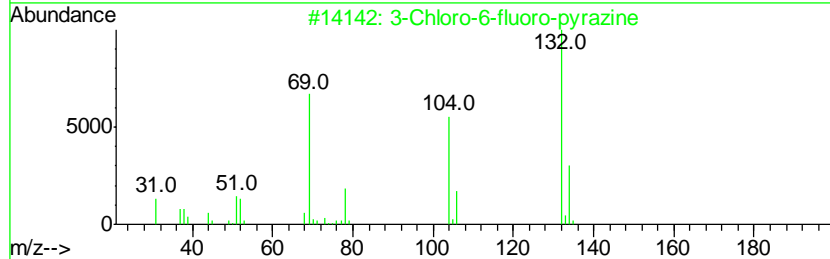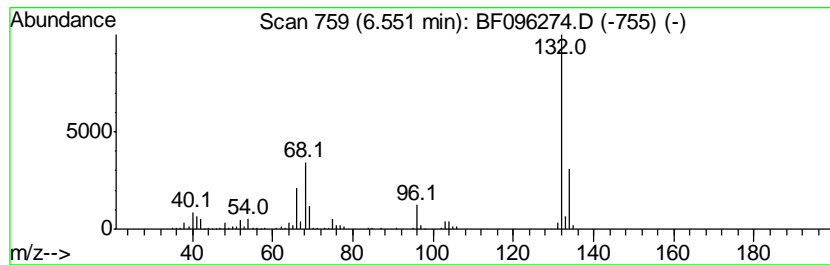

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062817\
Data File : BF096274.D
Acq On : 29 Jun 2017 3:41
Operator : SJ/MA
Sample : I3852-18 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-50-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.55	6.55	9.8	ng	416585	1	6.78	851405	20.0