


Data Path : Z:\HPCHEM1\BNA_F\Data\BF062817\
 Data File : BF096242.D
 Acq On : 28 Jun 2017 11:48
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 28 15:41:49 2017

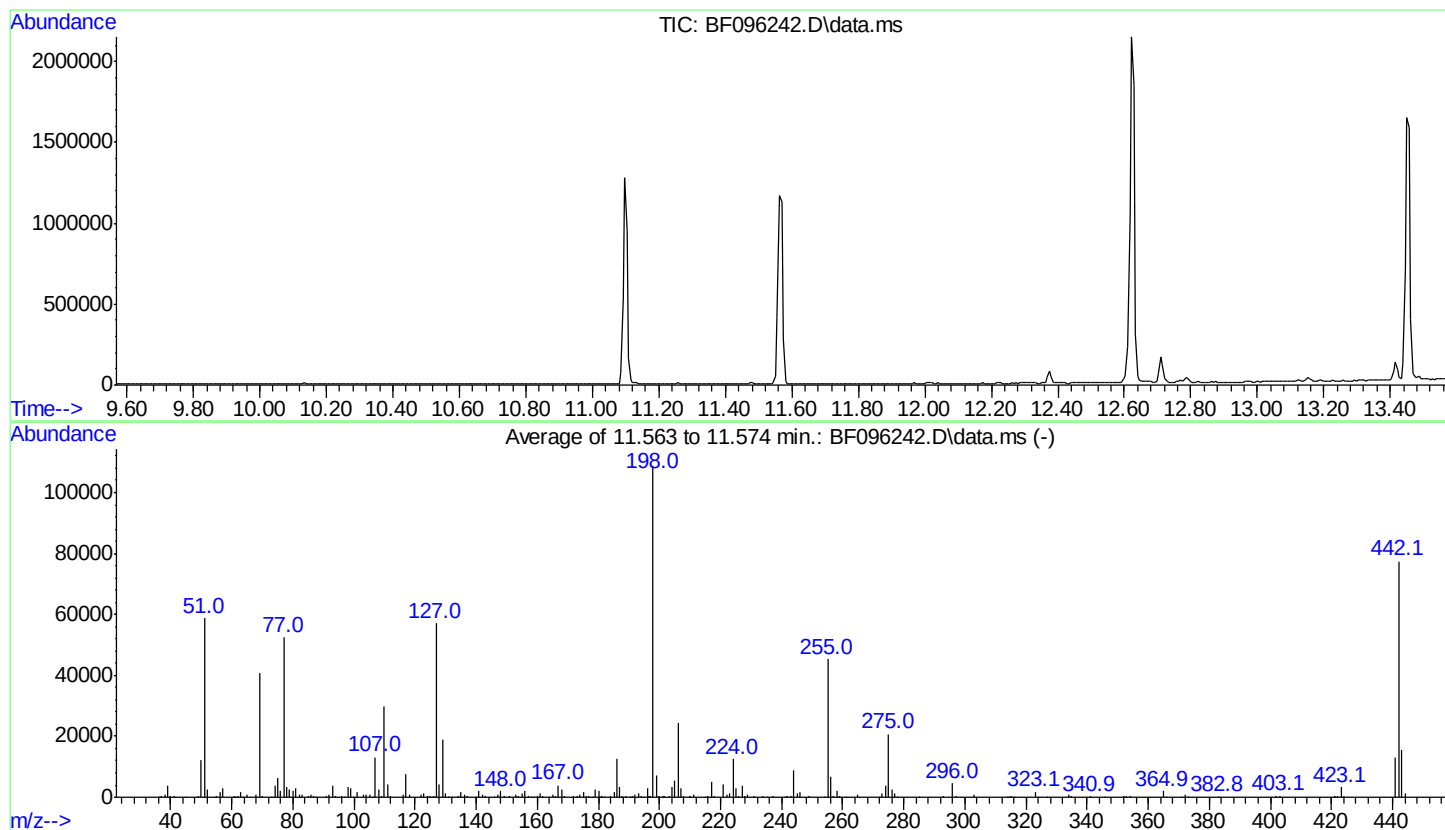

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.0	58795	PASS
68	69	0.00	2	1.6	665	PASS
69	198	0.00	100	37.4	40689	PASS
70	69	0.00	2	0.6	258	PASS
127	198	10	80	52.4	57007	PASS
197	198	0.00	2	0.4	461	PASS
198	198	100	100	100.0	108834	PASS
199	198	5	9	6.4	6961	PASS
275	198	10	60	18.9	20609	PASS
365	198	1	100	1.8	1965	PASS
441	442	0.01	24	17.1	13233	PASS
442	198	50	100	71.1	77405	PASS
443	442	15	24	20.0	15454	PASS