


Data Path : Z:\HPCHEM1\BNA F\Data\BF062817\
 Data File : BF096268.D
 Acq On : 29 Jun 2017 00:50
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 28 15:41:49 2017

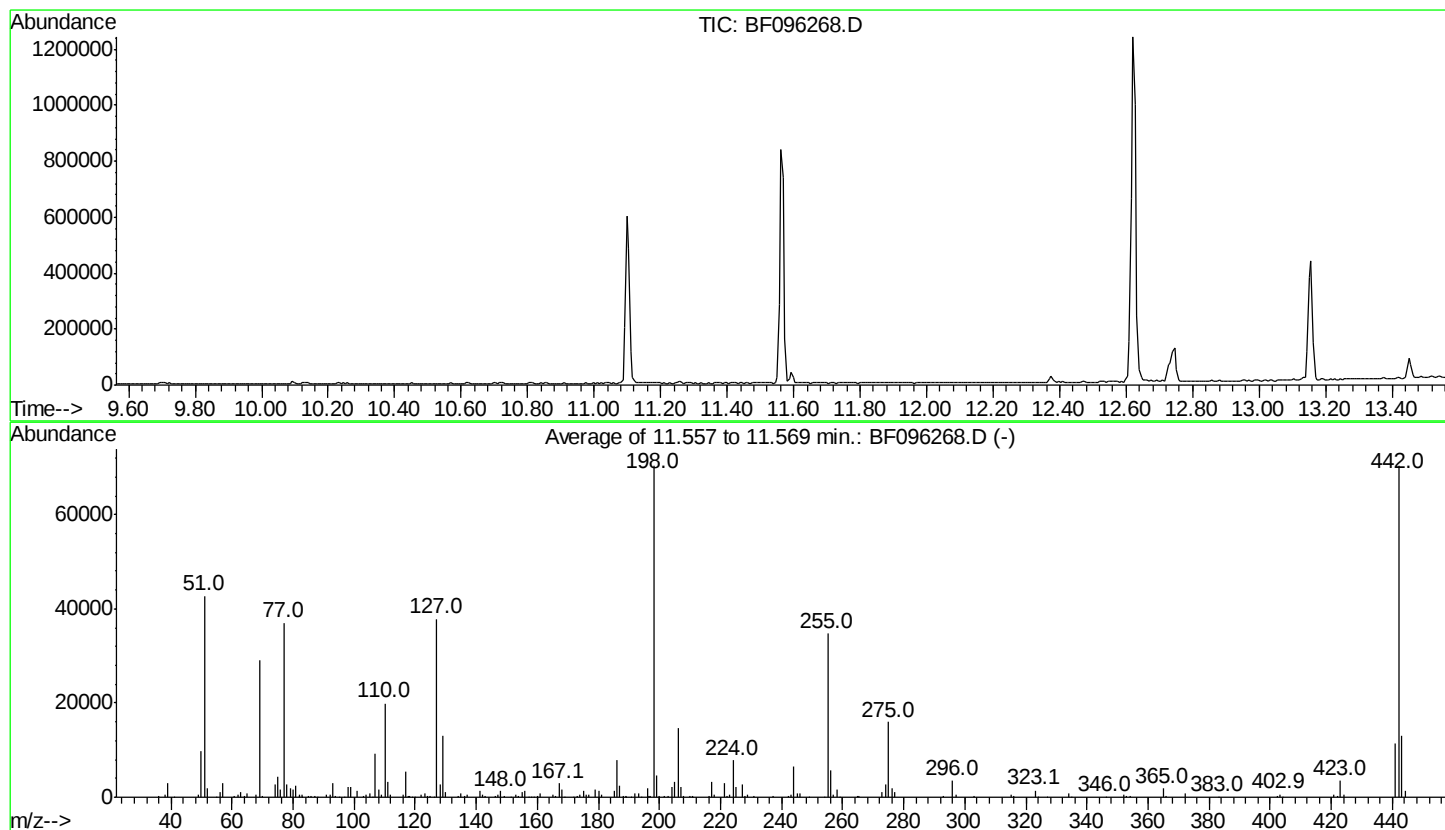

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.7	42776	PASS
68	69	0.00	2	1.5	436	PASS
69	198	0.00	100	41.5	29218	PASS
70	69	0.00	2	0.9	274	PASS
127	198	10	80	53.8	37885	PASS
197	198	0.00	2	0.5	354	PASS
198	198	100	100	100.0	70434	PASS
199	198	5	9	6.6	4650	PASS
275	198	10	60	22.6	15930	PASS
365	198	1	100	2.7	1868	PASS
441	442	0.01	24	16.3	11456	PASS
442	198	50	100	99.9	70387	PASS
443	442	15	24	18.7	13167	PASS