

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062821\
 Data File : BF124472.D
 Acq On : 28 Jun 2021 16:52
 Operator : JU/CG
 Sample : M2824-03RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ABN-1

Quant Time: Jun 28 17:21:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 28 16:01:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.692	152	38193	20.000	ng	0.00
21) Naphthalene-d8	7.975	136	139359	20.000	ng	# 0.00
39) Acenaphthene-d10	9.722	164	84347	20.000	ng	0.00
64) Phenanthrene-d10	11.210	188	164795	20.000	ng	0.00
76) Chrysene-d12	13.857	240	122379	20.000	ng	0.00
86) Perylene-d12	15.280	264	81106	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.322	112	290481	119.613	ng	0.01
7) Phenol-d6	6.345	99	321755	101.471	ng	0.00
23) Nitrobenzene-d5	7.263	82	277818	82.657	ng	0.00
42) 2,4,6-Tribromophenol	10.522	330	147227	146.098	ng	0.00
45) 2-Fluorobiphenyl	9.051	172	545512	79.226	ng	0.00
79) Terphenyl-d14	12.804	244	669998	82.001	ng	0.00
Target Compounds						
						Qvalue
19) n-Nitroso-di-n-propyla...	7.263	70	37323	17.502	ng	# 61
25) Isophorone	7.263	82	277816	48.077	ng	# 69
31) Naphthalene	7.992	128	45875	5.595	ng	97
32) Benzoic acid	7.792	122	269	7.369	ng	# 1
33) 4-Chloroaniline	7.992	127	6527	2.120	ng	# 38
50) Dimethylphthalate	9.728	163	17006	2.557	ng	# 1
51) 2,6-Dinitrotoluene	9.722	165	11869	7.726	ng	# 11
57) 2,4-Dinitrotoluene	9.722	165	11869	5.829	ng	# 17
67) 4-Bromophenyl-phenylether	10.522	248	10531	4.750	ng	# 1
70) Pentachlorophenol	10.792	266	107	6.272	ng	# 18
77) Benzidine	12.551	184	38845	15.838	ng	# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062821\
Data File : BF124472.D
Acq On : 28 Jun 2021 16:52
Operator : JU/CG
Sample : M2824-03RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ABN-1

Quant Time: Jun 28 17:21:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 28 16:01:42 2021
Response via : Initial Calibration




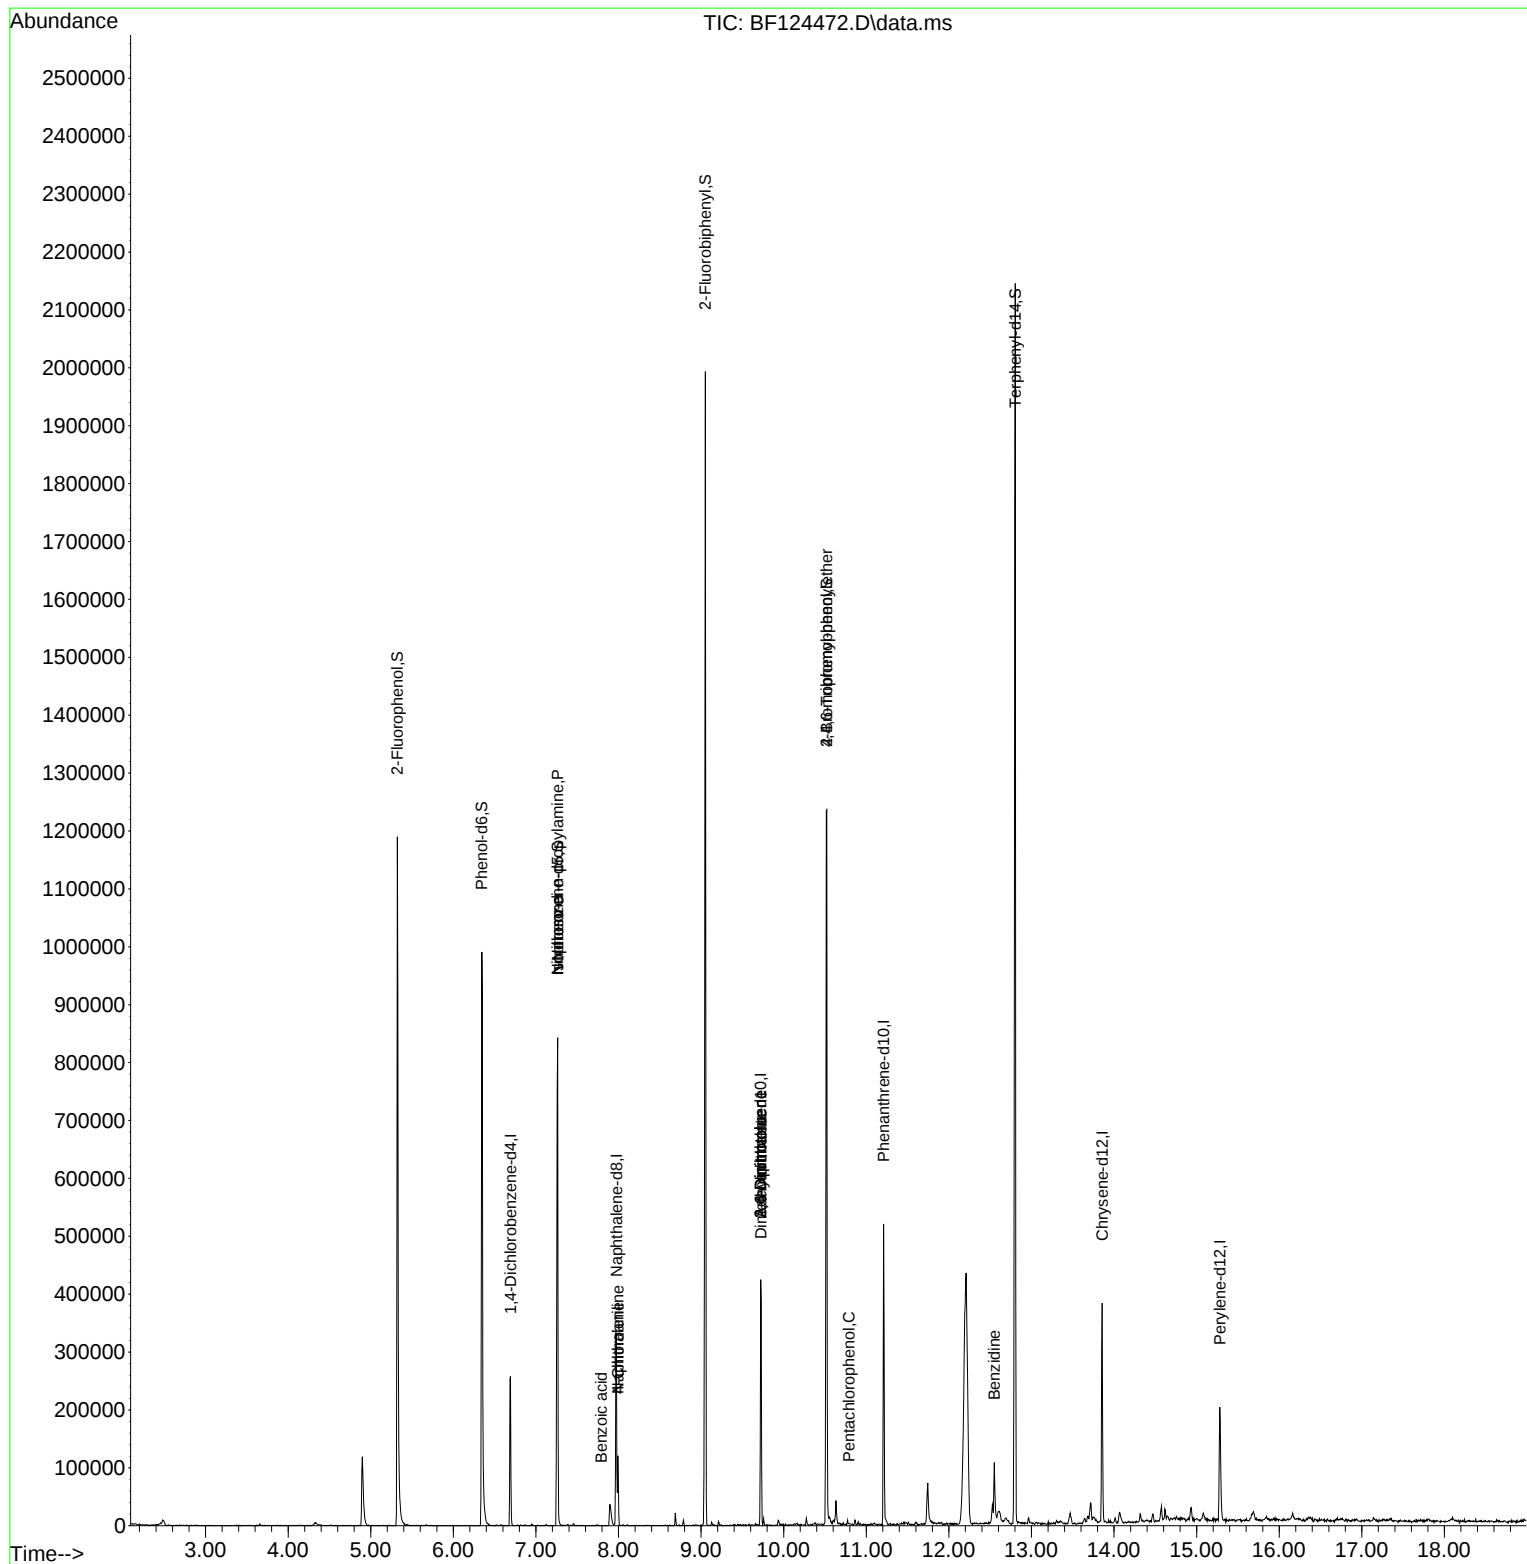


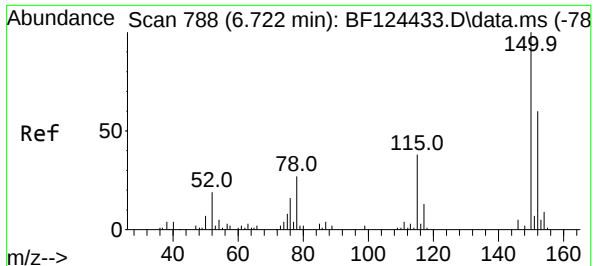

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.692 min Scan# 783
 Delta R.T. -0.001 min
 Lab File: BF124472.D
 Acq: 28 Jun 2021 16:52




Instrument :
 BNA_F
 ClientSampleId :
 ABN-1


Tgt Ion:152 Resp: 38193
 Ion Ratio Lower Upper
 152 100
 150 165.6 127.0 190.6
 115 58.5 54.3 81.5

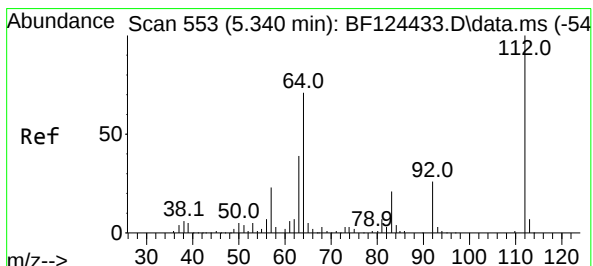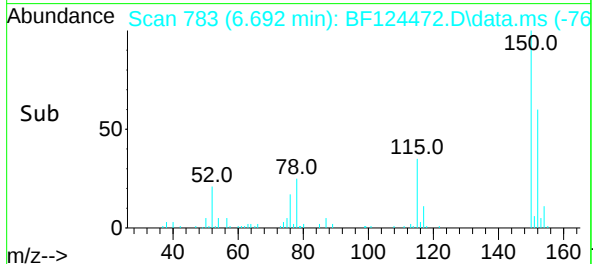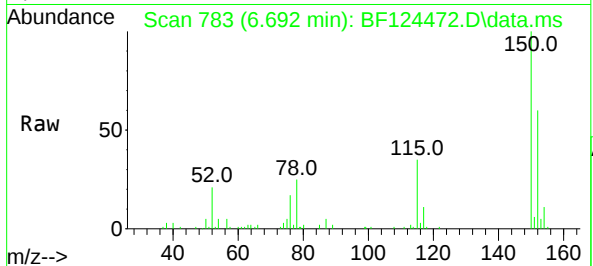

#5
 2-Fluorophenol
 Concen: 119.613 ng
 RT: 5.322 min Scan# 550
 Delta R.T. 0.012 min
 Lab File: BF124472.D
 Acq: 28 Jun 2021 16:52

Tgt Ion:112 Resp: 290481
 Ion Ratio Lower Upper
 112 100
 64 73.8 61.4 92.0
 63 42.7 33.0 49.4


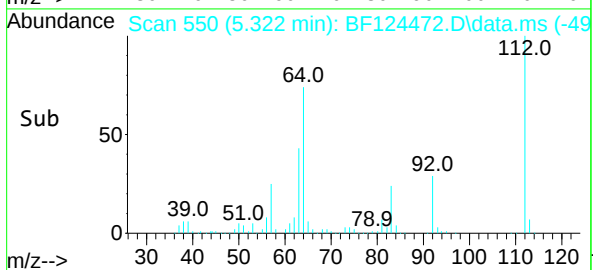

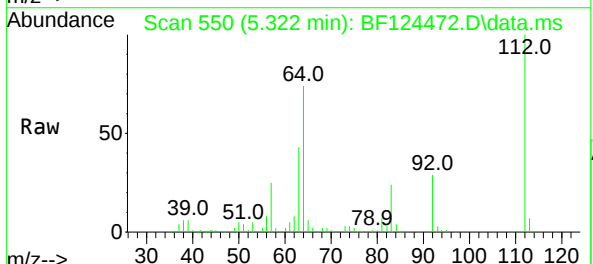


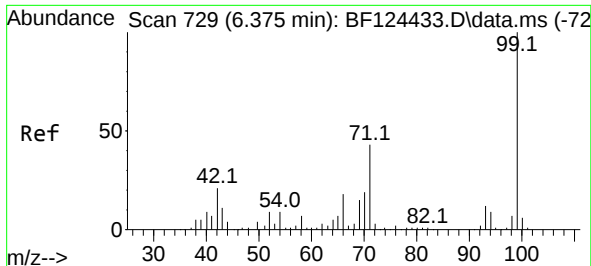

#7
Phenol-d6
Concen: 101.471 ng
RT: 6.345 min Scan# 724
Delta R.T. -0.000 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52




Instrument :
BNA_F
ClientSampleId :
ABN-1


Tgt Ion: 99 Resp: 321755
Ion Ratio Lower Upper
99 100
42 19.6 19.8 29.8#
71 46.5 31.1 46.7

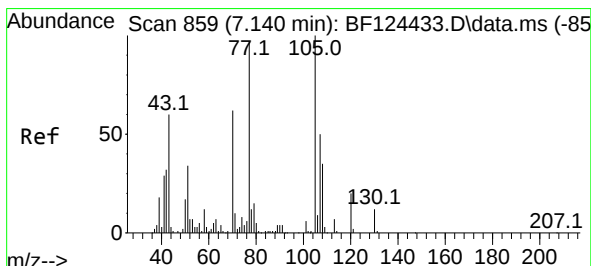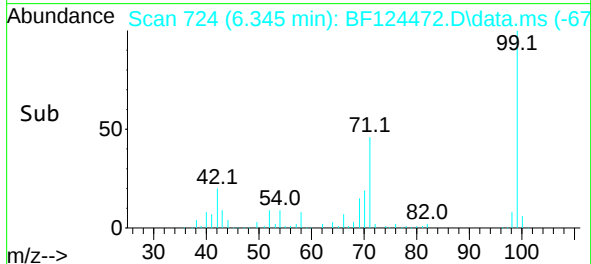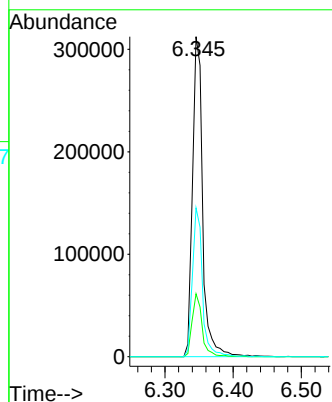

#19
n-Nitroso-di-n-propylamine
Concen: 17.502 ng
RT: 7.263 min Scan# 880
Delta R.T. 0.147 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52

Tgt Ion: 70 Resp: 37323
Ion Ratio Lower Upper
70 100
42 40.2 60.1 90.1#
101 0.0 7.4 11.2#
130 1.3 14.2 21.2#


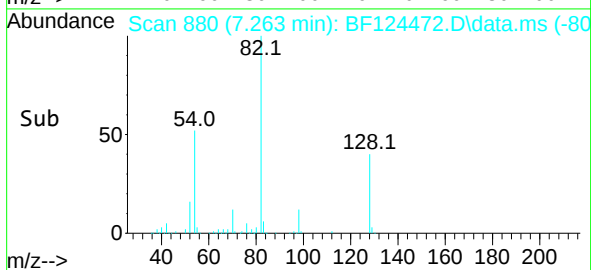

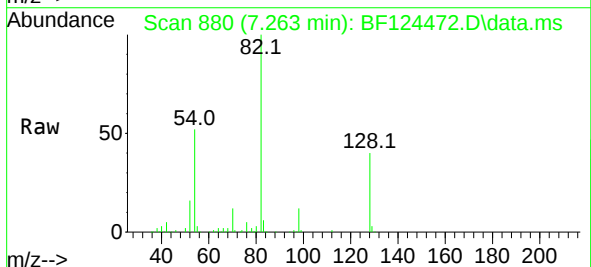




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.975 min Scan# 1001
Delta R.T. -0.000 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52




Instrument :
BNA_F
ClientSampled :
ABN-1


Tgt Ion:136	Resp:	139359
Ion Ratio	Lower	Upper
136	100	
137	10.1	8.7 13.1
54	7.2	9.8 14.6#
68	4.0	4.1 6.1#

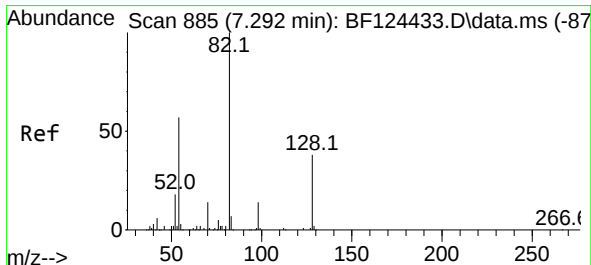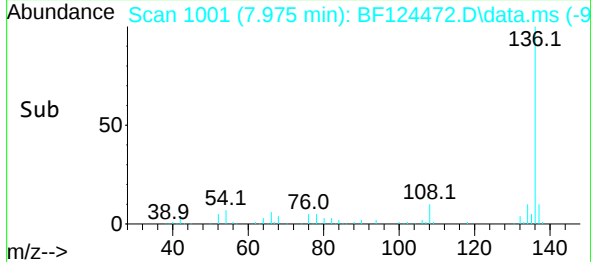

#23
Nitrobenzene-d5
Concen: 82.657 ng
RT: 7.263 min Scan# 880
Delta R.T. -0.000 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52

Tgt Ion: 82	Resp:	277818
Ion Ratio	Lower	Upper
82	100	
128	40.4	29.4 44.2
54	52.4	54.1 81.1#


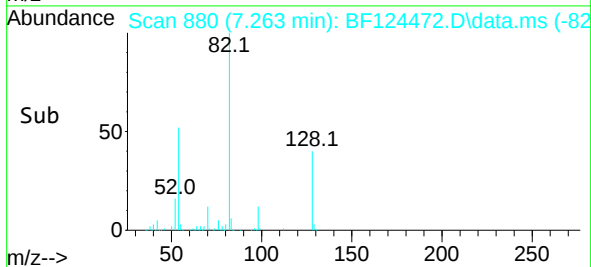
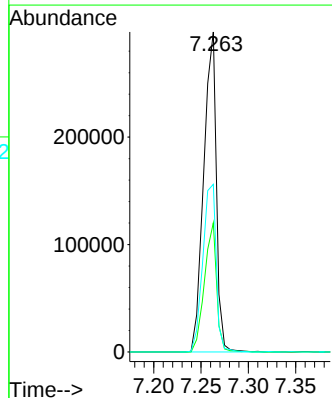
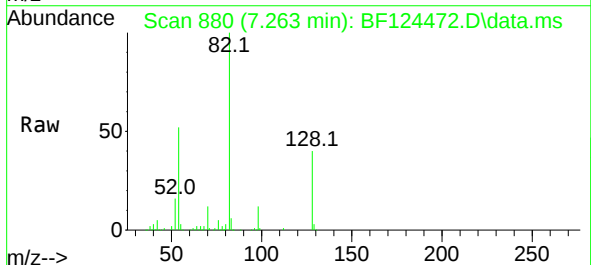




#25
Isophorone
Concen: 48.077 ng
RT: 7.263 min Scan# 880
Delta R.T. -0.259 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52




Instrument :
BNA_F
ClientSampleId :
ABN-1


Tgt Ion: 82 Resp: 277816
Ion Ratio Lower Upper
82 100
95 0.0 5.8 8.6#
138 0.0 11.8 17.8#

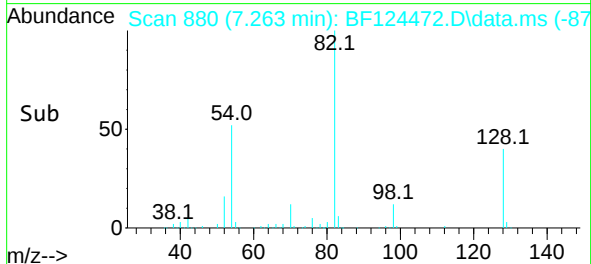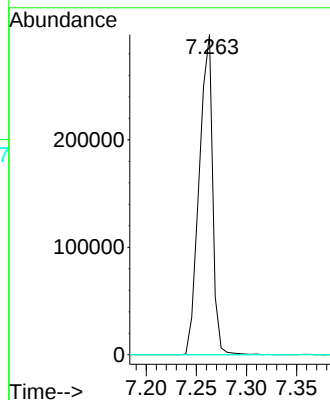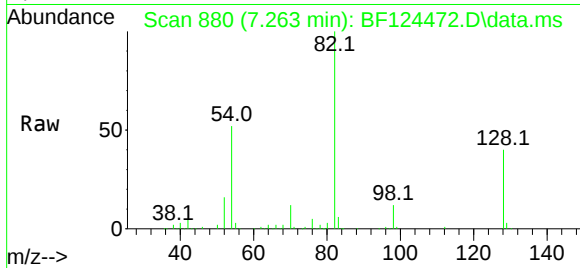

#31
Naphthalene
Concen: 5.595 ng
RT: 7.992 min Scan# 1004
Delta R.T. -0.006 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52

Tgt Ion: 128 Resp: 45875
Ion Ratio Lower Upper
128 100
129 11.0 8.9 13.3
127 15.8 10.8 16.2


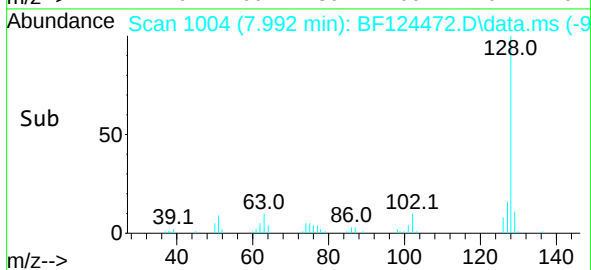
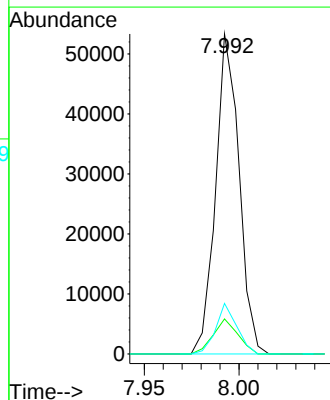
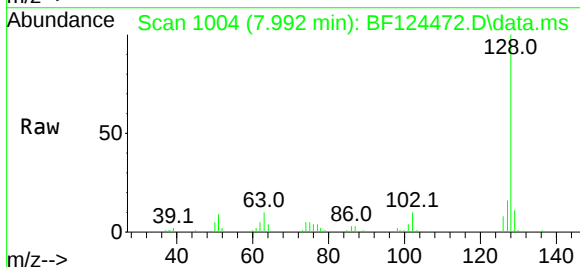


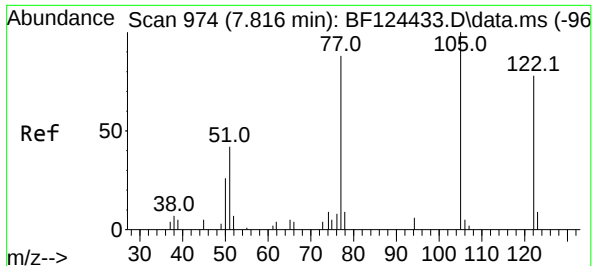

#32
Benzoic acid
Concen: 7.369 ng
RT: 7.792 min Scan# 970
Delta R.T. -0.006 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52




Instrument :
BNA_F
ClientSampleId :
ABN-1


Tgt Ion:122 Resp: 269
Ion Ratio Lower Upper
122 100
105 0.0 107.8 147.8#
77 0.0 81.6 121.6#

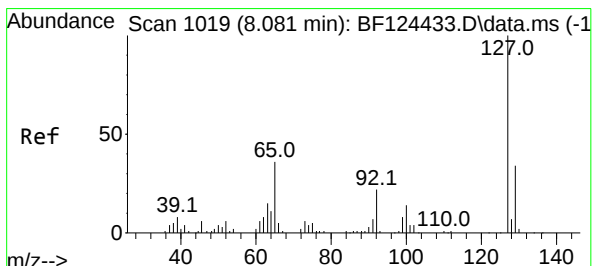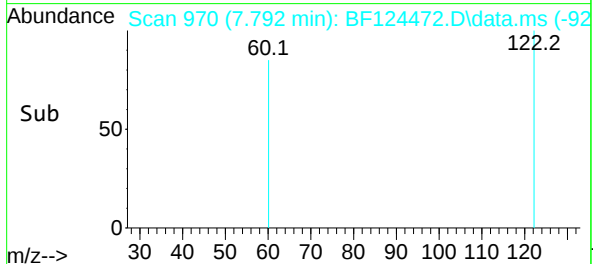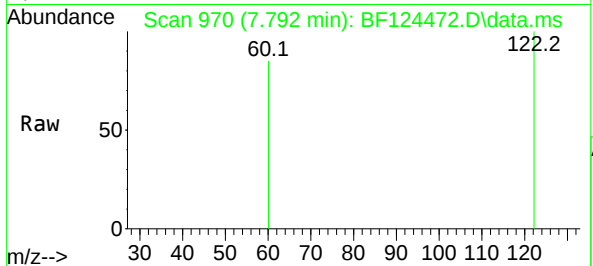

#33
4-Chloroaniline
Concen: 2.120 ng
RT: 7.992 min Scan# 1004
Delta R.T. -0.065 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52

Tgt Ion:127 Resp: 6527
Ion Ratio Lower Upper
127 100
129 69.4 25.7 38.5#
65 0.0 34.5 51.7#
92 0.0 17.4 26.0#


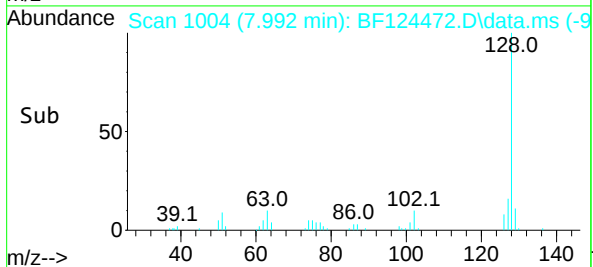

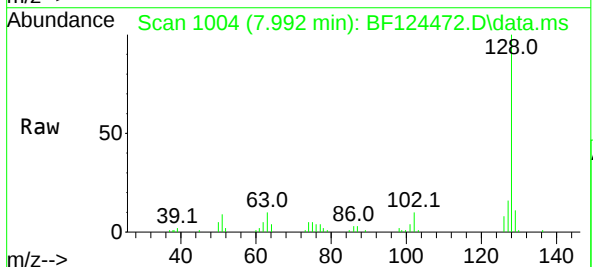




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.722 min Scan# 1298
Delta R.T. -0.006 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52




Instrument :
BNA_F
ClientSampled :
ABN-1


Tgt Ion:164 Resp: 84347
Ion Ratio Lower Upper
164 100
162 105.2 80.7 121.1
160 46.0 37.3 55.9

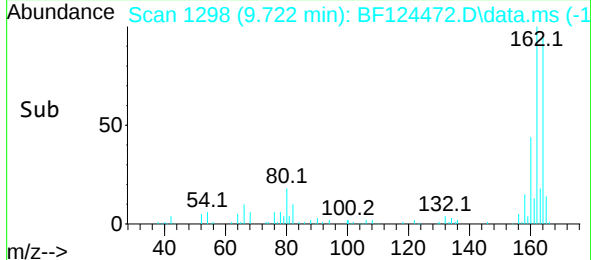

#42
2,4,6-Tribromophenol
Concen: 146.098 ng
RT: 10.522 min Scan# 1434
Delta R.T. -0.000 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52

Tgt Ion:330 Resp: 147227
Ion Ratio Lower Upper
330 100
332 96.6 77.1 115.7
141 37.6 27.9 41.9


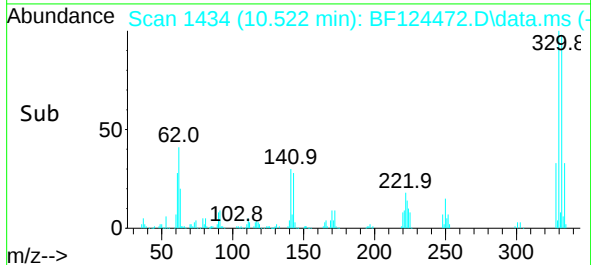

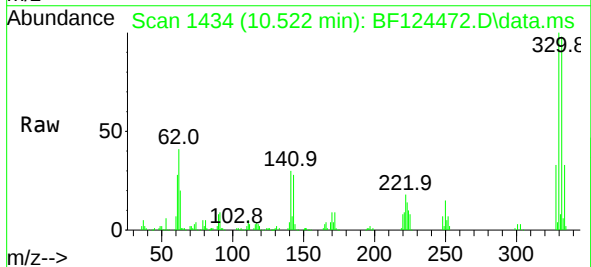


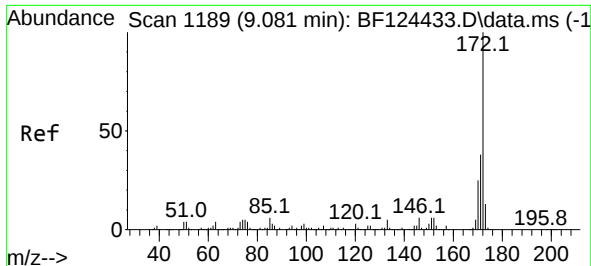

#45
2-Fluorobiphenyl
Concen: 79.226 ng
RT: 9.051 min Scan# 1184
Delta R.T. -0.000 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52




Instrument :
BNA_F
ClientSampleId :
ABN-1


Tgt Ion:172 Resp: 545512
Ion Ratio Lower Upper
172 100
171 38.2 28.1 42.1
170 23.5 19.2 28.8

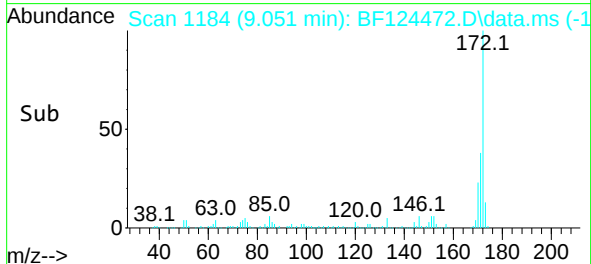

#50
Dimethylphthalate
Concen: 2.557 ng
RT: 9.728 min Scan# 1299
Delta R.T. 0.265 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52

Tgt Ion:163 Resp: 17006
Ion Ratio Lower Upper
163 100
194 0.0 3.1 4.7#
164 472.8 8.2 12.2#


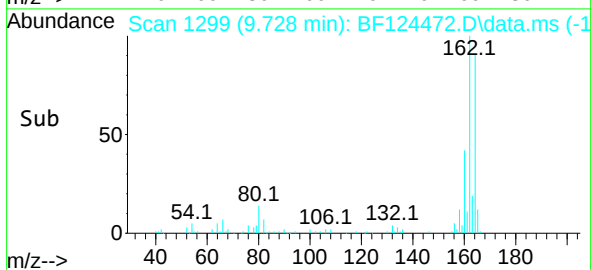

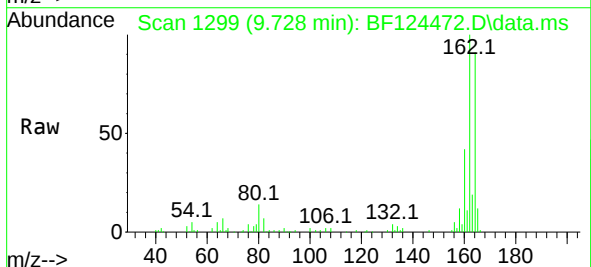




#51
2,6-Dinitrotoluene
Concen: 7.726 ng
RT: 9.722 min Scan# 1298
Delta R.T. 0.194 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52




Instrument :
BNA_F
ClientSampled :
ABN-1


Tgt Ion:165 Resp: 11869
Ion Ratio Lower Upper
165 100
63 0.0 67.7 101.5#
89 2.6 58.8 88.2#

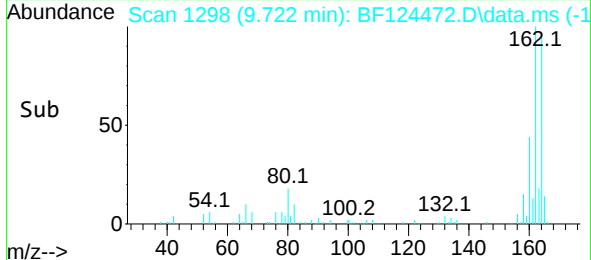

#57
2,4-Dinitrotoluene
Concen: 5.829 ng
RT: 9.722 min Scan# 1298
Delta R.T. -0.212 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52

Tgt Ion:165 Resp: 11869
Ion Ratio Lower Upper
165 100
63 0.0 43.5 65.3#
89 2.6 67.7 101.5#
182 0.0 2.1 3.1#


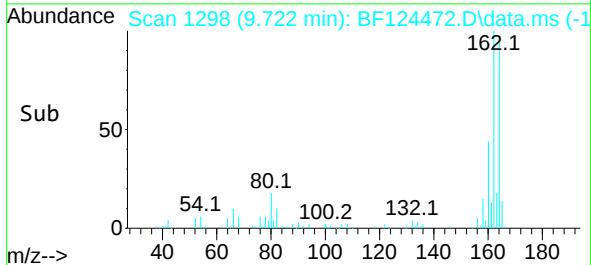

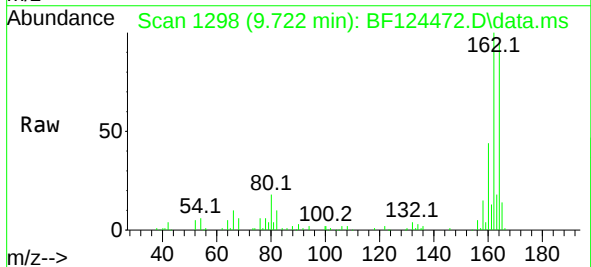


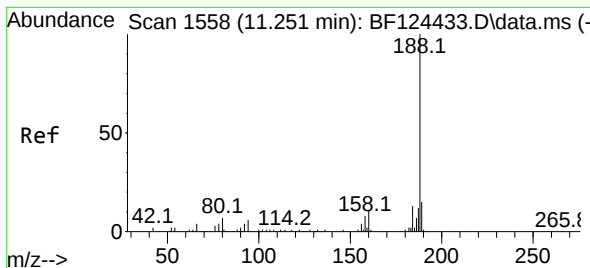

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.210 min Scan# 1551
Delta R.T. -0.006 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52




Instrument :
BNA_F
ClientSampleId :
ABN-1


Tgt Ion:188	Resp:	164795
Ion Ratio	Lower	Upper
188	100	
94	7.2	6.9 10.3
80	9.6	8.2 12.2

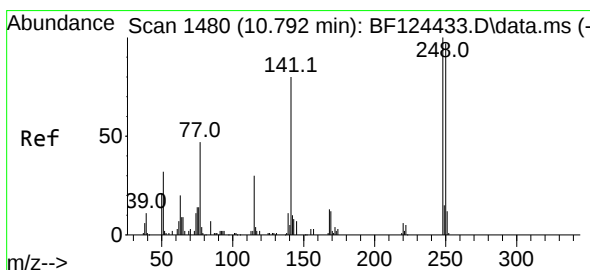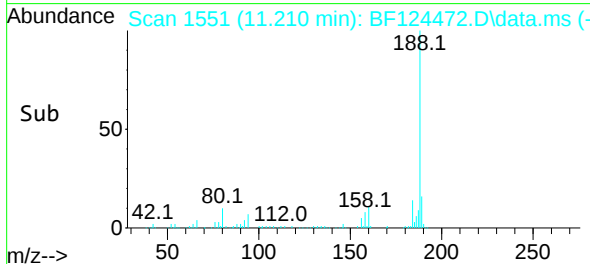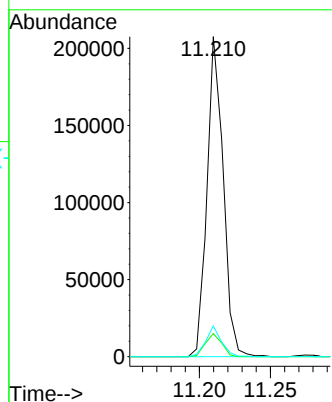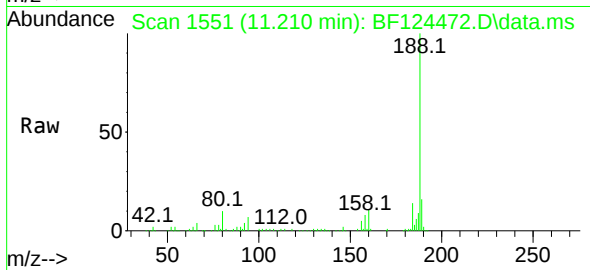

#67
4-Bromophenyl-phenylether
Concen: 4.750 ng
RT: 10.522 min Scan# 1434
Delta R.T. -0.235 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52

Tgt Ion:248	Resp:	10531
Ion Ratio	Lower	Upper
248	100	
250	206.9	77.4 116.2#
141	418.8	63.7 95.5#


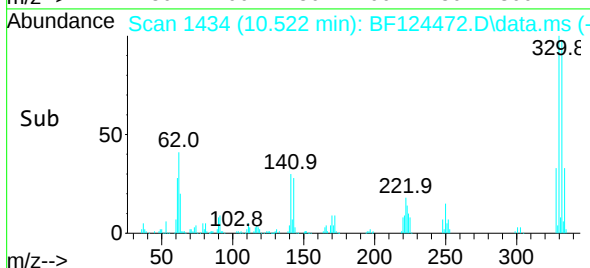

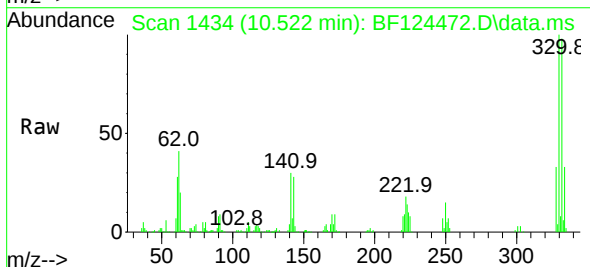


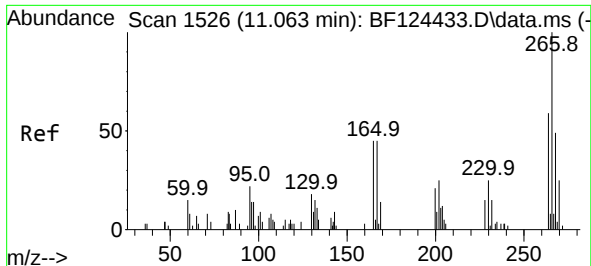

#70
 Pentachlorophenol
 Concen: 6.272 ng
 RT: 10.792 min Scan# 1480
 Delta R.T. -0.241 min
 Lab File: BF124472.D
 Acq: 28 Jun 2021 16:52




Instrument :
 BNA_F
 ClientSampled :
 ABN-1


Tgt Ion:266 Resp: 107
 Ion Ratio Lower Upper
 266 100
 268 0.0 51.6 77.4#
 264 0.0 52.6 78.8#

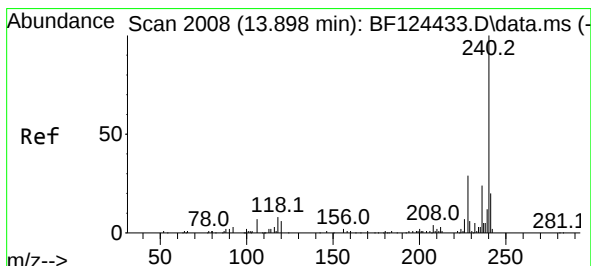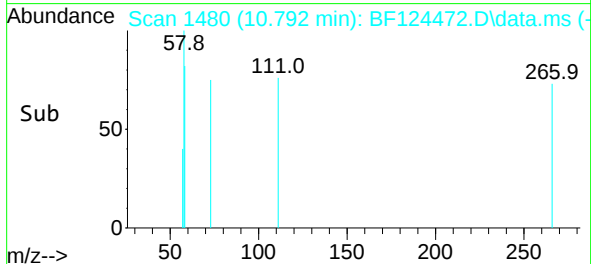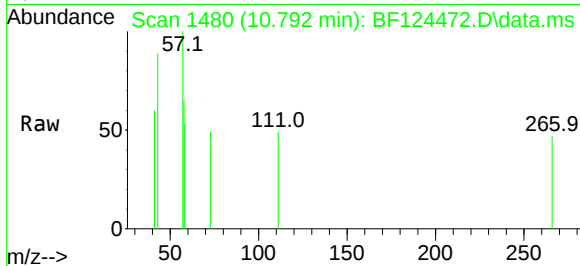

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 13.857 min Scan# 2001
 Delta R.T. -0.006 min
 Lab File: BF124472.D
 Acq: 28 Jun 2021 16:52

Tgt Ion:240 Resp: 122379
 Ion Ratio Lower Upper
 240 100
 120 7.8 7.2 10.8
 236 22.4 19.0 28.4


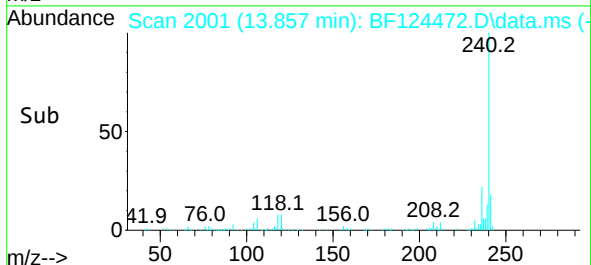

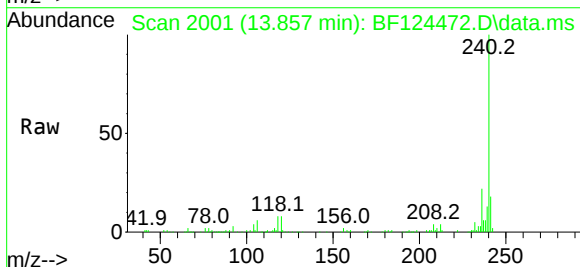




#77
Benzidine
Concen: 15.838 ng
RT: 12.551 min Scan# 1779
Delta R.T. -0.000 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52




Instrument :
BNA_F
ClientSampleId :
ABN-1


Tgt Ion:184 Resp: 38845
Ion Ratio Lower Upper
184 100
185 14.5 12.1 18.1
183 13.5 7.8 11.8#

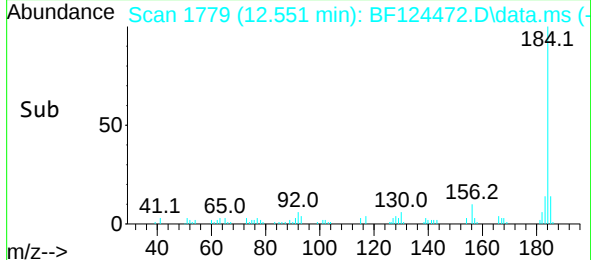

#79
Terphenyl-d14
Concen: 82.001 ng
RT: 12.804 min Scan# 1822
Delta R.T. -0.000 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52

Tgt Ion:244 Resp: 669998
Ion Ratio Lower Upper
244 100
212 7.3 5.7 8.5
122 8.3 9.7 14.5#

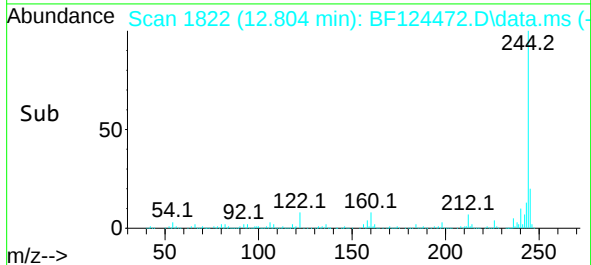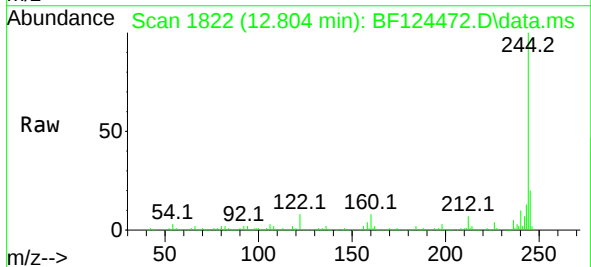

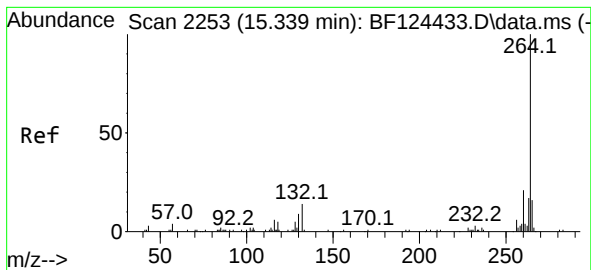

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.280 min Scan# 2243
Delta R.T. -0.006 min
Lab File: BF124472.D
Acq: 28 Jun 2021 16:52

Instrument :
BNA_F
ClientSampleId :
ABN-1

Tgt Ion:264 Resp: 81106
Ion Ratio Lower Upper
264 100
260 20.9 18.7 28.1
265 18.8 17.8 26.8

