
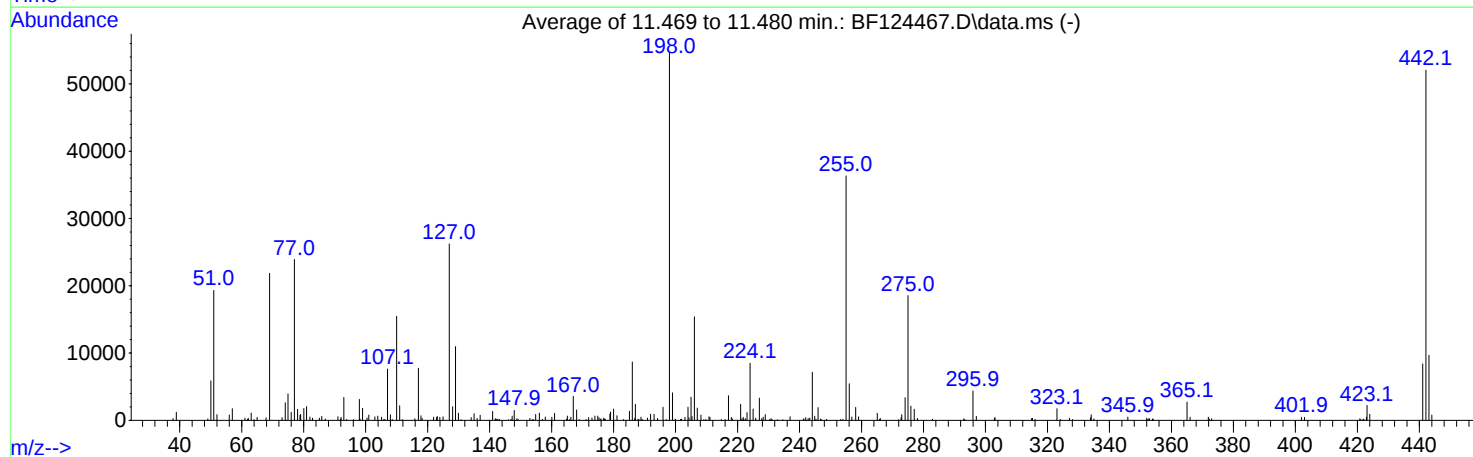


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062821\
 Data File : BF124467.D
 Acq On : 28 Jun 2021 13:17
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 28 16:01:42 2021

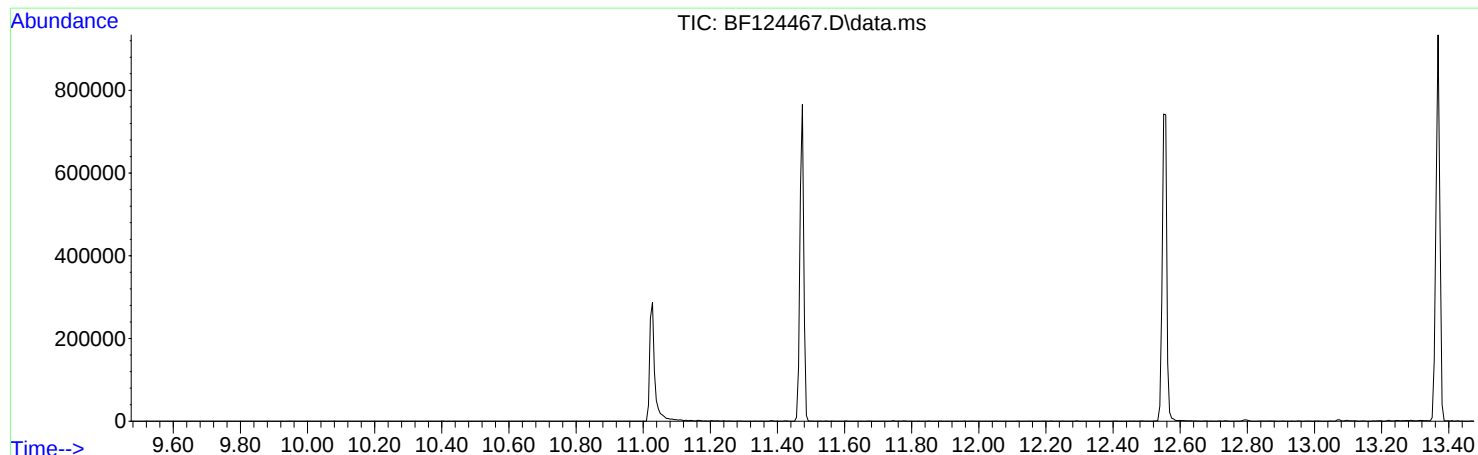




AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	19316	PASS
68	69	0.00	2	1.7	374	PASS
69	198	0.00	100	40.0	21861	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.0	26220	PASS
197	198	0.00	2	0.2	130	PASS
198	198	100	100	100.0	54669	PASS
199	198	5	9	7.5	4089	PASS
275	198	10	60	33.9	18558	PASS
365	198	1	100	5.0	2723	PASS
441	198	0.01	100	15.4	8403	PASS
442	442	50	100	100.0	52045	PASS
443	442	15	24	18.6	9688	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062821\
 Data File : BF124467.D
 Acq On : 28 Jun 2021 13:17
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 28 15:58:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 25 13:23:23 2021
 Response via : Initial Calibration

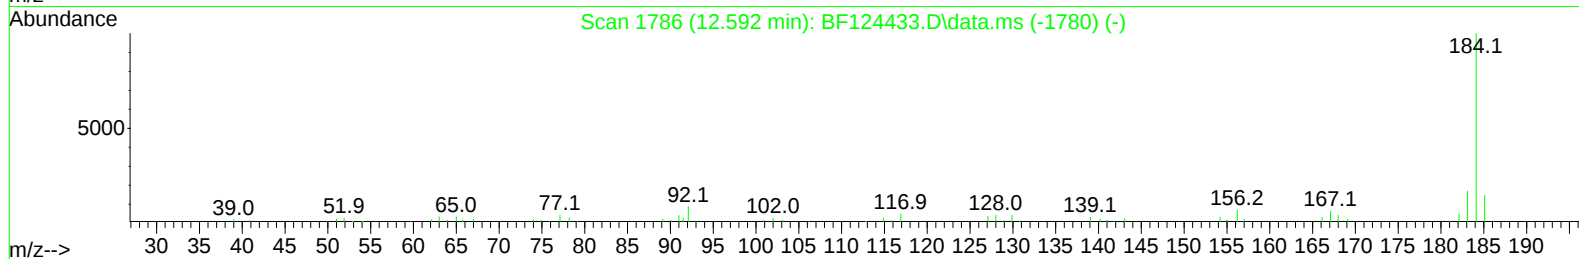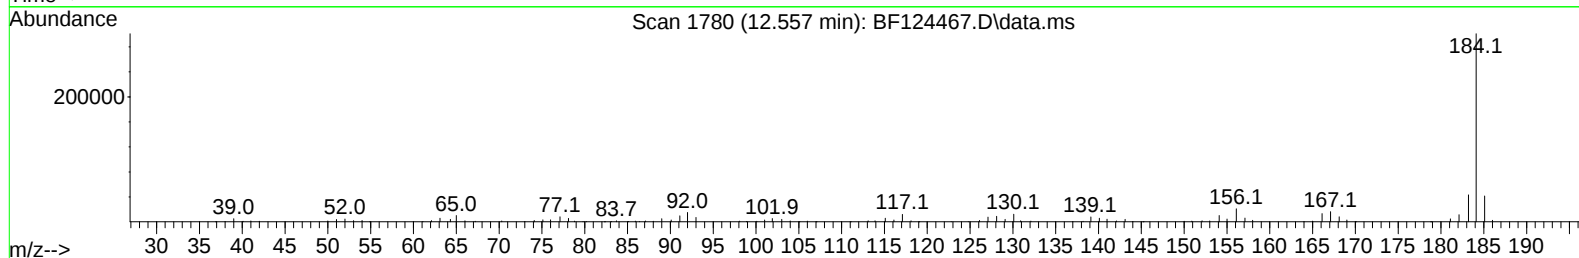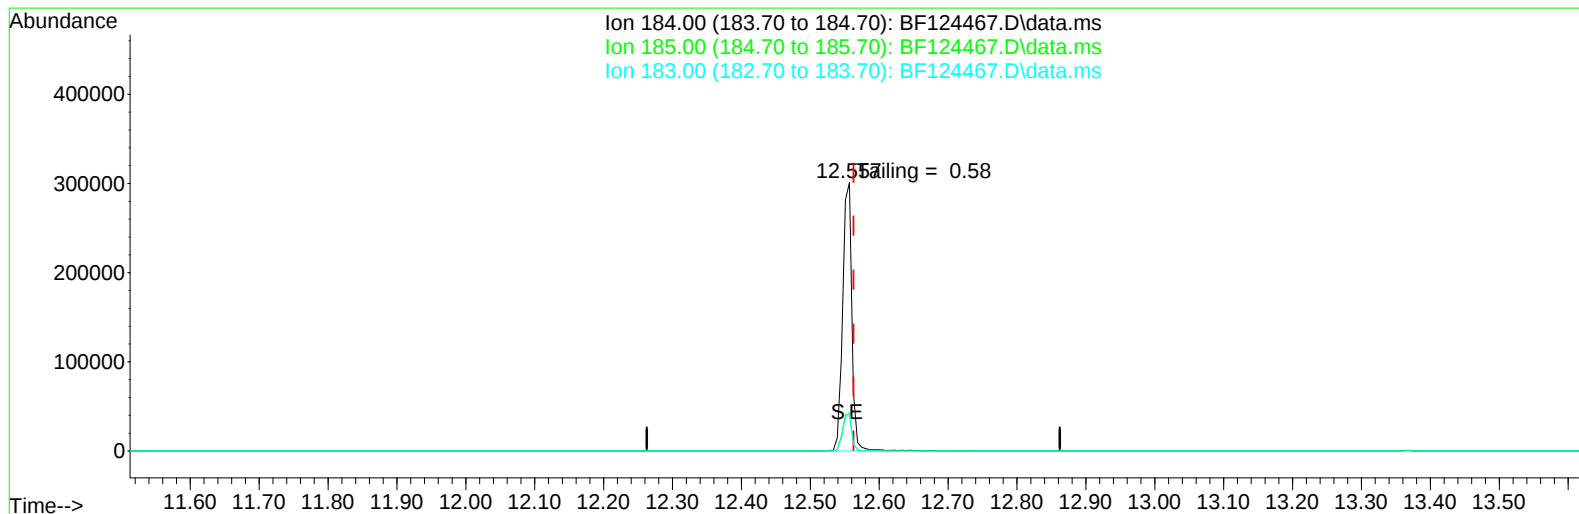

TIC: BF124467.D\data.ms

(77) Benzidine

12.557min (-0.006) 0.00 ng




response 278930

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.77
183.00	9.80	14.41#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062821\
Data File : BF124467.D
Acq On : 28 Jun 2021 13:17
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 28 15:58:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 25 13:23:23 2021
Response via : Initial Calibration

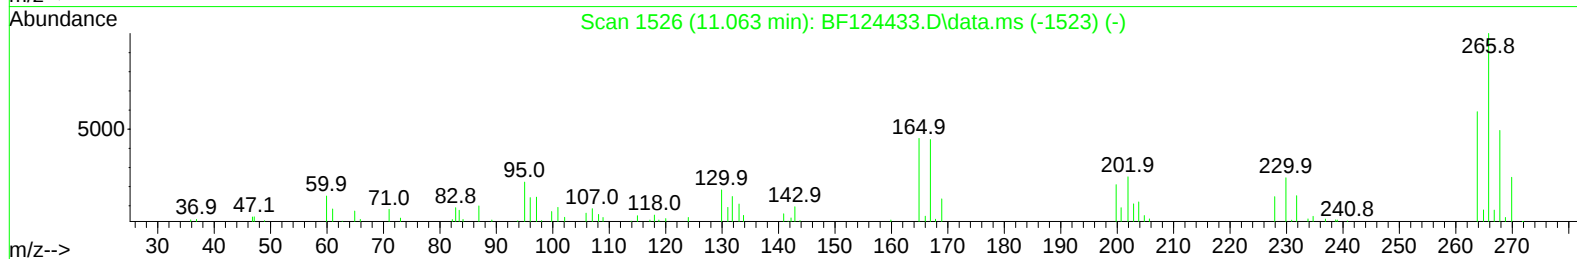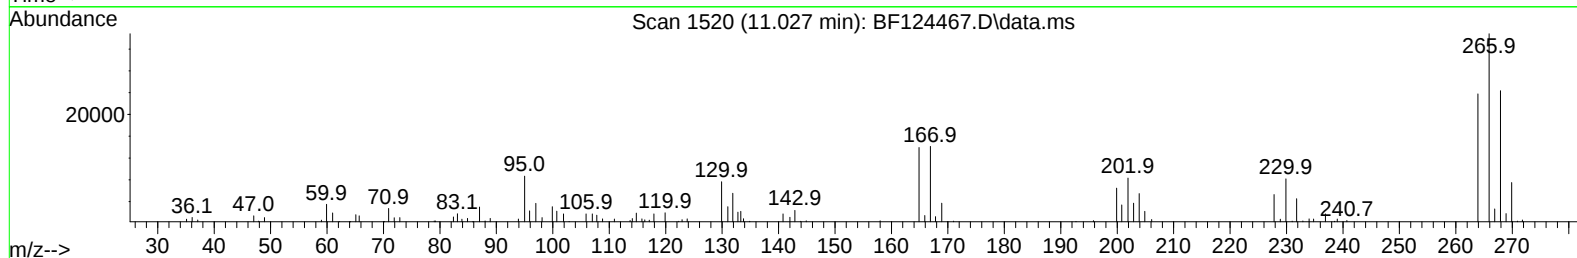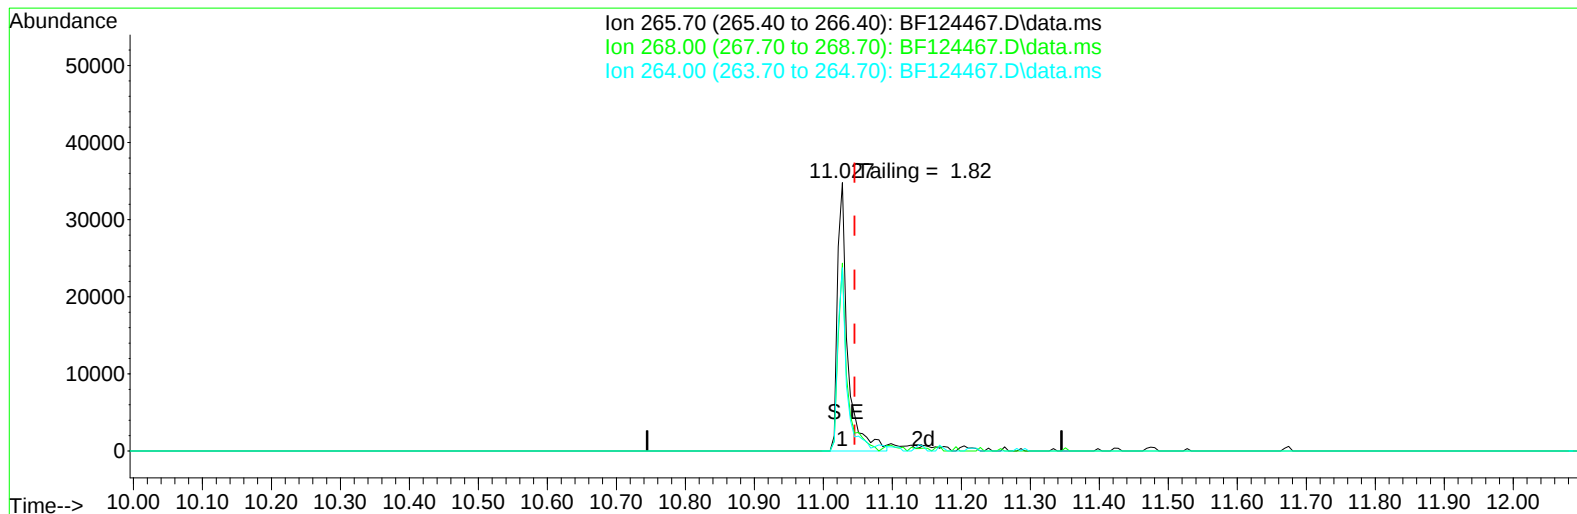

TIC: BF124467.D\data.ms

(70) Pentachlorophenol (C)

11.027min (-0.018) 28843.15 ng

response 35885

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	70.01
264.00	65.70	68.26
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
28/6/2021	BNA_F	<u>BF124467.D</u>
Compound Name	Response	Retention Time
DDT	139837	13.36
DDD	865	13.08
DDE	236	12.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1101	140938	0.78