

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062915\
 Data File : BF080217.D
 Acq On : 29 Jun 2015 20:30
 Operator : TP/IZ
 Sample : G2829-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-8

Quant Time: Jun 30 01:46:52 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 23 00:53:56 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.29	152	29699	20.00	ng	-0.03
21) Naphthalene-d8	8.58	136	112874	20.00	ng	-0.03
38) Acenaphthene-d10	10.36	164	58128	20.00	ng	-0.03
63) Phenanthrene-d10	11.86	188	115428	20.00	ng	-0.05
75) Chrysene-d12	14.89	240	127935	20.00	ng	-0.10
86) Perylene-d12	16.80	264	128093	20.00	ng	-0.13
System Monitoring Compounds						
5) 2-Fluorophenol	5.90	112	102908	61.34	ng	-0.03
7) Phenol-d6	6.89	99	80932	36.25	ng	-0.03
23) Nitrobenzene-d5	7.85	82	204759	105.61	ng	-0.02
41) 2,4,6-Tribromophenol	11.16	330	85947	151.21	ng	-0.02
44) 2-Fluorobiphenyl	9.66	172	392909	96.40	ng	-0.03
78) Terphenyl-d14	13.59	244	479818	87.59	ng	-0.08
Target Compounds						
9) Benzaldehyde	7.06	77	4350	3.38	ng	# 68
19) n-Nitroso-di-n-propylamine	7.85	70	26422	17.05	ng	# 58
25) Isophorone	7.85	82	204753	52.47	ng	# 58
49) Dimethylphthalate	10.05	163	9965	2.28	ng	# 98
50) 2,6-Dinitrotoluene	10.36	165	7717	8.81	ng	# 37
56) 2,4-Dinitrotoluene	10.36	165	7718	6.94	ng	# 31
66) 4-Bromophenyl-phenylether	11.16	248	5993	4.88	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062915\
Data File : BF080217.D
Acq On : 29 Jun 2015 20:30
Operator : TP/IZ
Sample : G2829-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-8

Quant Time: Jun 30 01:46:52 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 23 00:53:56 2015
Response via : Initial Calibration

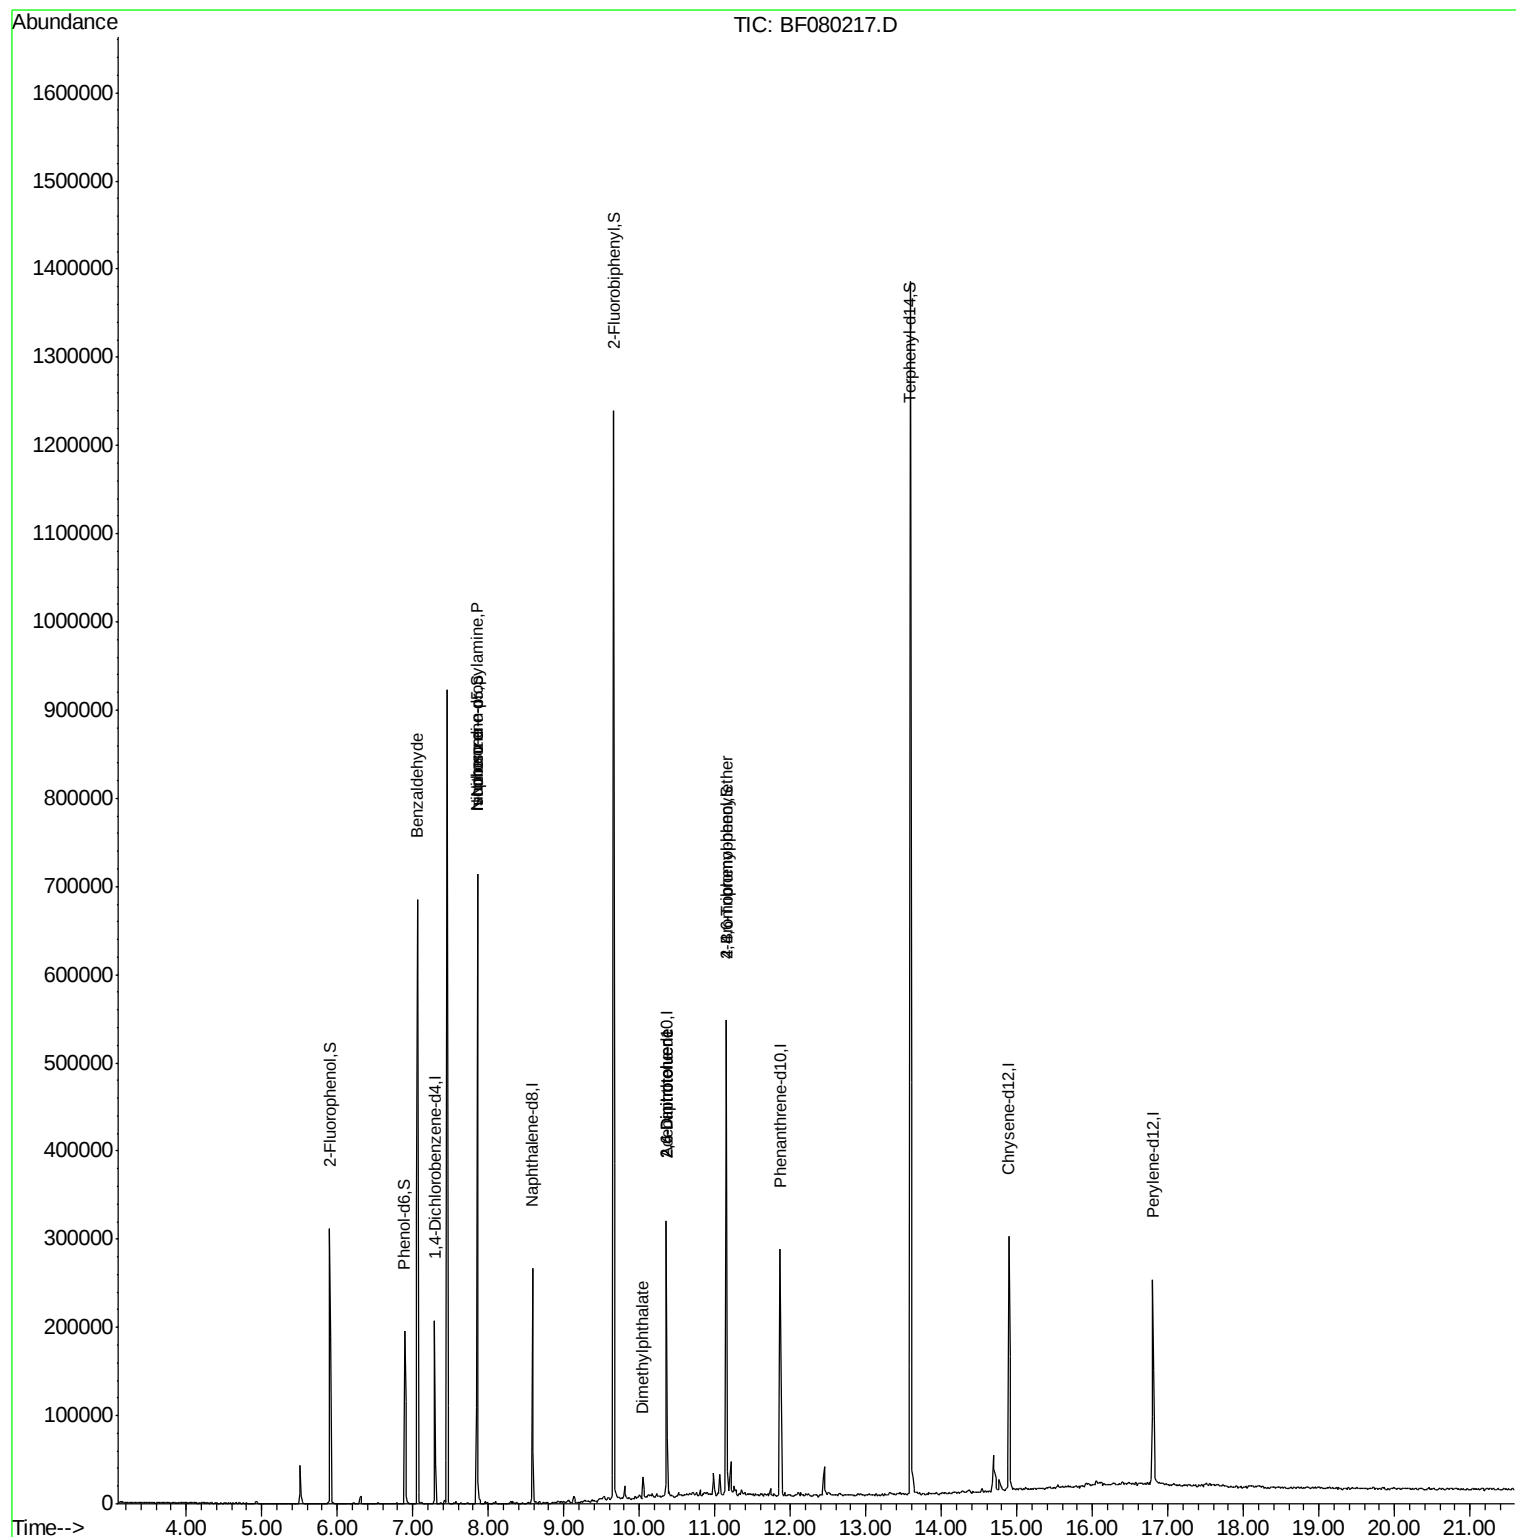



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.29 min Scan# 368

Delta R.T. -0.03 min

Lab File: BF080217.D

Acq: 29 Jun 2015 20:30

Instrument :

BNA_F

ClientSampleId :

MW-8


Tgt Ion:152 Resp: 29699

Ion Ratio Lower Upper

152 100

150 153.6 124.7 187.1




115 60.9 39.0 58.4#



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

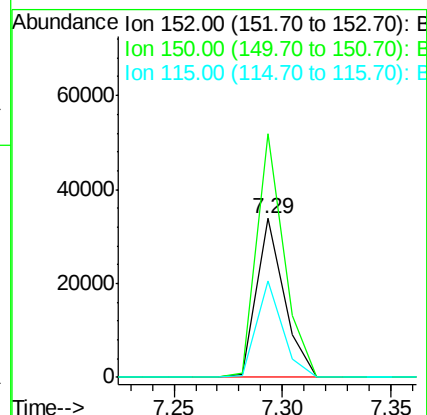

#5

2-Fluorophenol

Concen: 61.34 ng

RT: 5.90 min Scan# 246

Delta R.T. -0.03 min

Lab File: BF080217.D

Acq: 29 Jun 2015 20:30


Tgt Ion:112 Resp: 102908

Ion Ratio Lower Upper

112 100

64 71.6 39.7 59.5#



63 36.3 17.4 26.0#



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

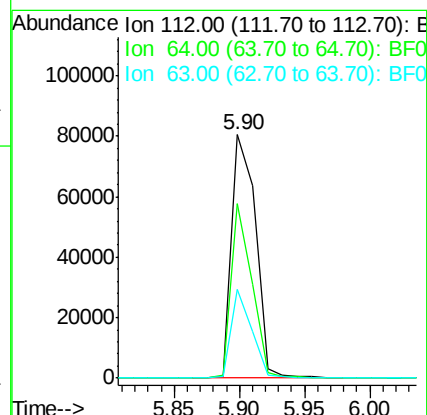



#7

Phenol-d6

Concen: 36.25 ng

RT: 6.89 min Scan# 333

Delta R.T. -0.03 min

Lab File: BF080217.D

Acq: 29 Jun 2015 20:30

Instrument :

BNA_F

ClientSampleId :

MW-8


Tgt Ion: 99 Resp: 80932

Ion Ratio Lower Upper

99 100

42 22.4 13.7 20.5#




71 35.2 14.2 21.2#

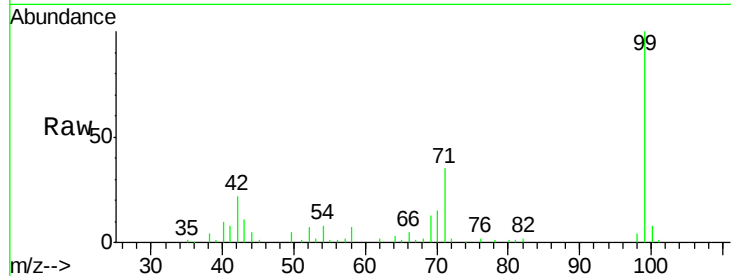

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

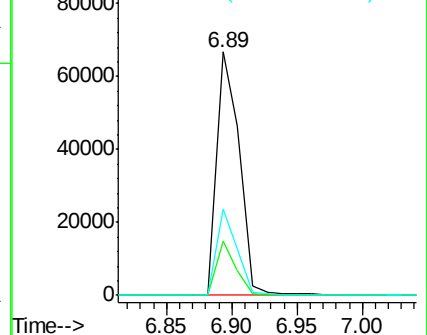

#9

Benzaldehyde

Concen: 3.38 ng

RT: 7.06 min Scan# 348

Delta R.T. 0.19 min

Lab File: BF080217.D

Acq: 29 Jun 2015 20:30


Tgt Ion: 77 Resp: 4350

Ion Ratio Lower Upper

77 100

105 86.4 91.6 131.6#



106 78.5 102.6 142.6#




Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E




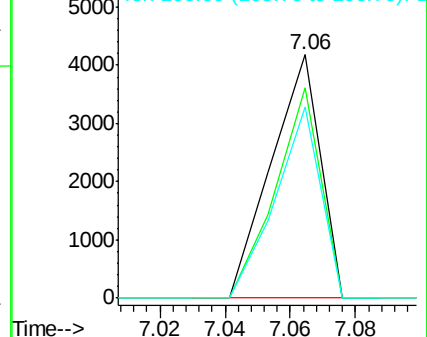




#19
n-Nitroso-di-n-propylamine
Concen: 17.05 ng
RT: 7.85 min Scan# 417
Delta R.T. 0.14 min
Lab File: BF080217.D
Acq: 29 Jun 2015 20:30




Instrument :
BNA_F
ClientSampled :
MW-8


Tgt Ion: 70 Resp: 26422
Ion Ratio Lower Upper
70 100
42 46.0 63.8 95.6#
101 0.0 9.2 13.8#
130 1.8 27.3 40.9#

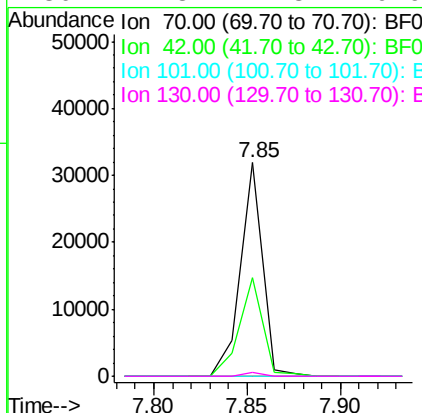

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.58 min Scan# 481
Delta R.T. -0.03 min
Lab File: BF080217.D
Acq: 29 Jun 2015 20:30

Tgt Ion: 136 Resp: 112874
Ion Ratio Lower Upper
136 100
137 11.1 9.0 13.6
54 9.8 8.2 12.2
68 7.3 5.8 8.6



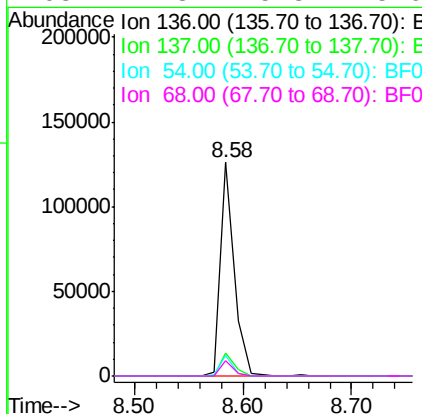





#23
 Nitrobenzene-d5
 Concen: 105.61 ng
 RT: 7.85 min Scan# 417
 Delta R.T. -0.02 min
 Lab File: BF080217.D
 Acq: 29 Jun 2015 20:30




Instrument :
 BNA_F
 ClientSampleId :
 MW-8


Tgt Ion: 82 Resp: 204759
 Ion Ratio Lower Upper
 82 100
 128 44.2 51.0 76.6#
 54 49.0 47.5 71.3

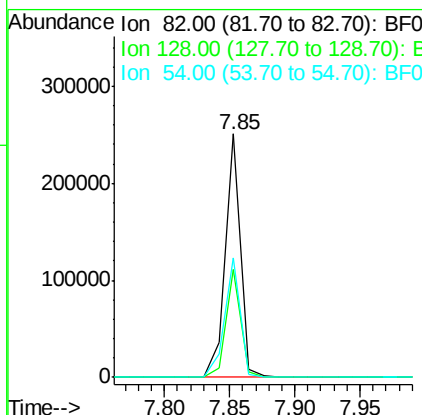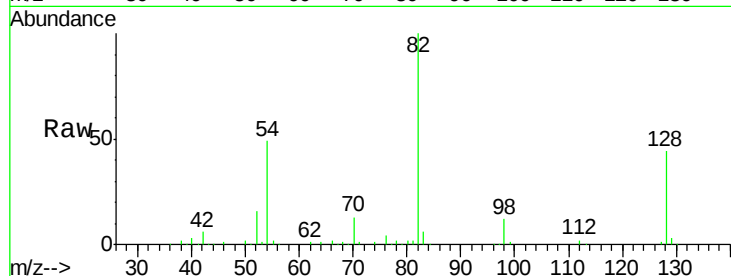

#25
 Isophorone
 Concen: 52.47 ng
 RT: 7.85 min Scan# 417
 Delta R.T. -0.29 min
 Lab File: BF080217.D
 Acq: 29 Jun 2015 20:30

Tgt Ion: 82 Resp: 204753
 Ion Ratio Lower Upper
 82 100
 95 0.0 4.0 6.0#
 138 0.0 18.3 27.5#

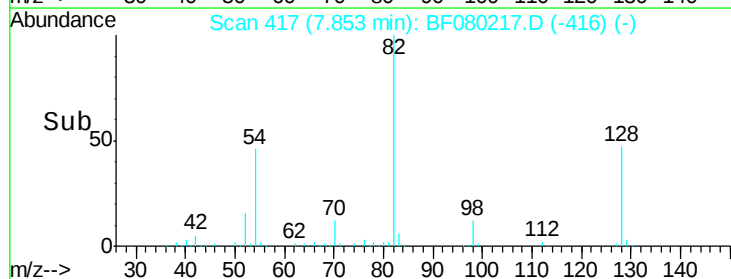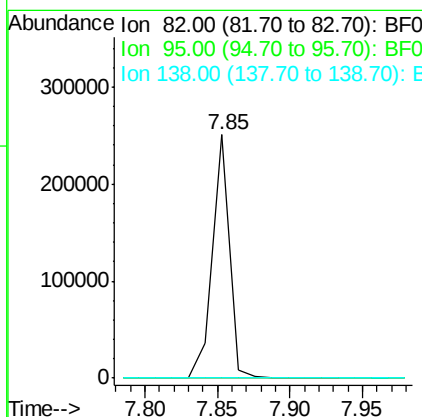


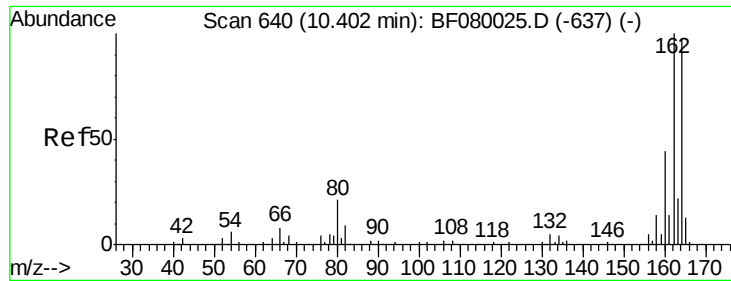




#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.36 min Scan# 636
 Delta R.T. -0.03 min
 Lab File: BF080217.D
 Acq: 29 Jun 2015 20:30

Instrument :
 BNA_F
 ClientSampleID :
 MW-8

Tgt Ion:164 Resp: 58128
 Ion Ratio Lower Upper
 164 100
 162 103.1 75.2 112.8
 160 44.8 31.5 47.3

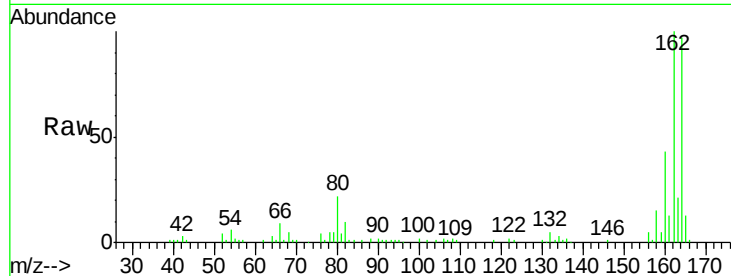


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E


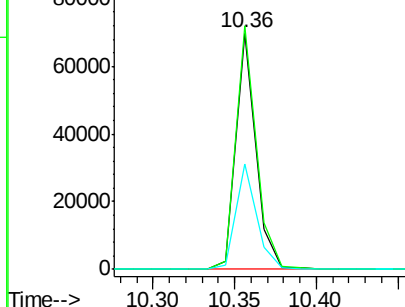



#41
 2,4,6-Tribromophenol
 Concen: 151.21 ng
 RT: 11.16 min Scan# 706
 Delta R.T. -0.02 min
 Lab File: BF080217.D
 Acq: 29 Jun 2015 20:30

Tgt Ion:330 Resp: 85947
 Ion Ratio Lower Upper
 330 100
 332 95.3 76.6 114.8
 141 35.1 29.7 44.5



Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E



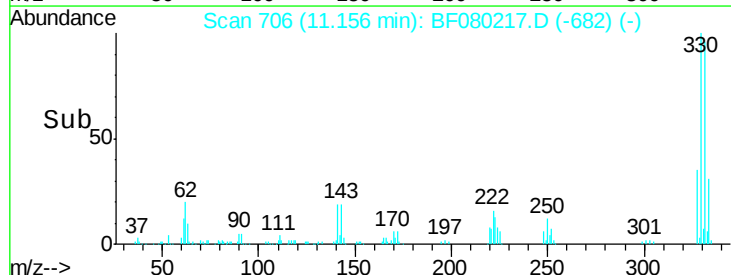
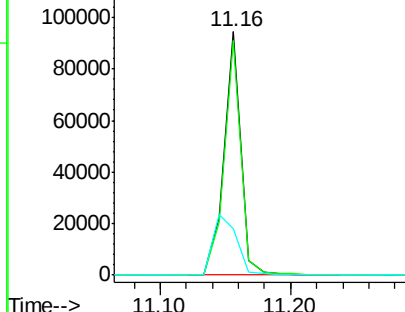


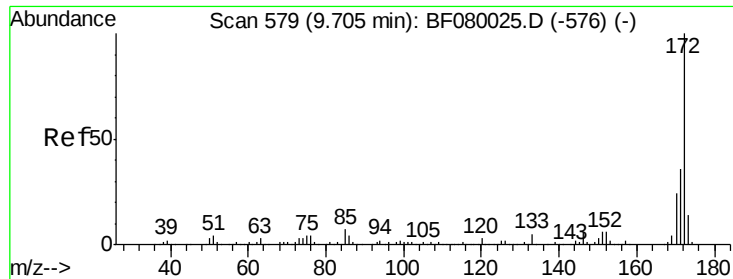

#44
 2-Fluorobiphenyl
 Concen: 96.40 ng
 RT: 9.66 min Scan# 575
 Delta R.T. -0.03 min
 Lab File: BF080217.D
 Acq: 29 Jun 2015 20:30




Instrument :
 BNA_F
 ClientSampled :
 MW-8


Tgt Ion:172 Resp: 392909
 Ion Ratio Lower Upper
 172 100
 171 35.5 26.1 39.1
 170 24.2 17.4 26.2

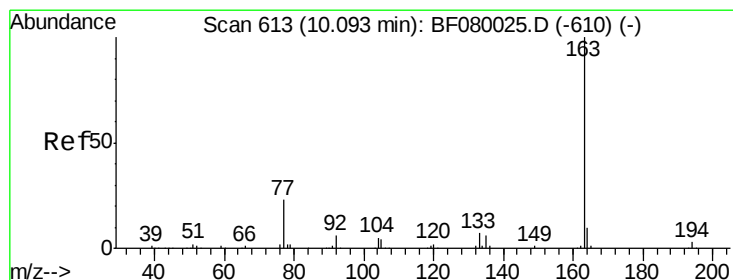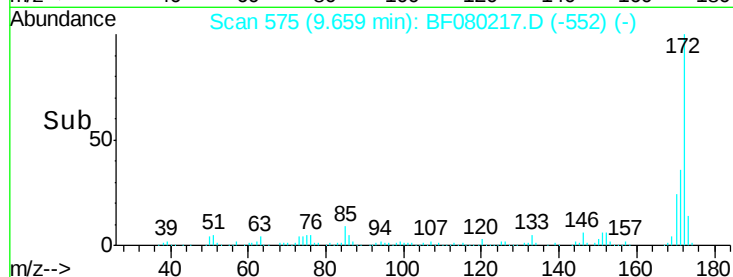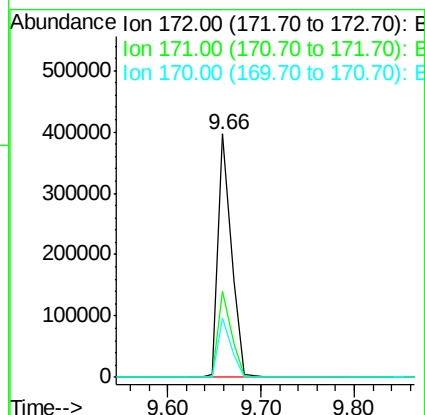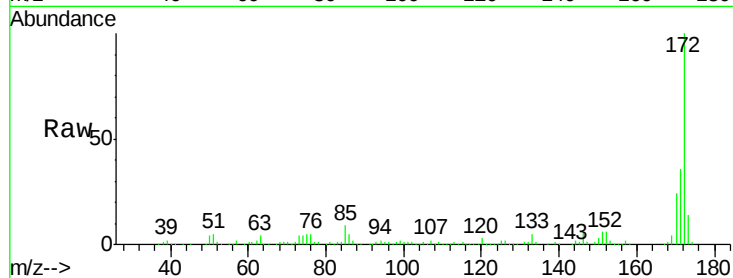

#49
 Dimethylphthalate
 Concen: 2.28 ng
 RT: 10.05 min Scan# 609
 Delta R.T. -0.03 min
 Lab File: BF080217.D
 Acq: 29 Jun 2015 20:30

Tgt Ion:163 Resp: 9965
 Ion Ratio Lower Upper
 163 100
 194 3.3 4.4 6.6#
 164 10.5 8.3 12.5

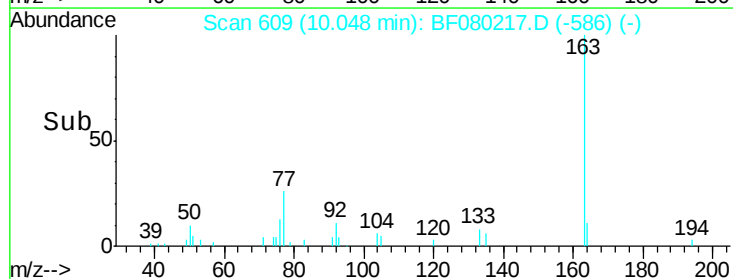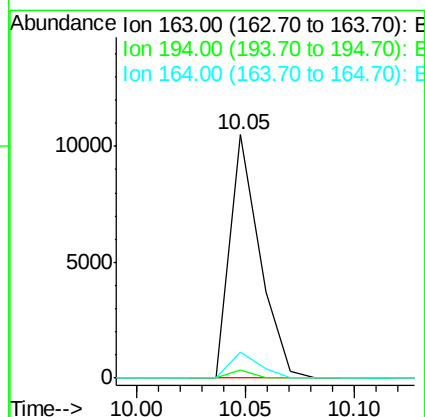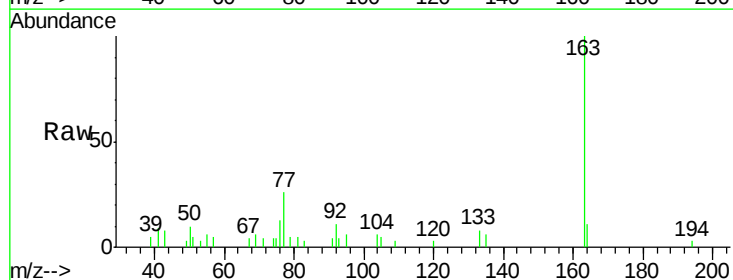


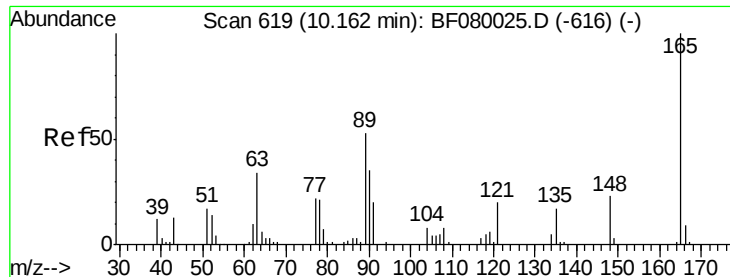




#50
 2,6-Dinitrotoluene
 Concen: 8.81 ng
 RT: 10.36 min Scan# 636
 Delta R.T. 0.21 min
 Lab File: BF080217.D
 Acq: 29 Jun 2015 20:30

Instrument :
 BNA_F
 ClientSampleId :
 MW-8

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	32.3	48.5#
89	0.0	28.6	43.0#

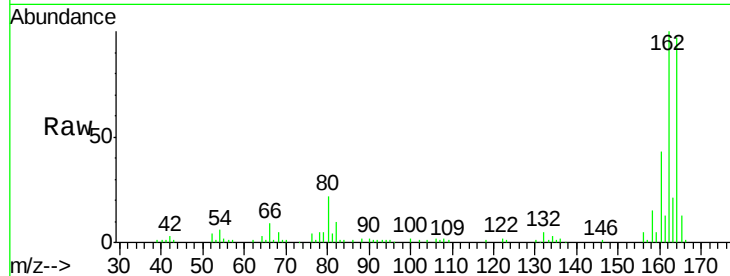




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0

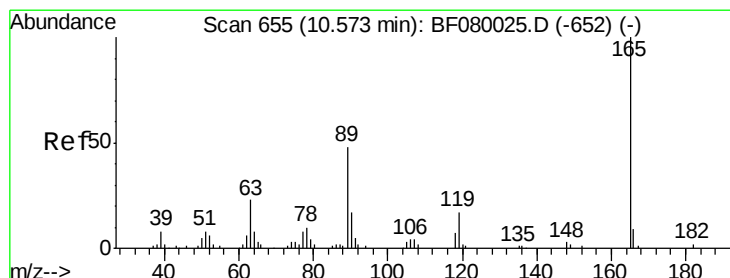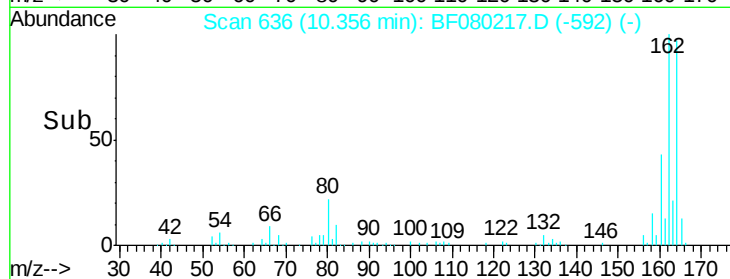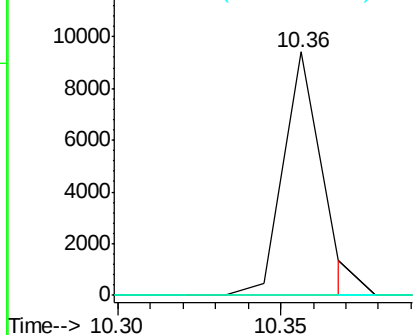


#56
 2,4-Dinitrotoluene
 Concen: 6.94 ng
 RT: 10.36 min Scan# 636
 Delta R.T. -0.19 min
 Lab File: BF080217.D
 Acq: 29 Jun 2015 20:30

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	29.8	44.6#
89	0.0	44.5	66.7#
182	0.0	3.0	4.4#

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0
 Ion 182.00 (181.70 to 182.70): E

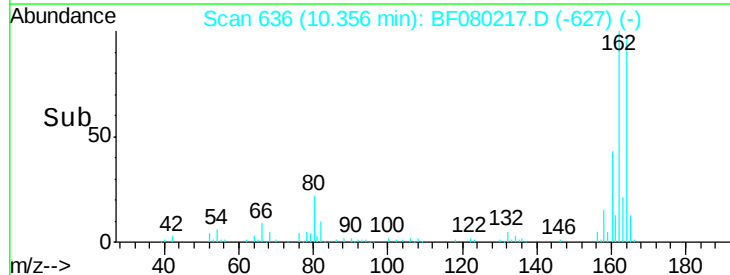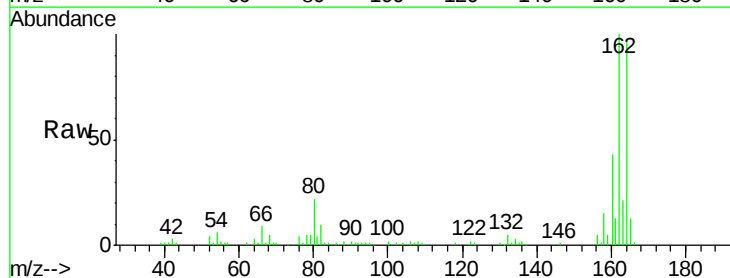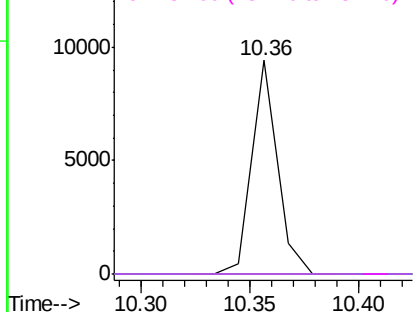


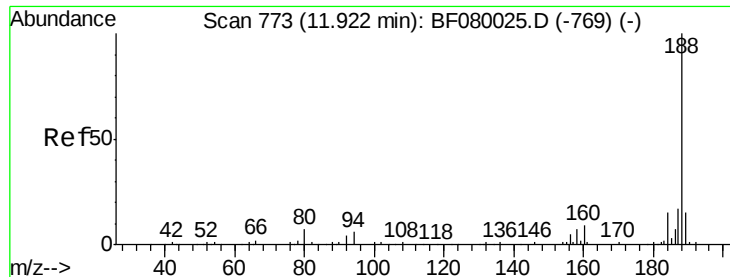




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.86 min Scan# 768
 Delta R.T. -0.05 min
 Lab File: BF080217.D
 Acq: 29 Jun 2015 20:30

Instrument :
 BNA_F
 ClientSampleId :
 MW-8

Tgt Ion:188 Resp: 115428
 Ion Ratio Lower Upper
 188 100
 94 12.1 11.1 16.7
 80 13.2 11.0 16.4

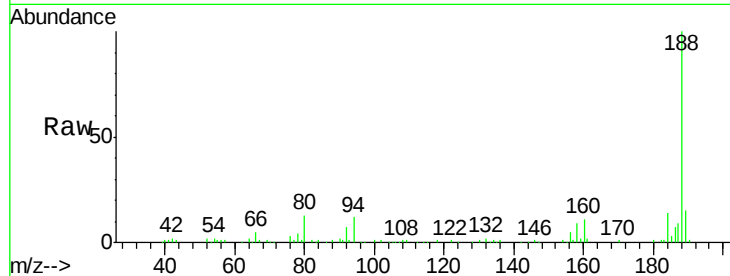


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

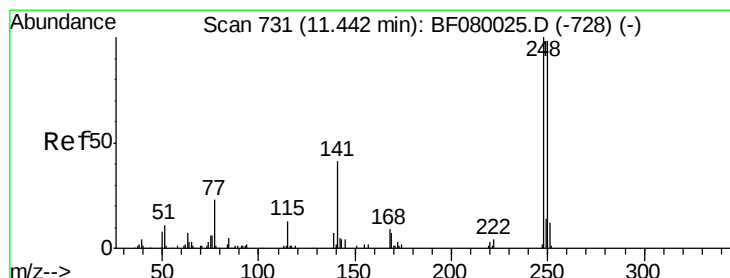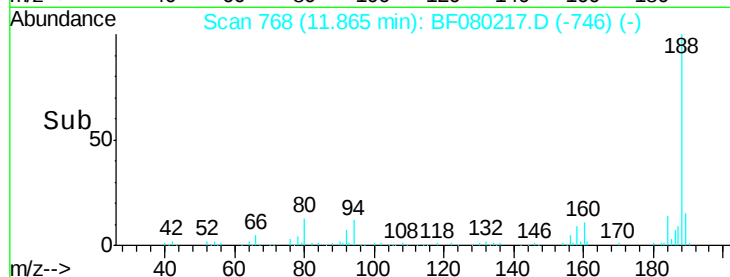
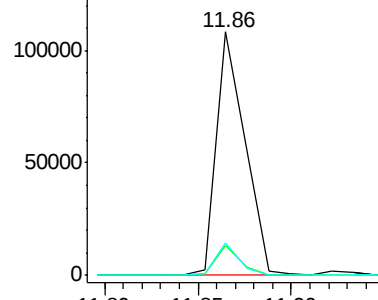



#66
 4-Bromophenyl-phenylether
 Concen: 4.88 ng
 RT: 11.16 min Scan# 706
 Delta R.T. -0.26 min
 Lab File: BF080217.D
 Acq: 29 Jun 2015 20:30

Tgt Ion:248 Resp: 5993
 Ion Ratio Lower Upper
 248 100
 250 187.0 78.5 117.7#
 141 297.5 59.0 88.6#

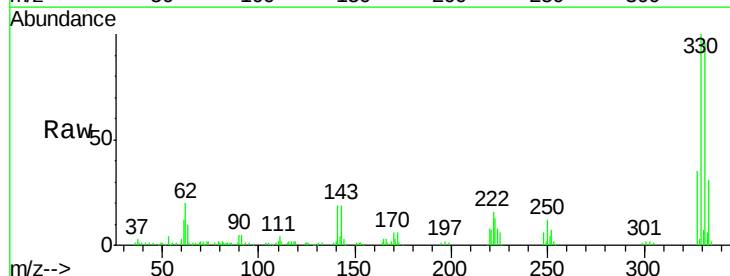

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

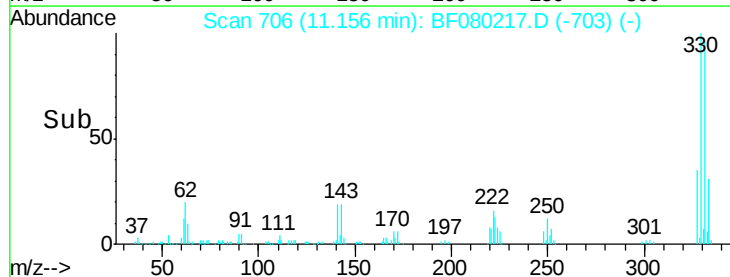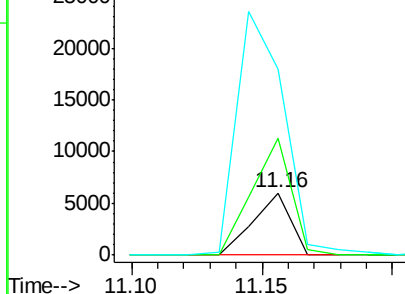



#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.89 min Scan# 1033

Delta R.T. -0.10 min

Lab File: BF080217.D

Acq: 29 Jun 2015 20:30

Instrument :

BNA_F

ClientSampleId :

MW-8


Tgt Ion:240 Resp: 127935

Ion Ratio Lower Upper

240 100

120 12.6 16.2 24.2#




236 25.4 18.4 27.6



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

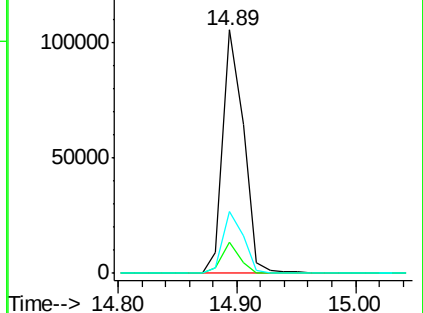

#78

Terphenyl-d14

Concen: 87.59 ng

RT: 13.59 min Scan# 919

Delta R.T. -0.08 min

Lab File: BF080217.D

Acq: 29 Jun 2015 20:30


Tgt Ion:244 Resp: 479818

Ion Ratio Lower Upper

244 100

212 7.5 4.3 6.5#



122 13.5 17.4 26.2#






Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

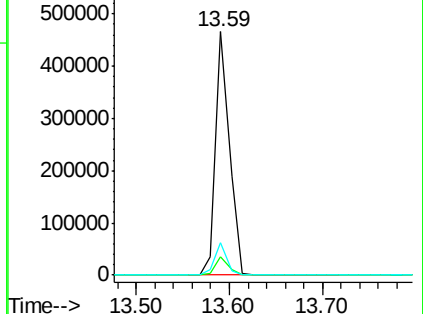

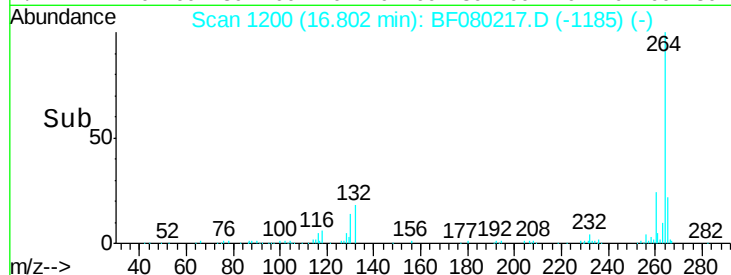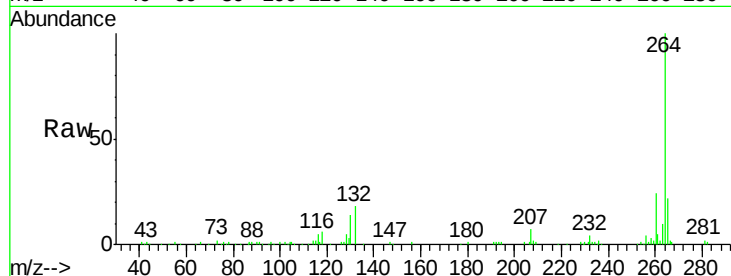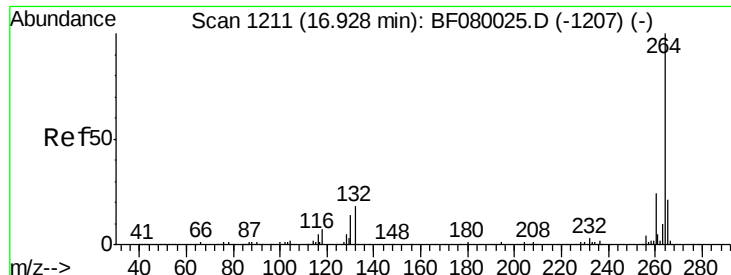

#86
Perylene-d12
Concen: 20.00 ng
RT: 16.80 min Scan# 1200
Delta R.T. -0.13 min
Lab File: BF080217.D
Acq: 29 Jun 2015 20:30

Instrument :
BNA_F
ClientSampleId :
MW-8

Tgt Ion:	264	Resp:	128093
Ion	Ratio	Lower	Upper
264	100		
260	23.8	16.7	25.1
265	21.6	17.2	25.8

