
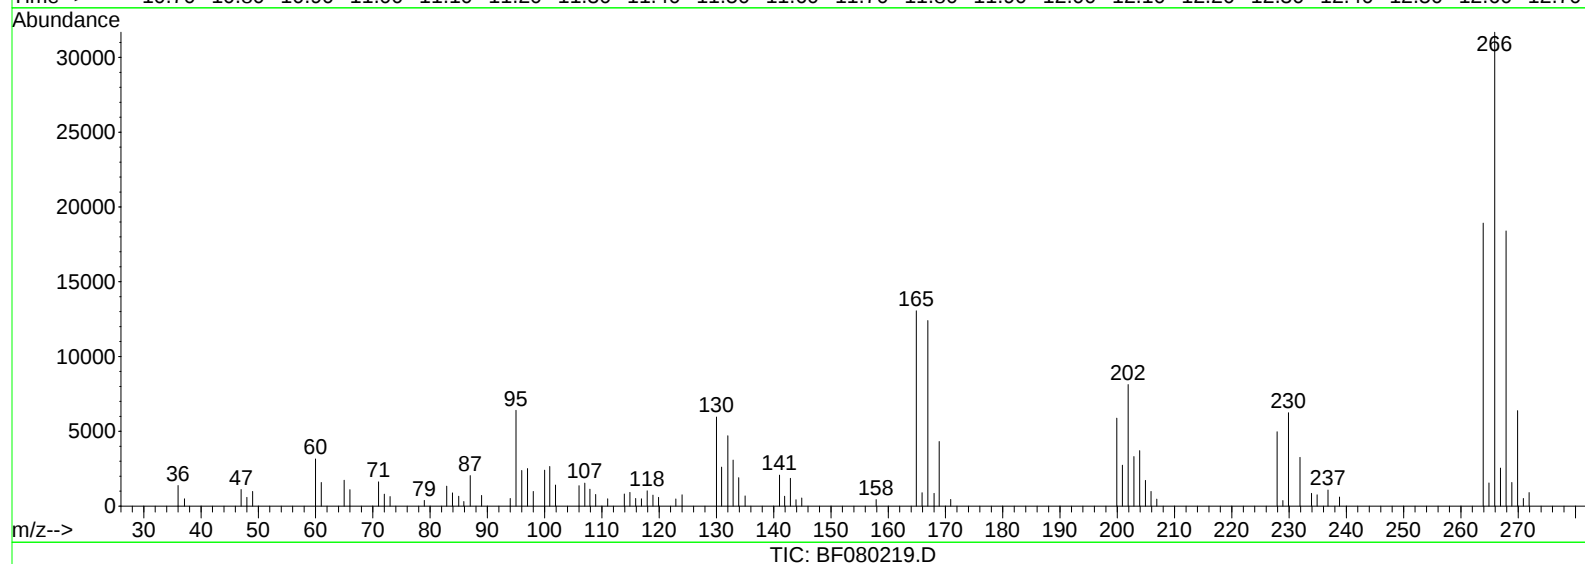


Data Path : Z:\HPCHEM1\BNA F\Data\BF062915\  
Data File : BF080219.D  
Acq On : 29 Jun 2015 22:53  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 06:44:59 2015  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jun 23 00:53:56 2015  
Response via : Initial Calibration

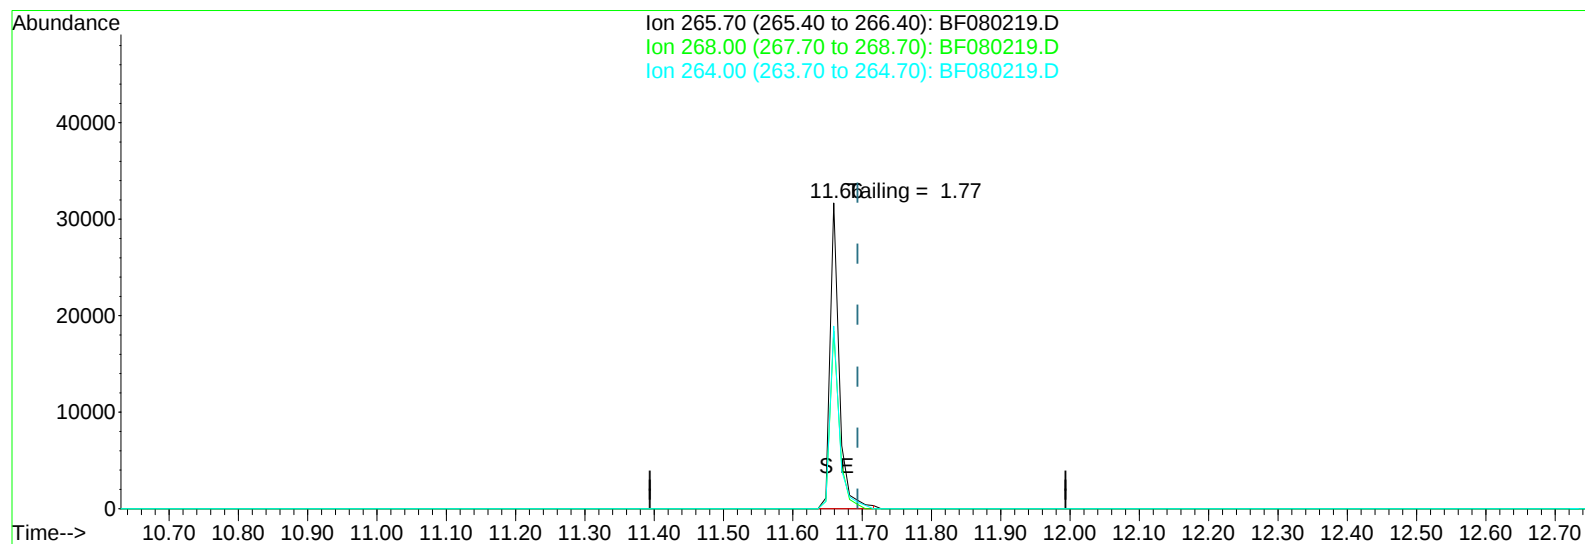

(69) Pentachlorophenol (C)



11.659min (-0.034) 0.00ng

response 29039

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 62.20 | 58.04 |
| 264.00 | 62.70 | 59.71 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA F\Data\BF062915\  
Data File : BF080219.D  
Acq On : 29 Jun 2015 22:53  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 06:44:59 2015  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jun 23 00:53:56 2015  
Response via : Initial Calibration

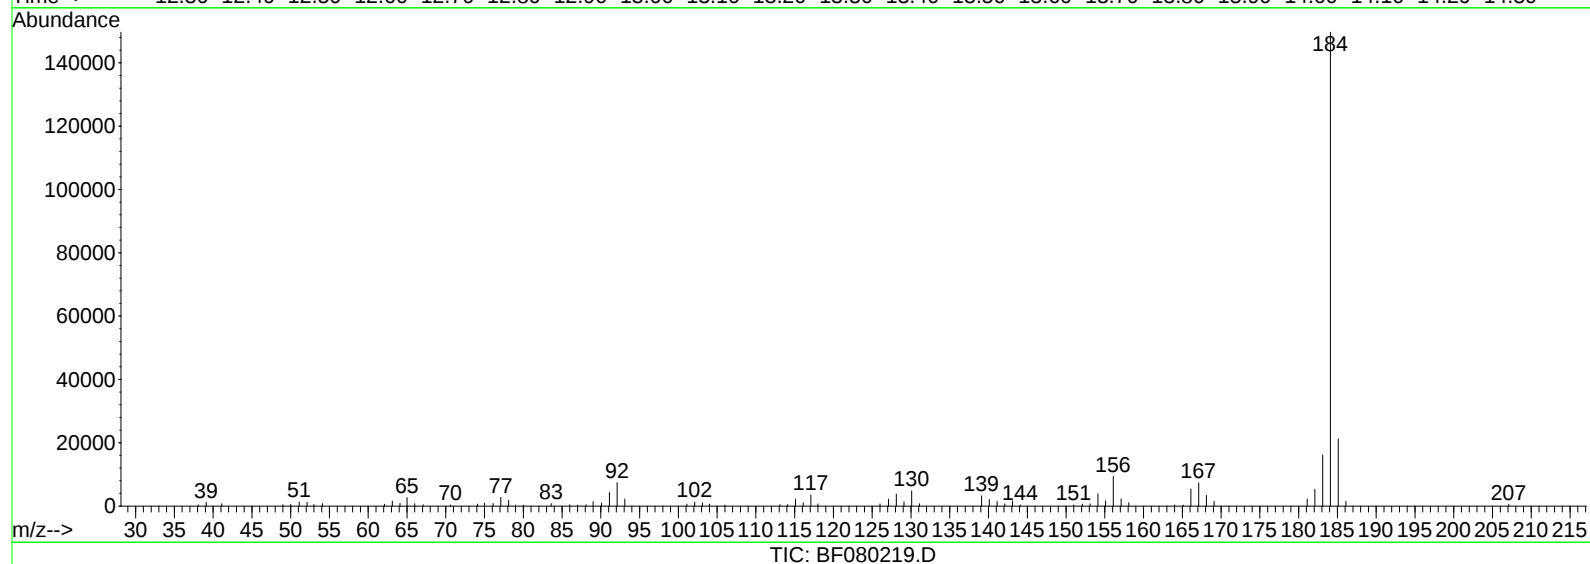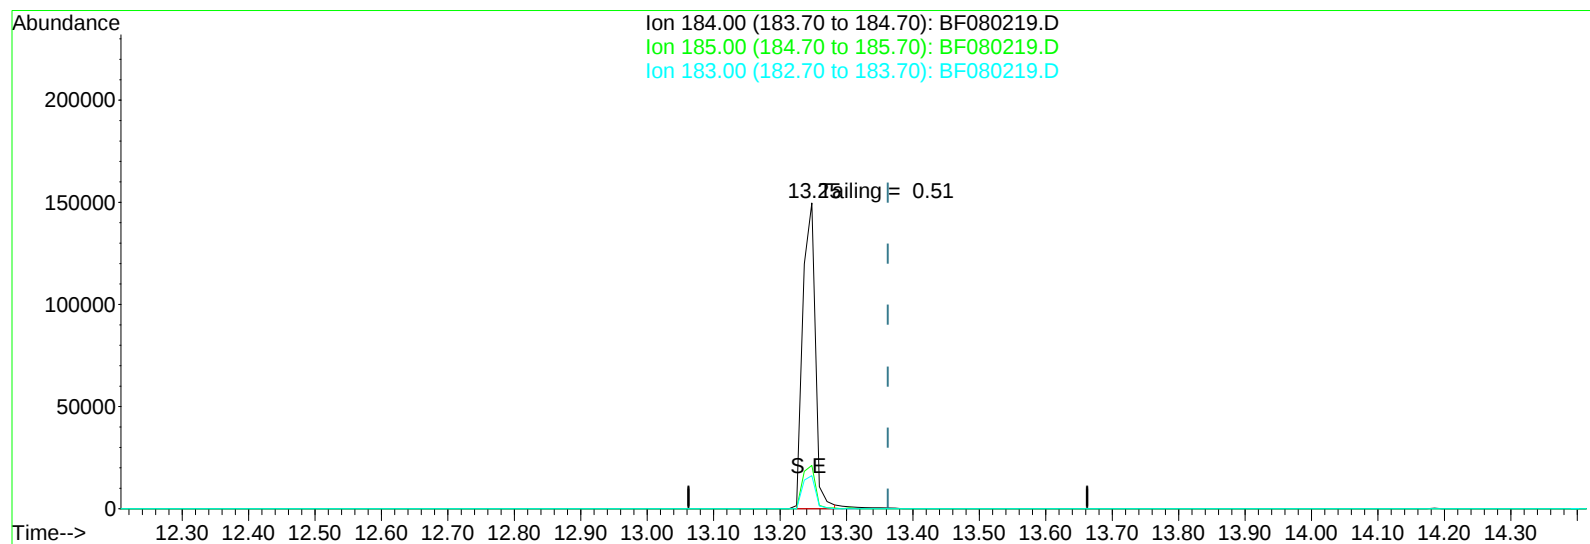

(76) Benzidine

13.248min (-0.114) 0.00ng

response 200300

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.70 | 14.15 |
| 183.00 | 9.50  | 10.80 |
| 0.00   | 0.00  | 0.00  |