


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062915\
 Data File : BF080203.D
 Acq On : 29 Jun 2015 11:28
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 23 00:53:56 2015

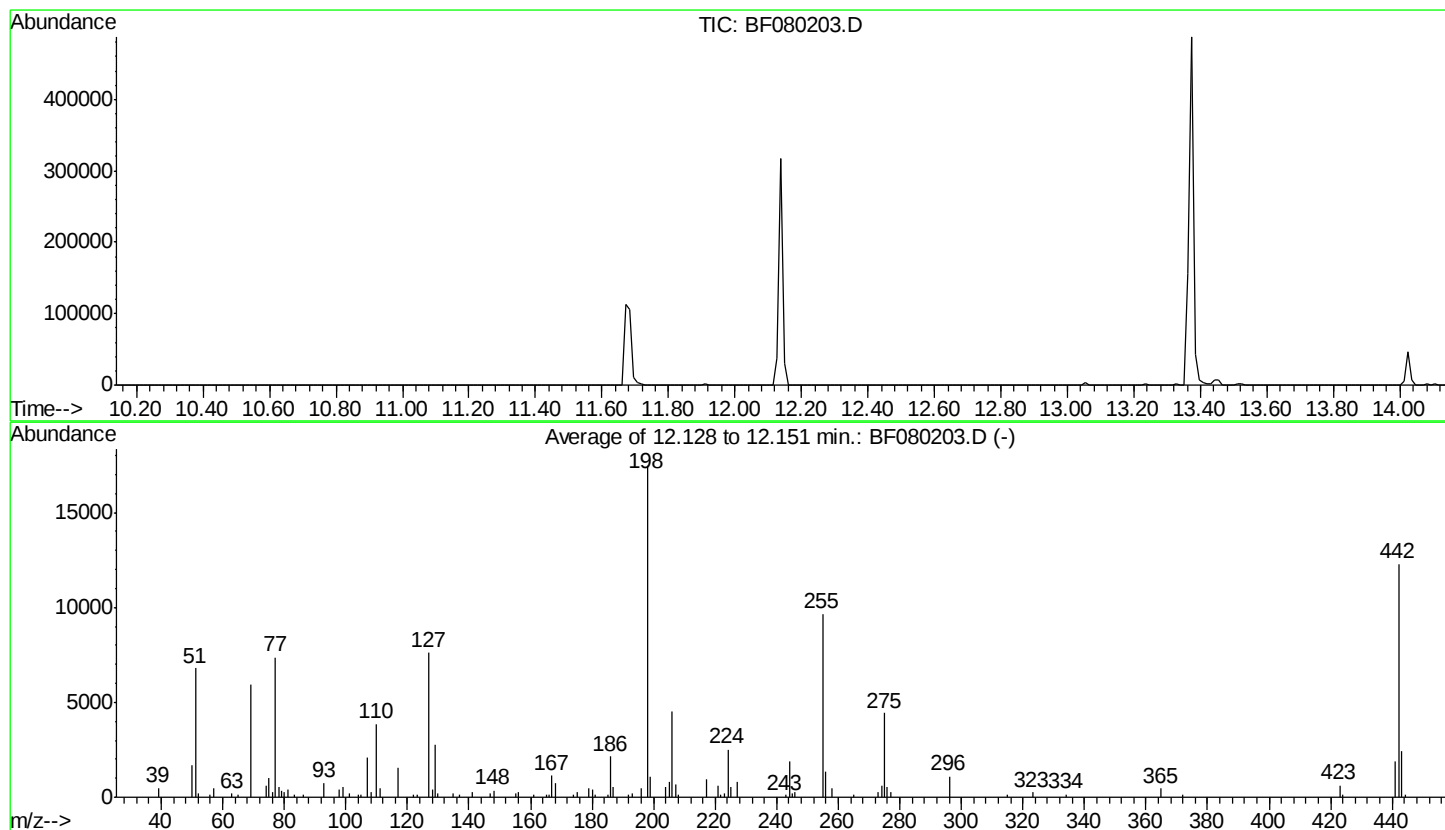

AutoFind: Scans 791, 792, 793; Background Corrected with Scan 788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	6804	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.9	5926	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.6	7615	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17475	PASS
199	198	5	9	6.0	1051	PASS
275	198	10	60	25.4	4433	PASS
365	198	1	100	2.5	441	PASS
441	442	0.01	24	15.6	1916	PASS
442	198	50	100	70.4	12302	PASS
443	442	15	24	19.9	2451	PASS