


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062915\
 Data File : BF080219.D
 Acq On : 29 Jun 2015 22:53
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 23 00:53:56 2015

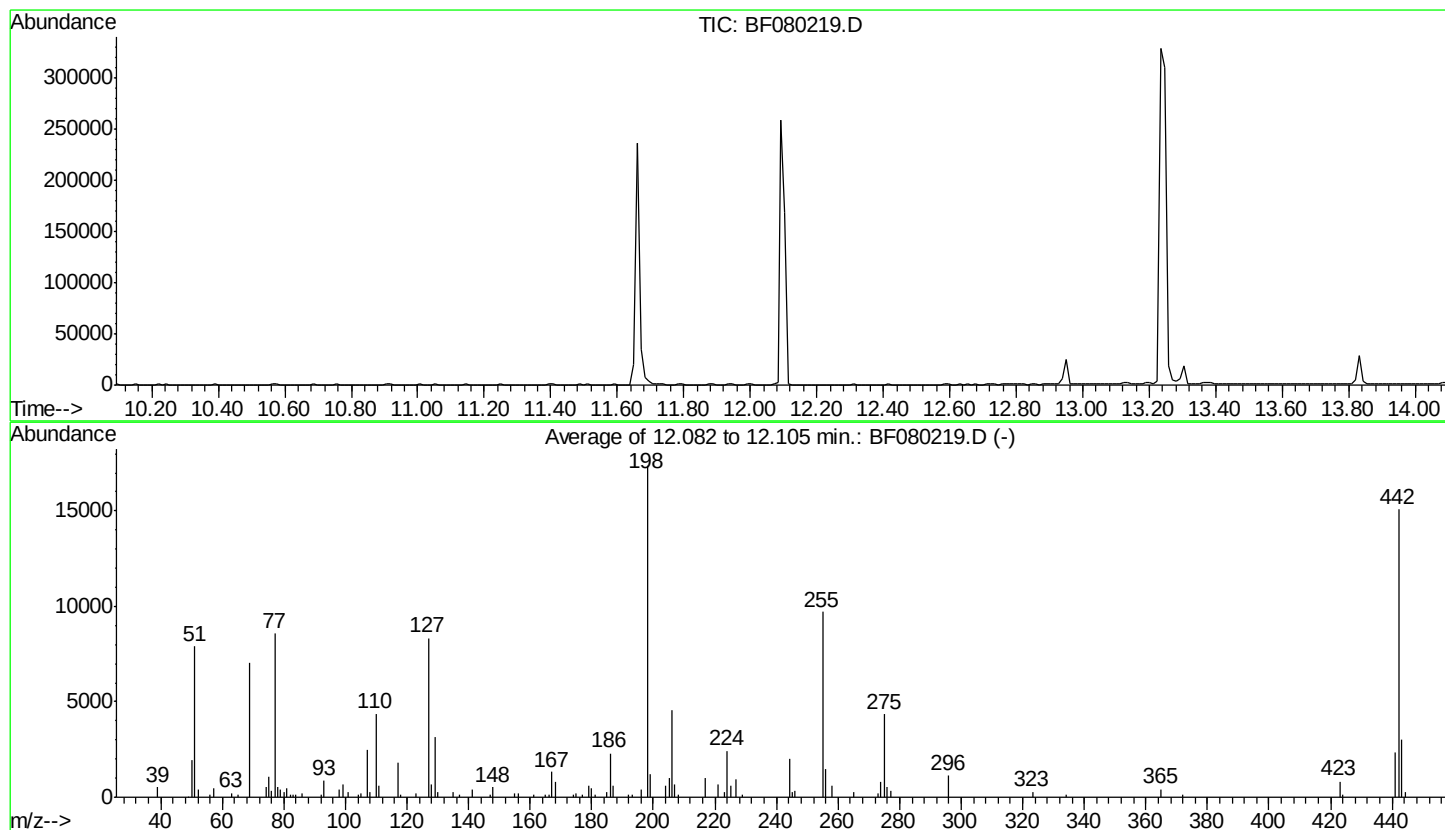

AutoFind: Scans 787, 788, 789; Background Corrected with Scan 785

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	7909	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.6	7049	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	8326	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17370	PASS
199	198	5	9	6.8	1188	PASS
275	198	10	60	24.9	4328	PASS
365	198	1	100	2.4	423	PASS
441	442	0.01	24	15.8	2375	PASS
442	198	50	100	86.8	15075	PASS
443	442	15	24	19.9	3004	PASS