



Phenanthrene

Response Ratio

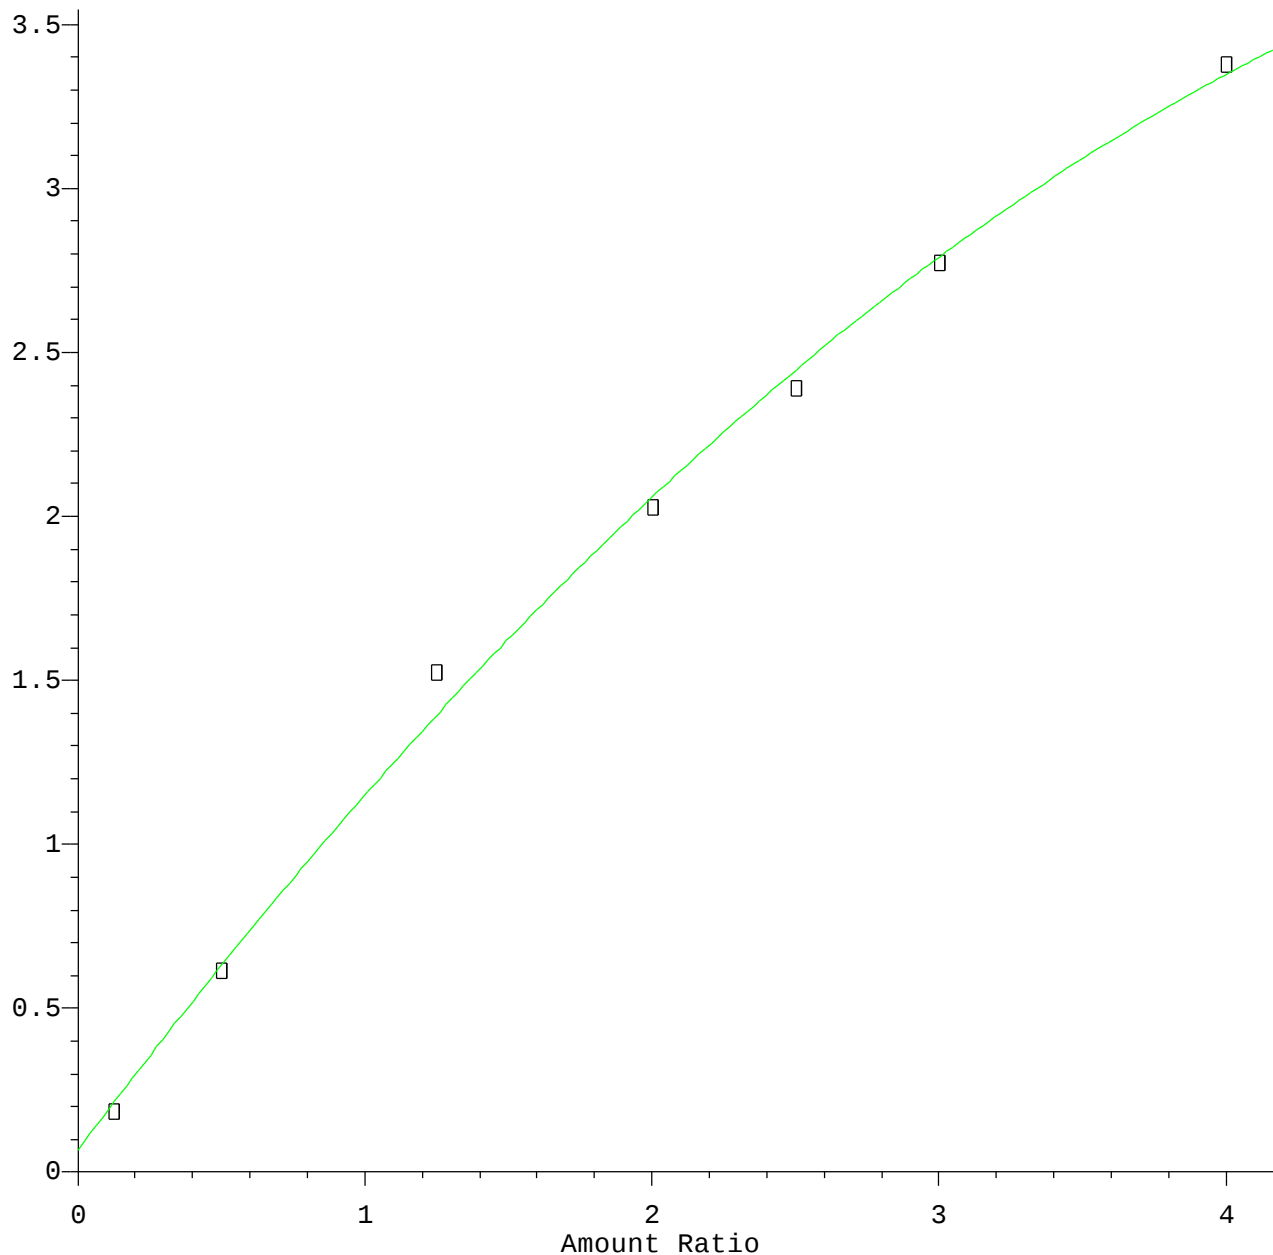


$R = -8.75e-002 A^2 + 1.17e+000 A + 6.77e-002$
Coef of Det (r^2) = 0.997 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF062916.M
Calibration Table Last Updated: Thu Jun 30 02:07:38 2016

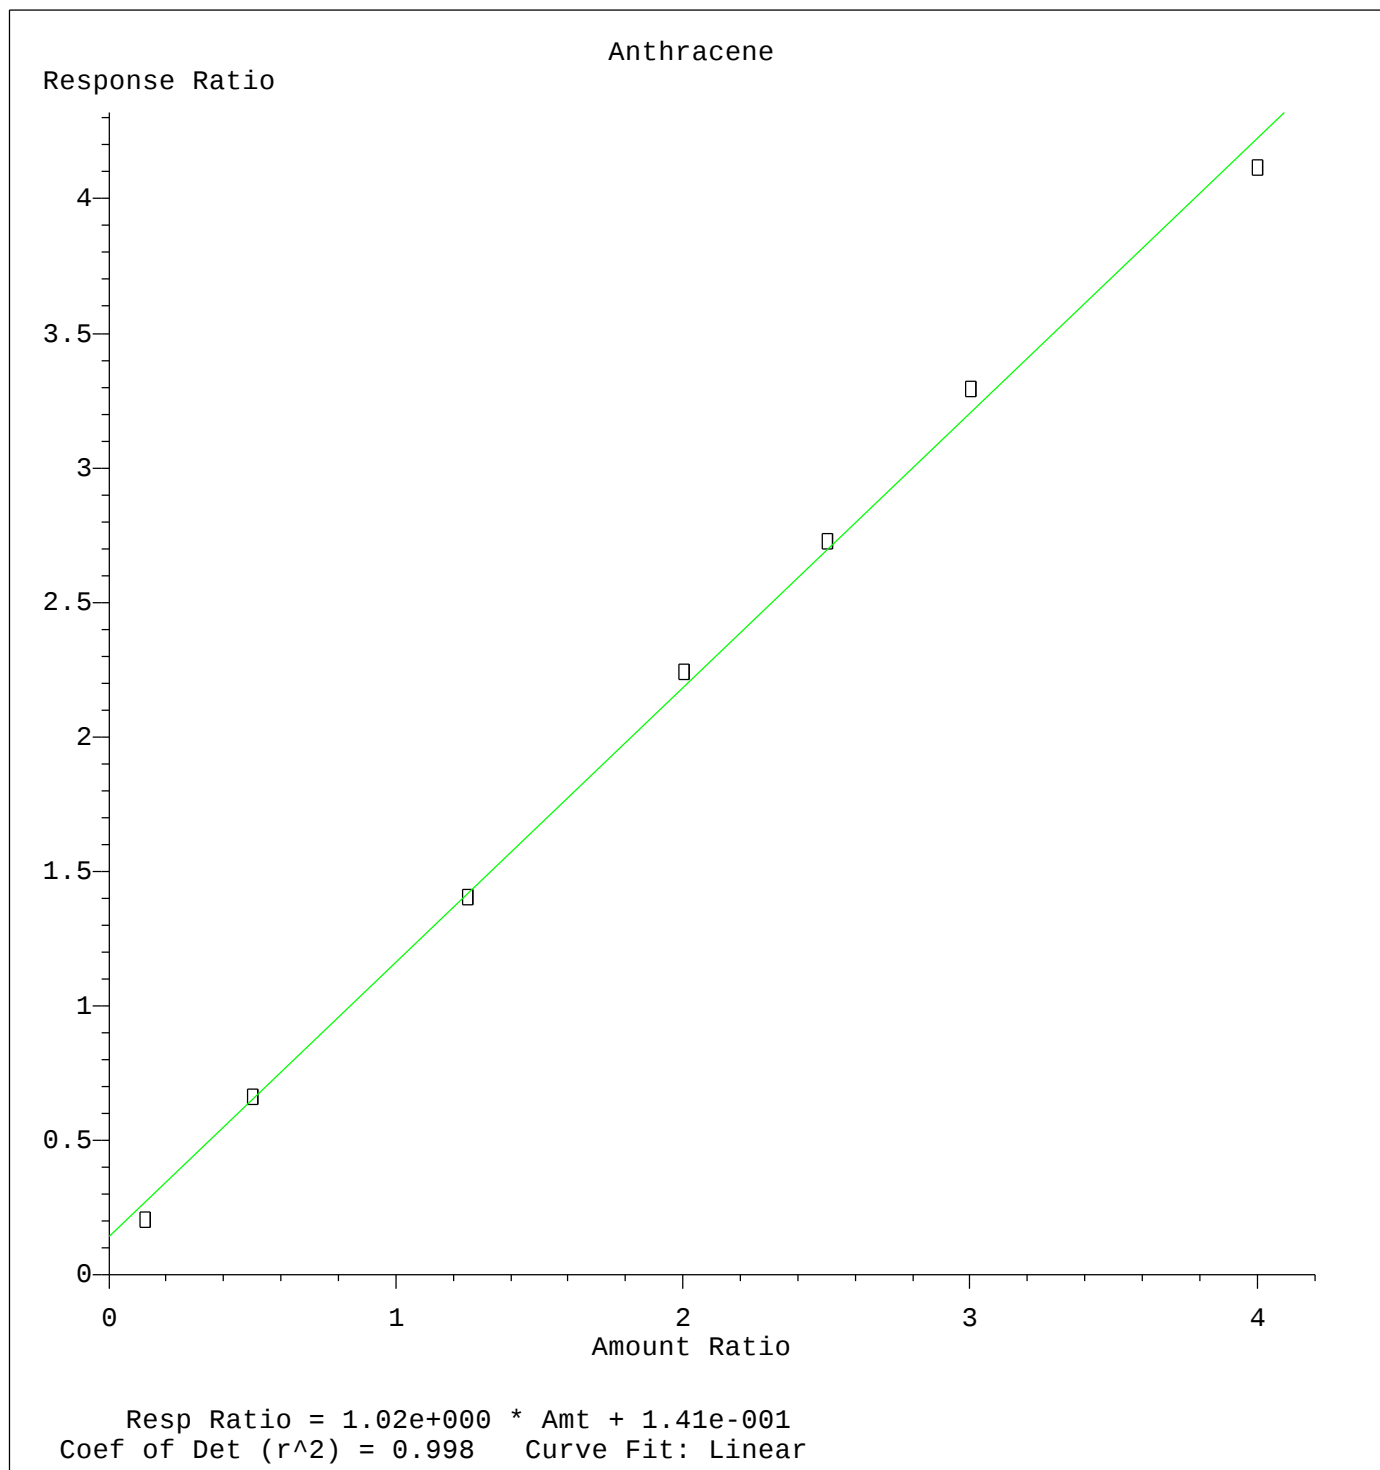


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF062916.M
Calibration Table Last Updated: Thu Jun 30 02:07:38 2016

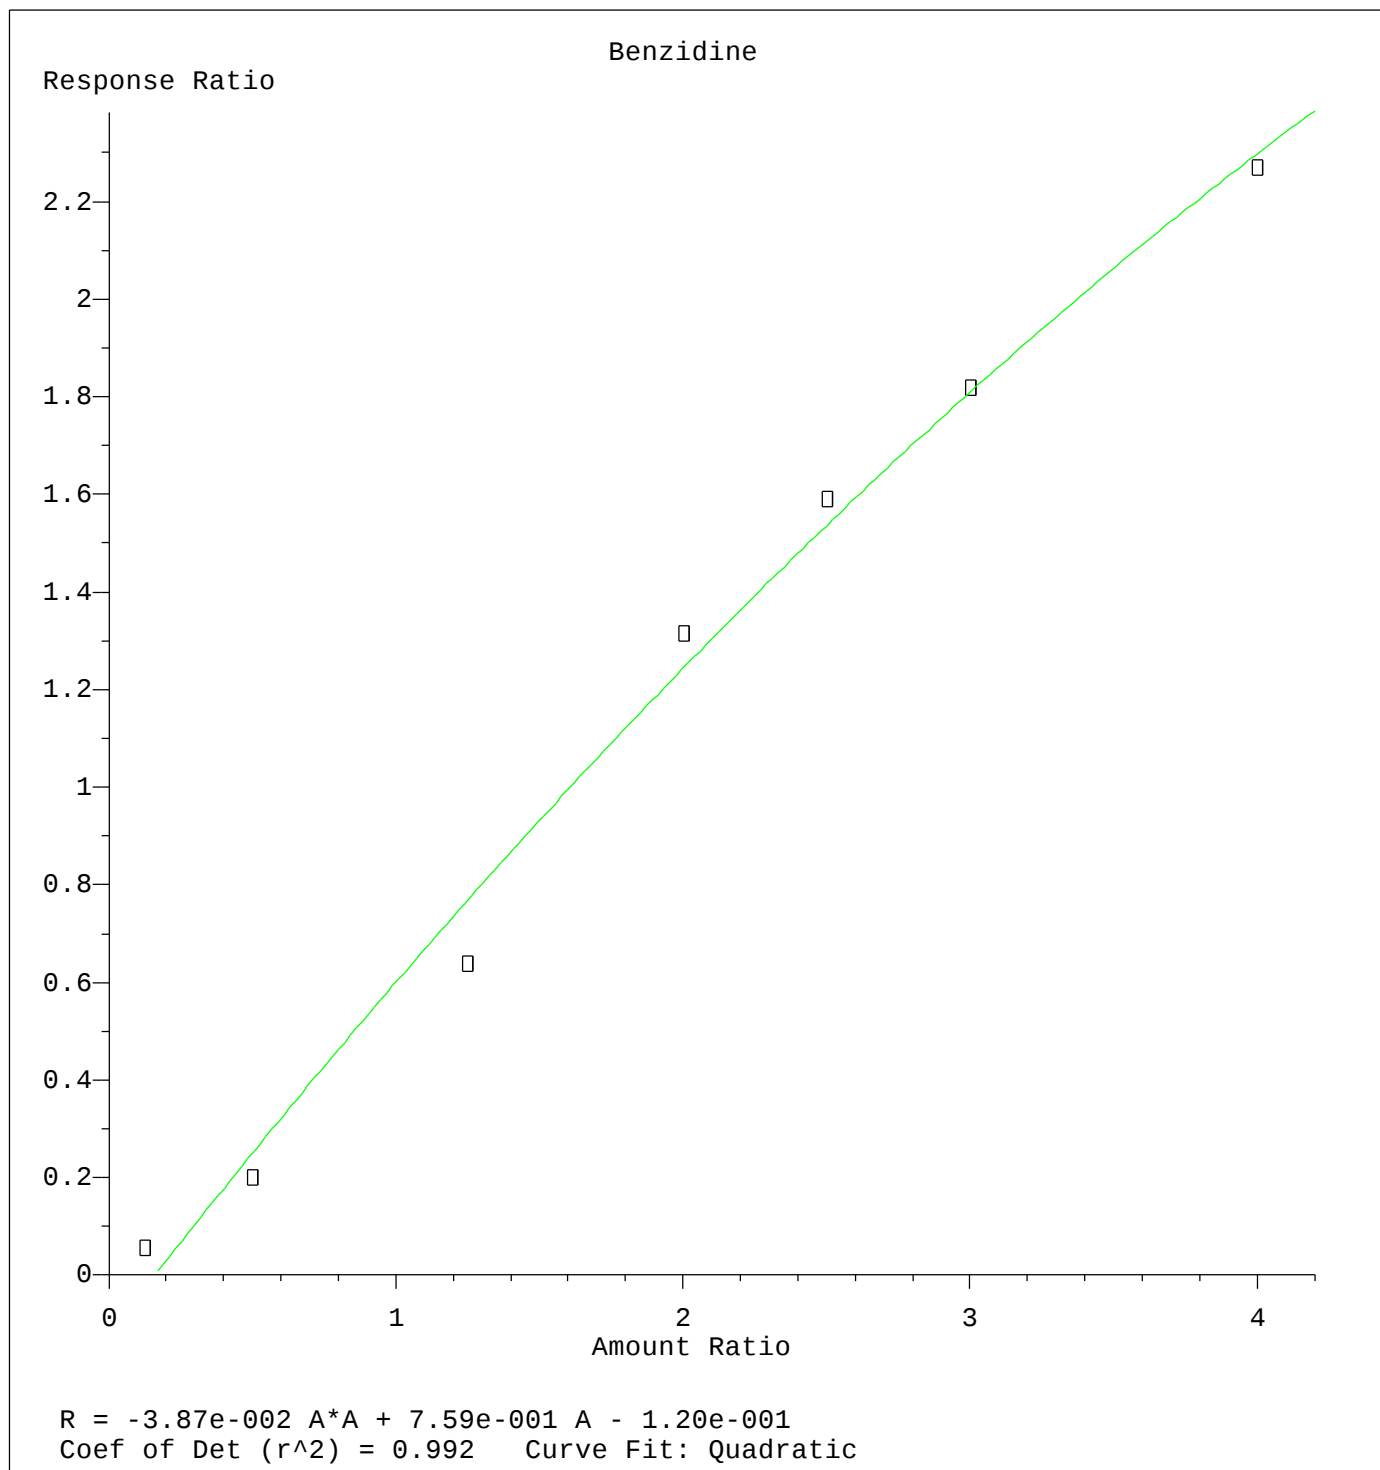

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF062916.M
Calibration Table Last Updated: Thu Jun 30 02:07:38 2016


Terphenyl-d14

Response Ratio

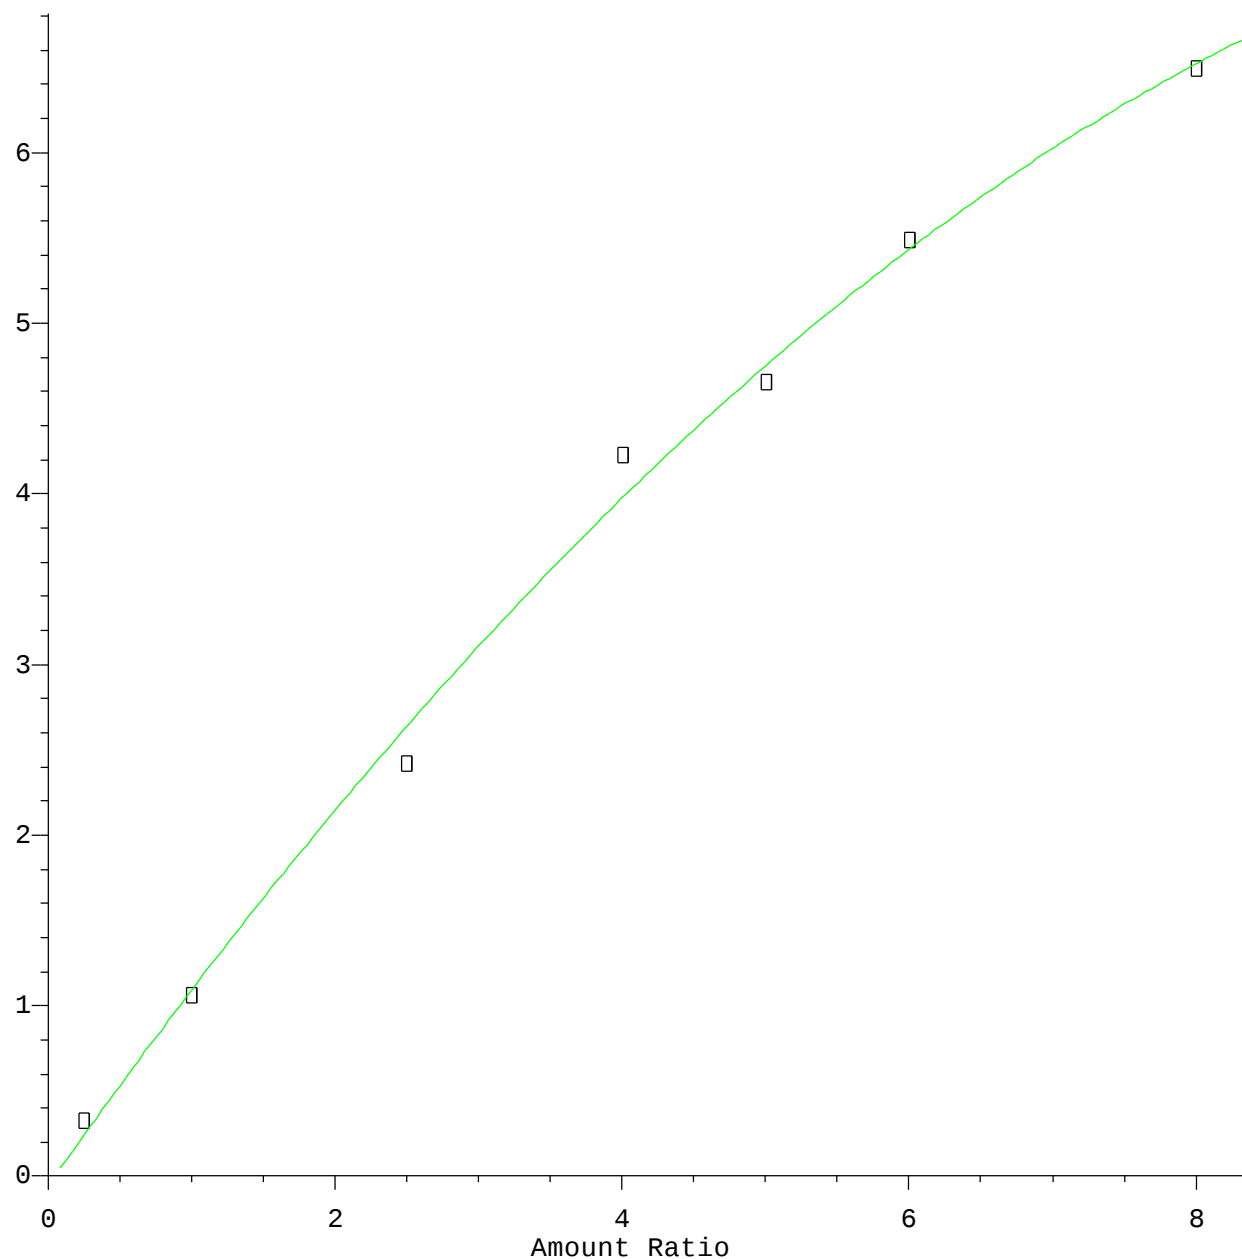


$R = -4.64e-002 A^2 + 1.19e+000 A - 5.62e-002$
Coef of Det (r^2) = 0.996 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF062916.M
Calibration Table Last Updated: Thu Jun 30 02:07:38 2016

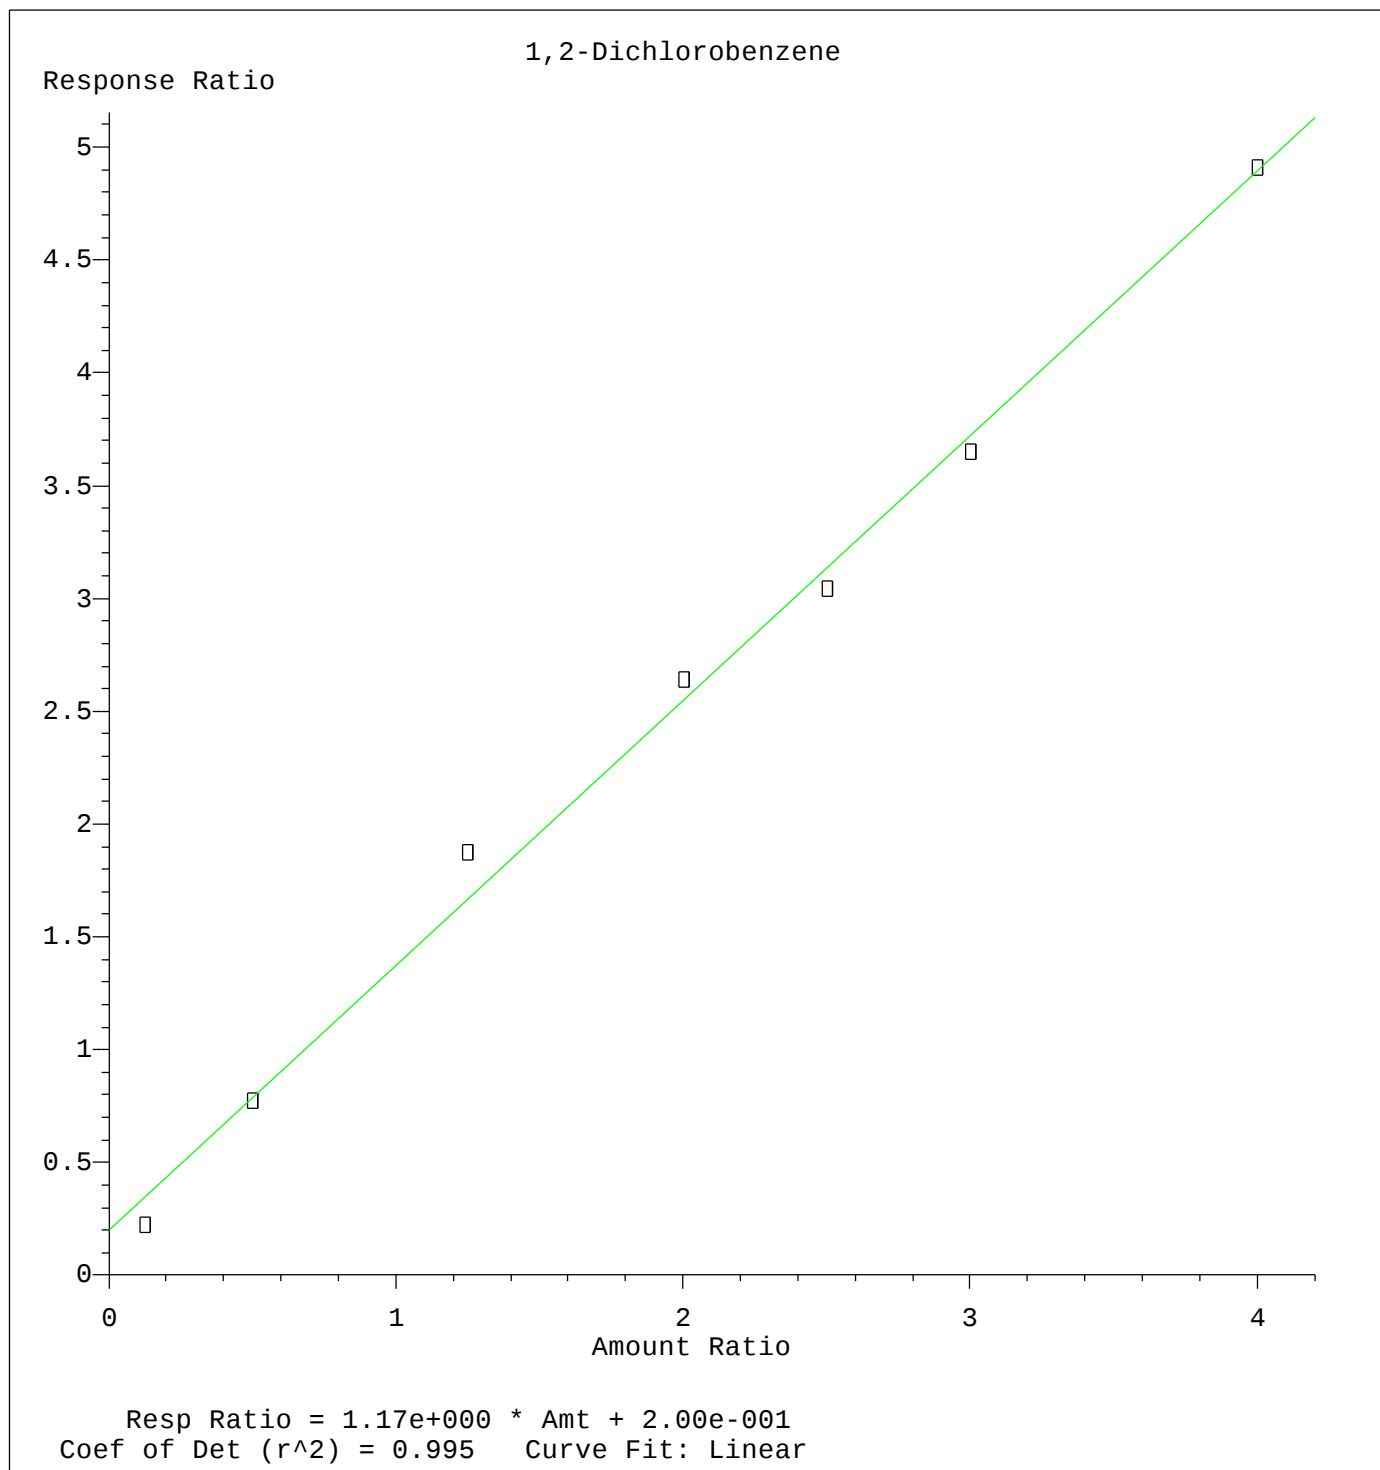


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF062916.M
Calibration Table Last Updated: Thu Jun 30 02:07:38 2016

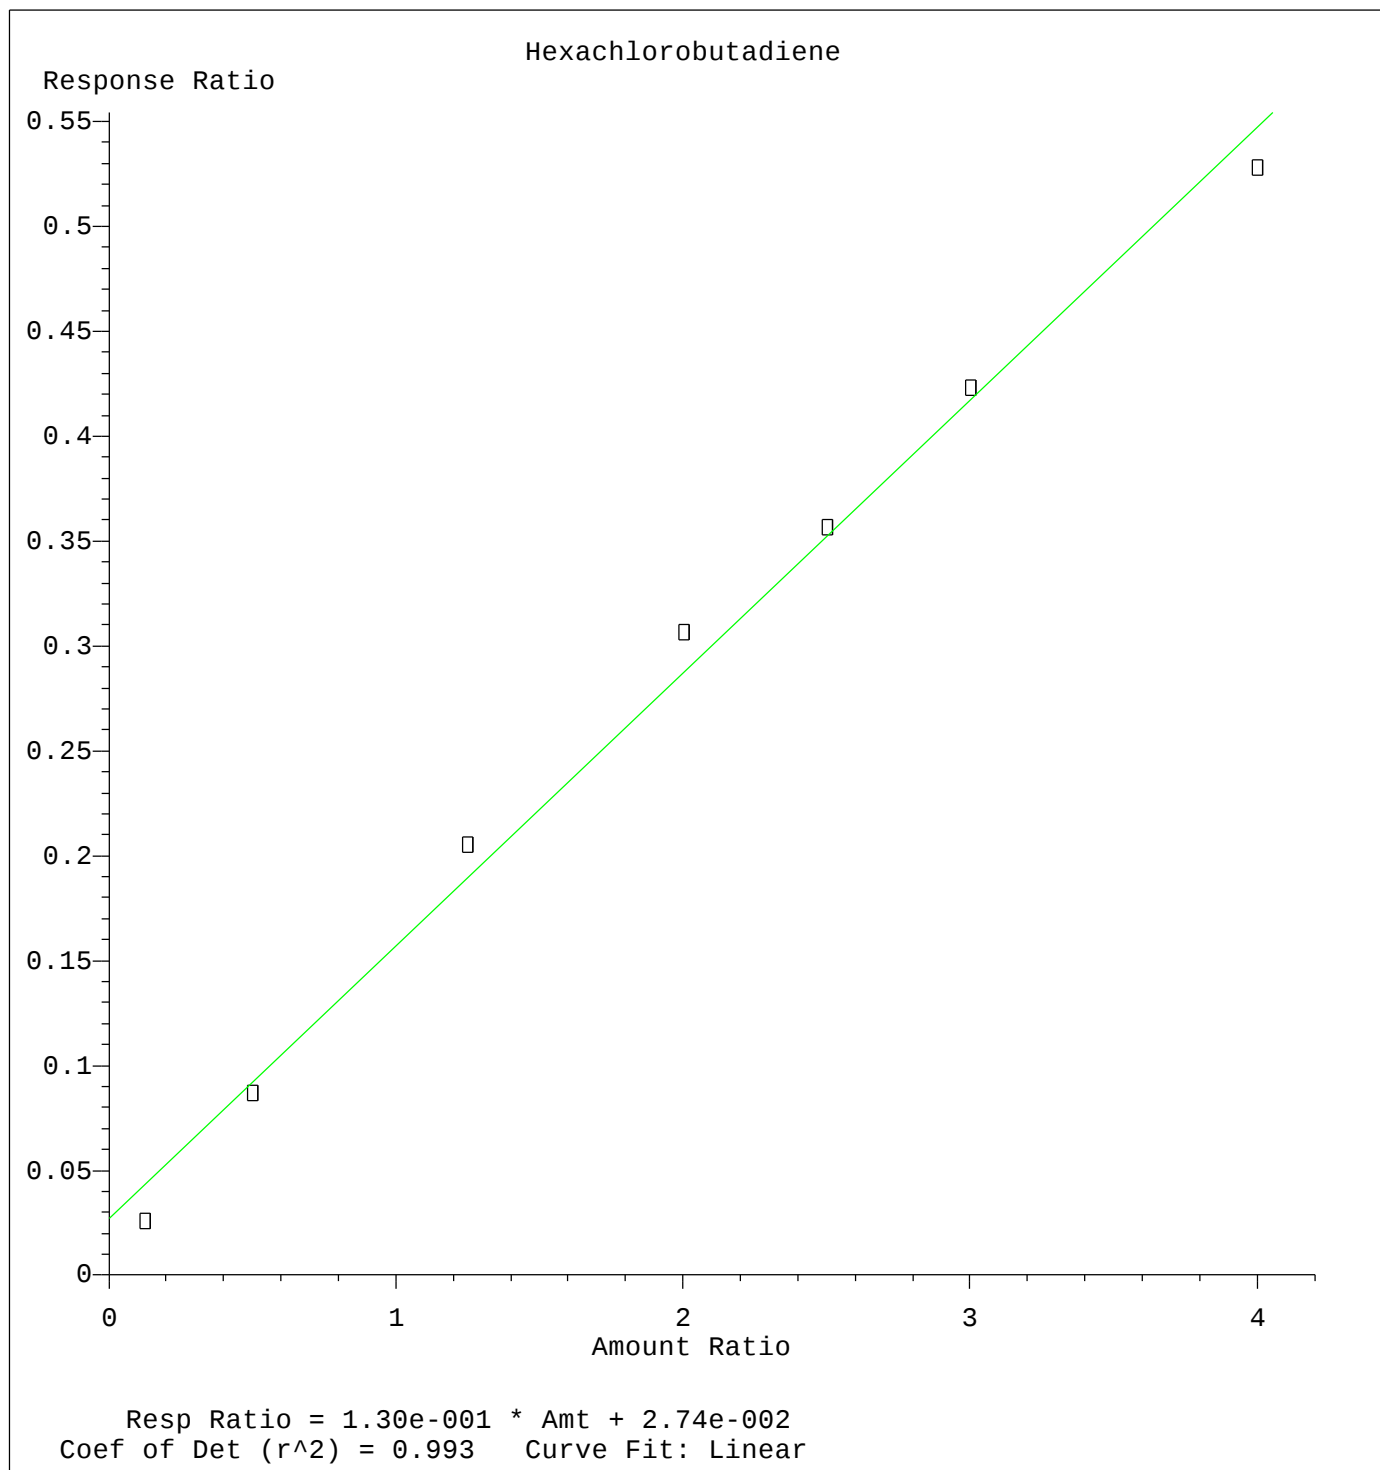

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF062916.M
Calibration Table Last Updated: Thu Jun 30 02:07:38 2016

1,2,4,5-Tetrachlorobenzene

Response Ratio

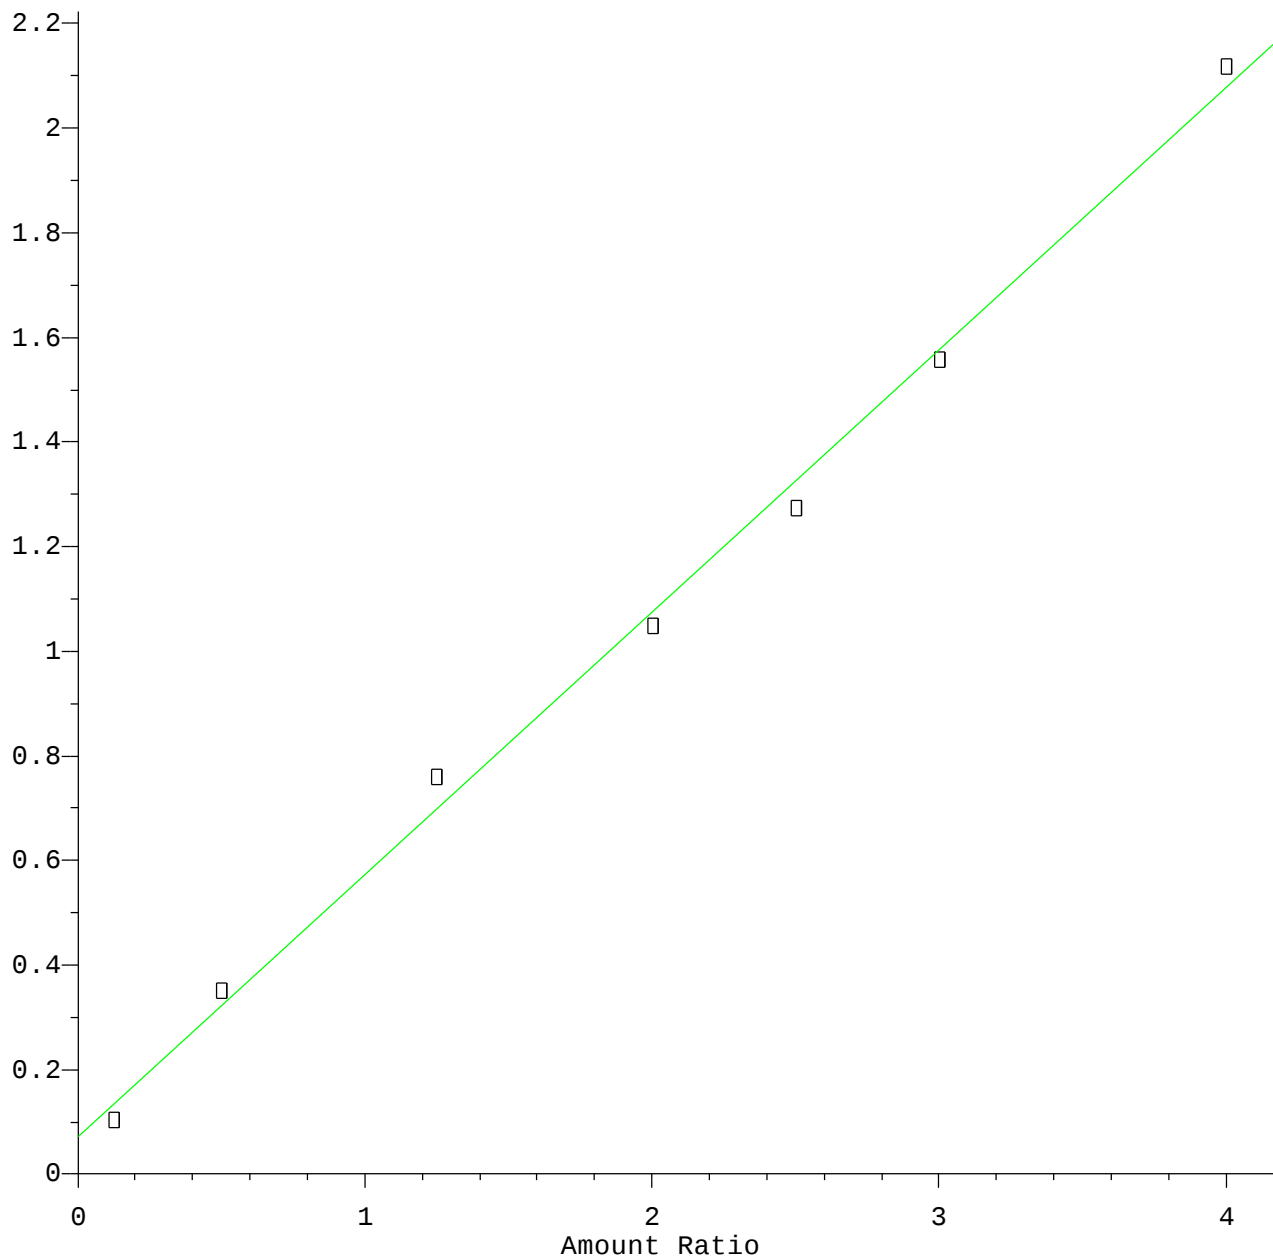


Resp Ratio = $5.02 \times 10^{-1} \times \text{Amt} + 6.95 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF062916.M
Calibration Table Last Updated: Thu Jun 30 02:07:38 2016

2-Fluorobiphenyl

Response Ratio

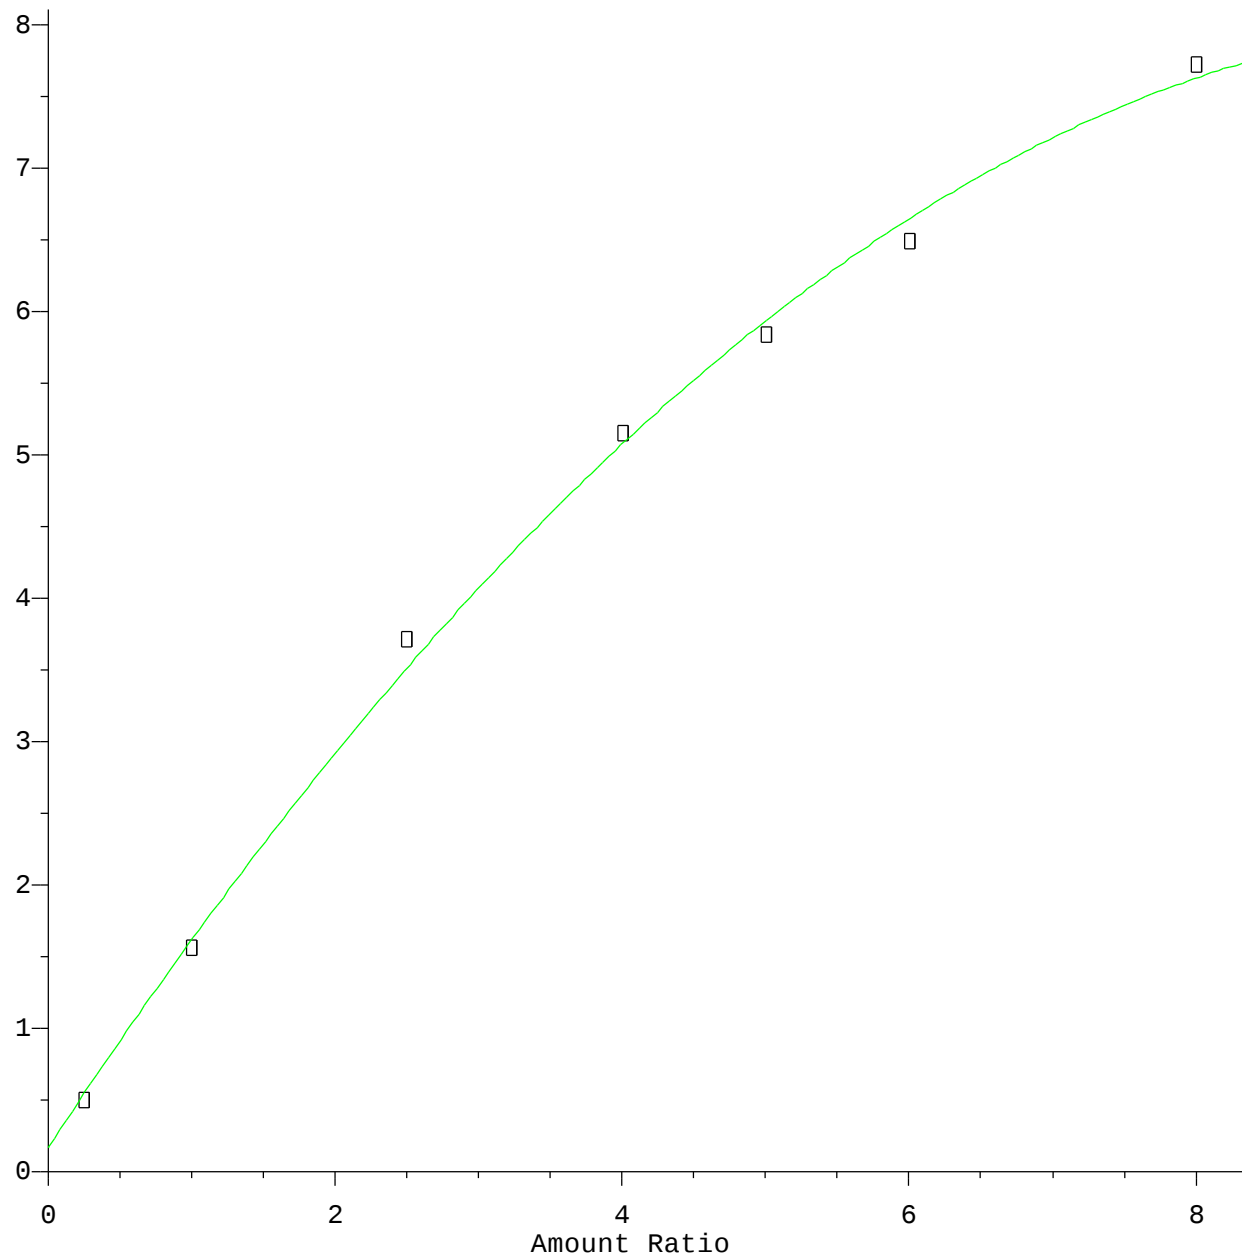


$R = -7.36e-002 A^2 + 1.52e+000 A + 1.71e-001$
Coef of Det (r^2) = 0.998 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF062916.M
Calibration Table Last Updated: Thu Jun 30 02:07:38 2016

1,1'-Biphenyl

Response Ratio

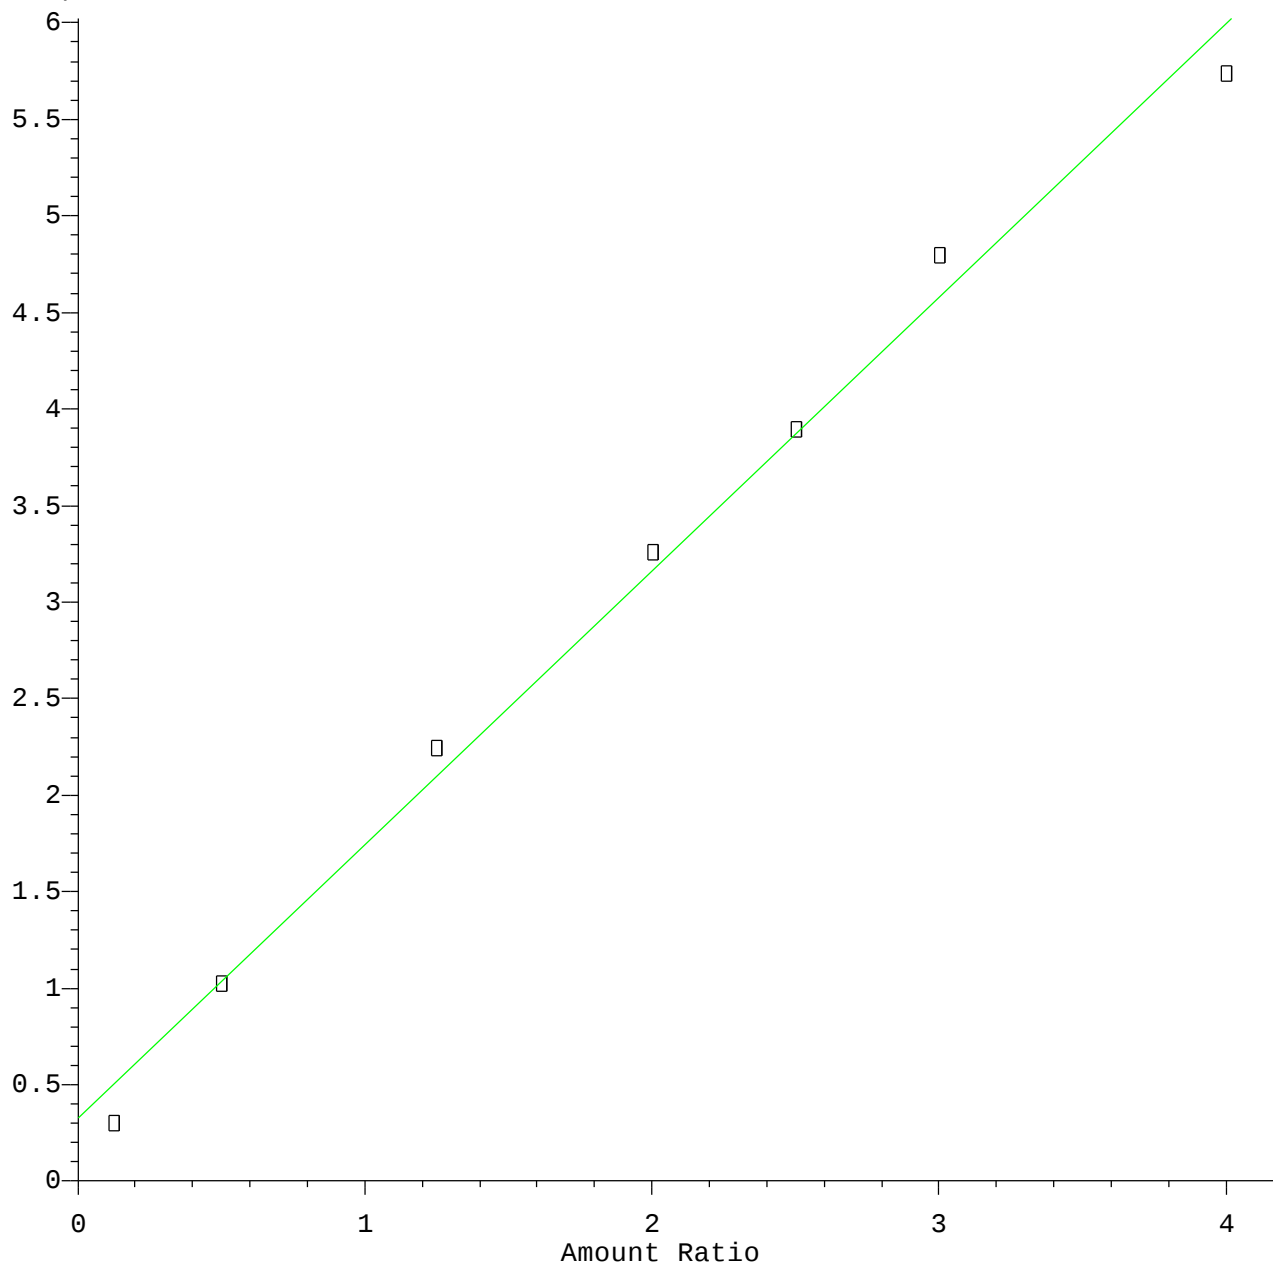


Resp Ratio = 1.42e+000 * Amt + 3.26e-001
Coef of Det (r^2) = 0.992 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF062916.M
Calibration Table Last Updated: Thu Jun 30 02:07:38 2016

2-Chloronaphthalene

Response Ratio

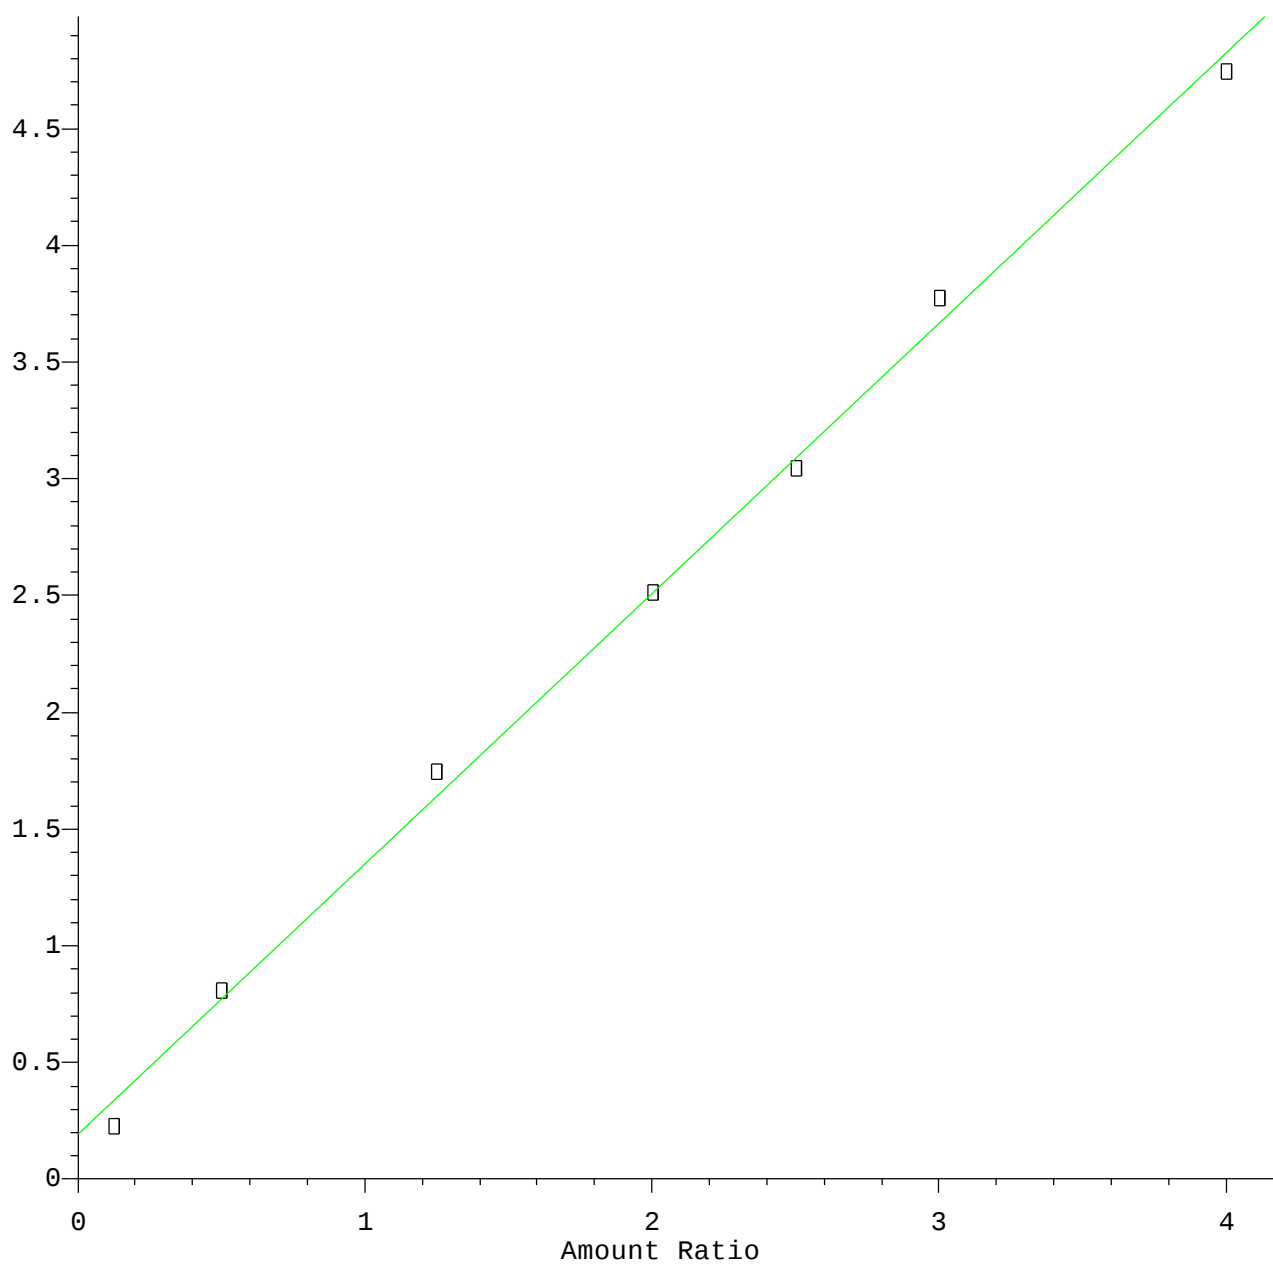


Resp Ratio = $1.16 \times 10^0 \times \text{Amt} + 1.94 \times 10^{-1}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF062916.M
Calibration Table Last Updated: Thu Jun 30 02:07:38 2016


Dimethylphthalate

Response Ratio

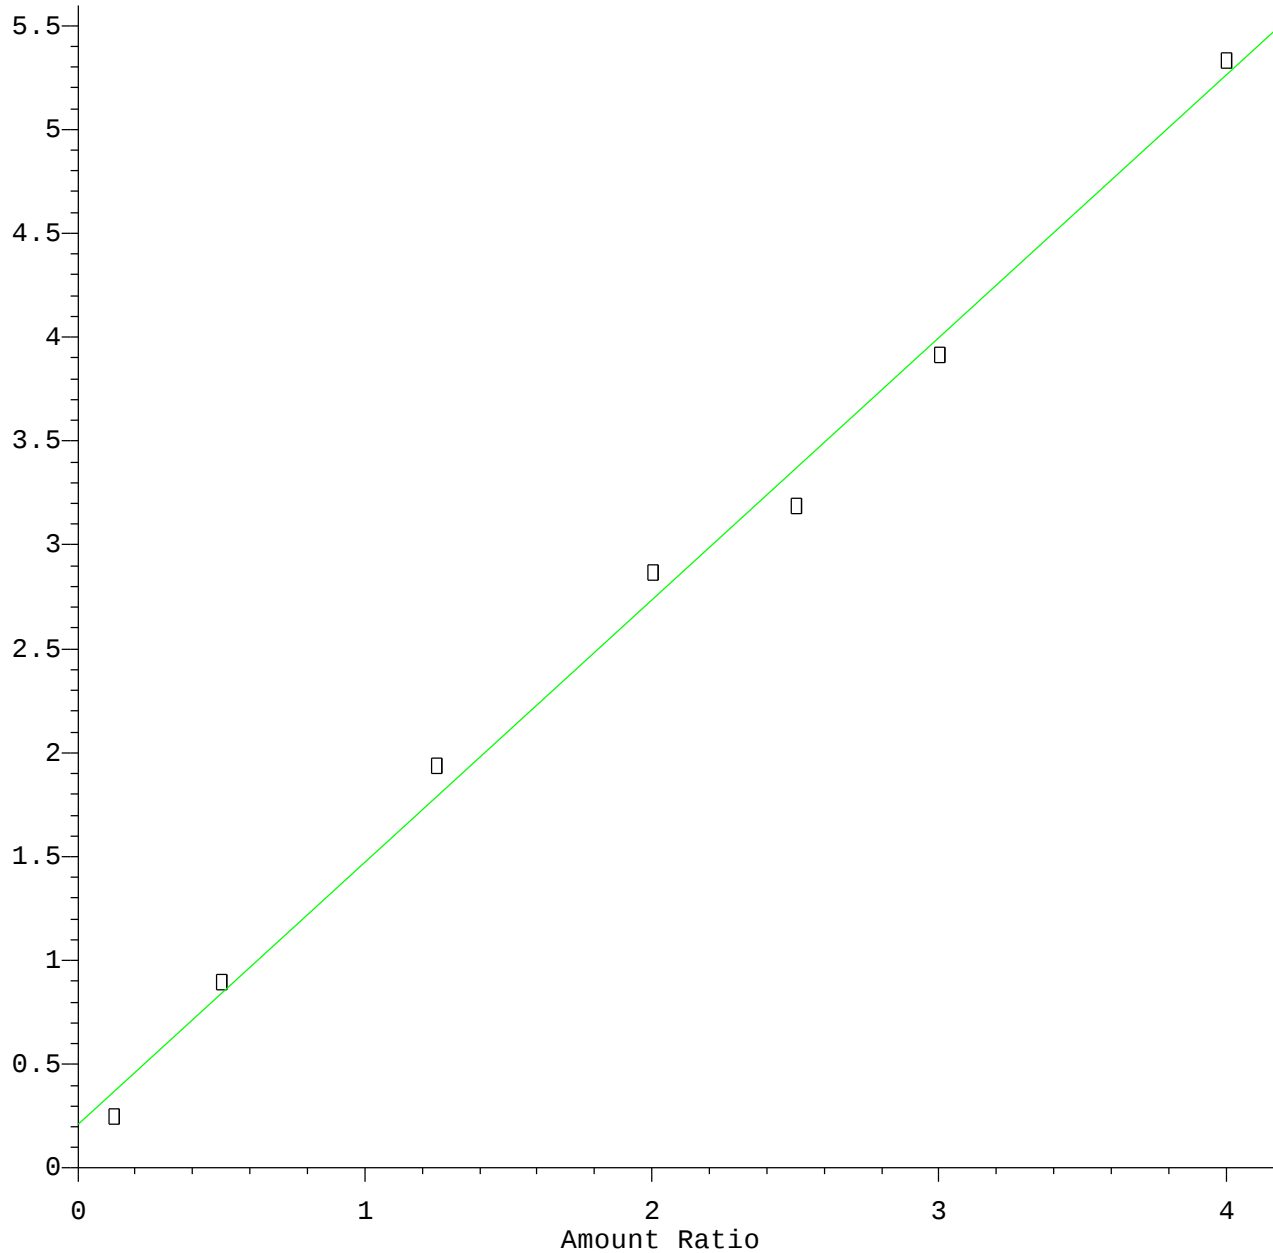

Resp Ratio = 1.26e+000 * Amt + 2.11e-001
Coef of Det (r^2) = 0.995 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF062916.M
Calibration Table Last Updated: Thu Jun 30 02:07:38 2016

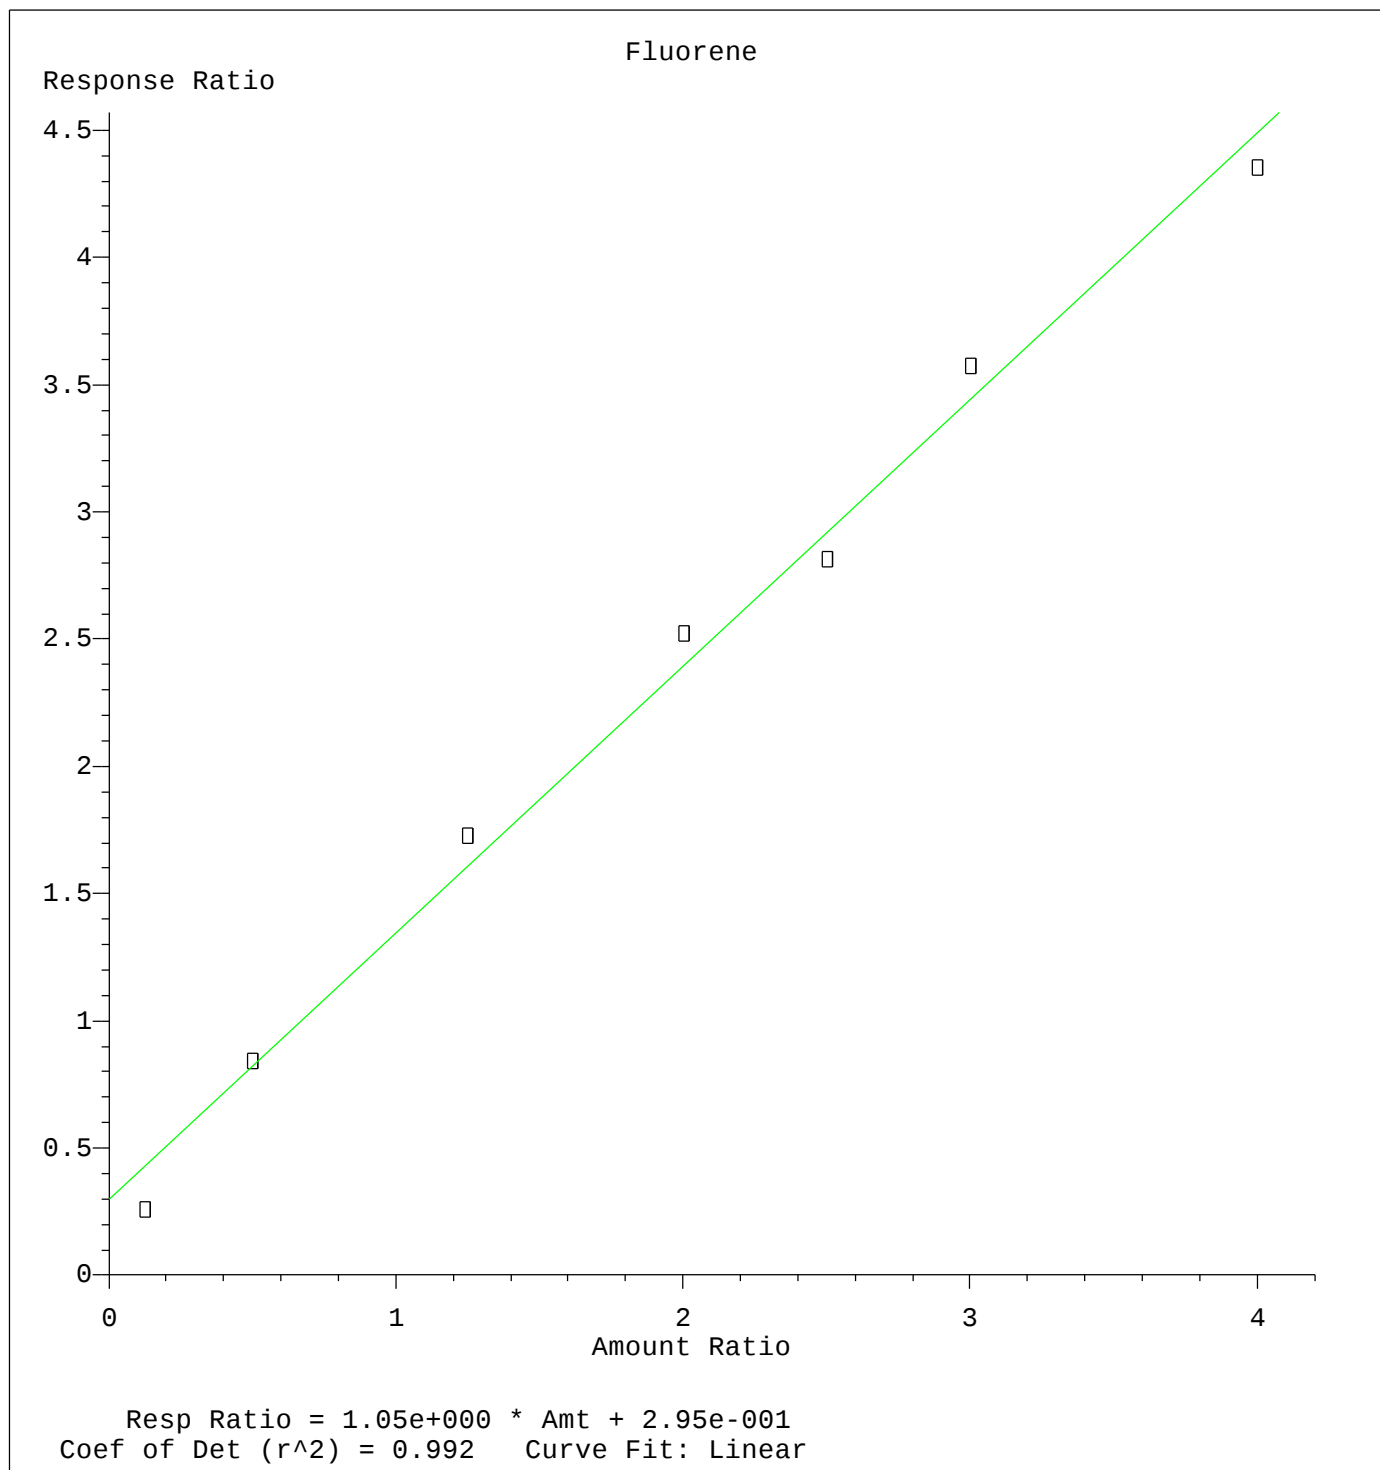

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF062916.M
Calibration Table Last Updated: Thu Jun 30 02:07:38 2016

4-Chlorophenyl-phenylether


Response Ratio

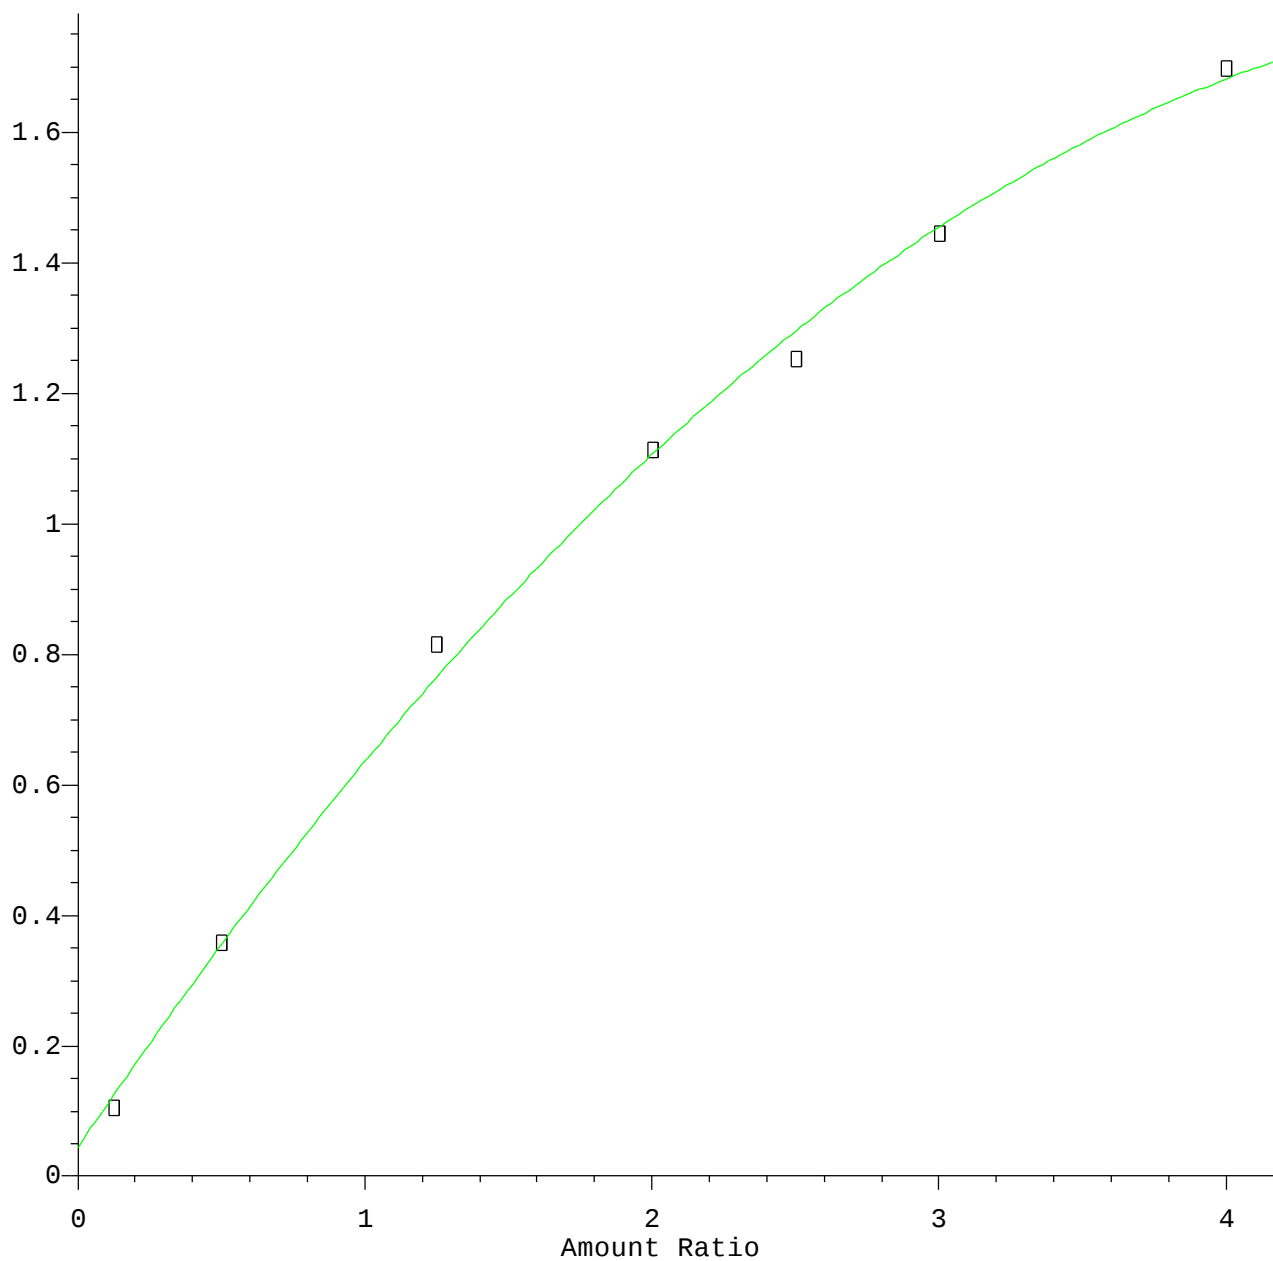

$R = -6.08e-002 A^2 + 6.52e-001 A + 4.42e-002$
Coef of Det (r^2) = 0.997 Curve Fit: Quadratic


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF062916.M
Calibration Table Last Updated: Thu Jun 30 02:07:38 2016

4,6-Dinitro-2-methylphenol

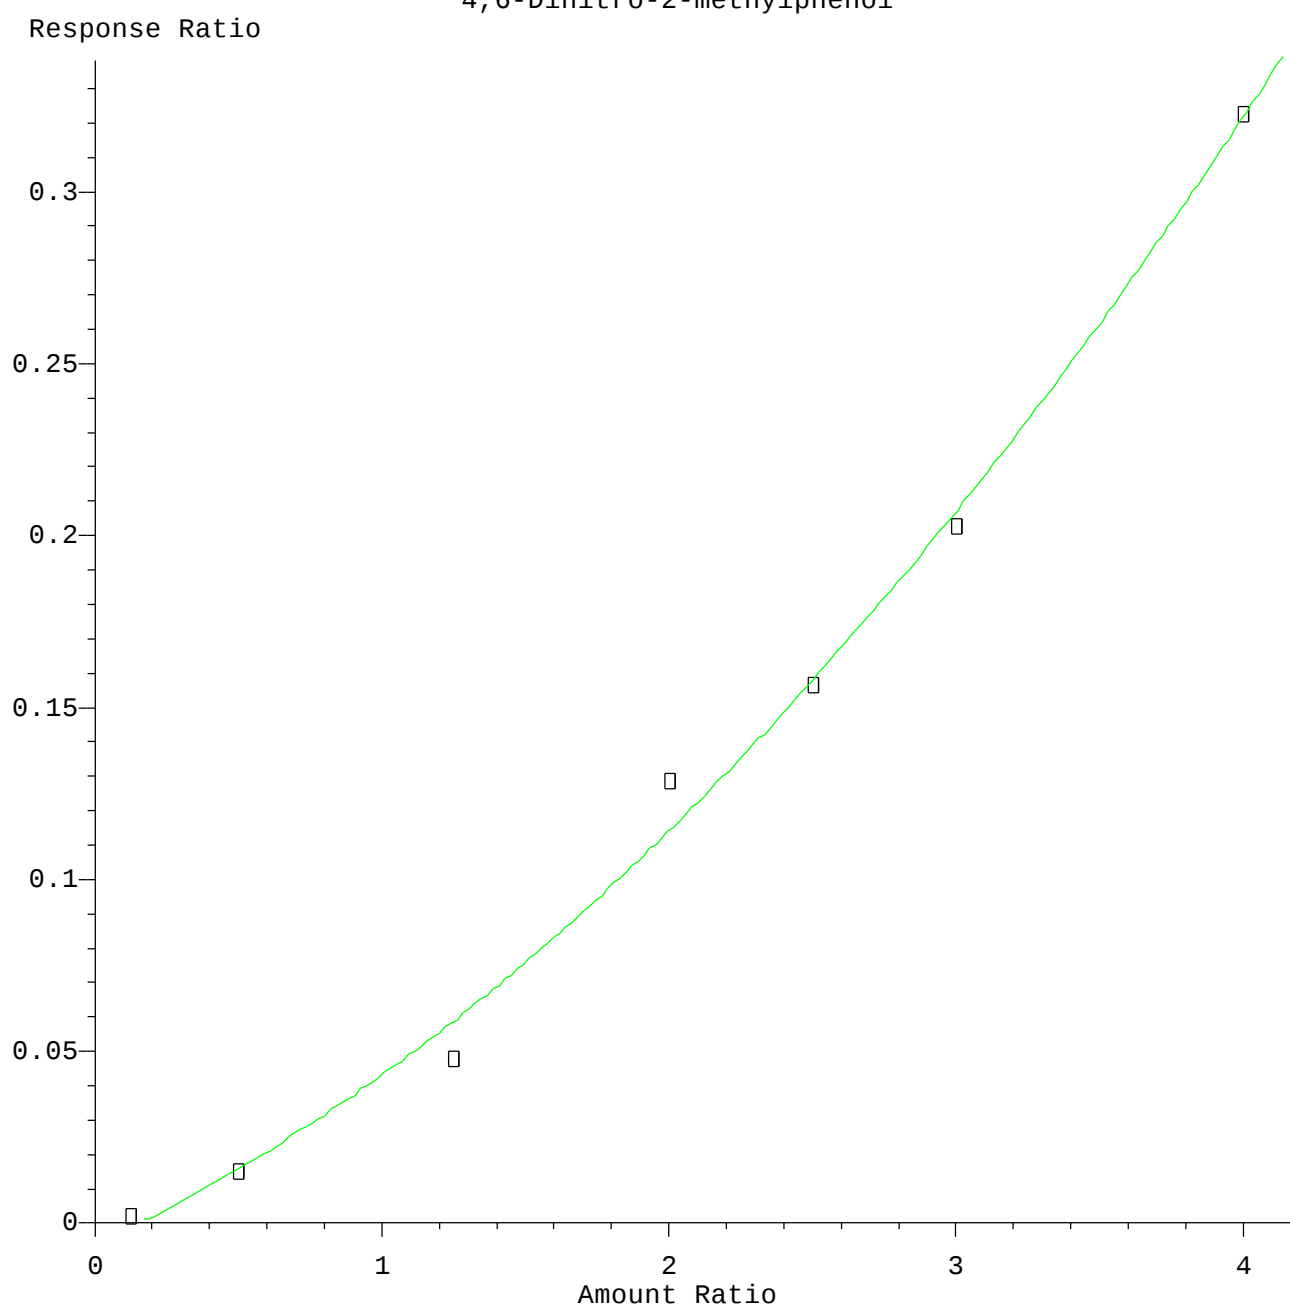

$R = 1.09e-002 A^2 + 3.83e-002 A - 6.13e-003$
Coef of Det (r^2) = 0.995 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF062916.M
Calibration Table Last Updated: Thu Jun 30 02:07:38 2016

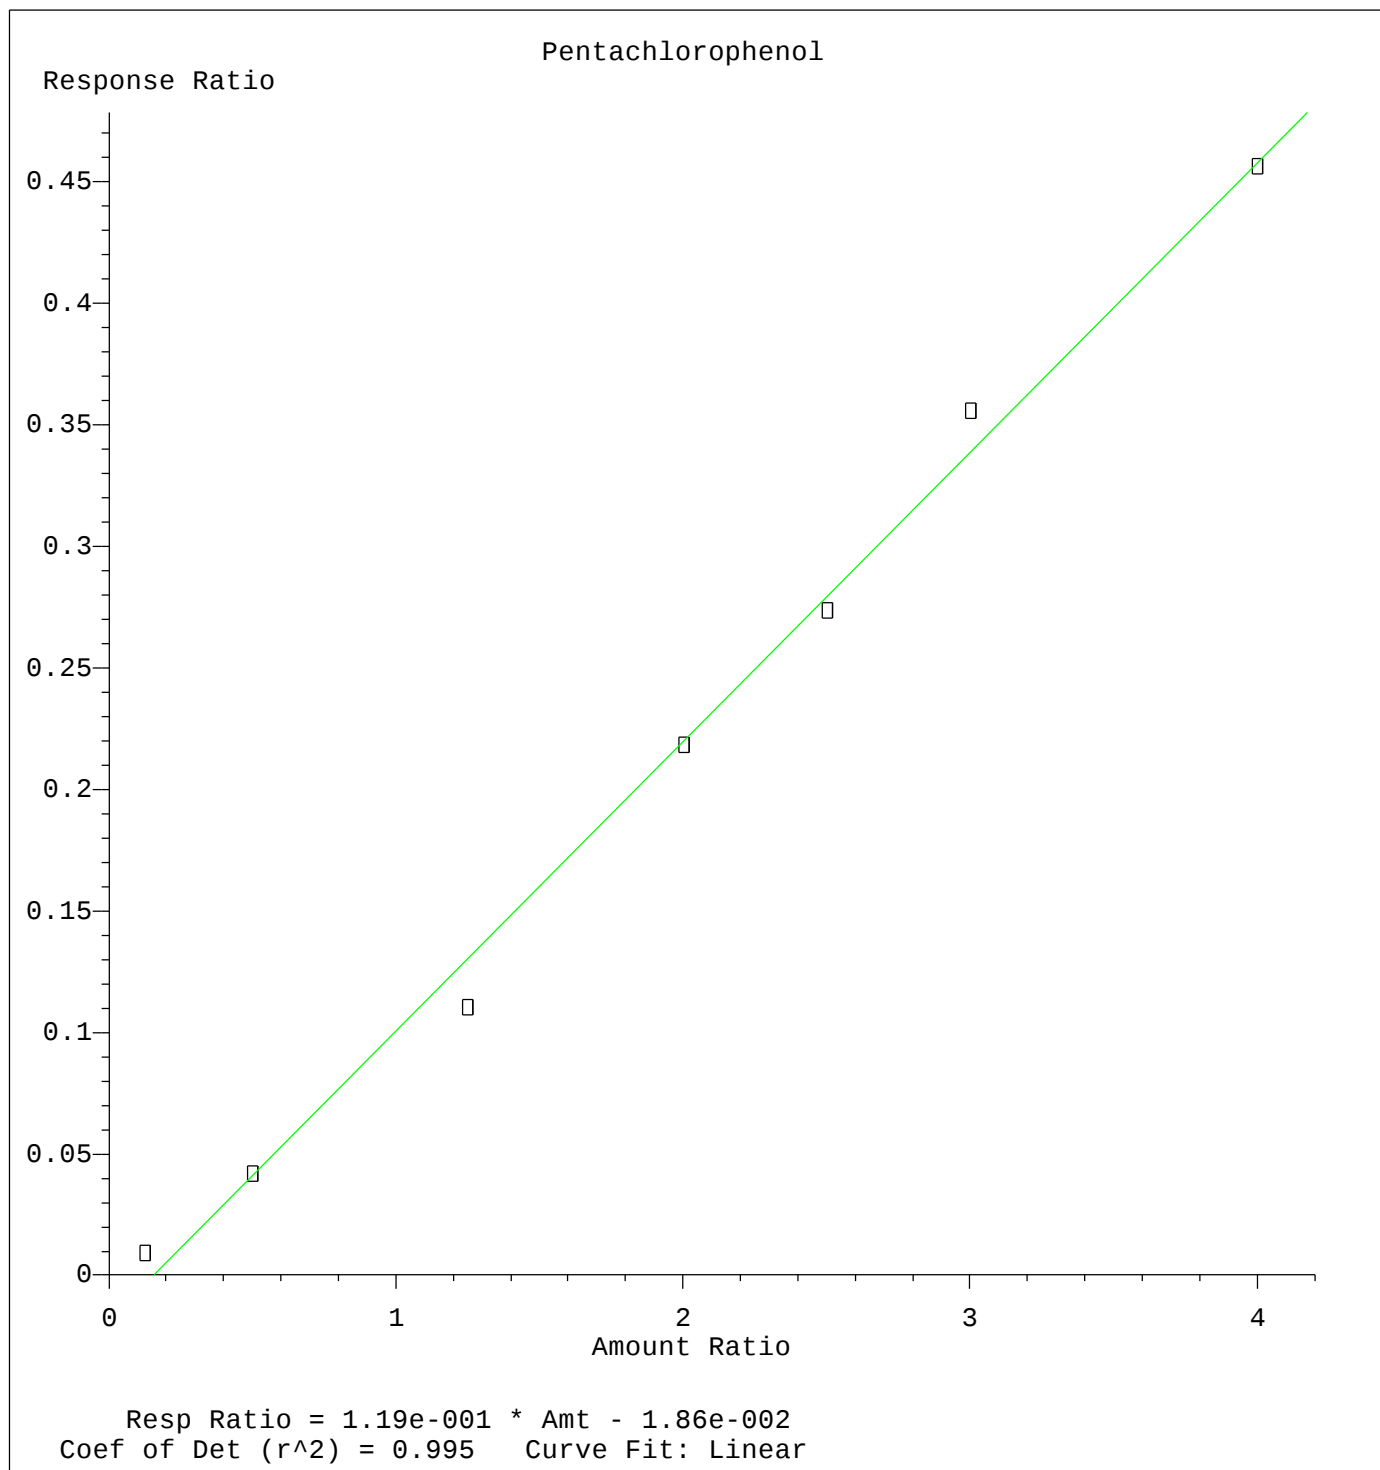

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF062916.M
Calibration Table Last Updated: Thu Jun 30 02:07:38 2016