

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062916\
 Data File : BF088522.D
 Acq On : 30 Jun 2016 6:14
 Operator : UM/SJ
 Sample : H3830-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TILCON-GF-018

Quant Time: Jun 30 07:12:35 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF062916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 30 02:07:38 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	126991	20.00	ng	0.00
21) Naphthalene-d8	8.10	136	437423	20.00	ng	-0.01
38) Acenaphthene-d10	9.85	164	171845	20.00	ng	-0.01
63) Phenanthrene-d10	11.34	188	316789	20.00	ng	0.00
75) Chrysene-d12	13.95	240	296903	20.00	ng	-0.01
86) Perylene-d12	15.37	264	272441	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	743790	90.70	ng	0.00
7) Phenol-d6	6.46	99	1121012	106.90	ng	0.00
23) Nitrobenzene-d5	7.38	82	576666	69.24	ng	-0.01
41) 2,4,6-Tribromophenol	10.64	330	154162	117.01	ng	0.00
44) 2-Fluorobiphenyl	9.19	172	967556	92.54	ng	0.00
78) Terphenyl-d14	12.91	244	779082	49.74	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	9.58	163	68854	3.00	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062916\
Data File : BF088522.D
Acq On : 30 Jun 2016 6:14
Operator : UM/SJ
Sample : H3830-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TILCON-GF-018

Quant Time: Jun 30 07:12:35 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF062916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 30 02:07:38 2016
Response via : Initial Calibration

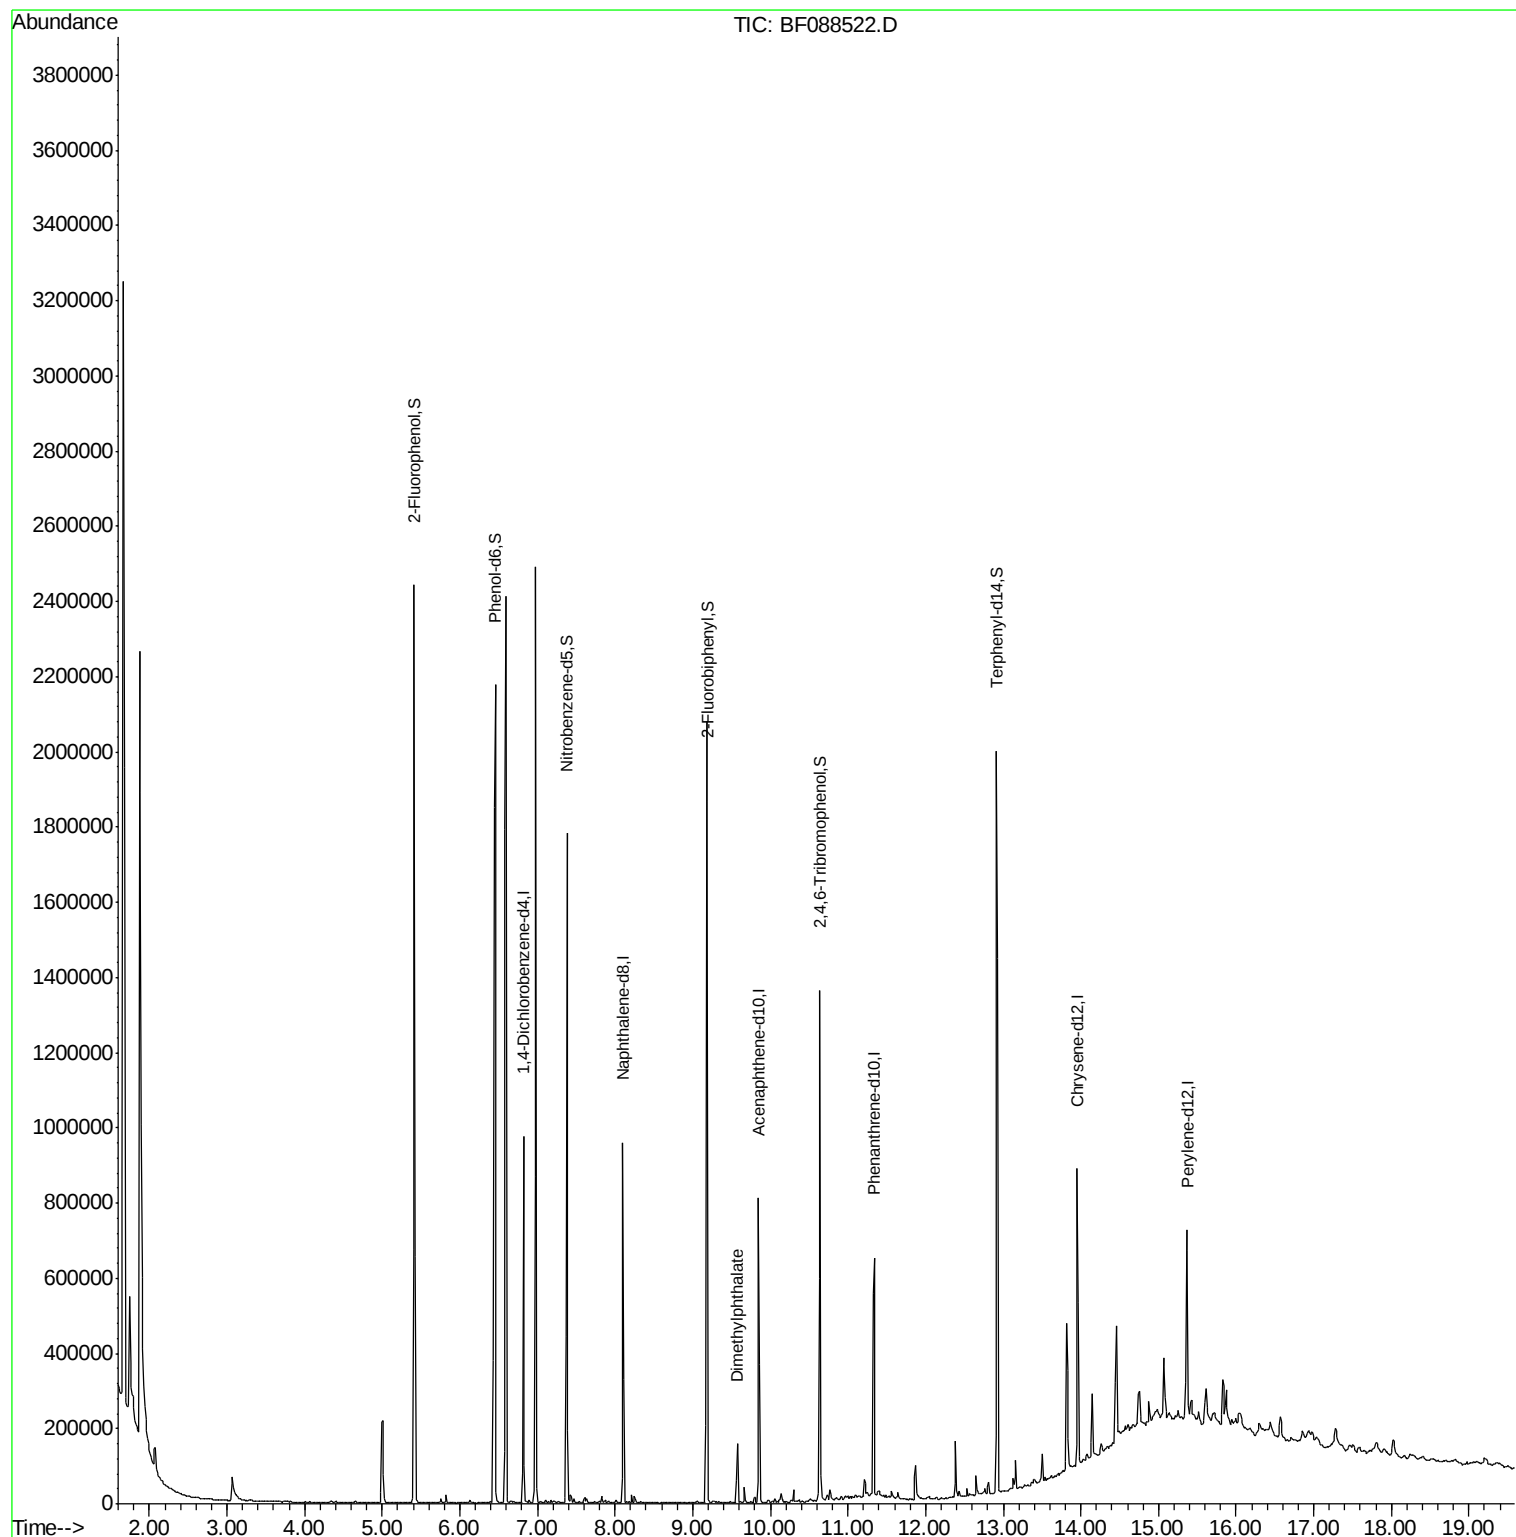

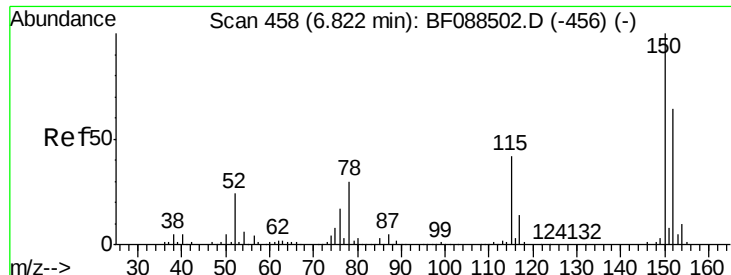

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.82 min Scan# 458

Delta R.T. 0.00 min

Lab File: BF088522.D

Acq: 30 Jun 2016 6:14

Instrument :

BNA_F

ClientSampleId :

TILCON-GF-018


Tot Ion:152 Resp: 126991

Ion Ratio Lower Upper

152 100

150 154.7 124.5 186.7




115 66.7 52.3 78.5

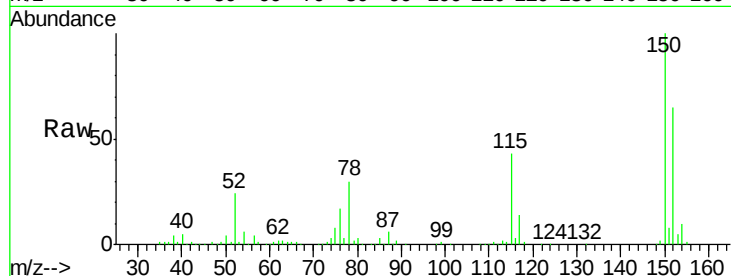

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

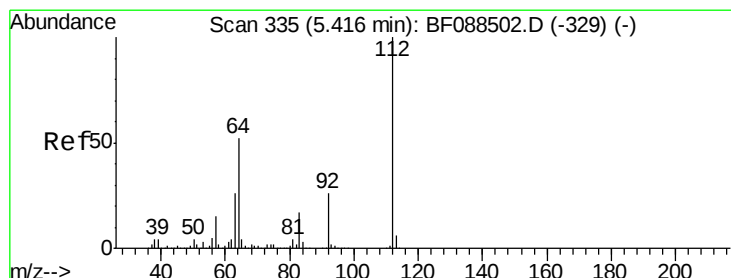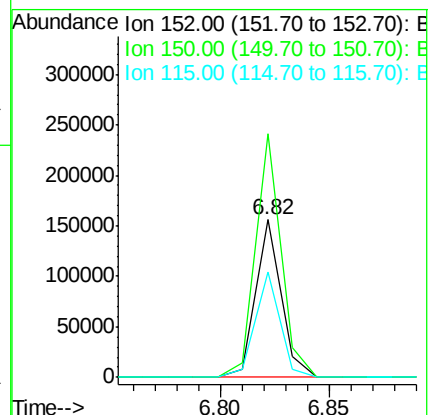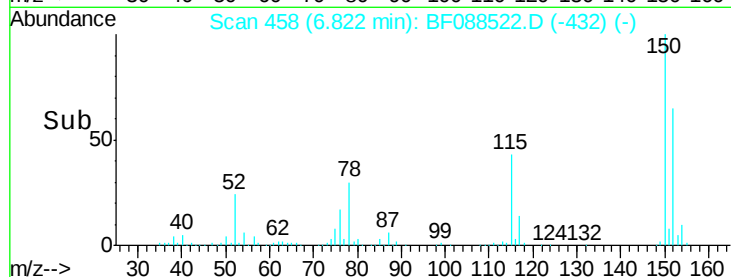

#5

2-Fluorophenol

Concen: 90.70 ng

RT: 5.42 min Scan# 335

Delta R.T. 0.00 min

Lab File: BF088522.D

Acq: 30 Jun 2016 6:14


Tgt Ion:112 Resp: 743790

Ion Ratio Lower Upper

112 100

64 66.0 41.5 62.3#



63 34.0 20.6 31.0#

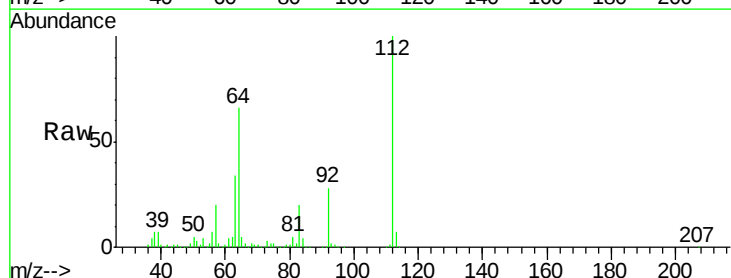


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

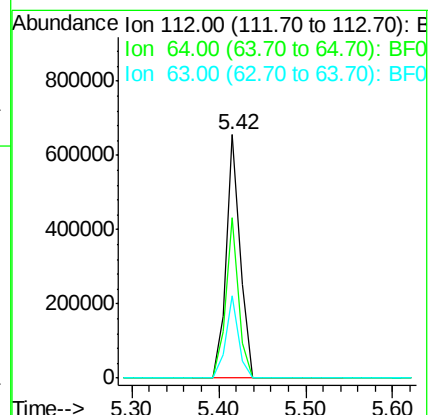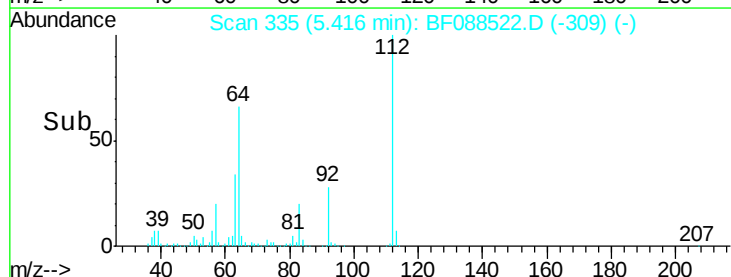

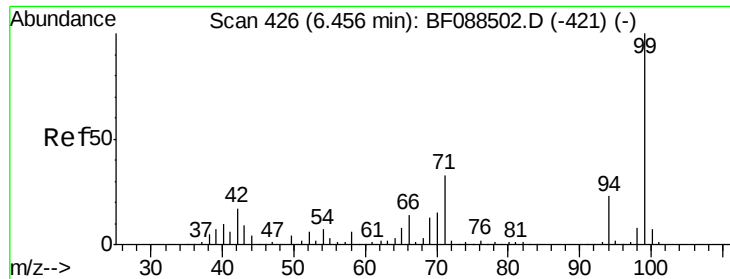

#7

Phenol-d6

Concen: 106.90 ng

RT: 6.46 min Scan# 426

Delta R.T. 0.00 min

Lab File: BF088522.D

Acq: 30 Jun 2016 6:14

Instrument :

BNA_F

ClientSampleId :

TILCON-GF-018


Tot Ion: 99 Resp: 1121012

Ion Ratio Lower Upper

99 100

42 14.0 13.4 20.0




71 30.7 26.1 39.1

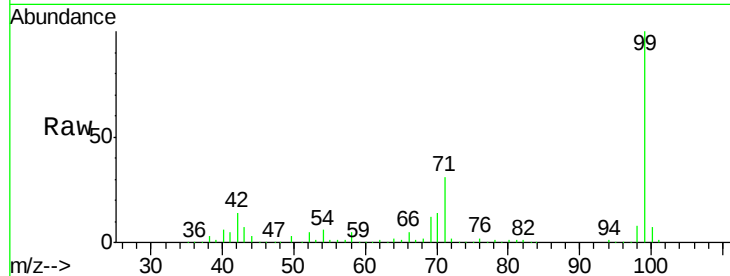

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

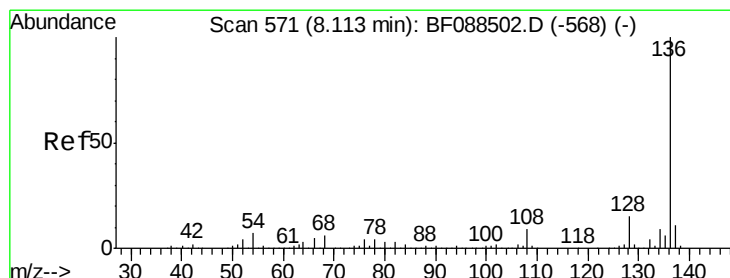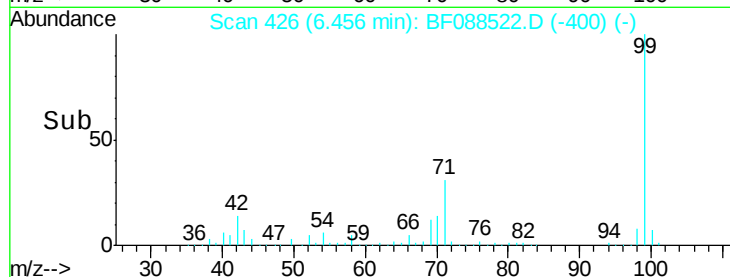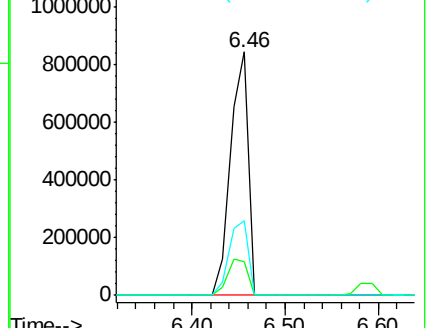

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.10 min Scan# 570

Delta R.T. -0.01 min

Lab File: BF088522.D

Acq: 30 Jun 2016 6:14

Tgt Ion: 136 Resp: 437423


Ion Ratio Lower Upper

136 100

137 11.2 8.5 12.7

54 10.2 5.4 8.2#

68 8.5 4.9 7.3#


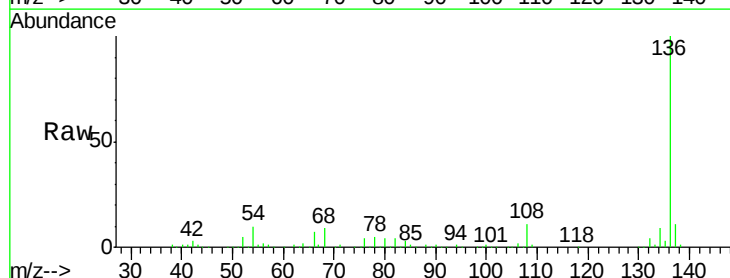



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

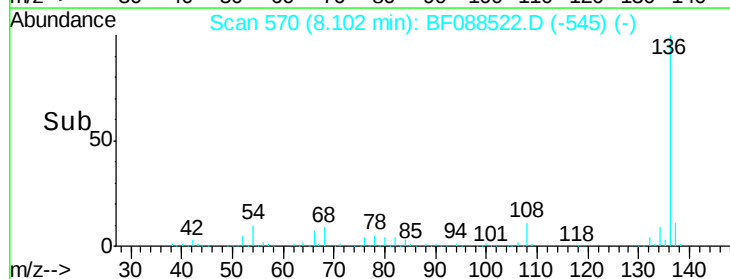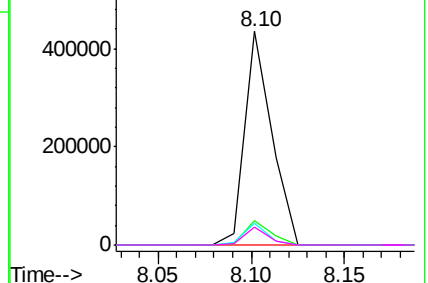


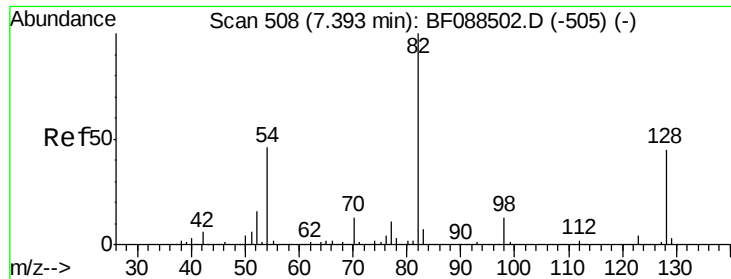




#23
 Nitrobenzene-d5
 Concen: 69.24 ng
 RT: 7.38 min Scan# 507
 Delta R.T. -0.01 min
 Lab File: BF088522.D
 Acq: 30 Jun 2016 6:14

Instrument :
 BNA_F
 ClientSampleId :
 TILCON-GF-018

Tot Ion	82	Resp	576666
Ion Ratio	Lower	Upper	
82	100		
128	39.3	35.8	53.8
54	50.6	37.1	55.7

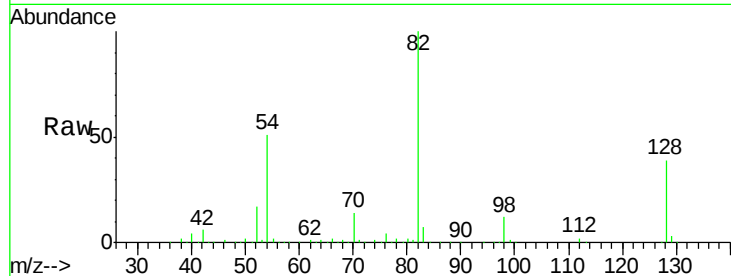


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

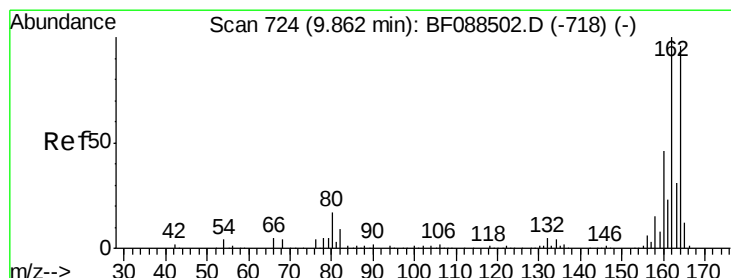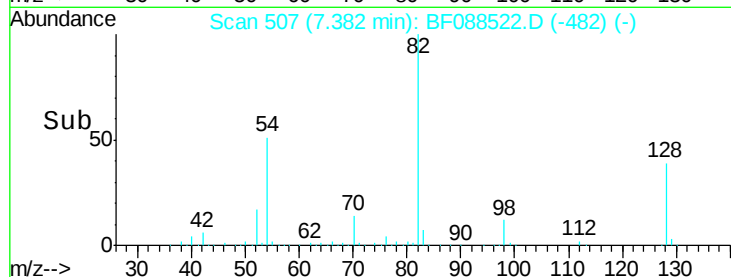
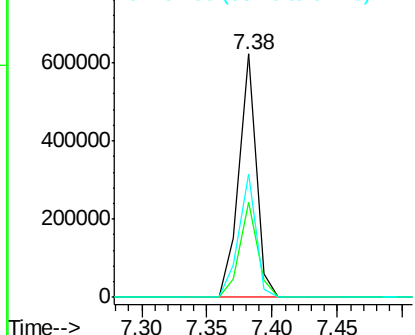



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.85 min Scan# 723
 Delta R.T. -0.01 min
 Lab File: BF088522.D
 Acq: 30 Jun 2016 6:14

Tgt Ion	164	Resp	171845
Ion Ratio	Lower	Upper	
164	100		
162	104.1	83.7	125.5
160	46.9	38.9	58.3

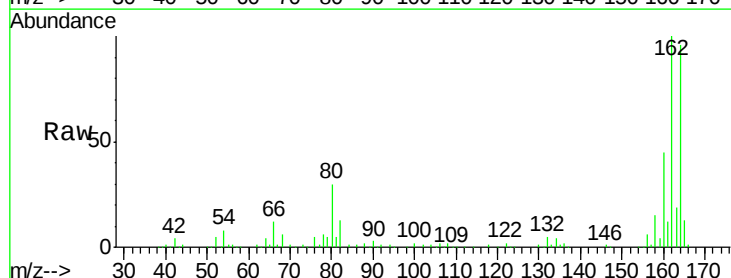

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

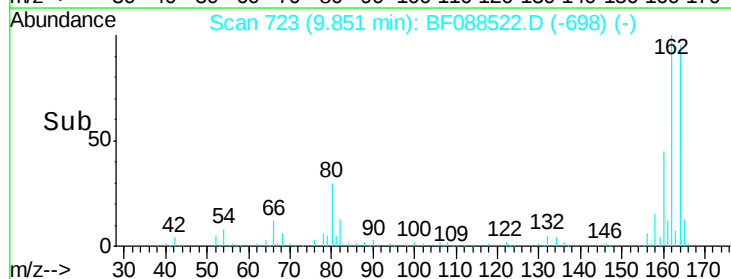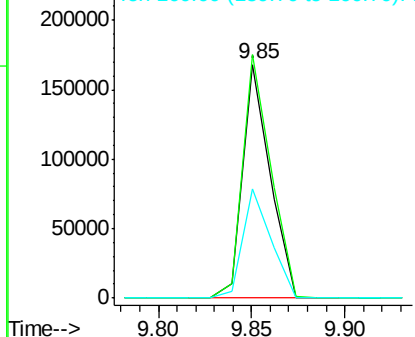


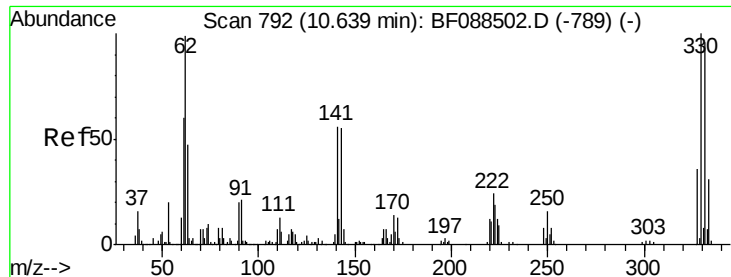




#41
 2,4,6-Tribromophenol
 Concen: 117.01 ng
 RT: 10.64 min Scan# 792
 Delta R.T. 0.00 min
 Lab File: BF088522.D
 Acq: 30 Jun 2016 6:14

Instrument :
 BNA_F
 ClientSampleId :
 TILCON-GF-018

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.8	0.0	0.0#
141	43.1	0.0	0.0#

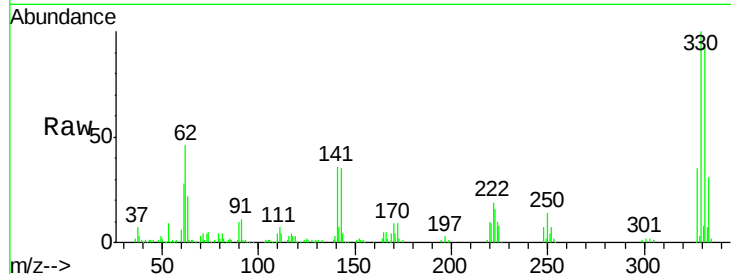


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

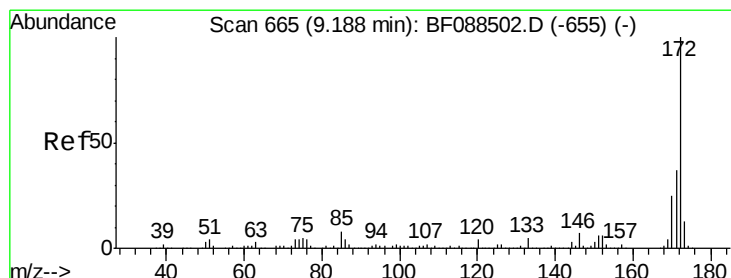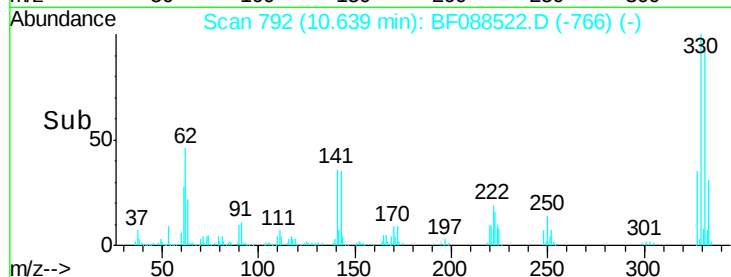
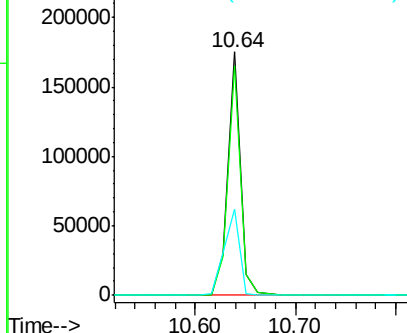



#44
 2-Fluorobiphenyl
 Concen: 92.54 ng
 RT: 9.19 min Scan# 665
 Delta R.T. 0.00 min
 Lab File: BF088522.D
 Acq: 30 Jun 2016 6:14

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.5	29.3	43.9
170	23.8	19.8	29.8

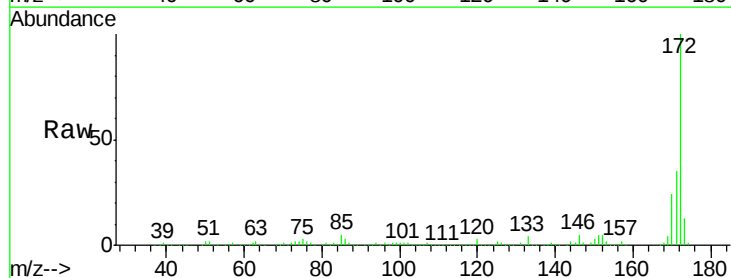

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

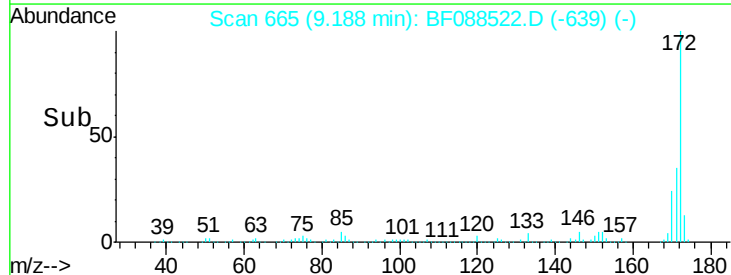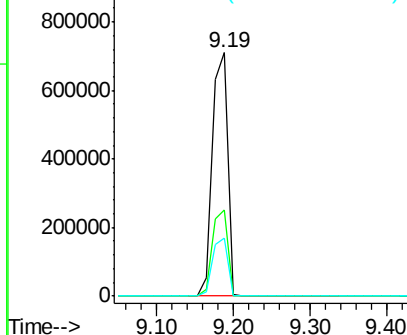


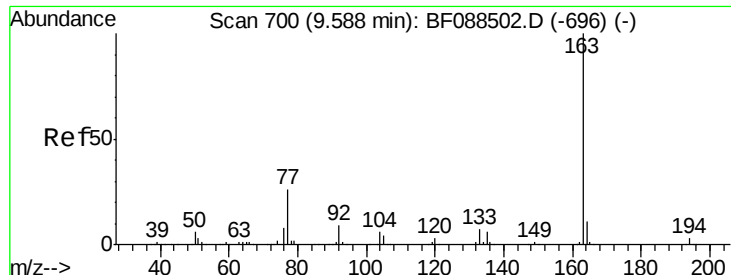




#49
Dimethylphthalate
Concen: 3.00 ng
RT: 9.58 min Scan# 699
Delta R.T. -0.01 min
Lab File: BF088522.D
Acq: 30 Jun 2016 6:14

Instrument :
BNA_F
ClientSampleId :
TILCON-GF-018

Tot Ion:163 Resp: 68854
Ion Ratio Lower Upper
163 100
194 3.4 2.6 4.0
164 9.7 8.5 12.7

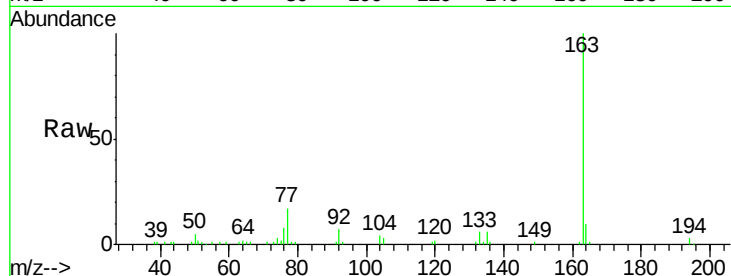


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

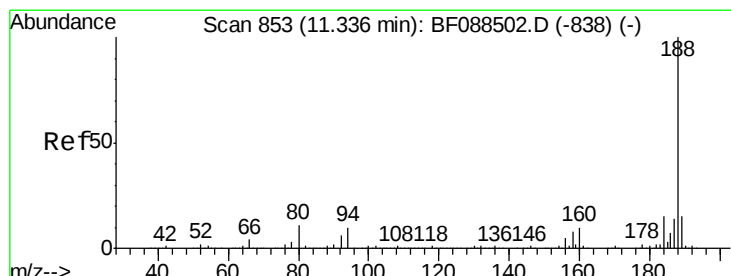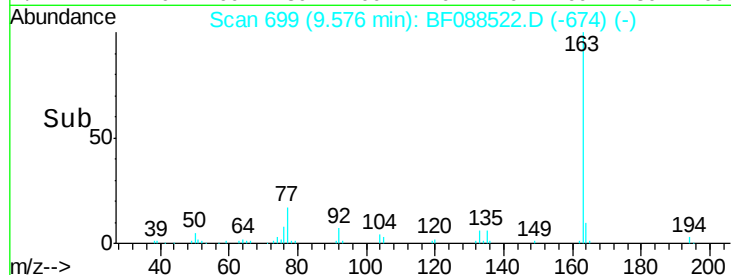
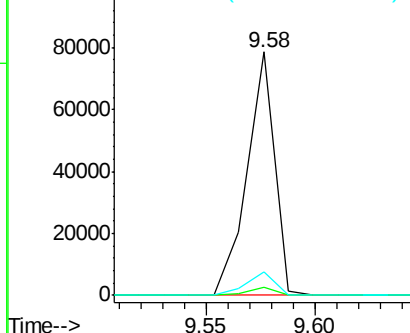



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.34 min Scan# 853
Delta R.T. 0.00 min
Lab File: BF088522.D
Acq: 30 Jun 2016 6:14

Tgt Ion:188 Resp: 316789
Ion Ratio Lower Upper
188 100
94 7.5 7.8 11.8#
80 8.0 8.7 13.1#

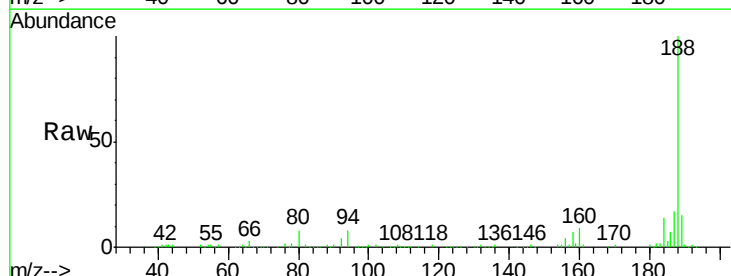

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

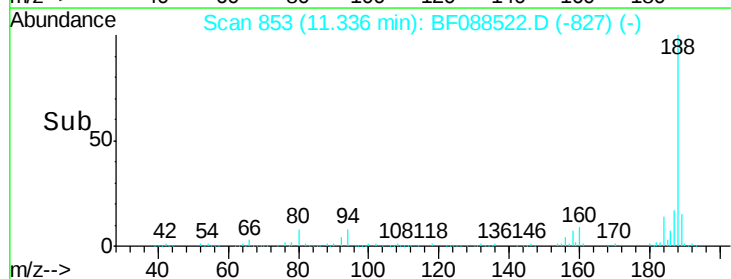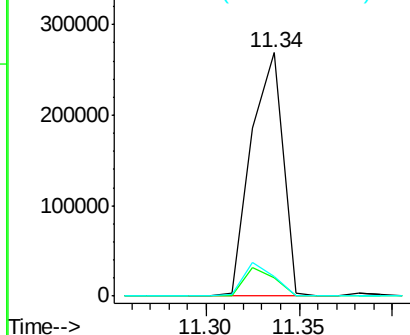

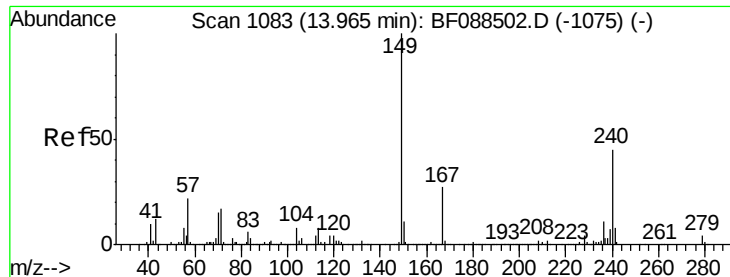

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.95 min Scan# 1082

Delta R.T. -0.01 min

Lab File: BF088522.D

Acq: 30 Jun 2016 6:14

Instrument :

BNA_F

ClientSampleId :

TILCON-GF-018


Tot Ion:240 Resp: 296903

Ion Ratio Lower Upper

240 100

120 19.0 7.1 10.7#




236 26.1 20.3 30.5

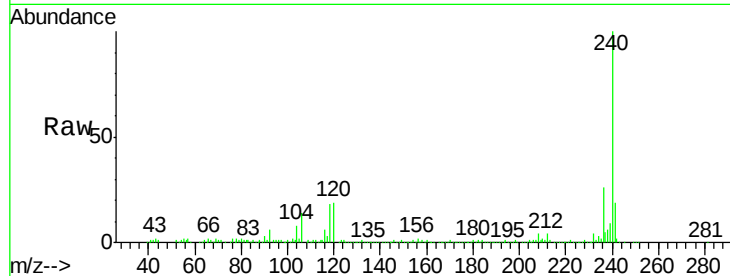

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

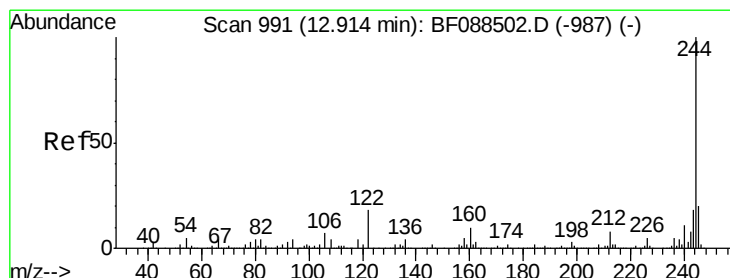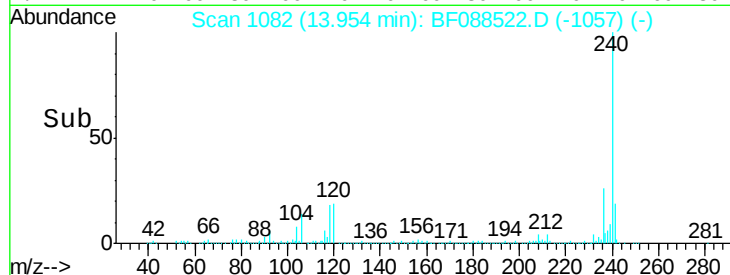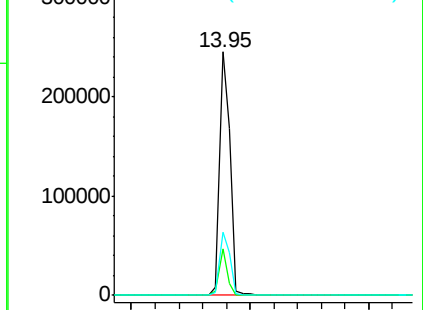

#78

Terphenyl-d14

Concen: 49.74 ng

RT: 12.91 min Scan# 991

Delta R.T. 0.00 min

Lab File: BF088522.D

Acq: 30 Jun 2016 6:14


Tgt Ion:244 Resp: 779082

Ion Ratio Lower Upper

244 100

212 8.0 6.5 9.7



122 19.3 14.8 22.2

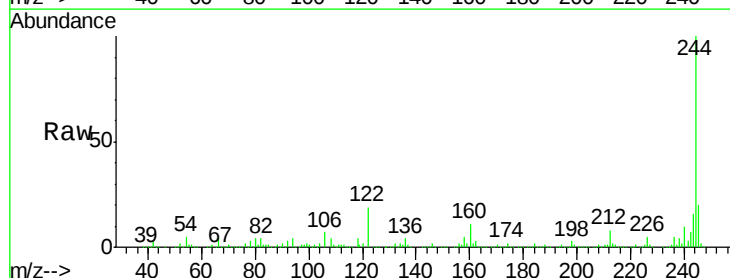


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

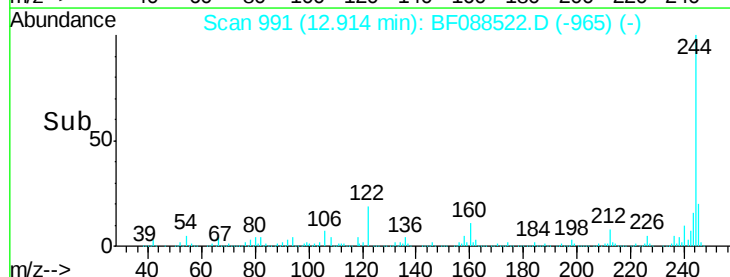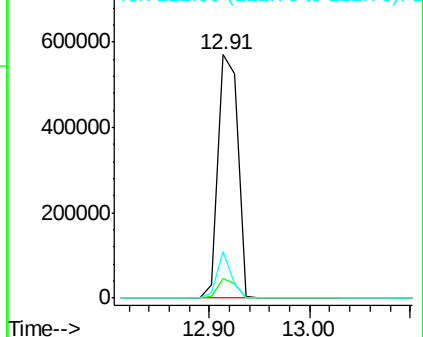


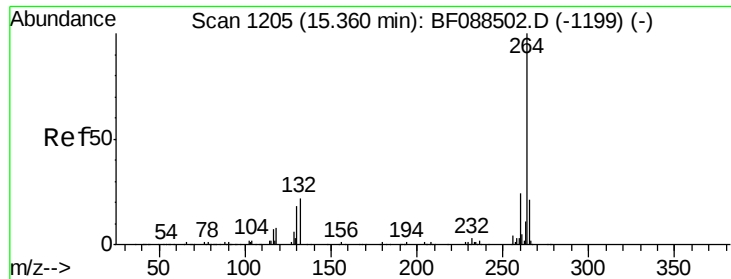

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.37 min Scan# 1206
Delta R.T. 0.01 min
Lab File: BF088522.D
Acq: 30 Jun 2016 6:14

Instrument :
BNA_F
ClientSampleId :
TILCON-GF-018

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.6	19.3	28.9
265	20.8	17.1	25.7

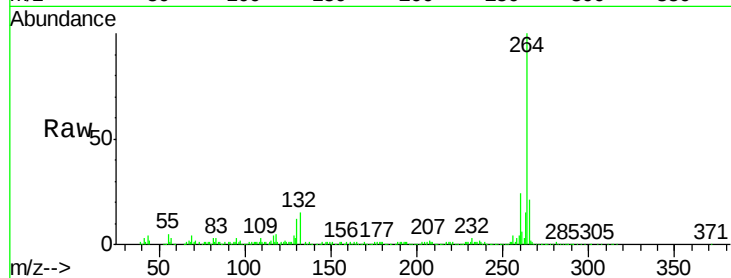

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

