


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062916\
 Data File : BF088497.D
 Acq On : 29 Jun 2016 17:10
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 30 02:07:38 2016

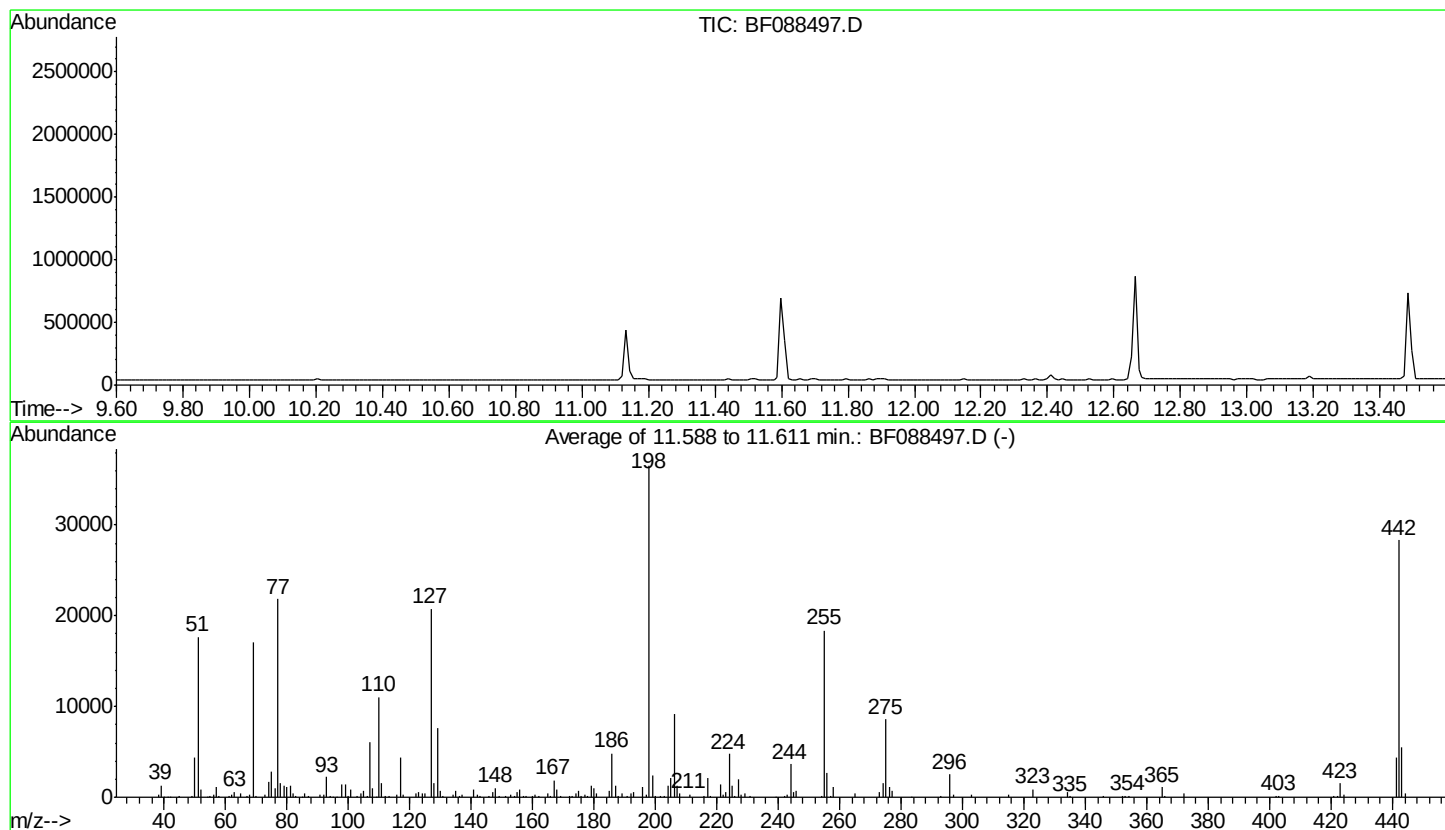

AutoFind: Scans 875, 876, 877; Background Corrected with Scan 872

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.3	17646	PASS
68	69	0.00	2	1.4	235	PASS
69	198	0.00	100	46.6	17025	PASS
70	69	0.00	2	0.9	155	PASS
127	198	10	80	56.9	20787	PASS
197	198	0.00	2	0.9	322	PASS
198	198	100	100	100.0	36561	PASS
199	198	5	9	6.6	2406	PASS
275	198	10	60	23.5	8595	PASS
365	198	1	100	2.9	1076	PASS
441	442	0.01	24	15.3	4327	PASS
442	198	50	100	77.6	28367	PASS
443	442	15	24	19.4	5499	PASS