

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062917\
 Data File : BF096307.D
 Acq On : 29 Jun 2017 22:25
 Operator : SJ/MA
 Sample : I3882-06 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G52-1.5-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.957	485	488	496	rVB	21288	23824	1.71%	0.330%
2	5.375	551	559	563	rBV	139367	124347	8.91%	1.724%
3	6.393	728	732	737	rBV	131189	121201	8.68%	1.681%
4	6.534	752	756	760	rVB	149658	117064	8.39%	1.623%
5	6.769	792	796	800	rBV	1266026	1074730	77.01%	14.902%
6	6.928	819	823	826	rBV	97419	84153	6.03%	1.167%
7	7.322	886	890	893	rBV	82878	64797	4.64%	0.898%
8	8.051	1009	1014	1018	rBV	1622818	1395576	100.00%	19.351%
9	9.128	1193	1197	1200	rVB	140241	112241	8.04%	1.556%
10	9.692	1290	1293	1296	rBV4	13423	16693	1.20%	0.231%
11	9.804	1307	1312	1316	rBV2	1386792	1218776	87.33%	16.899%
12	10.586	1441	1445	1449	rBV2	57108	49800	3.57%	0.691%
13	10.733	1465	1470	1474	rBV2	17855	26496	1.90%	0.367%
14	11.169	1540	1544	1546	rBV2	16587	17616	1.26%	0.244%
15	11.286	1560	1564	1567	rBV	1112418	953156	68.30%	13.216%
16	11.592	1612	1616	1619	rBV4	15522	19842	1.42%	0.275%
17	12.863	1829	1832	1839	rVB	101341	95676	6.86%	1.327%
18	13.916	2007	2011	2015	rBV	1124176	1003895	71.93%	13.920%
19	15.339	2250	2253	2258	rVB	569052	692050	49.59%	9.596%


Sum of corrected areas: 7211933

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062917\
Data File : BF096307.D
Acq On : 29 Jun 2017 22:25
Operator : SJ/MA
Sample : I3882-06 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G52-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

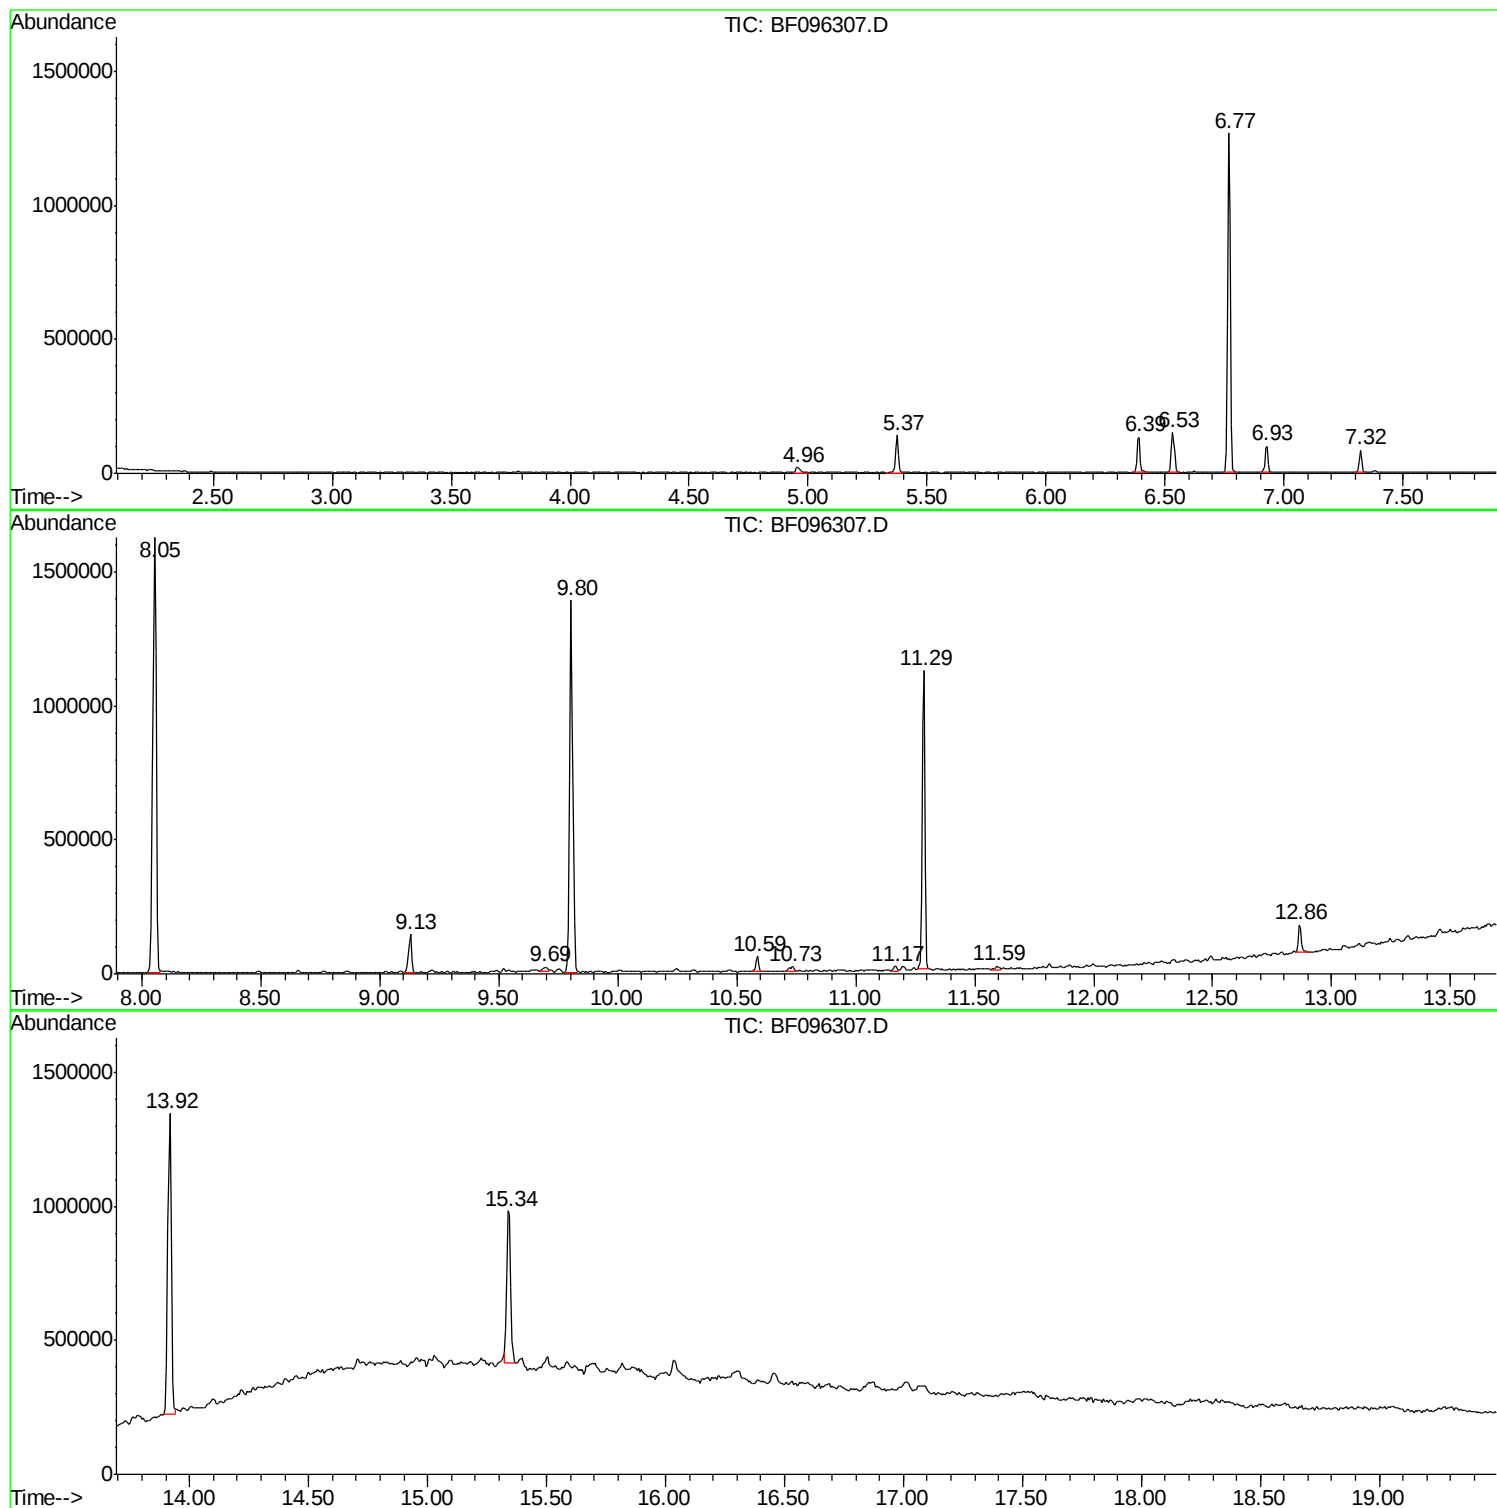

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062917\
Data File : BF096307.D
Acq On : 29 Jun 2017 22:25
Operator : SJ/MA
Sample : I3882-06 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G52-1.5-3










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.53 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.53	2.18 ng	117064	1,4-Dichlorobenzene-d4	6.77

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Aminoindole	132	C8H8N2	005192-03-0	10
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		1-Aminoindan	133	C9H11N	034698-41-4	9

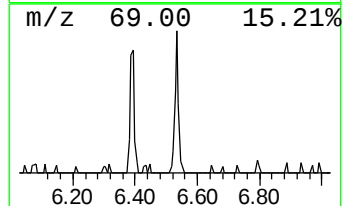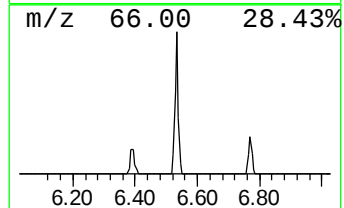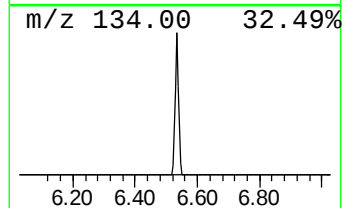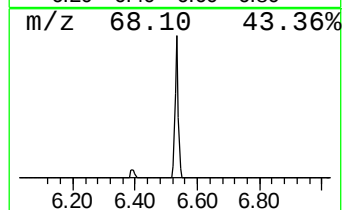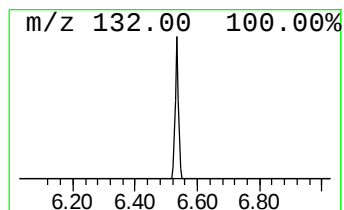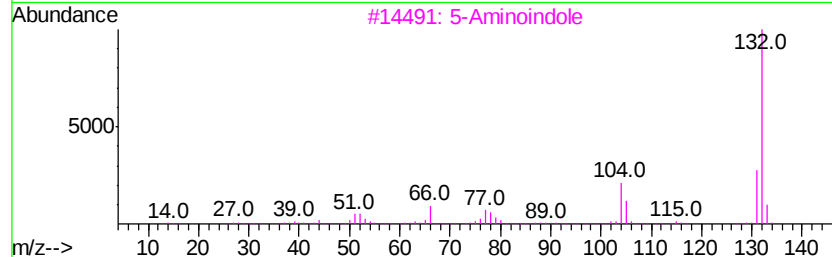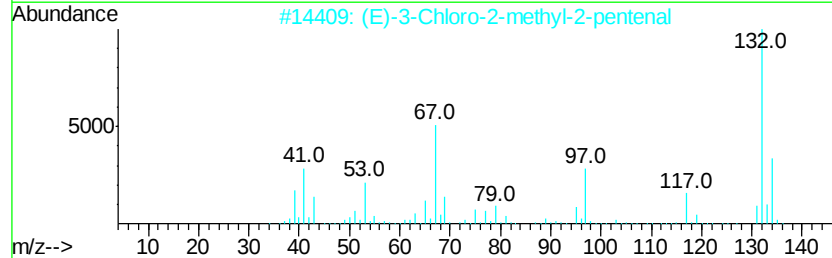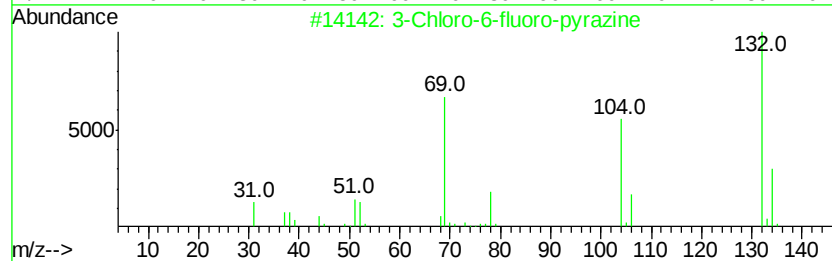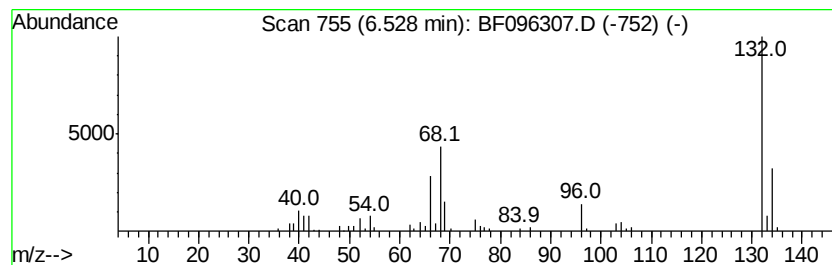

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062917\
Data File : BF096307.D
Acq On : 29 Jun 2017 22:25
Operator : SJ/MA
Sample : I3882-06 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G52-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.53	6.53	2.2	ng	117064	1	6.77	1074730	20.0