


Data Path : Z:\HPCHEM1\BNA F\Data\BF062917\
 Data File : BF096282.D
 Acq On : 29 Jun 2017 10:46
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 28 15:41:49 2017

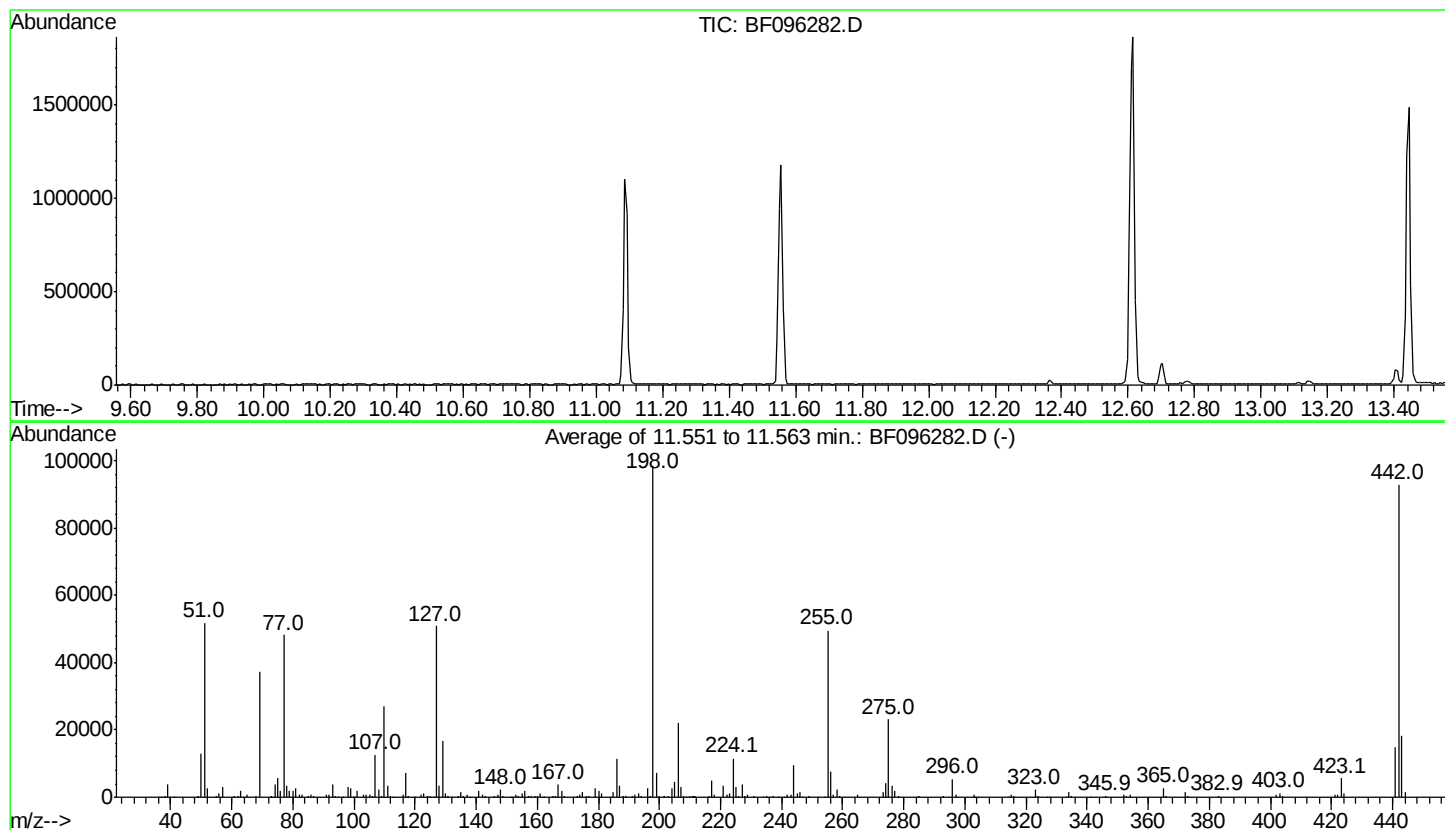

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.5	51726	PASS
68	69	0.00	2	1.2	445	PASS
69	198	0.00	100	38.0	37400	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.7	50941	PASS
197	198	0.00	2	0.5	532	PASS
198	198	100	100	100.0	98493	PASS
199	198	5	9	7.3	7185	PASS
275	198	10	60	23.5	23115	PASS
365	198	1	100	2.8	2712	PASS
441	442	0.01	24	16.1	14973	PASS
442	198	50	100	94.3	92856	PASS
443	442	15	24	19.6	18162	PASS