


Data Path : Z:\HPCHEM1\BNA F\Data\BF062917\
 Data File : BF096295.D
 Acq On : 29 Jun 2017 16:51
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 28 15:41:49 2017

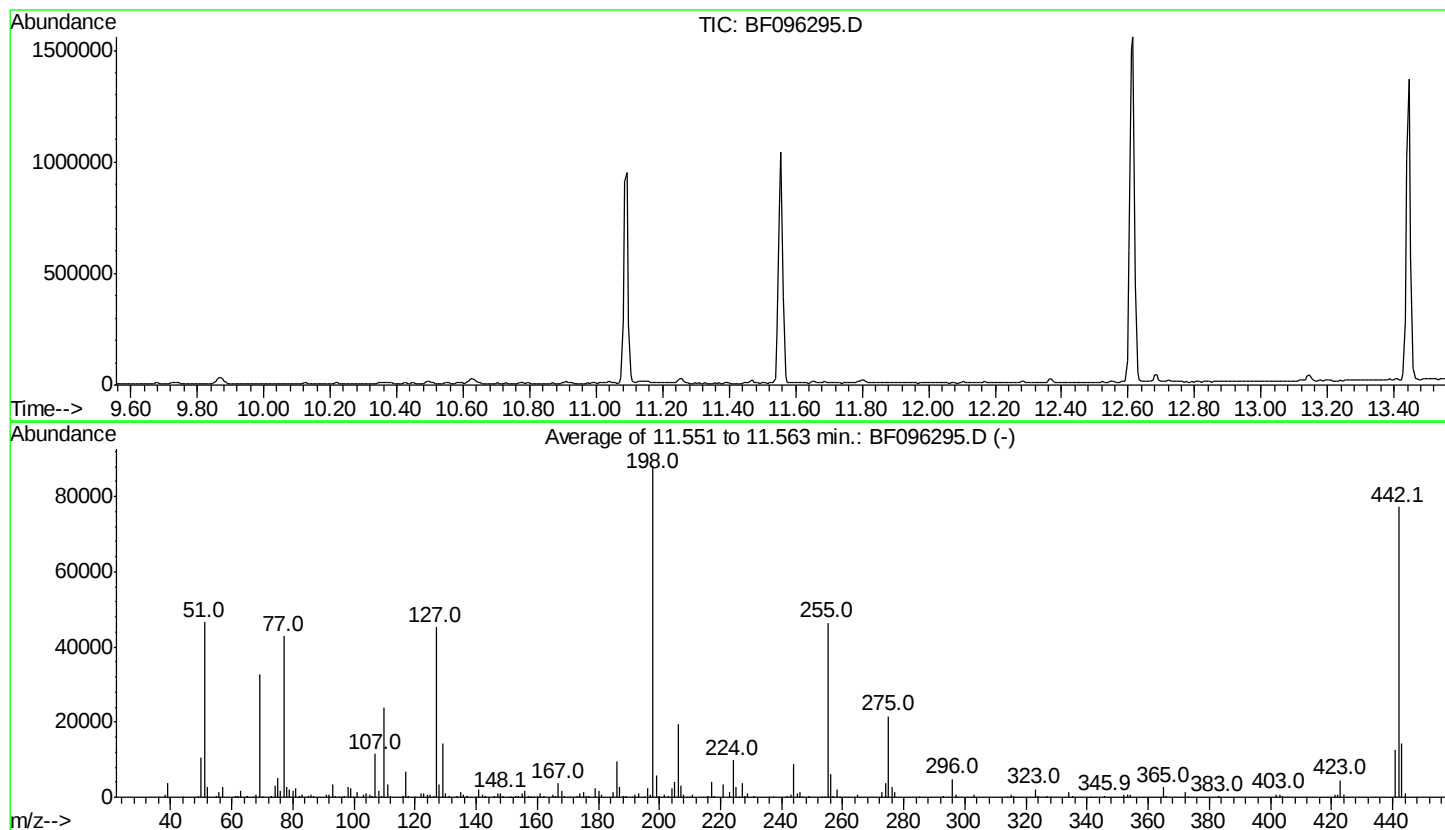

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.9	46660	PASS
68	69	0.00	2	1.7	571	PASS
69	198	0.00	100	37.0	32649	PASS
70	69	0.00	2	0.4	124	PASS
127	198	10	80	51.2	45189	PASS
197	198	0.00	2	0.7	656	PASS
198	198	100	100	100.0	88229	PASS
199	198	5	9	6.6	5804	PASS
275	198	10	60	24.4	21536	PASS
365	198	1	100	3.0	2681	PASS
441	442	0.01	24	16.2	12519	PASS
442	198	50	100	87.5	77221	PASS
443	442	15	24	18.6	14338	PASS