

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062918\
 Data File : BF106975.D
 Acq On : 29 Jun 2018 16:12
 Operator : JU/SJ
 Sample : J3677-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 147-149-B1(6-8)

Quant Time: Jun 29 18:26:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 29 11:40:02 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	72739	20.00	ng	0.00
21) Naphthalene-d8	8.24	136	267261	20.00	ng	-0.01
38) Acenaphthene-d10	10.00	164	122660	20.00	ng	-0.01
63) Phenanthrene-d10	11.49	188	206797	20.00	ng	-0.01
75) Chrysene-d12	14.15	240	196866	20.00	ng	-0.02
86) Perylene-d12	15.69	264	150013	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	426469	99.28	ng	0.00
7) Phenol-d6	6.60	99	530362	98.87	ng	-0.02
23) Nitrobenzene-d5	7.52	82	324652	67.51	ng	-0.02
41) 2,4,6-Tribromophenol	10.79	330	146885	103.32	ng	-0.01
44) 2-Fluorobiphenyl	9.31	172	604050	83.01	ng	-0.02
78) Terphenyl-d14	13.07	244	575463	70.81	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	9.70	163	67532	7.341	ng	# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062918\
Data File : BF106975.D
Acq On : 29 Jun 2018 16:12
Operator : JU/SJ
Sample : J3677-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
147-149-B1(6-8)

Quant Time: Jun 29 18:26:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 11:40:02 2018
Response via : Initial Calibration

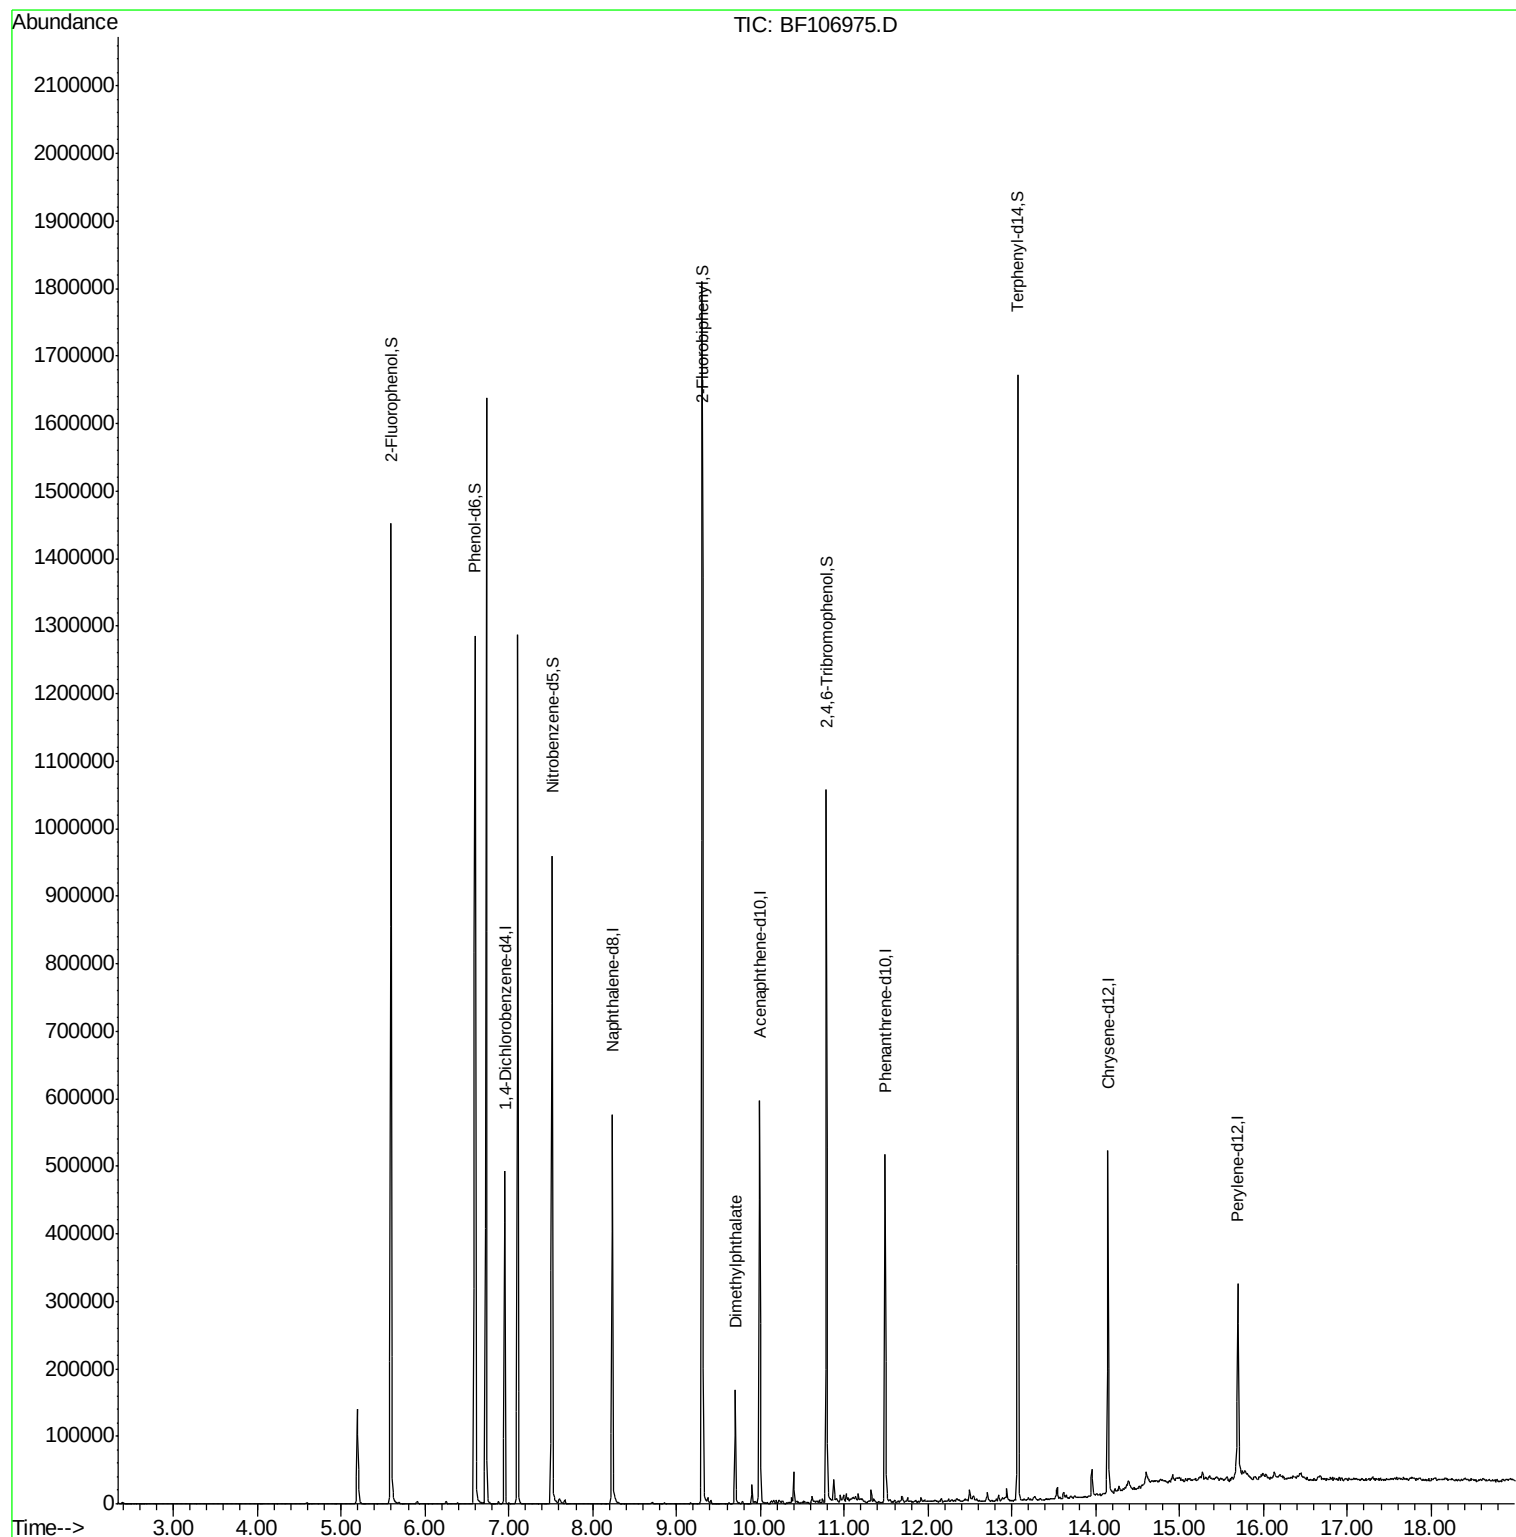

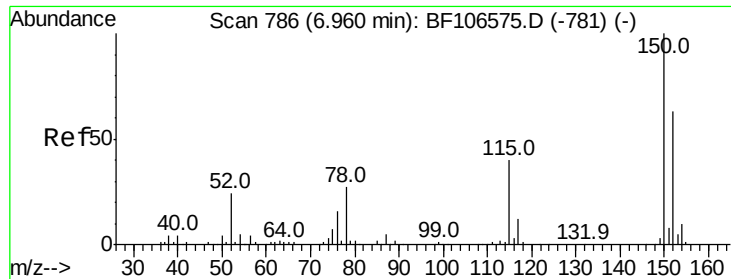


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.95 min Scan# 785
Delta R.T. -0.01 min
Lab File: BF106975.D
Acq: 29 Jun 2018 16:12

Instrument :
BNA_F
ClientSampleId :
147-149-B1(6-8)

Tot Ion:152 Resp: 72739
Ion Ratio Lower Upper
152 100
150 152.2 124.6 186.8
115 57.0 50.1 75.1

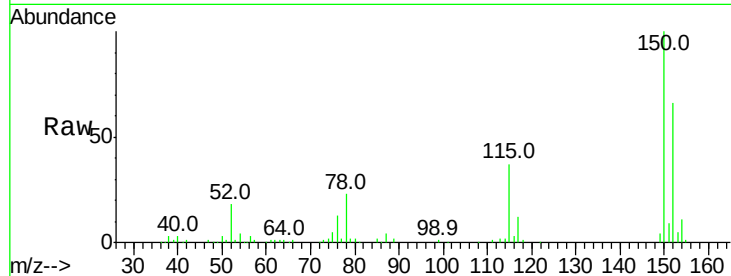


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

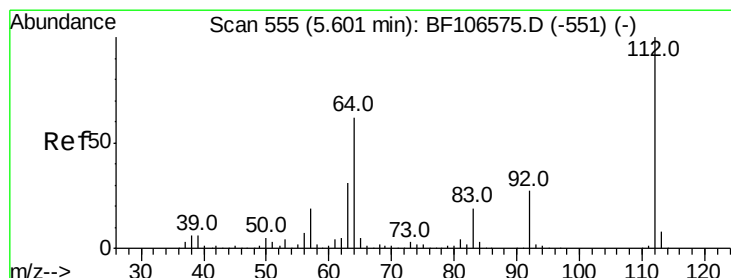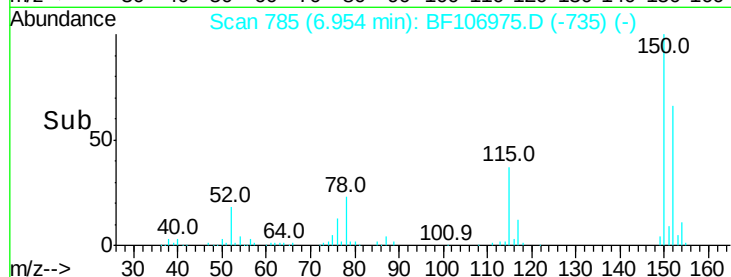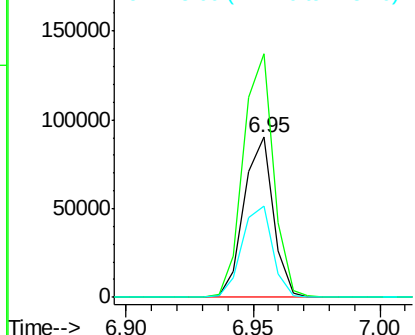



#5


2-Fluorophenol
Concen: 99.279 ng
RT: 5.60 min Scan# 554
Delta R.T. -0.01 min
Lab File: BF106975.D
Acq: 29 Jun 2018 16:12

Tgt Ion:112 Resp: 426469
Ion Ratio Lower Upper
112 100
64 58.6 47.9 71.9
63 29.6 23.7 35.5

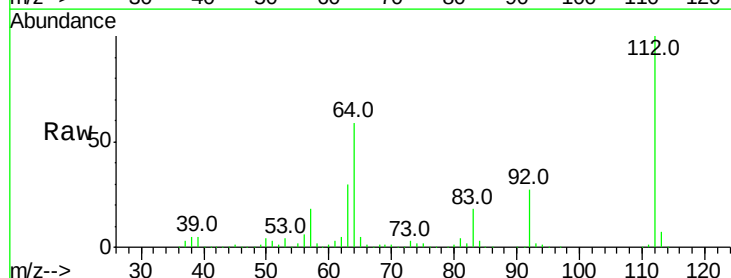

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

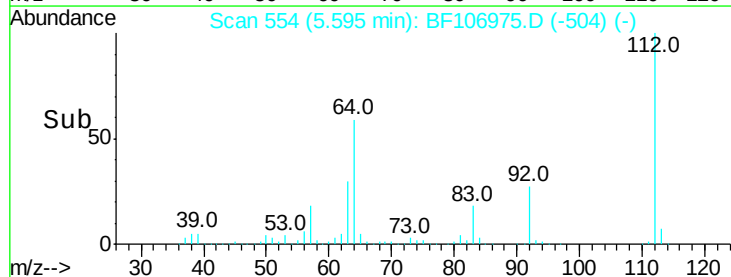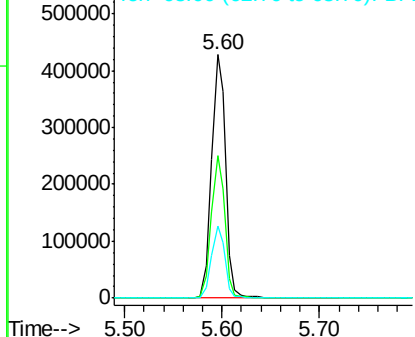

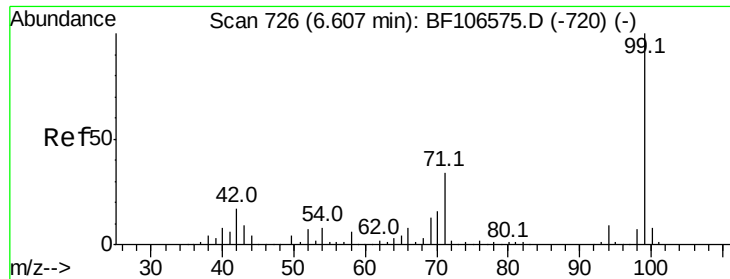

#7

Phenol-d6

Concen: 98.866 ng

RT: 6.60 min Scan# 724

Delta R.T. -0.02 min

Lab File: BF106975.D

Acq: 29 Jun 2018 16:12

Instrument :

BNA_F

ClientSampleId :

147-149-B1(6-8)


Tot Ion: 99 Resp: 530362

Ion Ratio Lower Upper




99 100

42 17.0 14.5 21.7

71 34.3 25.4 38.0

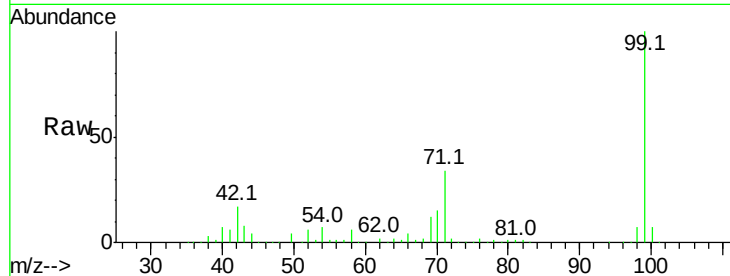

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

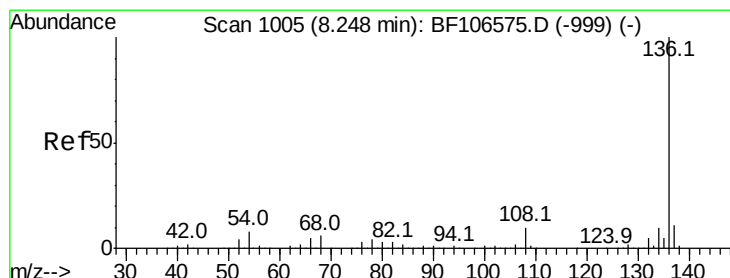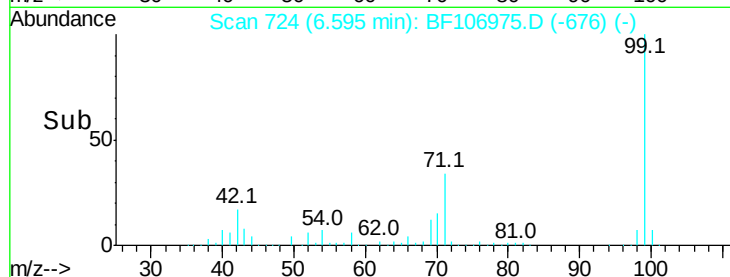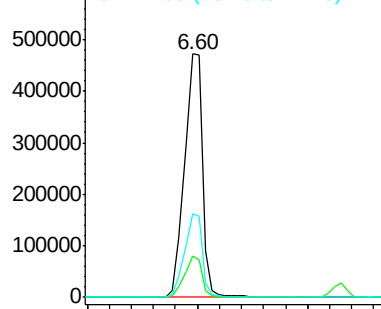

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.24 min Scan# 1003

Delta R.T. -0.01 min

Lab File: BF106975.D

Acq: 29 Jun 2018 16:12

Tgt Ion: 136 Resp: 267261


Ion Ratio Lower Upper

136 100



137 10.6 8.9 13.3


54 7.6 6.6 9.8

68 5.9 5.0 7.4

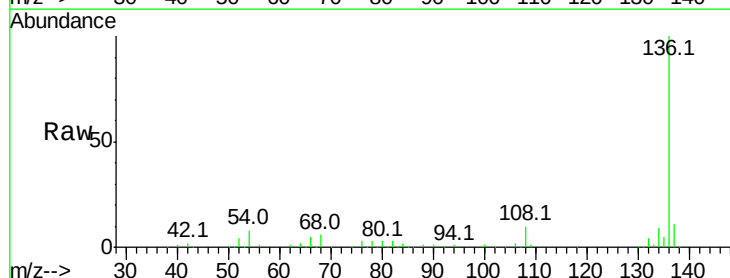

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

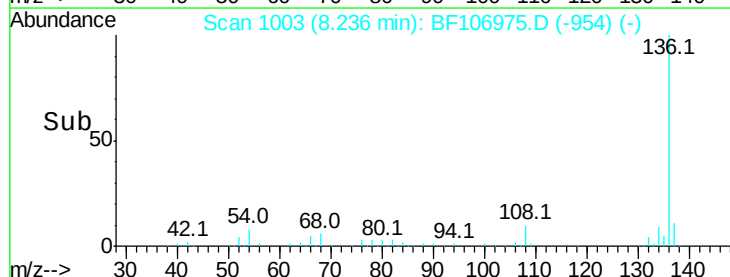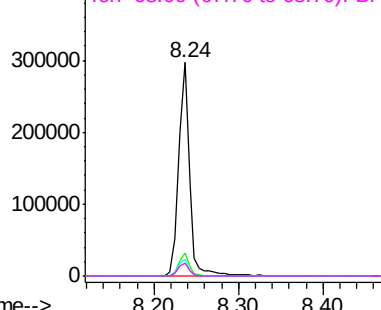


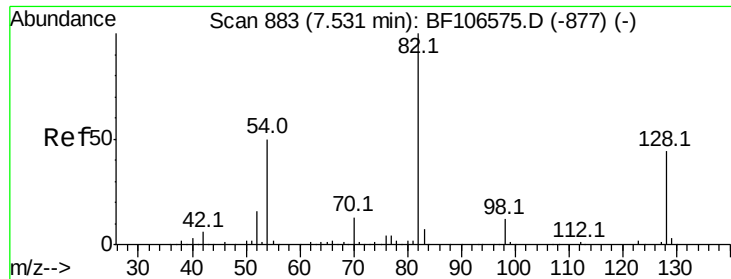




#23
 Nitrobenzene-d5
 Concen: 67.507 ng
 RT: 7.52 min Scan# 881
 Delta R.T. -0.02 min
 Lab File: BF106975.D
 Acq: 29 Jun 2018 16:12

Instrument :
 BNA_F
 ClientSampleId :
 147-149-B1(6-8)

Tot Ion	82	Resp	324652
Ion Ratio	Lower	Upper	
82	100		
128	45.9	36.1	54.1
54	47.5	41.4	62.2

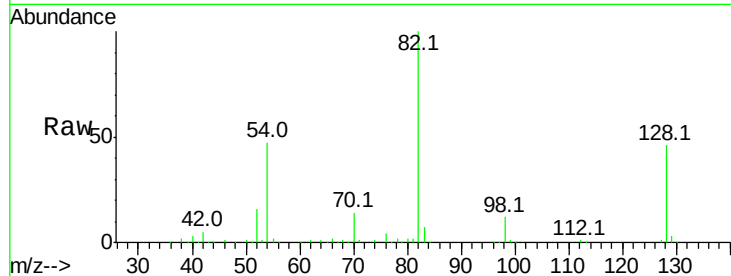


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

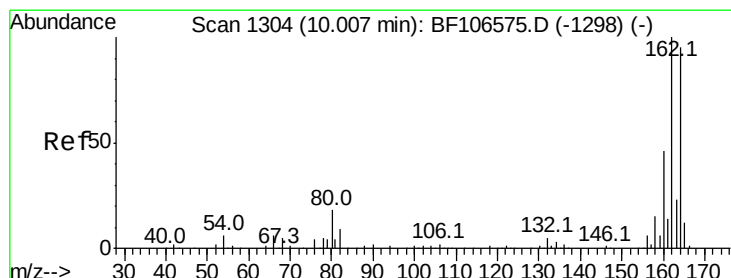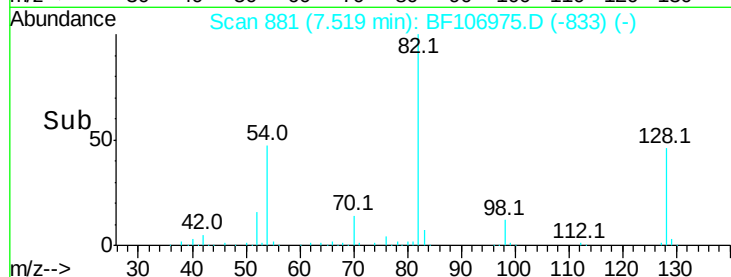
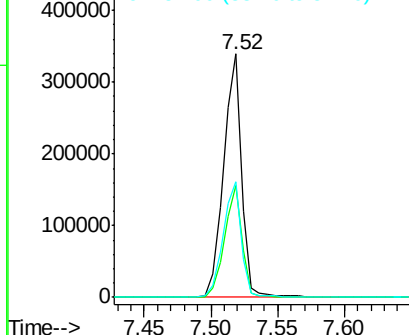



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 10.00 min Scan# 1302
 Delta R.T. -0.01 min
 Lab File: BF106975.D
 Acq: 29 Jun 2018 16:12

Tgt Ion	164	Resp	122660
Ion Ratio	Lower	Upper	
164	100		
162	97.0	86.1	129.1
160	43.0	38.3	57.5

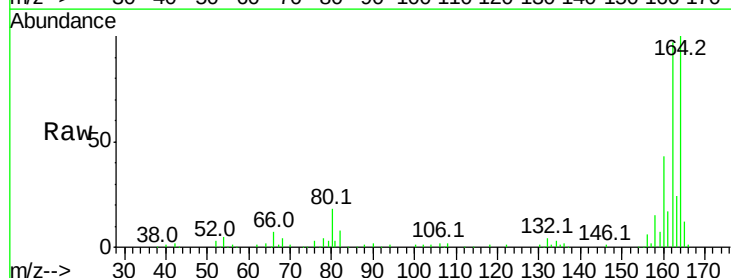

Abundance Ion 164.00 (163.70 to 164.70): BF1
 Ion 162.00 (161.70 to 162.70): BF1
 Ion 160.00 (159.70 to 160.70): BF1



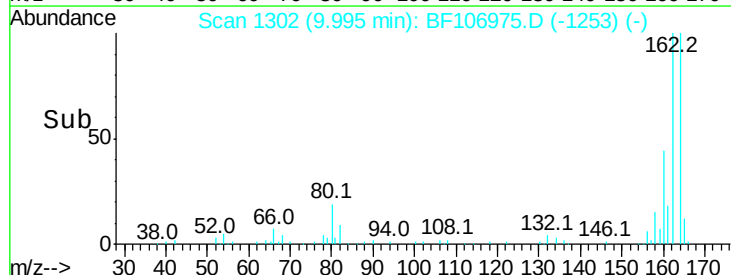
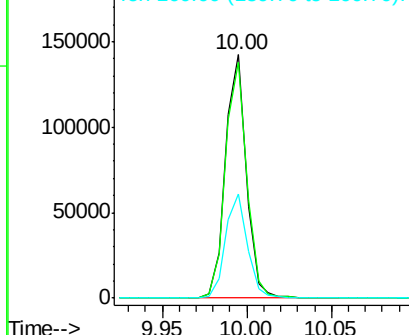


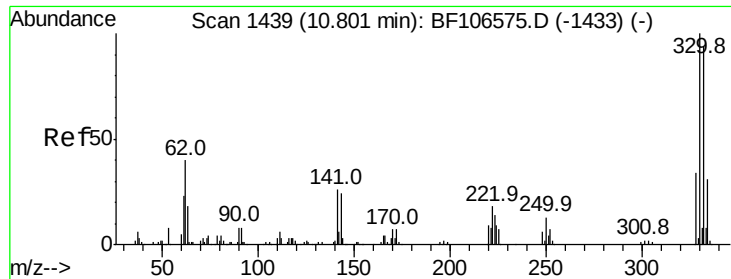

#41
 2,4,6-Tribromophenol
 Concen: 103.319 ng
 RT: 10.79 min Scan# 1437
 Delta R.T. -0.01 min
 Lab File: BF106975.D
 Acq: 29 Jun 2018 16:12




Instrument :
 BNA_F
 ClientSampleId :
 147-149-B1(6-8)


Tot Ion	Ratio	Lower	Upper
330	100		
332	97.1	77.0	115.6
141	23.2	29.9	44.9#

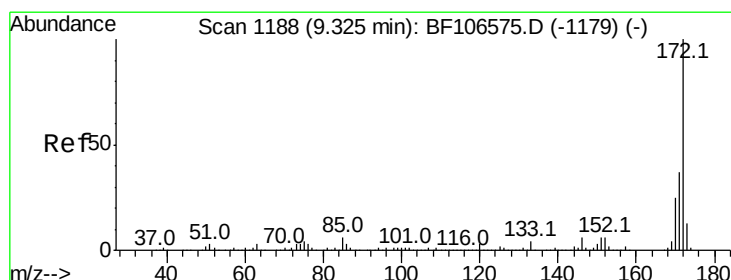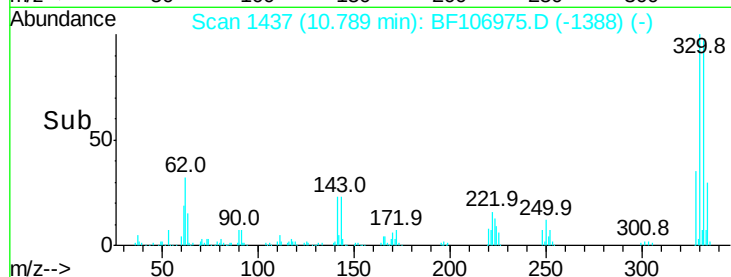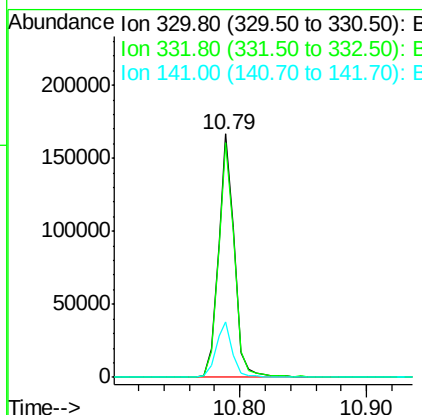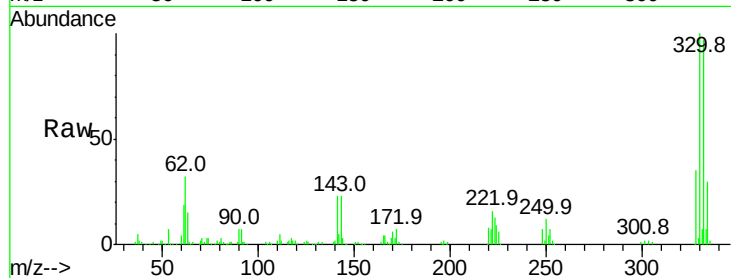

#44
 2-Fluorobiphenyl
 Concen: 83.009 ng
 RT: 9.31 min Scan# 1185
 Delta R.T. -0.02 min
 Lab File: BF106975.D
 Acq: 29 Jun 2018 16:12

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.6	29.7	44.5
170	24.2	19.6	29.4


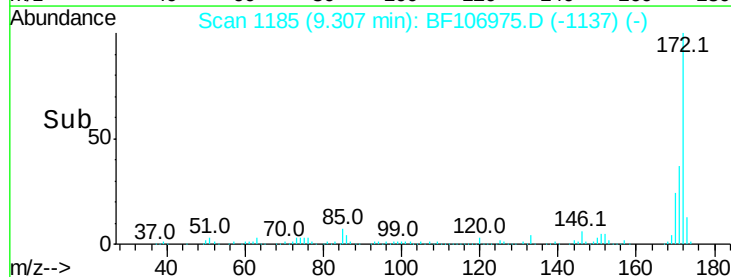
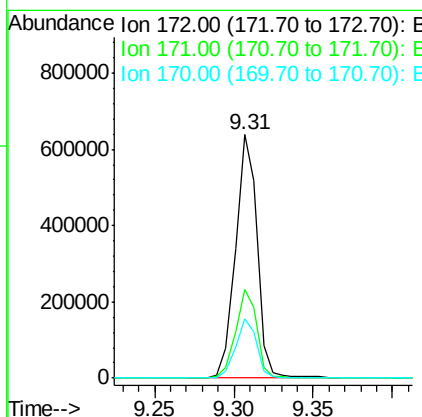
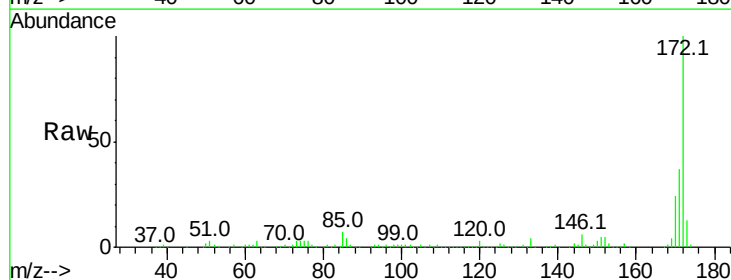


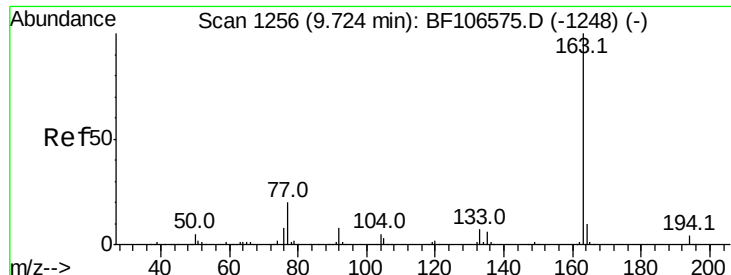

#49
Dimethylphthalate
Concen: 7.341 ng
RT: 9.70 min Scan# 1252
Delta R.T. -0.02 min
Lab File: BF106975.D
Acq: 29 Jun 2018 16:12




Instrument :
BNA_F
ClientSampleId :
147-149-B1(6-8)


Tot Ion:163 Resp: 67532
Ion Ratio Lower Upper
163 100
194 4.1 2.7 4.1#
164 10.7 8.2 12.2

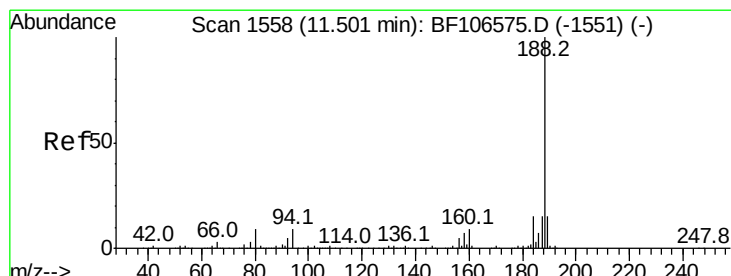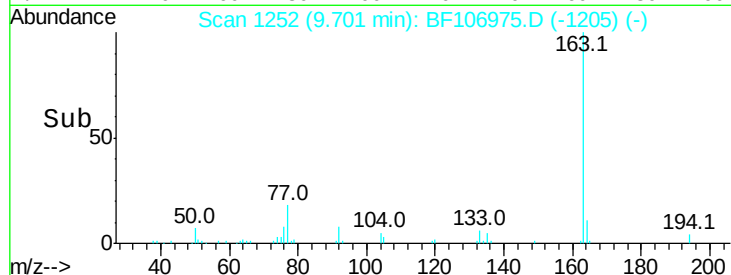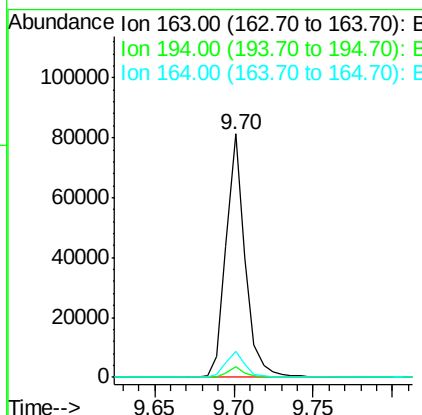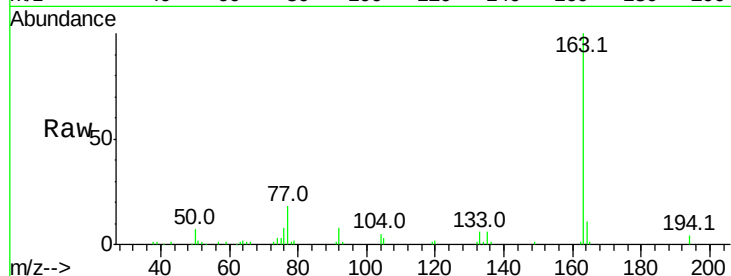

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.49 min Scan# 1556
Delta R.T. -0.01 min
Lab File: BF106975.D
Acq: 29 Jun 2018 16:12

Tgt Ion:188 Resp: 206797
Ion Ratio Lower Upper
188 100
94 8.0 8.5 12.7#
80 8.6 9.2 13.8#

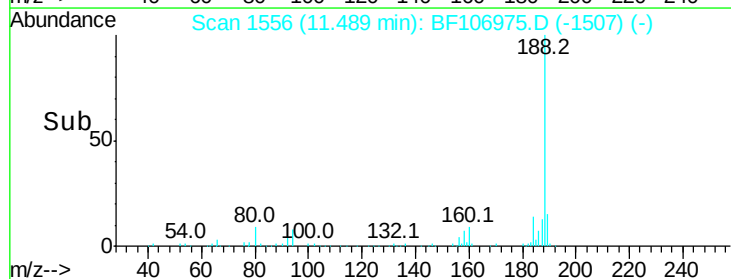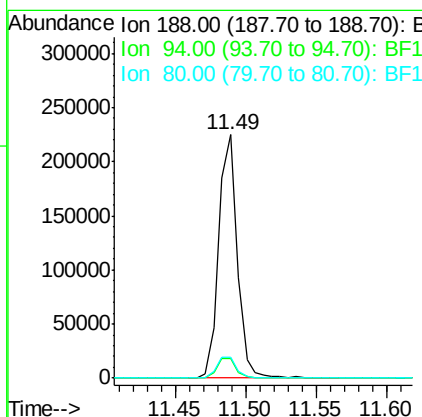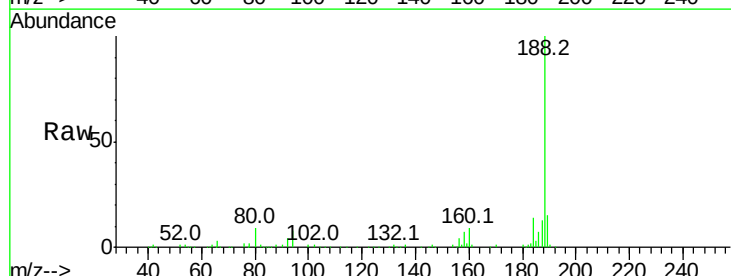

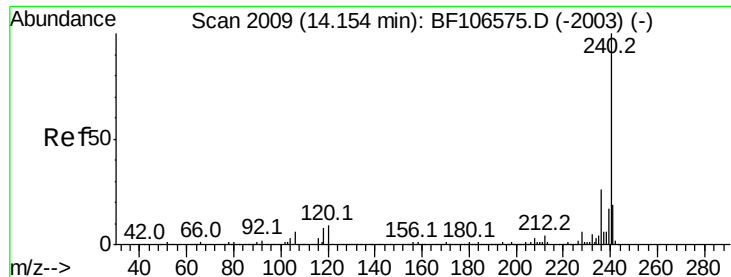

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.15 min Scan# 2008

Delta R.T. -0.02 min

Lab File: BF106975.D

Acq: 29 Jun 2018 16:12

Instrument :

BNA_F

ClientSampleId :

147-149-B1(6-8)


Tot Ion:240 Resp: 196866

Ion Ratio Lower Upper

240 100

120 8.4 9.5 14.3#




236 25.2 20.7 31.1

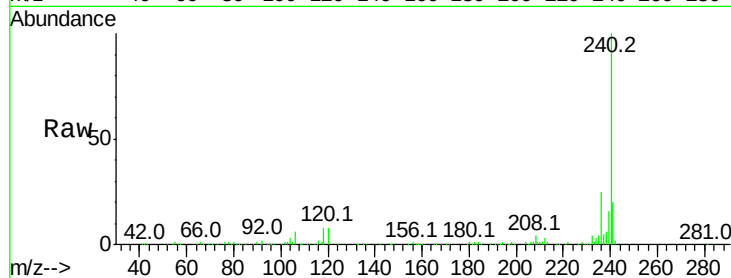

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

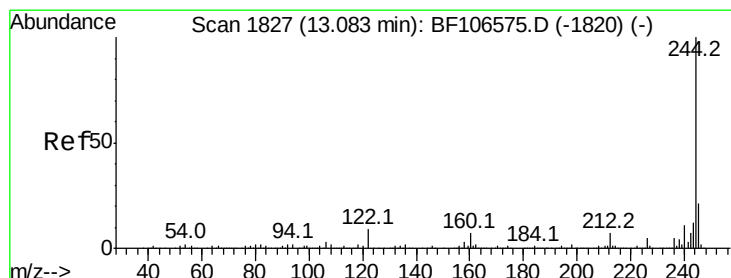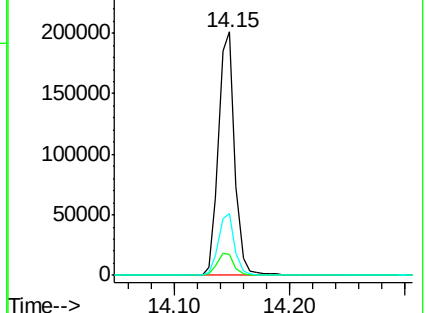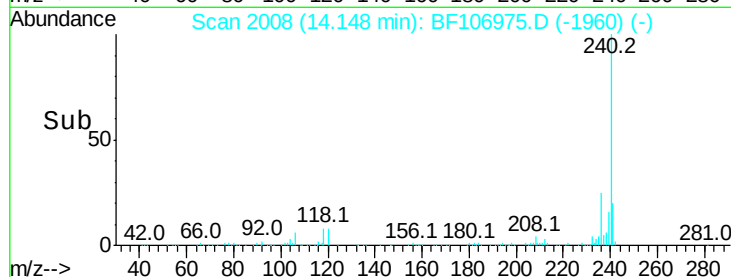

#78

Terphenyl-d14

Concen: 70.807 ng

RT: 13.07 min Scan# 1825

Delta R.T. -0.01 min

Lab File: BF106975.D

Acq: 29 Jun 2018 16:12


Tgt Ion:244 Resp: 575463

Ion Ratio Lower Upper

244 100

212 6.4 5.4 8.0



122 8.7 11.0 16.4#

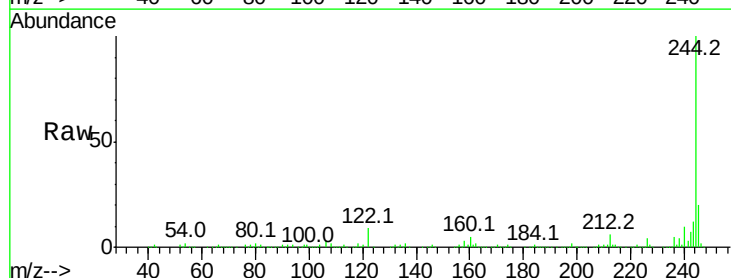


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

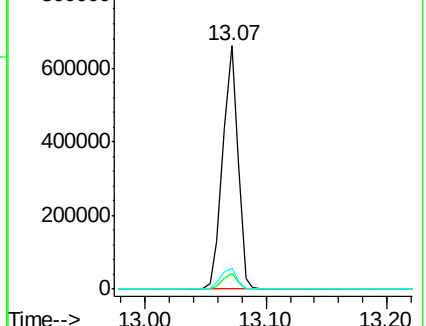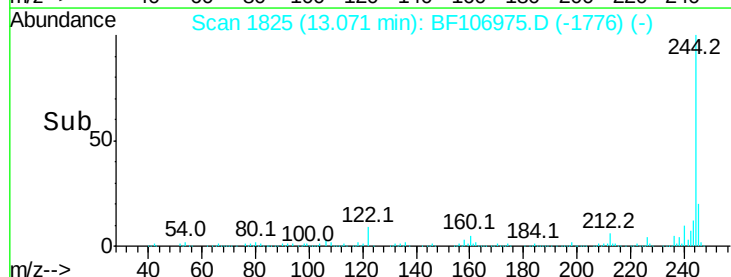

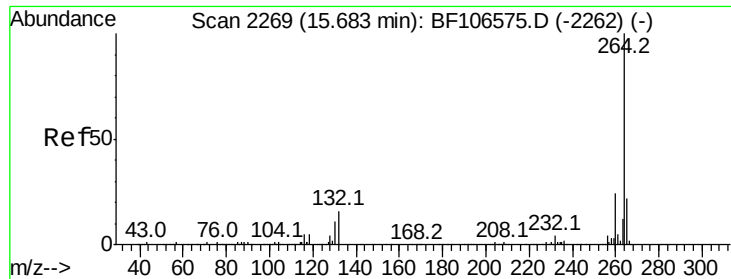

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.69 min Scan# 2271
Delta R.T. -0.02 min
Lab File: BF106975.D
Acq: 29 Jun 2018 16:12

Instrument :
BNA_F
ClientSampleId :
147-149-B1(6-8)

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.0	19.2	28.8
265	21.2	17.5	26.3

