


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062918\
 Data File : BF106988.D
 Acq On : 29 Jun 2018 22:27
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 29 14:38:29 2018

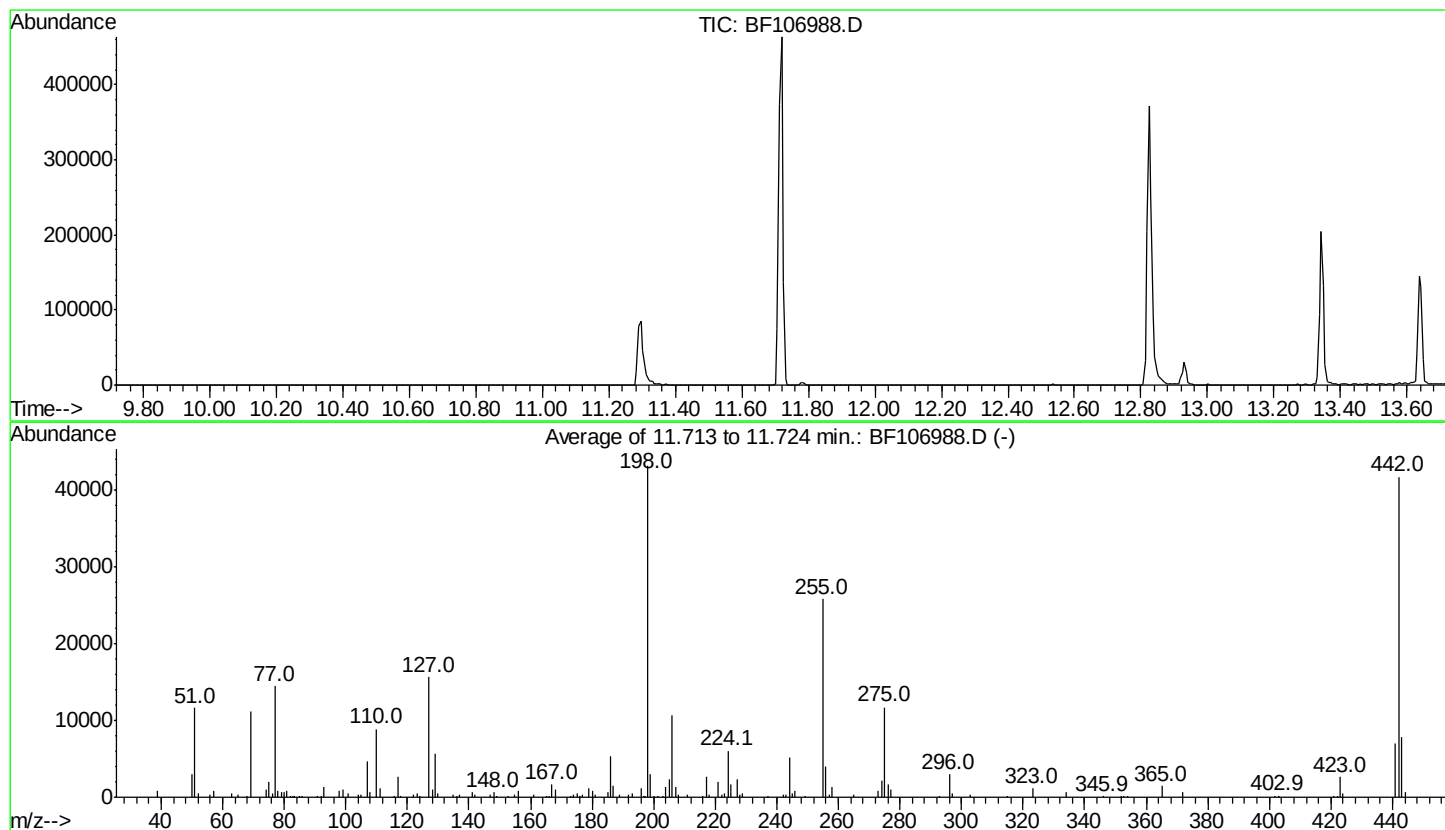

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	11637	PASS
68	69	0.00	2	0.9	101	PASS
69	198	0.00	100	25.8	11123	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	36.2	15617	PASS
197	198	0.00	2	0.3	114	PASS
198	198	100	100	100.0	43162	PASS
199	198	5	9	6.9	2994	PASS
275	198	10	60	27.1	11711	PASS
365	198	1	100	3.4	1481	PASS
441	443	0.01	100	88.3	6983	PASS
442	198	50	100	96.6	41680	PASS
443	442	15	24	19.0	7905	PASS