
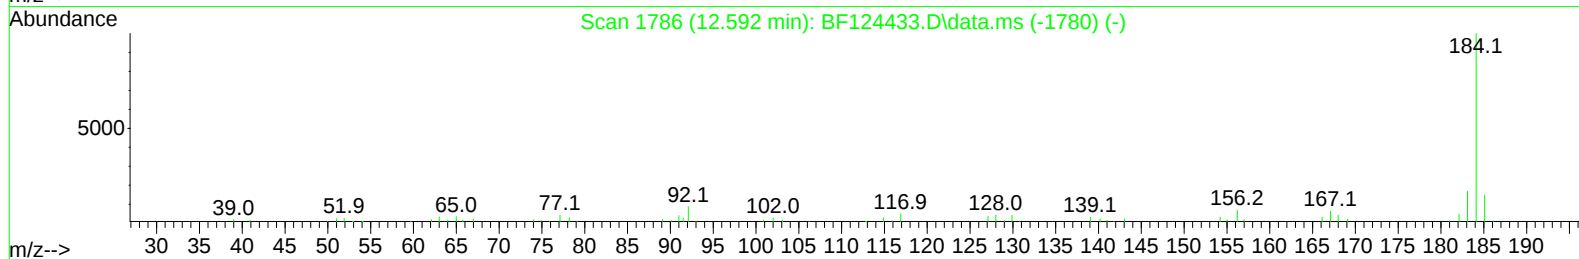
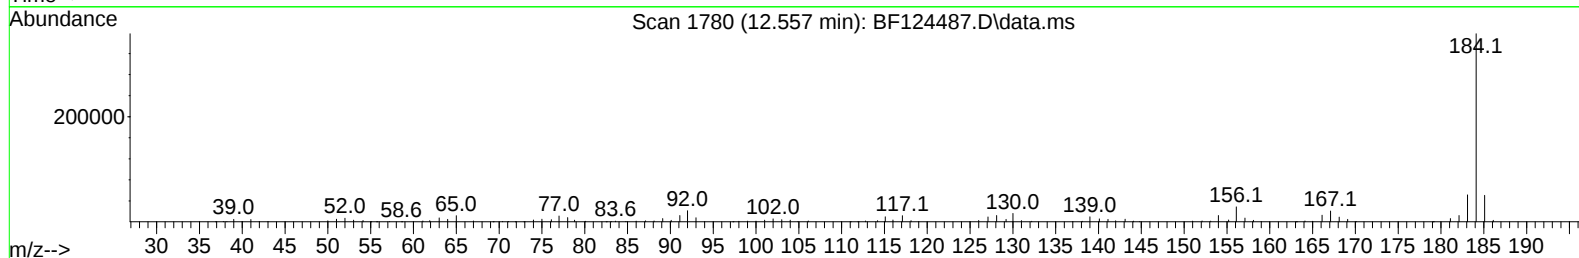


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062921\  
Data File : BF124487.D  
Acq On    : 29 Jun 2021  11:41  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jun 29 12:27:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 28 16:01:42 2021
Response via : Initial Calibration

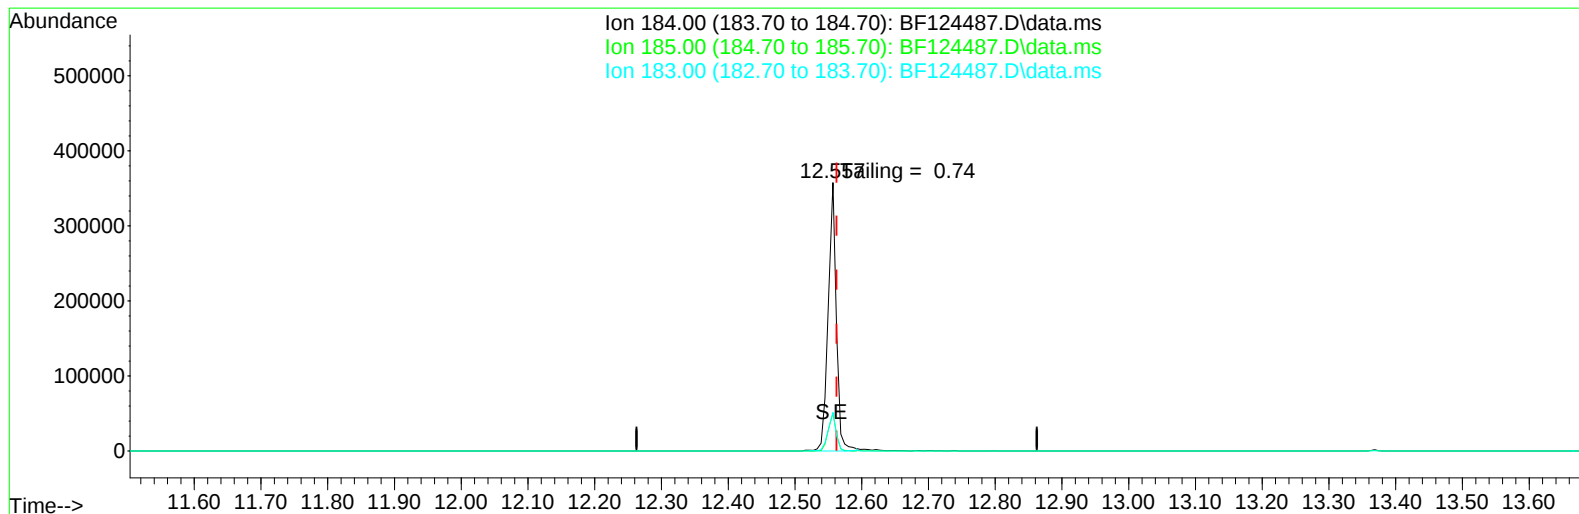

TIC: BF124487.D\data.ms

(77) Benzidine




12.557min (-0.006) 0.00 ng

response **309035**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.15
183.00	9.80	14.36#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062921\
Data File : BF124487.D
Acq On : 29 Jun 2021 11:41
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 12:27:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 28 16:01:42 2021
Response via : Initial Calibration

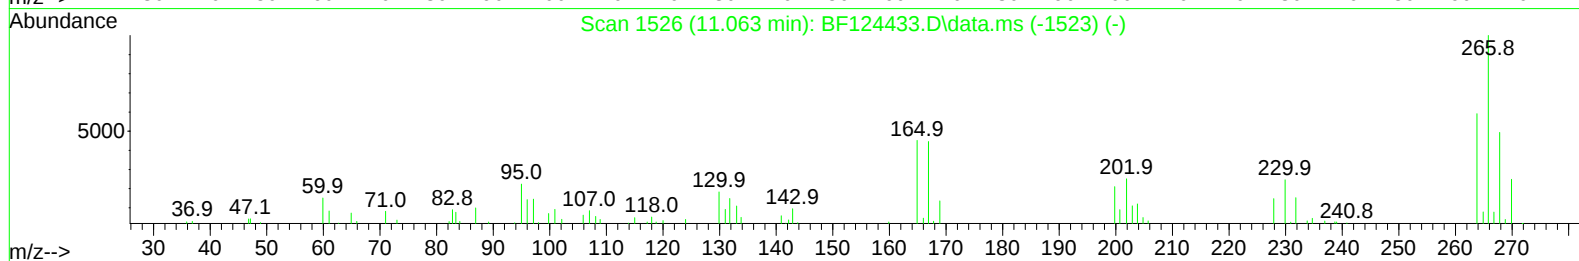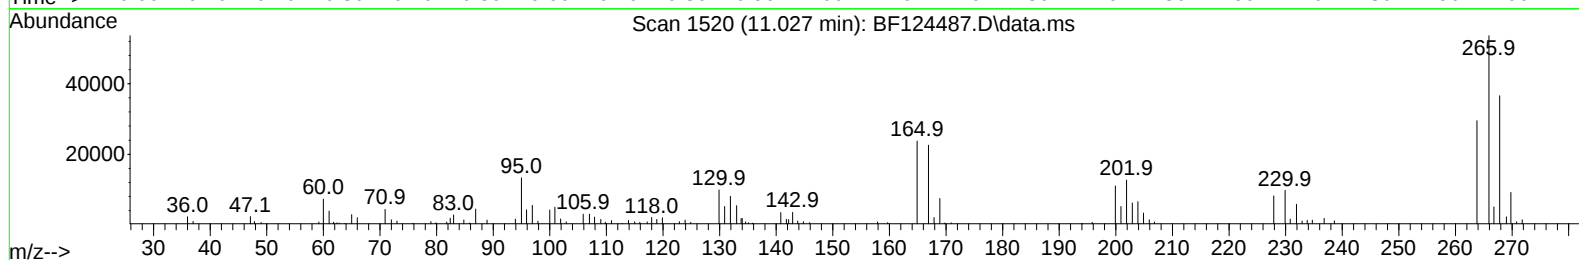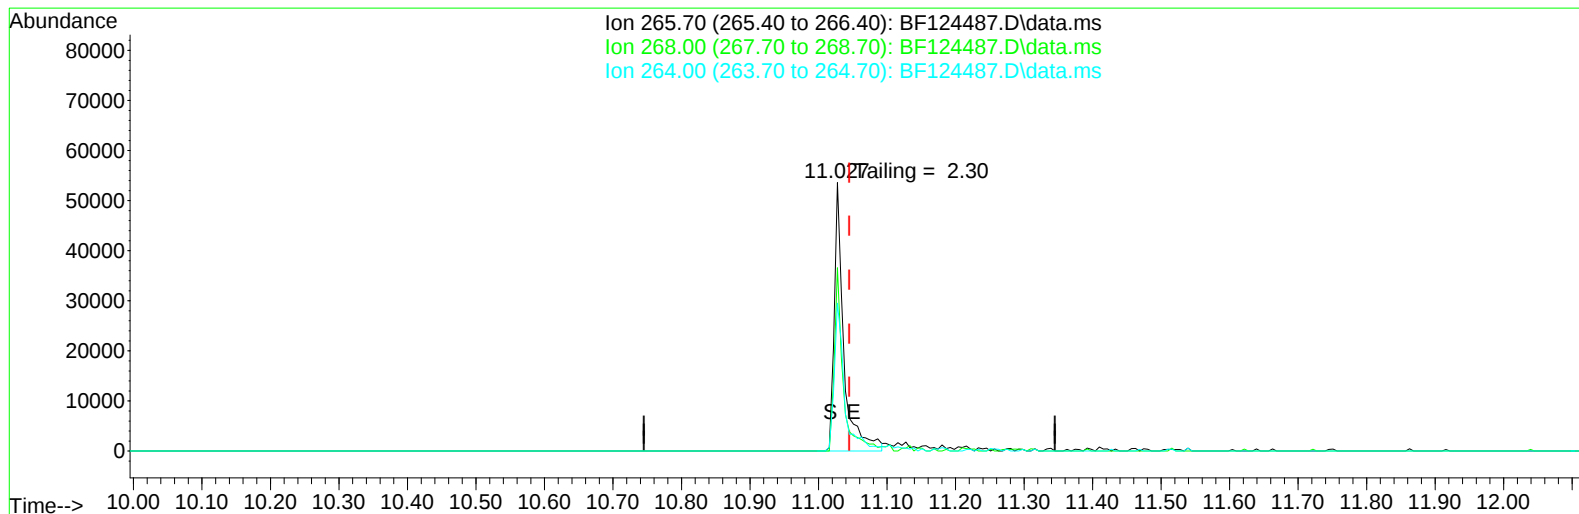

TIC: BF124487.D\data.ms

(70) Pentachlorophenol (C)

11.027min (-0.018) 23420.42 ng

response 53659

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	68.29
264.00	65.70	55.08
0.00	0.00	0.00