
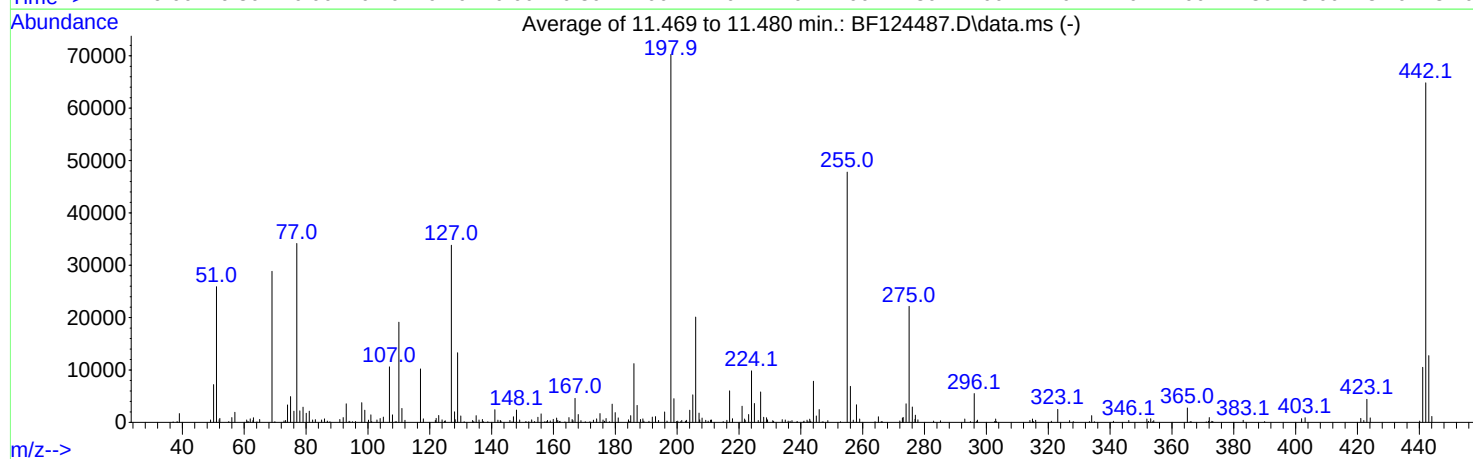


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062921\
 Data File : BF124487.D
 Acq On : 29 Jun 2021 11:41
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 29 12:49:33 2021

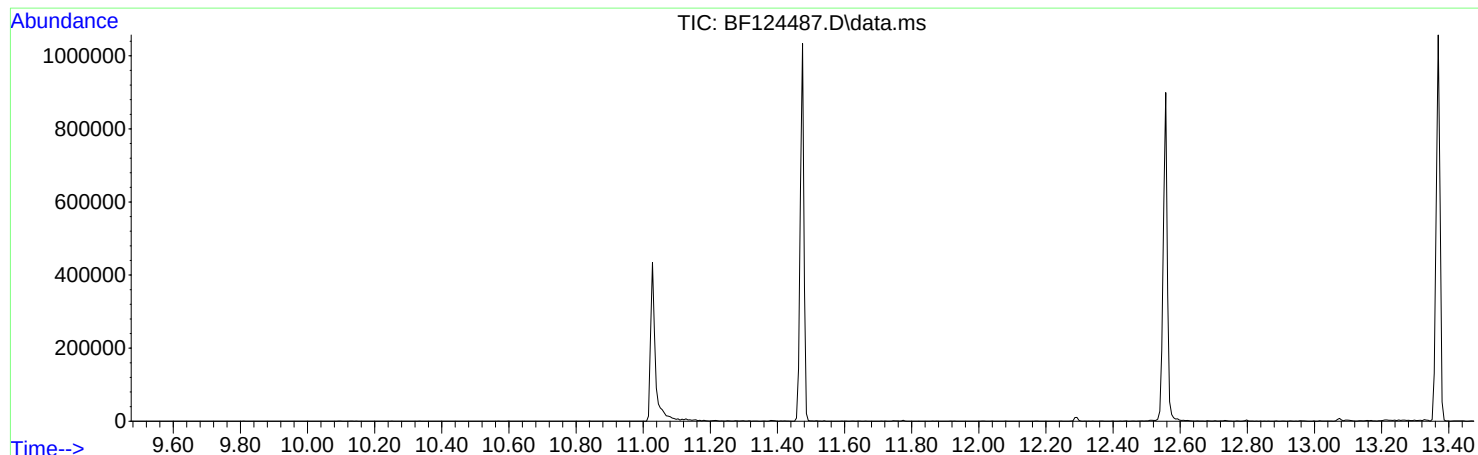

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	25907	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.1	28855	PASS
70	69	0.00	2	0.4	113	PASS
127	198	10	80	48.2	33833	PASS
197	198	0.00	2	0.3	244	PASS
198	198	100	100	100.0	70248	PASS
199	198	5	9	6.4	4512	PASS
275	198	10	60	31.5	22146	PASS
365	198	1	100	3.9	2758	PASS
441	198	0.01	100	15.0	10510	PASS
442	442	50	100	100.0	64835	PASS
443	442	15	24	19.6	12729	PASS