
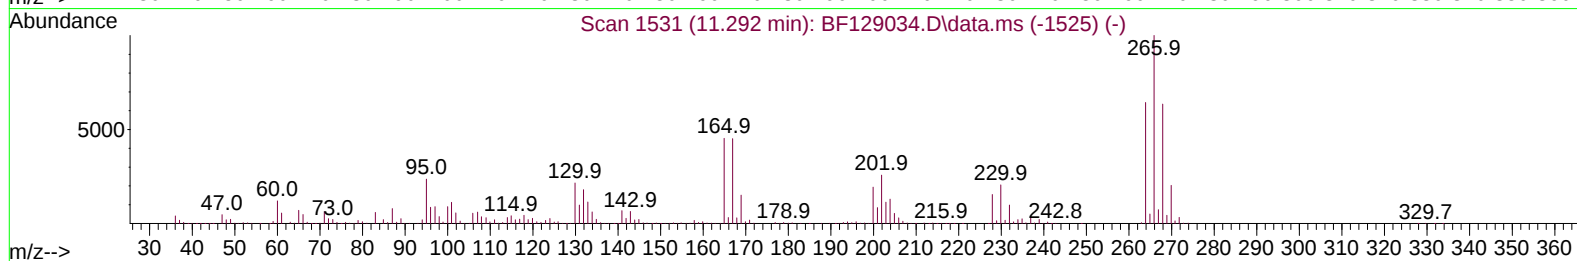
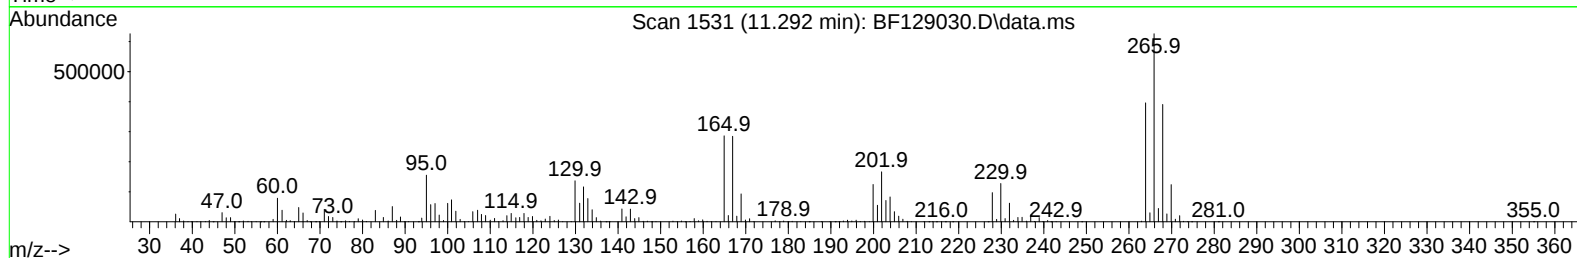


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062922\
Data File : BF129030.D
Acq On : 29 Jun 2022 12:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 17:07:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

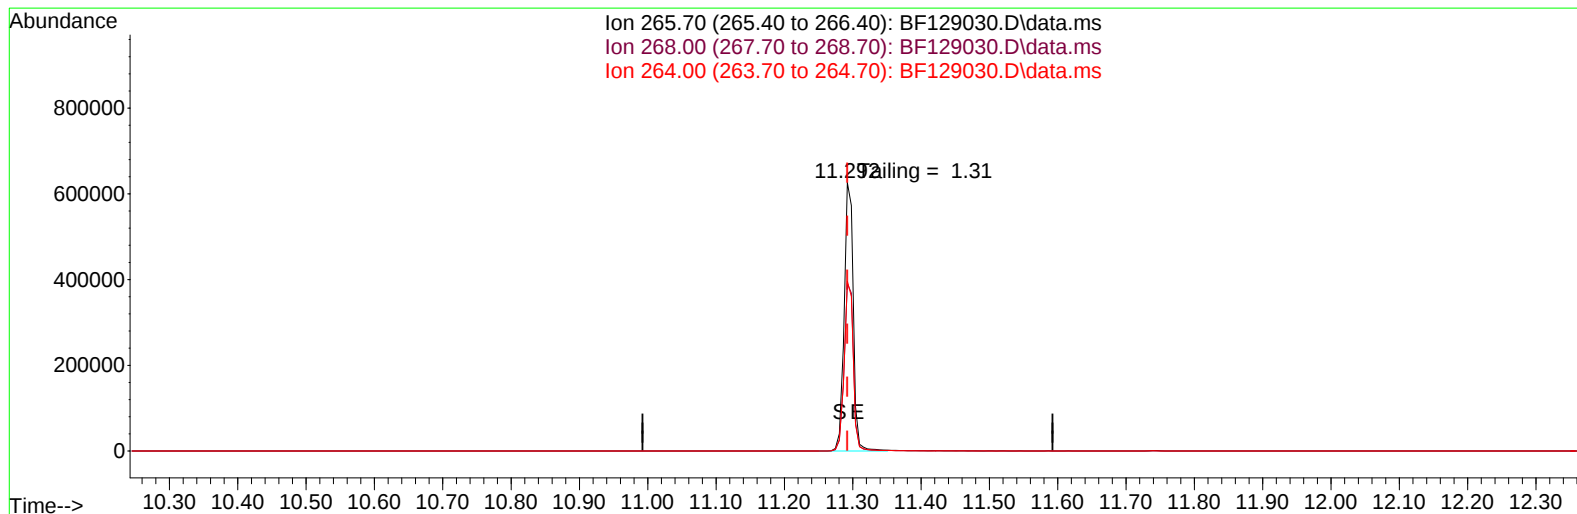

TIC: BF129030.D\data.ms

(70) Pentachlorophenol (C)




11.292min (-0.000) 262318.47 ng

response 579259

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.43
264.00	61.80	63.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062922\
Data File : BF129030.D
Acq On : 29 Jun 2022 12:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 17:07:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

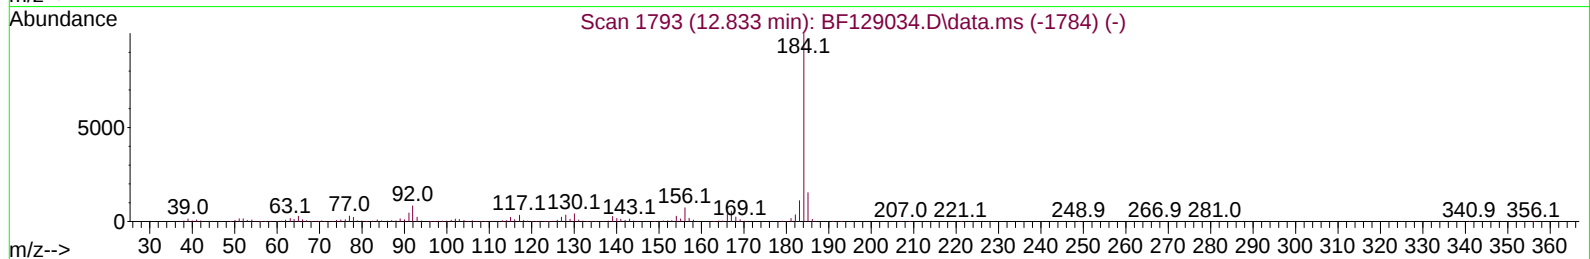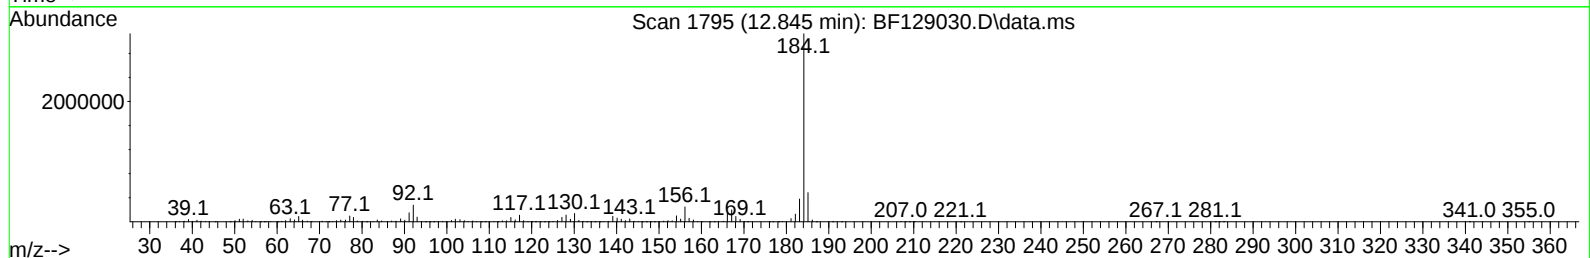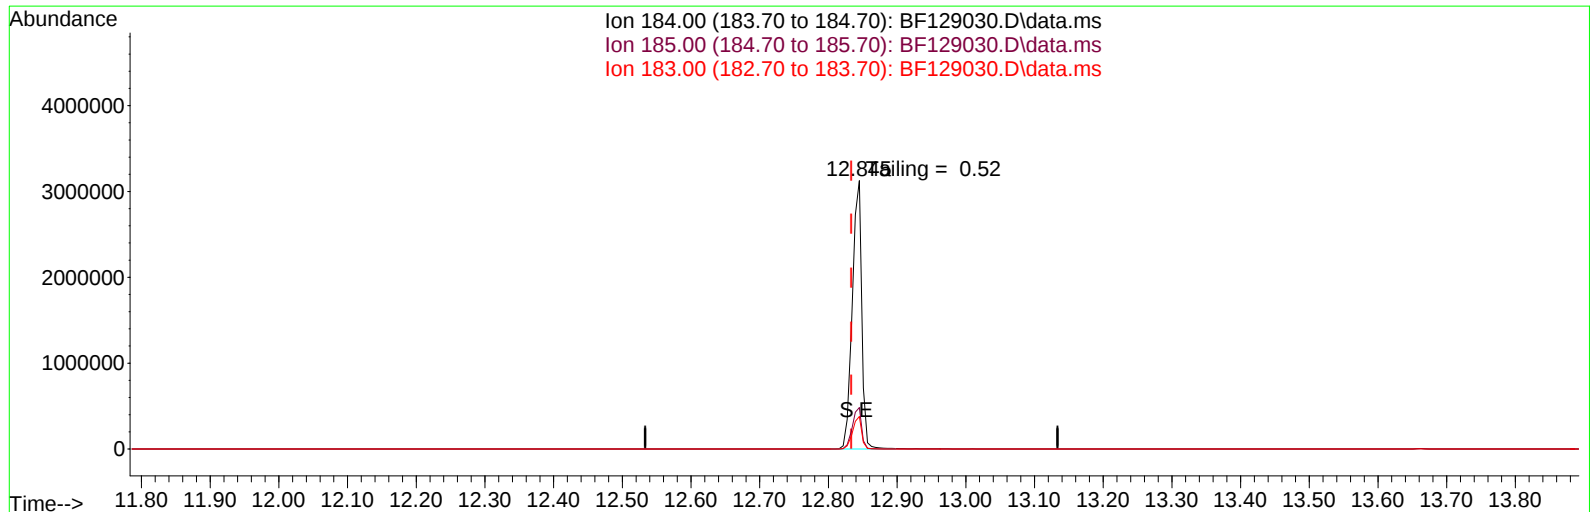

TIC: BF129030.D\data.ms

(77) Benzidine

12.845min (+ 0.012) 10266.43 ng m

response 3004259

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	15.49
183.00	11.60	12.13
0.00	0.00	0.00