

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062922\
 Data File : BF129039.D
 Acq On : 29 Jun 2022 16:58
 Operator : CG\JU
 Sample : PB145630BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145630BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.593	557	562	565	rBV	7345301	7514184	52.64%	9.673%
2	6.581	724	730	733	rBV	7385748	7432164	52.07%	9.567%
3	6.957	790	794	797	rBV	2991922	2361381	16.54%	3.040%
4	7.522	884	890	893	rBV	6718270	7058593	49.45%	9.086%
5	8.240	1007	1012	1016	rBV	3786969	3357029	23.52%	4.321%
6	9.316	1189	1195	1198	rBV	12060081	13146719	92.10%	16.923%
7	9.998	1305	1311	1315	rBV	4228643	3862802	27.06%	4.972%
8	10.792	1439	1446	1449	rBV	6919573	6090621	42.67%	7.840%
9	11.492	1559	1565	1568	rBV	4858676	4048302	28.36%	5.211%
10	13.086	1831	1836	1839	rBV	13567374	14274185	100.00%	18.375%
11	14.145	2012	2016	2019	rBV	4332200	3742161	26.22%	4.817%
12	14.239	2027	2032	2038	rBV	326022	374275	2.62%	0.482%
13	15.280	2206	2209	2214	rVB	170475	176907	1.24%	0.228%
14	15.674	2270	2276	2288	rBV	2696208	3707909	25.98%	4.773%
15	16.145	2352	2356	2364	rVB	183214	282032	1.98%	0.363%
16	16.692	2444	2449	2455	rBV	142210	254395	1.78%	0.327%




Sum of corrected areas: 77683659

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062922\
Data File : BF129039.D
Acq On : 29 Jun 2022 16:58
Operator : CG\JU
Sample : PB145630BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145630BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

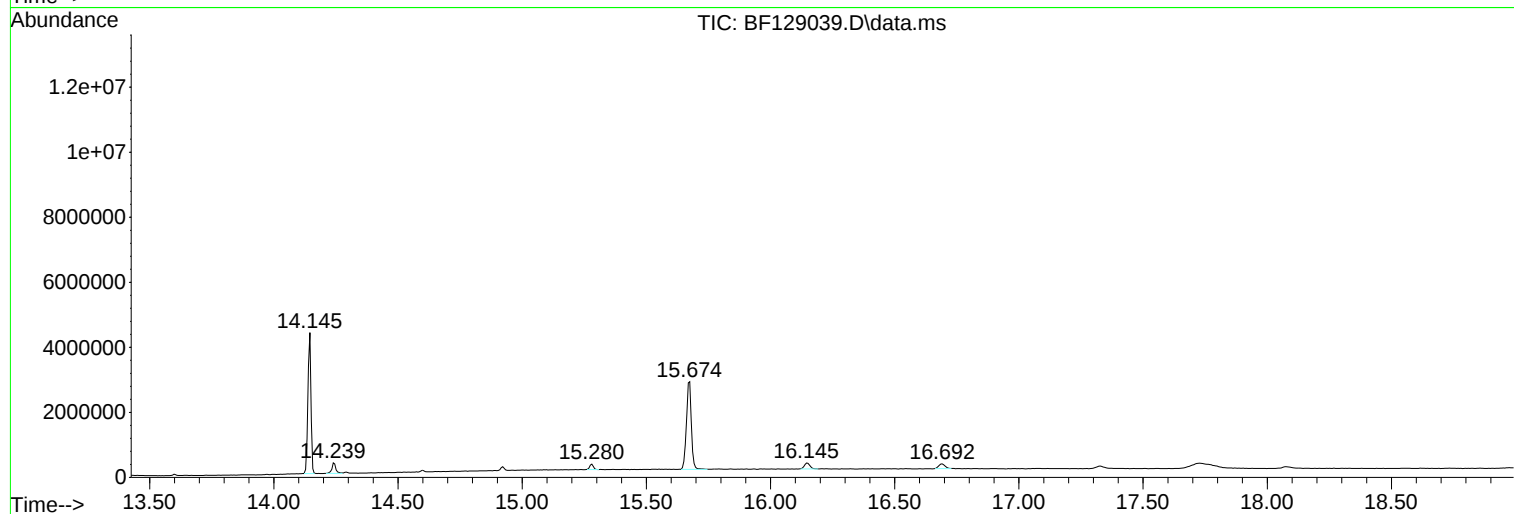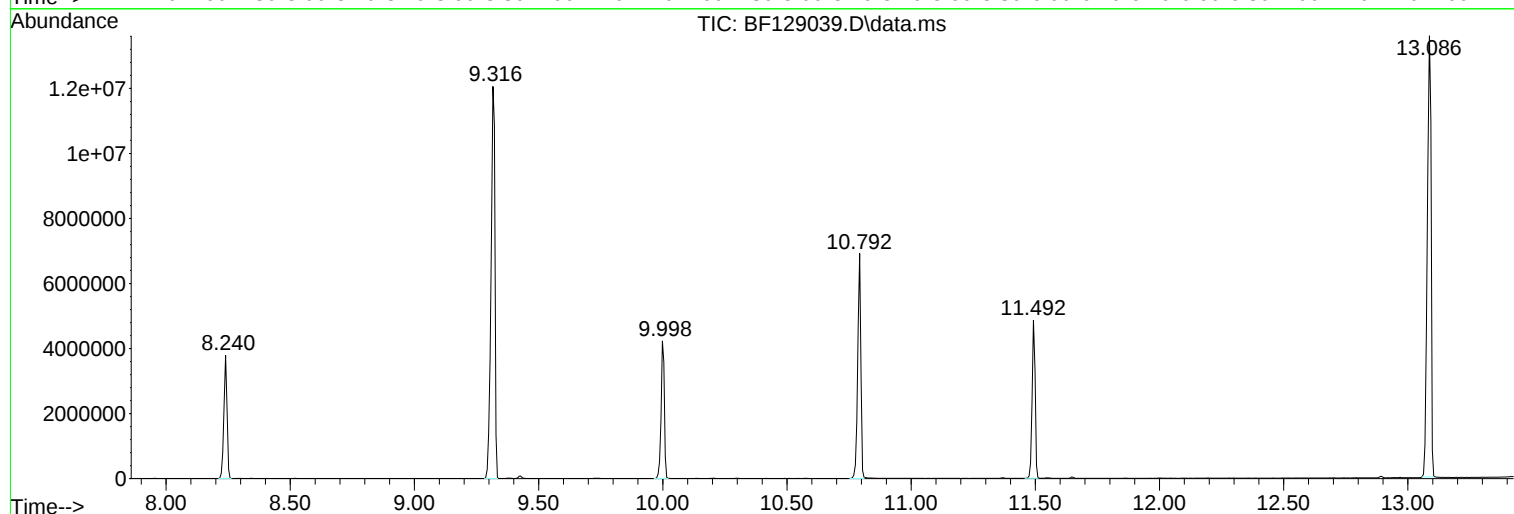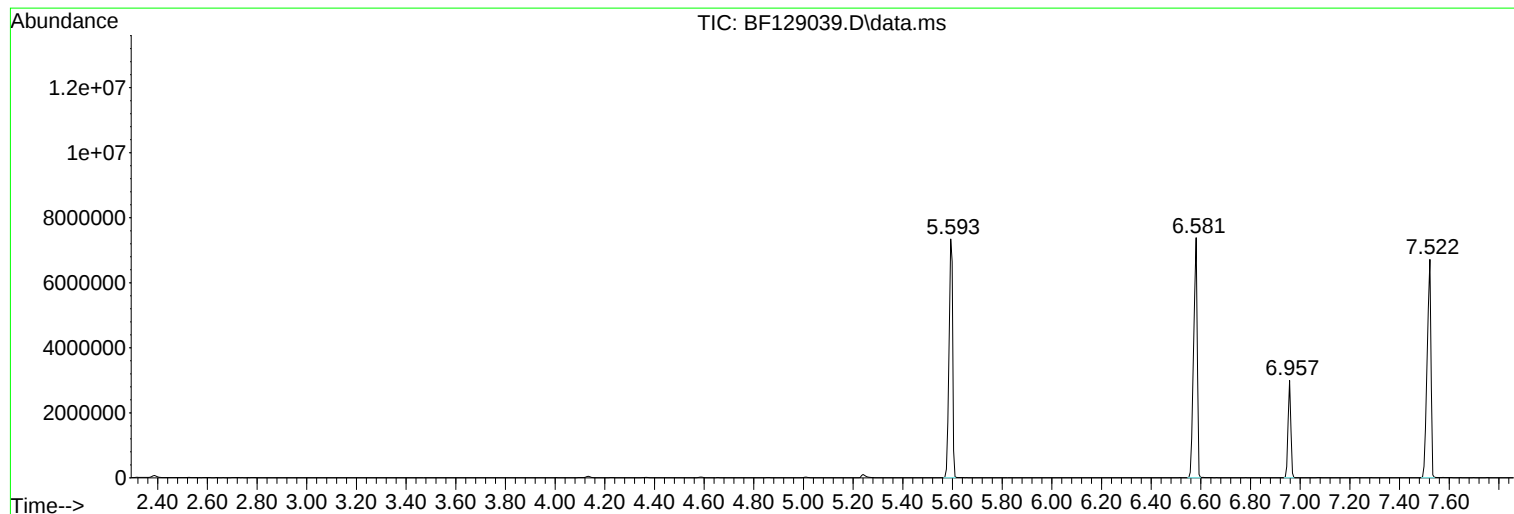

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062922\
Data File : BF129039.D
Acq On : 29 Jun 2022 16:58
Operator : CG\JU
Sample : PB145630BL
Misc :
ALS Vial : 10 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB145630BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.		
14.239	2.00 ng	374275	Chrysene-d12	14.145		
Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Triphenylphosphine oxide	278	C18H15OP	000791-28-6	93
2		(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19NO3S	1000483-83-4	91
3		Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	64
4		4-Nitro-4'-methyldiphenylsulfone	277	C13H11NO4S	004094-37-5	46
5		Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	38

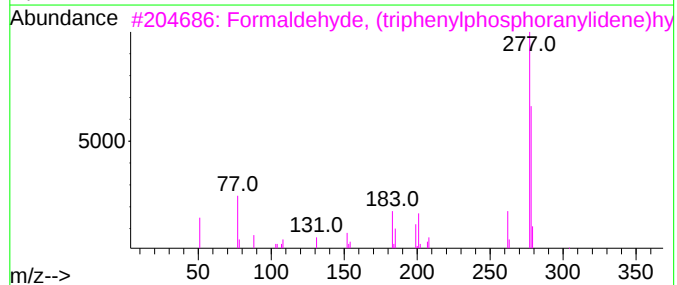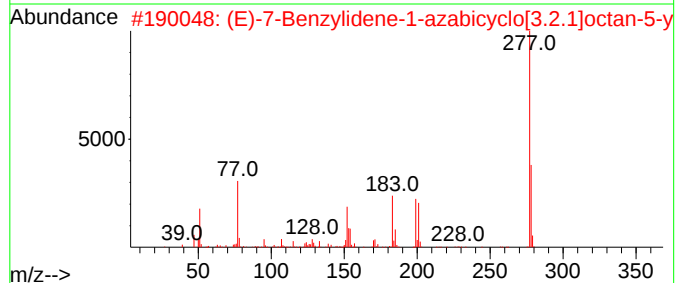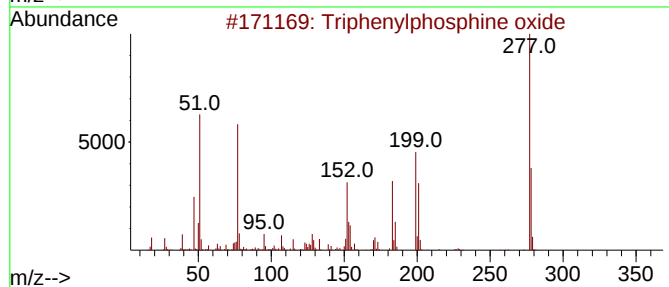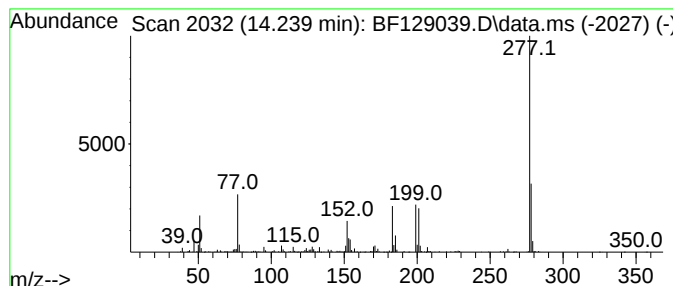

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062922\
Data File : BF129039.D
Acq On : 29 Jun 2022 16:58
Operator : CG\JU
Sample : PB145630BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145630BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.239	2.0	ng	374275	5	14.145	3742160	20.0