
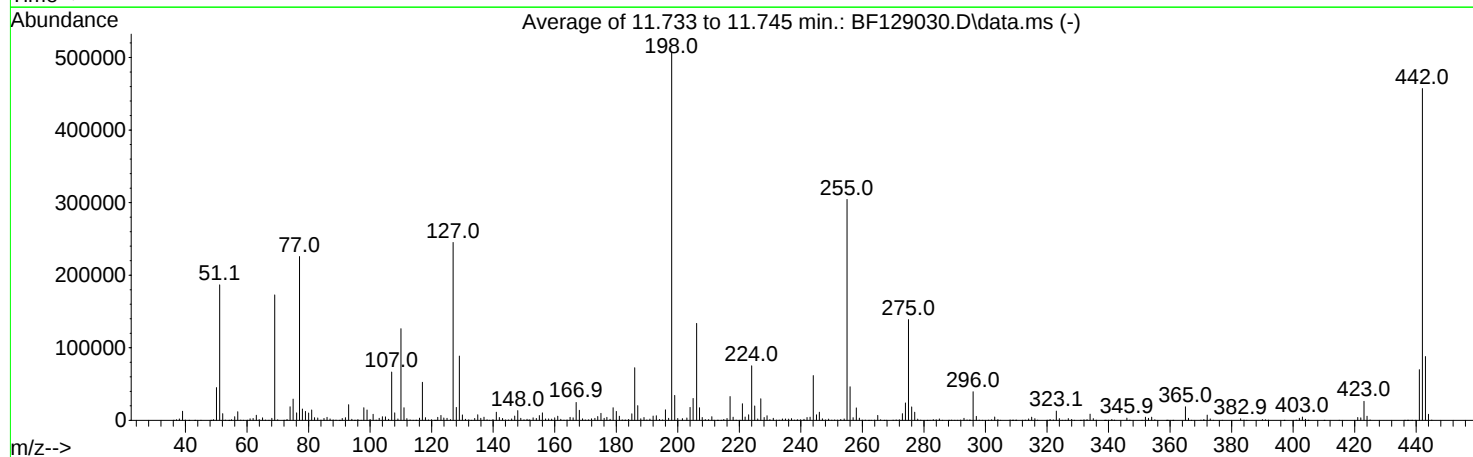


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062922\
 Data File : BF129030.D
 Acq On : 29 Jun 2022 12:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 29 17:05:31 2022

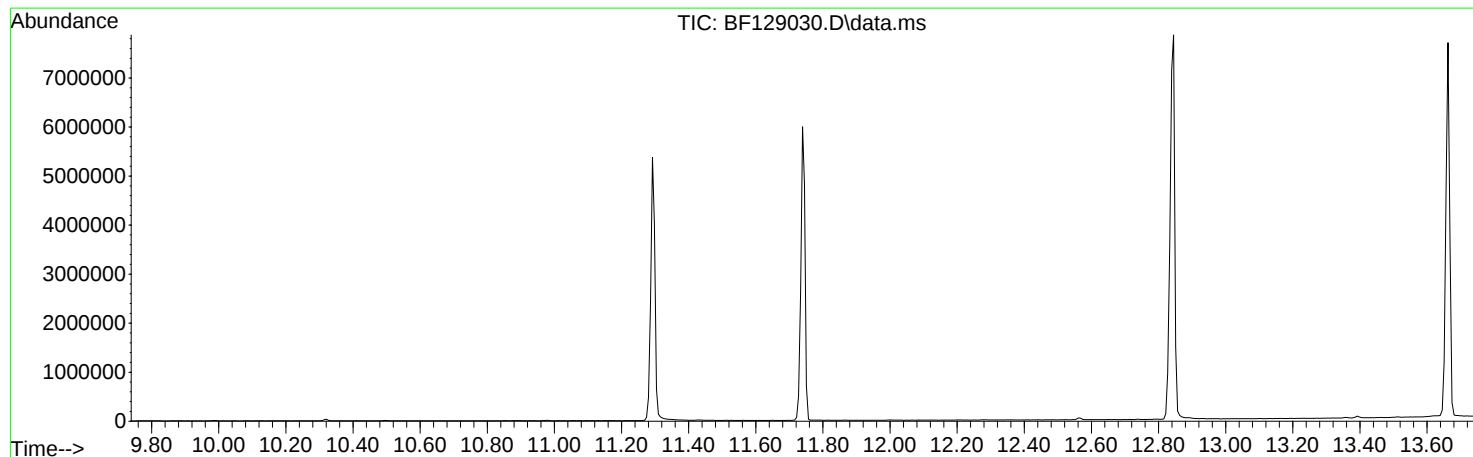

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	186816	PASS
68	69	0.00	2	1.7	2959	PASS
69	198	0.00	100	34.1	172783	PASS
70	69	0.00	2	0.6	953	PASS
127	198	10	80	48.4	245141	PASS
197	198	0.00	2	0.6	2798	PASS
198	198	100	100	100.0	506880	PASS
199	198	5	9	6.8	34483	PASS
275	198	10	60	27.4	138973	PASS
365	198	1	100	3.7	18749	PASS
441	198	0.01	100	13.8	70003	PASS
442	442	50	100	100.0	457237	PASS
443	442	15	24	19.2	87904	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/29/2022	BNA_F	<u>BF129030.D</u>
Compound Name	Response	Retention Time
DDT	1140576	13.66
DDD	2083	13.35
DDE	0	12.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2083	1142659	0.18

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062922\
Data File : BF129030.D
Acq On : 29 Jun 2022 12:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 29 17:07:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

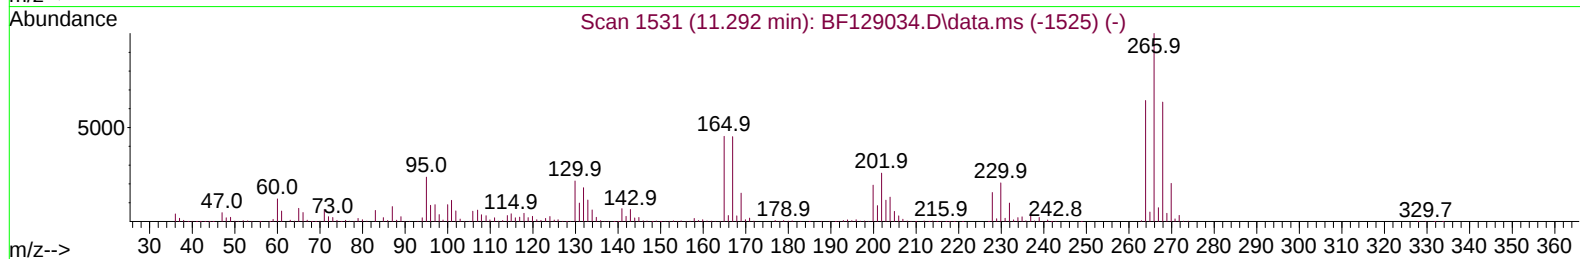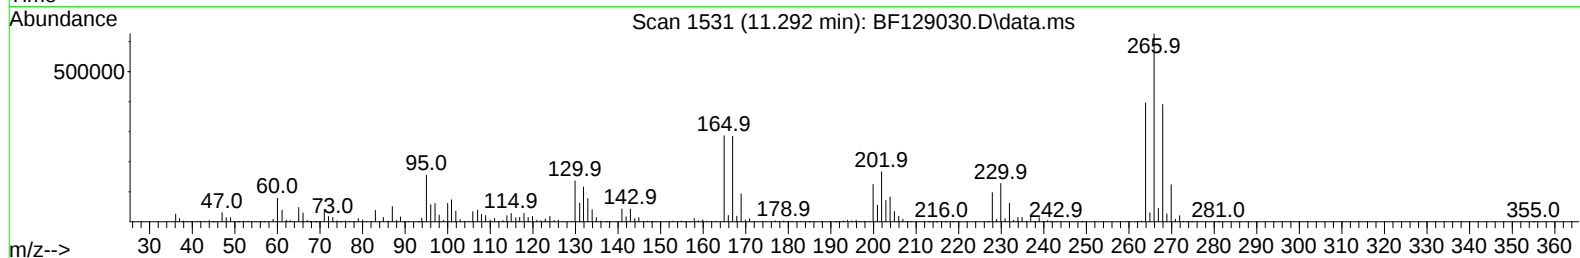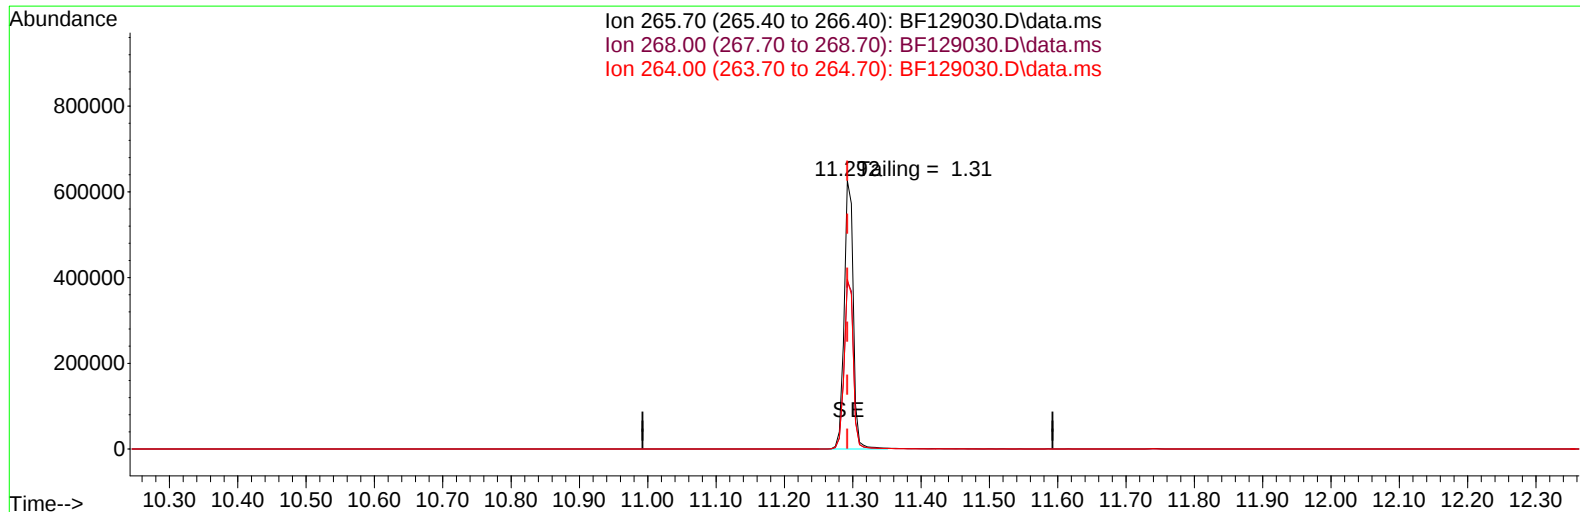

TIC: BF129030.D\data.ms

(70) Pentachlorophenol (C)

11.292min (-0.000) 262318.47 ng




response 579259

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.43
264.00	61.80	63.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062922\
Data File : BF129030.D
Acq On : 29 Jun 2022 12:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 29 17:07:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

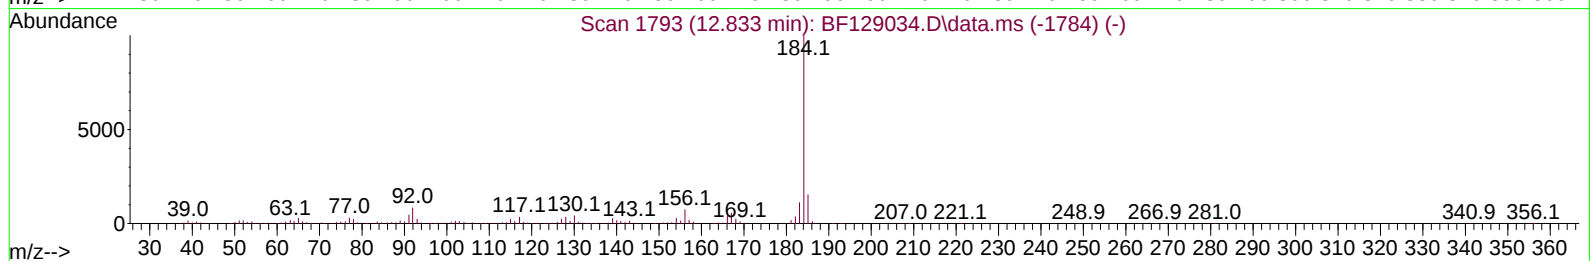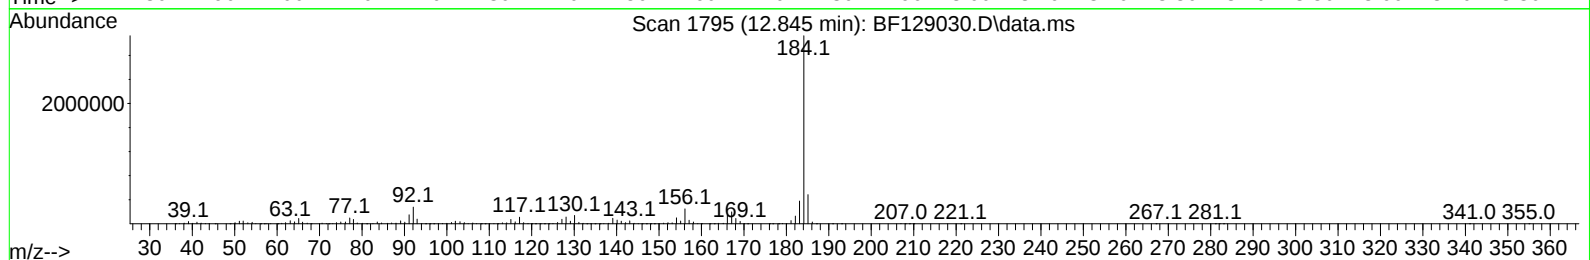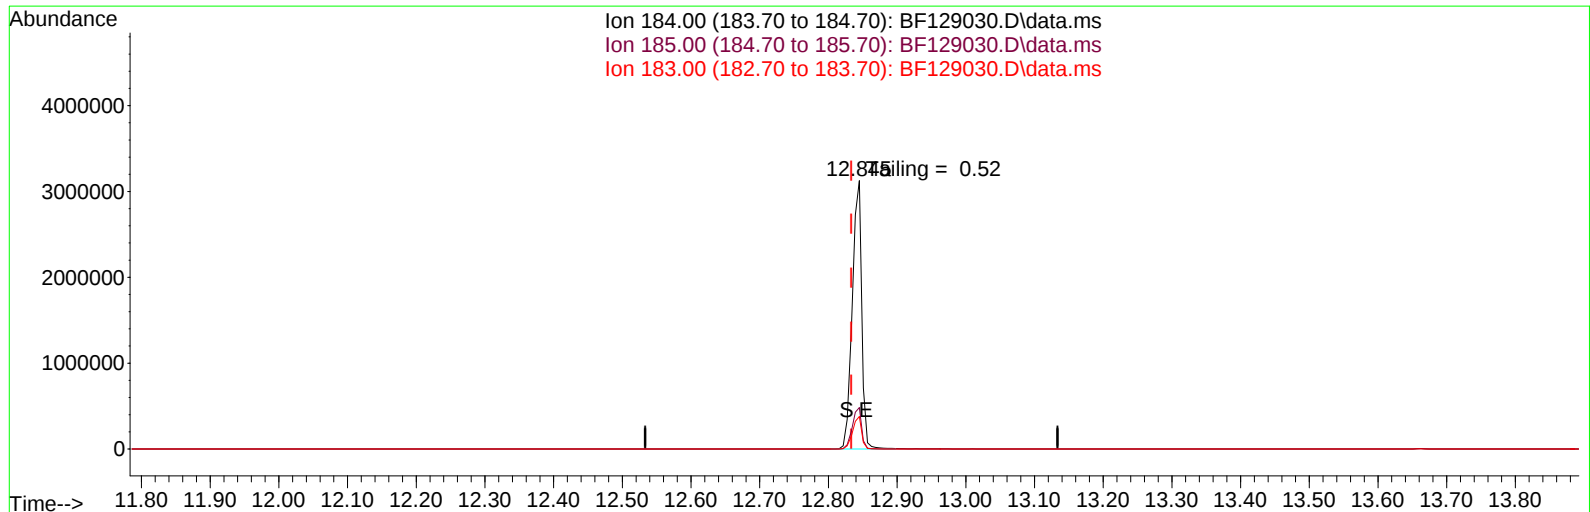

TIC: BF129030.D\data.ms

(77) Benzidine

12.845min (+ 0.012) 10266.43 ng m

response 3004259

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	15.49
183.00	11.60	12.13
0.00	0.00	0.00