

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063015\
 Data File : BF080234.D
 Acq On : 30 Jun 2015 14:13
 Operator : TP/IZ
 Sample : PB84280BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB84280BL

Quant Time: Jul 01 01:15:04 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 23 00:53:56 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.28	152	32249	20.00	ng	-0.05
21) Naphthalene-d8	8.57	136	126795	20.00	ng	-0.05
38) Acenaphthene-d10	10.34	164	65153	20.00	ng	-0.05
63) Phenanthrene-d10	11.88	188	134707	20.00	ng	-0.03
75) Chrysene-d12	15.01	240	144755	20.00	ng	0.01
86) Perylene-d12	16.99	264	141243	20.00	ng	0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.90	112	213467	117.17	ng	-0.03
7) Phenol-d6	6.89	99	284144	117.21	ng	-0.03
23) Nitrobenzene-d5	7.84	82	162029	74.39	ng	-0.03
41) 2,4,6-Tribromophenol	11.14	330	70136	110.09	ng	-0.03
44) 2-Fluorobiphenyl	9.66	172	309400	67.72	ng	-0.03
78) Terphenyl-d14	13.65	244	417976	67.44	ng	-0.02
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.84	70	20052	11.91	ng	# 61
25) Isophorone	7.84	82	162057	36.97	ng	# 58
50) 2,6-Dinitrotoluene	10.34	165	8187	8.34	ng	# 37
56) 2,4-Dinitrotoluene	10.34	165	8188	6.57	ng	# 31
66) 4-Bromophenyl-phenylether	11.14	248	5308	3.71	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063015\
Data File : BF080234.D
Acq On : 30 Jun 2015 14:13
Operator : TP/IZ
Sample : PB84280BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84280BL

Quant Time: Jul 01 01:15:04 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 23 00:53:56 2015
Response via : Initial Calibration

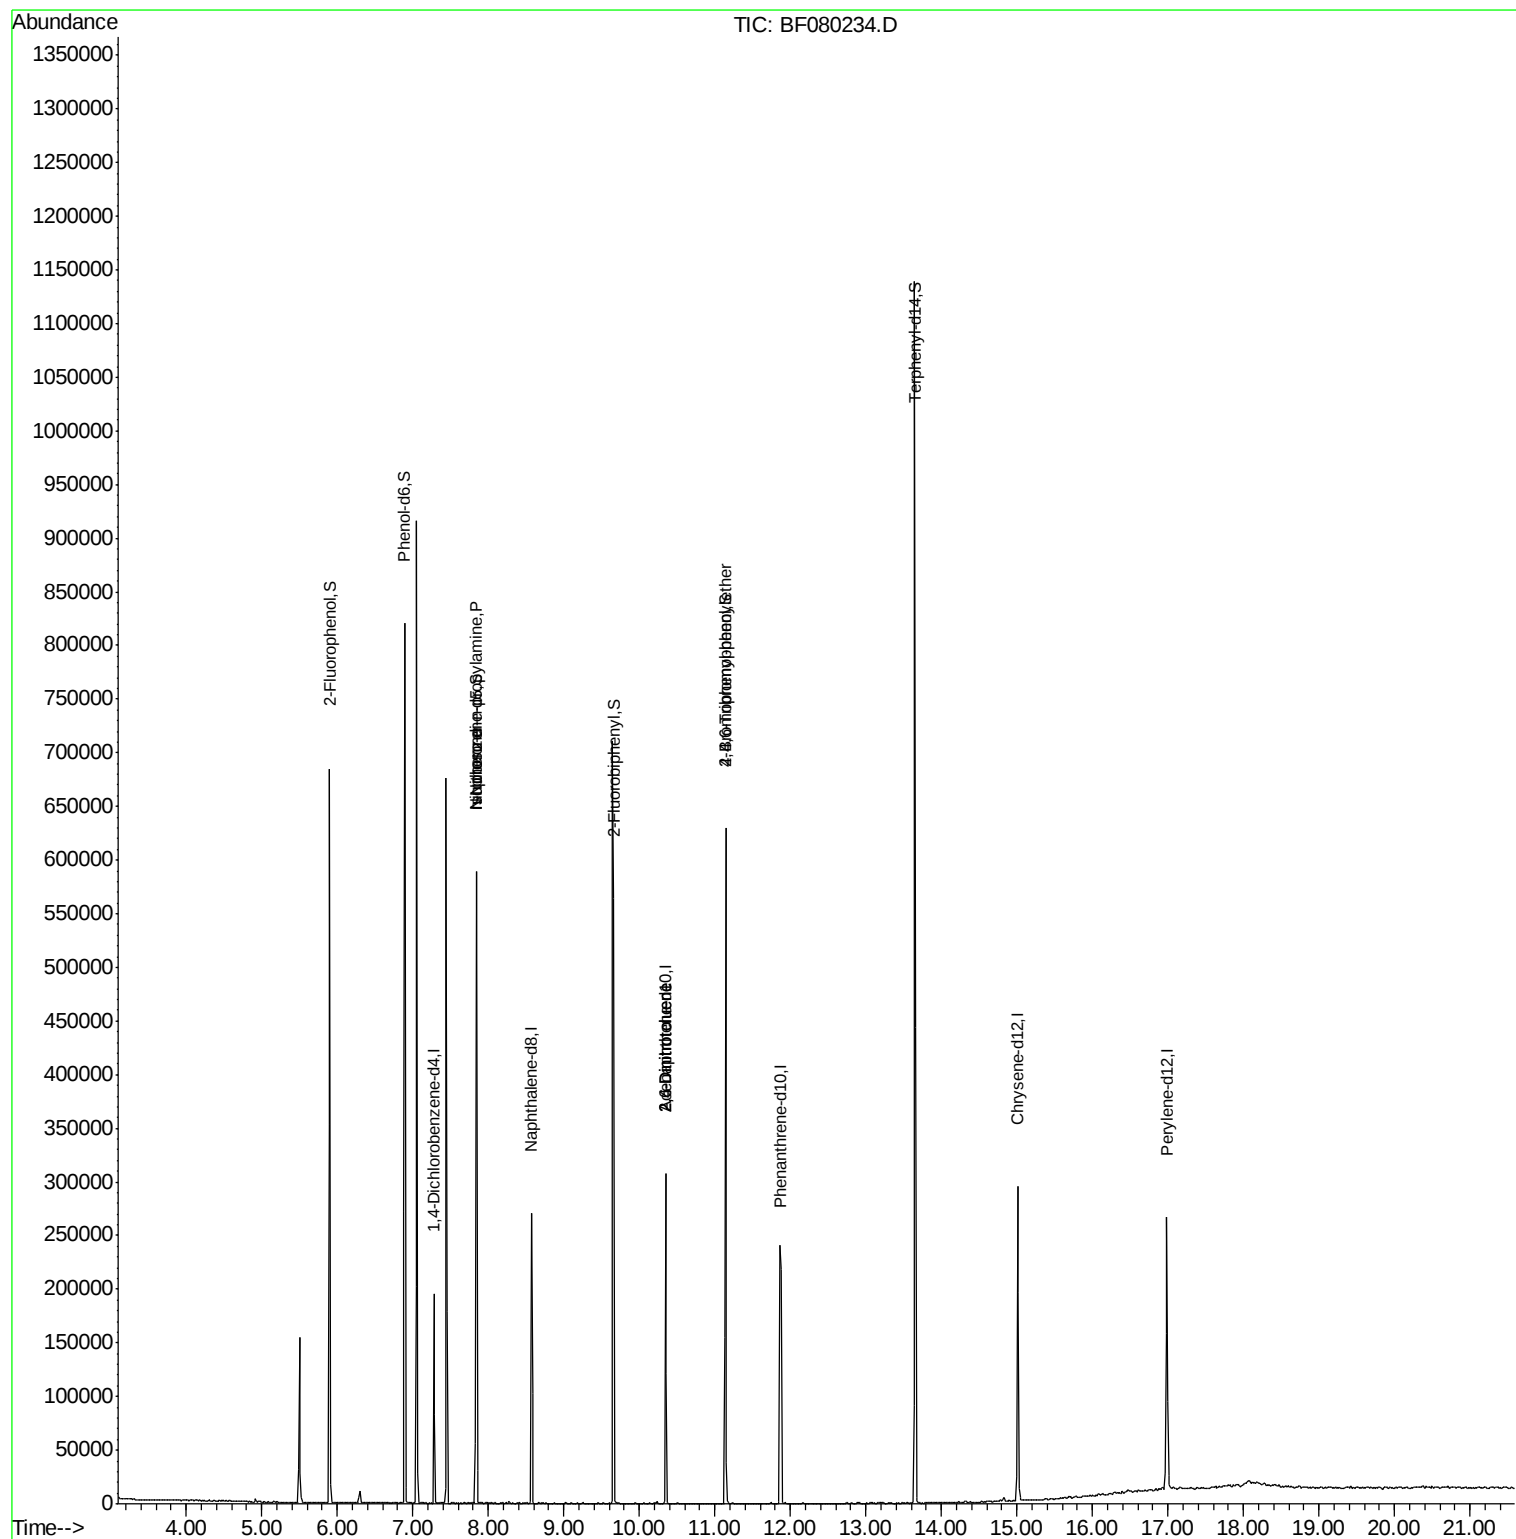







#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.28 min Scan# 367
Delta R.T. -0.05 min
Lab File: BF080234.D
Acq: 30 Jun 2015 14:13

Instrument :
BNA_F
ClientSampleId :
PB84280BL




Tgt Ion:152 Resp: 32249
Ion Ratio Lower Upper
152 100
150 159.7 124.7 187.1
115 66.6 39.0 58.4#

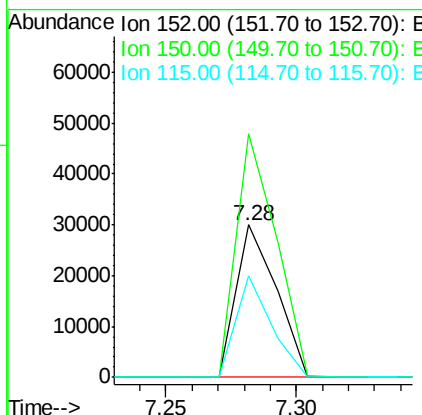


#5

2-Fluorophenol
Concen: 117.17 ng
RT: 5.90 min Scan# 246
Delta R.T. -0.03 min
Lab File: BF080234.D
Acq: 30 Jun 2015 14:13

Tgt Ion:112 Resp: 213467
Ion Ratio Lower Upper
112 100
64 52.2 39.7 59.5
63 26.2 17.4 26.0#

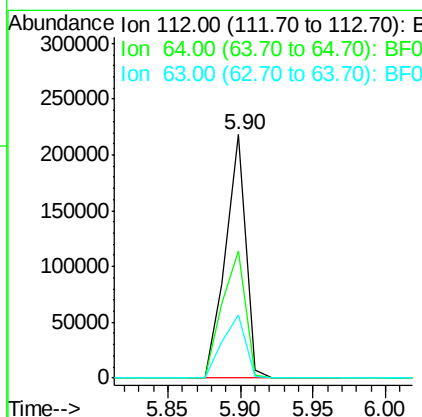

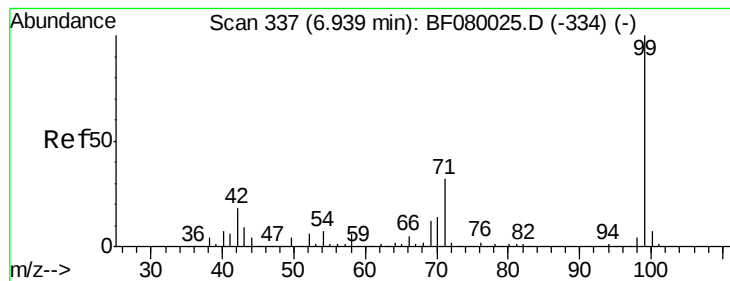

#7

Phenol-d6

Concen: 117.21 ng

RT: 6.89 min Scan# 333

Delta R.T. -0.03 min

Lab File: BF080234.D

Acq: 30 Jun 2015 14:13

Instrument :

BNA_F

ClientSampleId :

PB84280BL


Tgt Ion: 99 Resp: 284144

Ion Ratio Lower Upper

99 100

42 15.5 13.7 20.5




71 29.5 14.2 21.2#

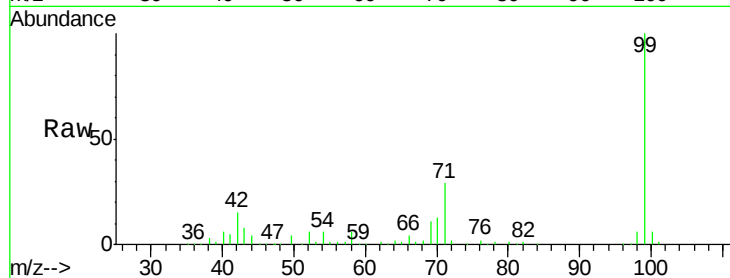

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

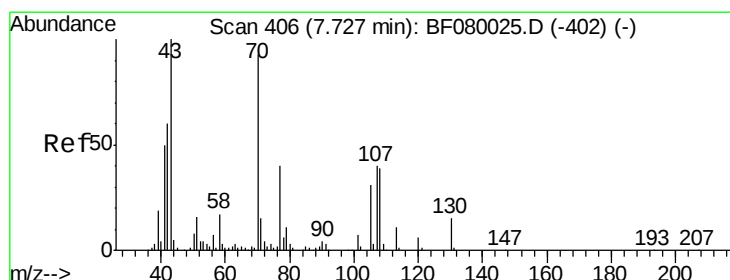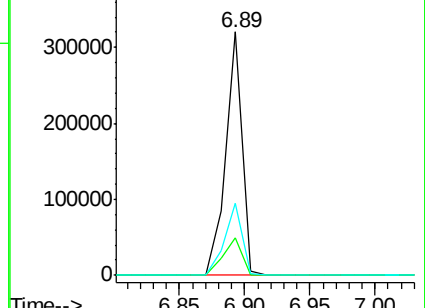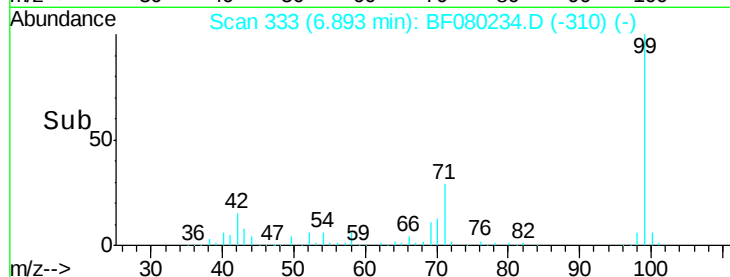

#19

n-Nitroso-di-n-propylamine

Concen: 11.91 ng

RT: 7.84 min Scan# 416

Delta R.T. 0.13 min

Lab File: BF080234.D

Acq: 30 Jun 2015 14:13

Tgt Ion: 70 Resp: 20052


Ion Ratio Lower Upper

70 100

42 50.6 63.8 95.6#

101 0.0 9.2 13.8#

130 1.4 27.3 40.9#


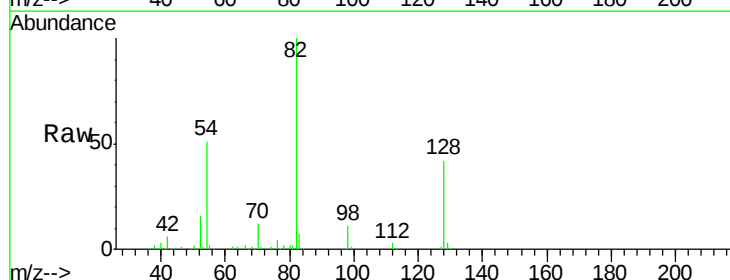



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

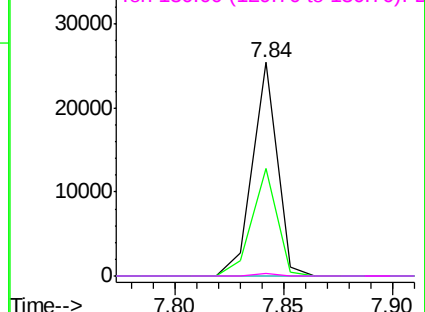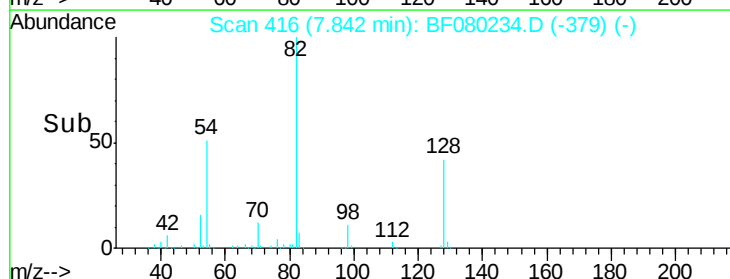


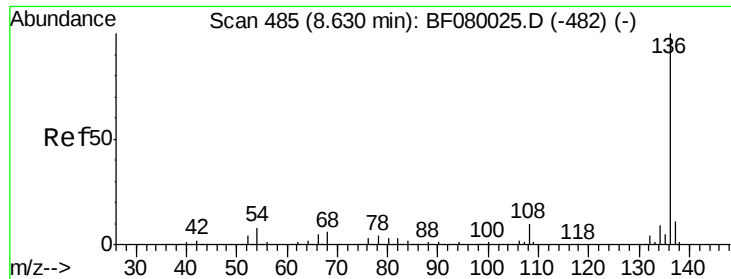




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.57 min Scan# 480
Delta R.T. -0.05 min
Lab File: BF080234.D
Acq: 30 Jun 2015 14:13

Instrument :
BNA_F
ClientSampleId :
PB84280BL

Tgt Ion:	136	Resp:	126795
Ion	Ratio	Lower	Upper
136	100		
137	11.4	9.0	13.6
54	10.9	8.2	12.2
68	7.8	5.8	8.6




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

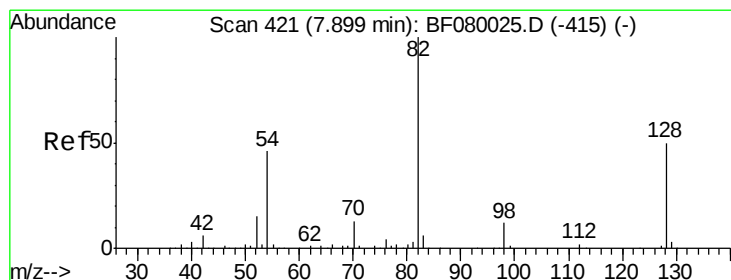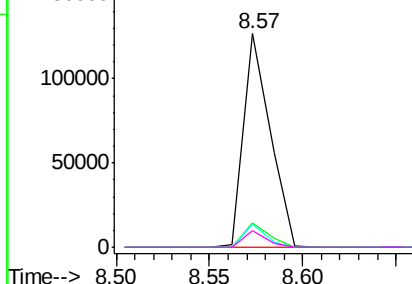




#23
Nitrobenzene-d5
Concen: 74.39 ng
RT: 7.84 min Scan# 416
Delta R.T. -0.03 min
Lab File: BF080234.D
Acq: 30 Jun 2015 14:13

Tgt Ion:	82	Resp:	162029
Ion	Ratio	Lower	Upper
82	100		
128	42.2	51.0	76.6#
54	51.4	47.5	71.3



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

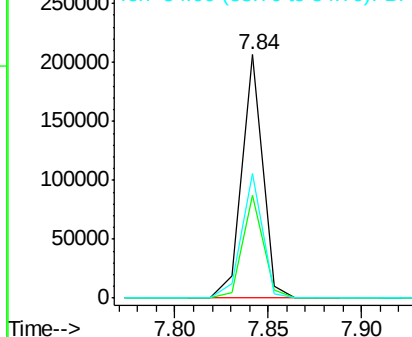

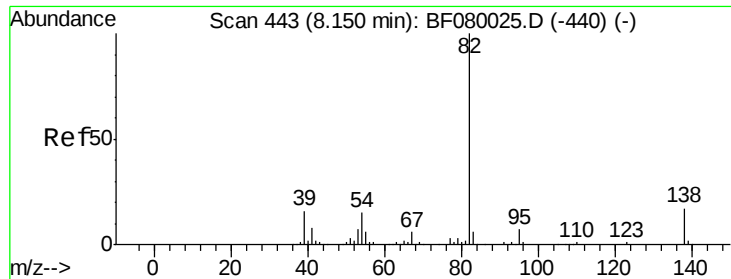

#25

Isophorone

Concen: 36.97 ng

RT: 7.84 min Scan# 416

Delta R.T. -0.30 min

Lab File: BF080234.D

Acq: 30 Jun 2015 14:13

Instrument :

BNA_F

ClientSampled :

PB84280BL


Tgt Ion: 82 Resp: 162057

Ion Ratio Lower Upper

82 100

95 0.0 4.0 6.0#




138 0.0 18.3 27.5#



Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 95.00 (94.70 to 95.70): BF0

Ion 138.00 (137.70 to 138.70): E

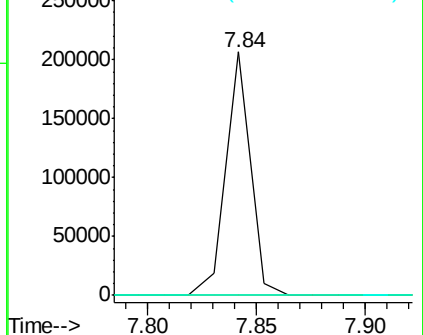

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 10.34 min Scan# 635

Delta R.T. -0.05 min

Lab File: BF080234.D

Acq: 30 Jun 2015 14:13


Tgt Ion: 164 Resp: 65153

Ion Ratio Lower Upper

164 100

162 100.8 75.2 112.8



160 44.7 31.5 47.3




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E




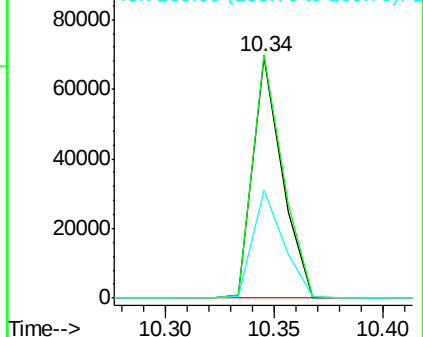




#41
 2,4,6-Tribromophenol
 Concen: 110.09 ng
 RT: 11.14 min Scan# 705
 Delta R.T. -0.03 min
 Lab File: BF080234.D
 Acq: 30 Jun 2015 14:13




Instrument :
 BNA_F
 ClientSampleId :
 PB84280BL


Tgt Ion:330 Resp: 70136
 Ion Ratio Lower Upper
 330 100
 332 94.6 76.6 114.8
 141 35.3 29.7 44.5

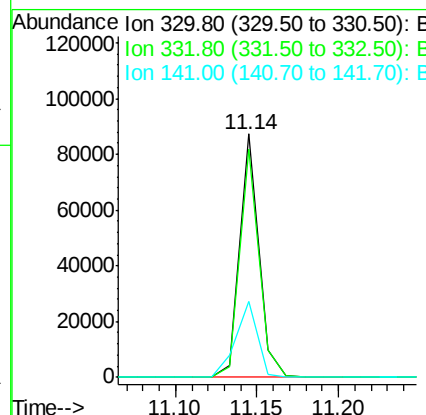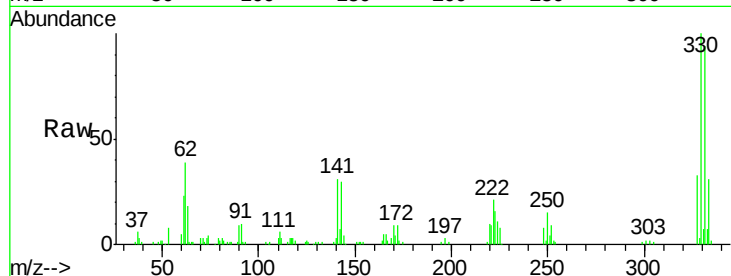

#44
 2-Fluorobiphenyl
 Concen: 67.72 ng
 RT: 9.66 min Scan# 575
 Delta R.T. -0.03 min
 Lab File: BF080234.D
 Acq: 30 Jun 2015 14:13

Tgt Ion:172 Resp: 309400
 Ion Ratio Lower Upper
 172 100
 171 35.0 26.1 39.1
 170 23.9 17.4 26.2

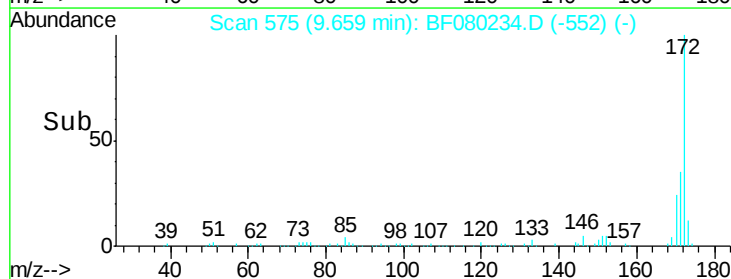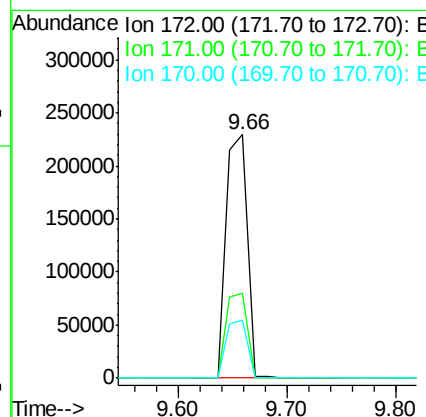


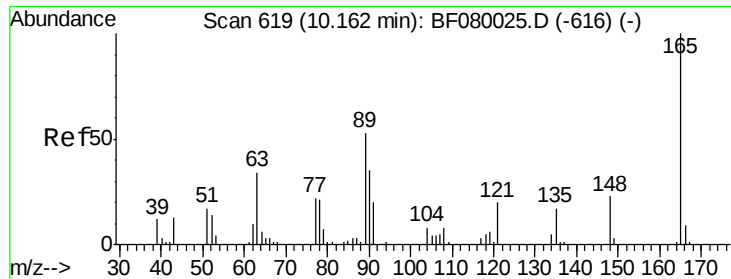

#50
 2,6-Dinitrotoluene
 Concen: 8.34 ng
 RT: 10.34 min Scan# 635
 Delta R.T. 0.19 min
 Lab File: BF080234.D
 Acq: 30 Jun 2015 14:13

Instrument :
 BNA_F
 ClientSampleId :
 PB84280BL




Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	32.3	48.5#
89	0.0	28.6	43.0#

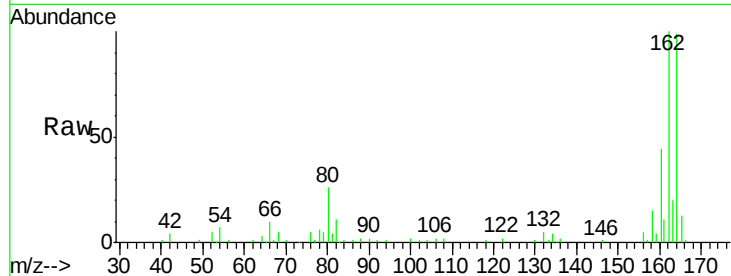

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

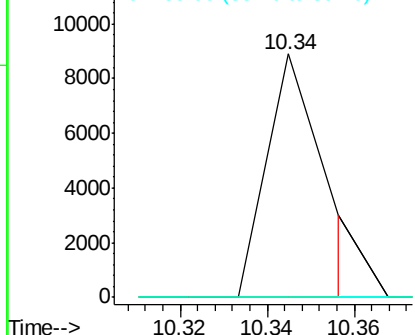

#56
 2,4-Dinitrotoluene
 Concen: 6.57 ng
 RT: 10.34 min Scan# 635
 Delta R.T. -0.21 min
 Lab File: BF080234.D
 Acq: 30 Jun 2015 14:13




Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	29.8	44.6#
89	0.0	44.5	66.7#
182	0.0	3.0	4.4#


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

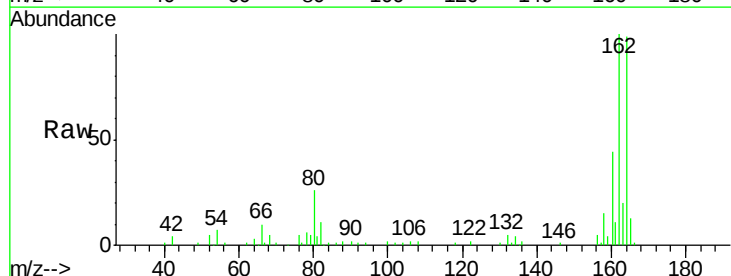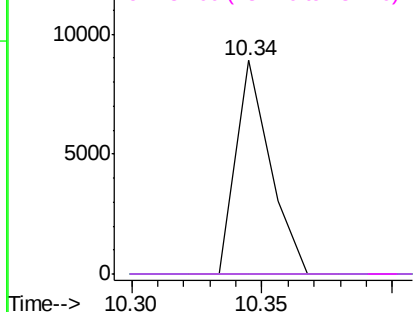


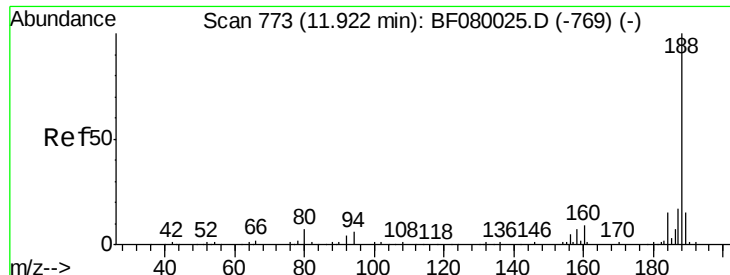




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.88 min Scan# 769
 Delta R.T. -0.03 min
 Lab File: BF080234.D
 Acq: 30 Jun 2015 14:13

Instrument :
 BNA_F
 ClientSampleId :
 PB84280BL

Tgt Ion:188 Resp: 134707
 Ion Ratio Lower Upper
 188 100
 94 5.6 11.1 16.7#
 80 5.9 11.0 16.4#

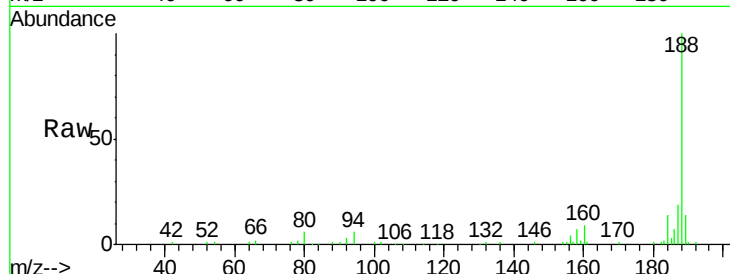


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

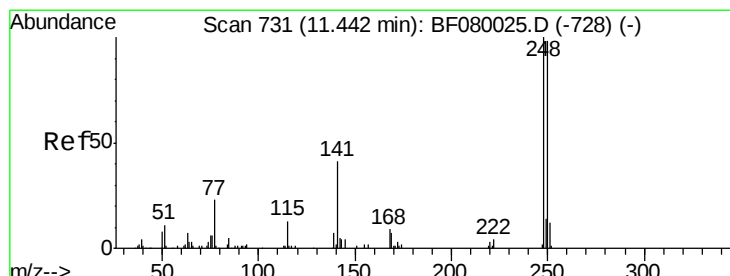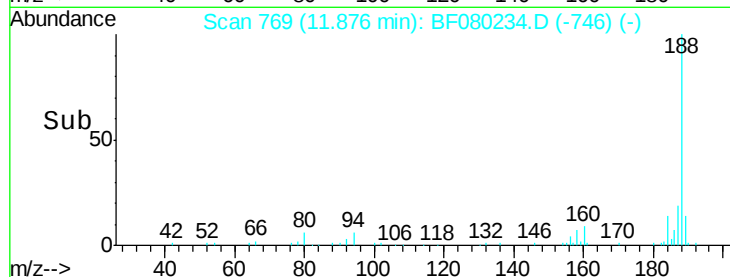
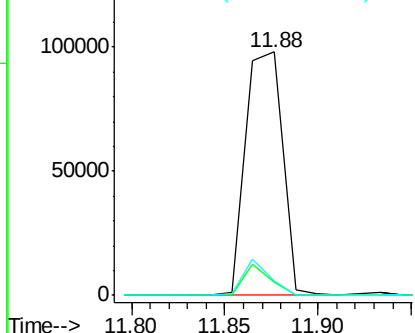



#66
 4-Bromophenyl-phenylether
 Concen: 3.71 ng
 RT: 11.14 min Scan# 705
 Delta R.T. -0.27 min
 Lab File: BF080234.D
 Acq: 30 Jun 2015 14:13

Tgt Ion:248 Resp: 5308
 Ion Ratio Lower Upper
 248 100
 250 197.2 78.5 117.7#
 141 413.2 59.0 88.6#

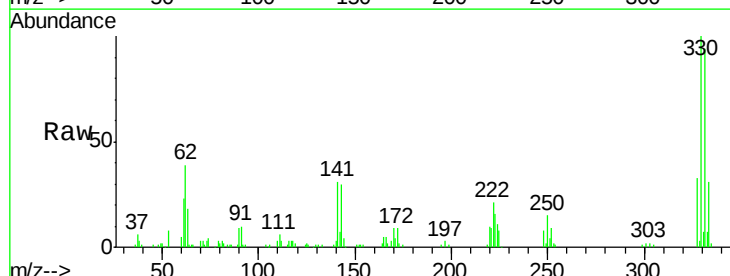

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

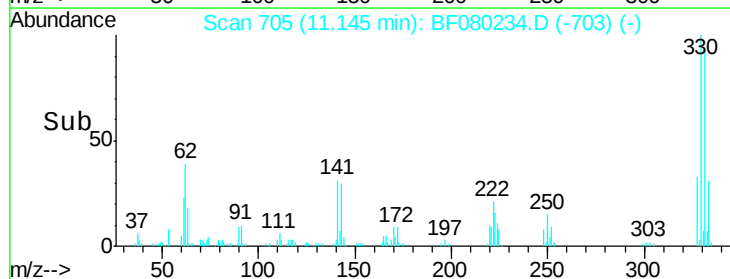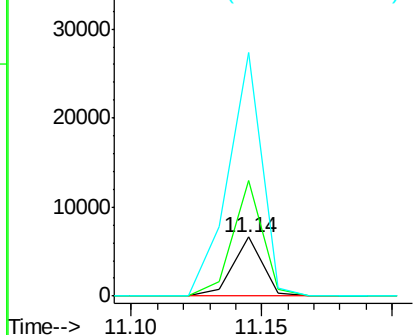

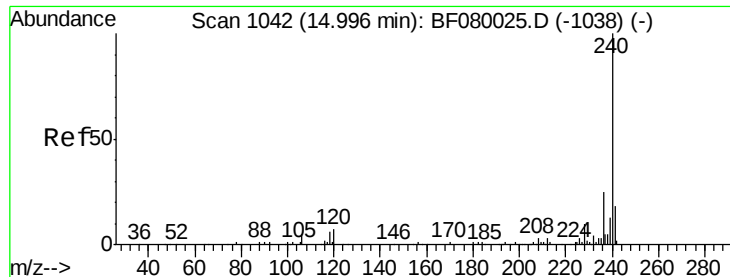

#75

Chrysene-d12

Concen: 20.00 ng

RT: 15.01 min Scan# 1043

Delta R.T. 0.01 min

Lab File: BF080234.D

Acq: 30 Jun 2015 14:13

Instrument :

BNA_F

ClientSampleId :

PB84280BL


Tgt Ion:240 Resp: 144755

Ion Ratio Lower Upper

240 100

120 13.4 16.2 24.2#




236 26.1 18.4 27.6

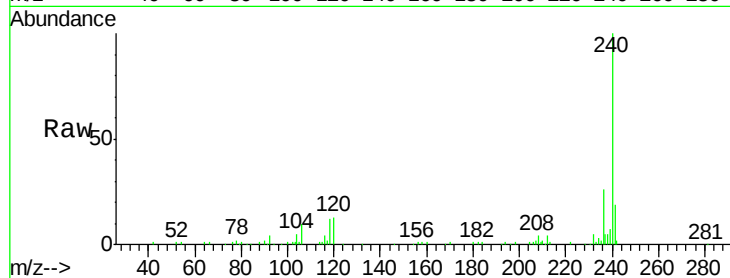

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

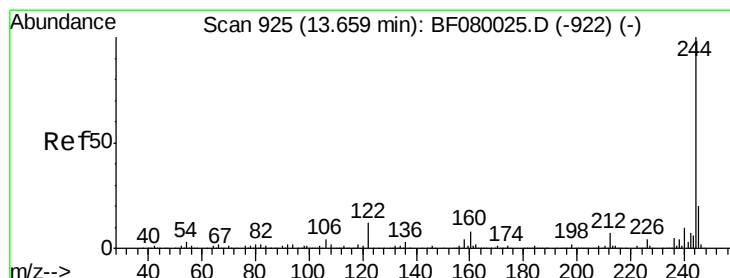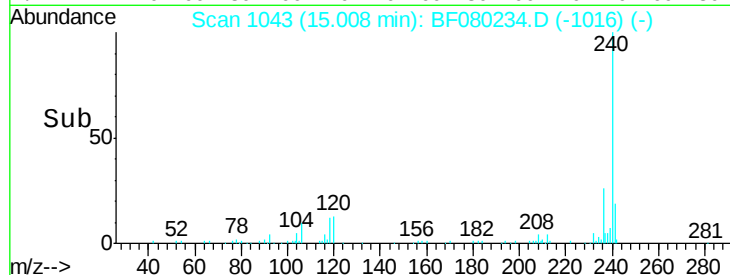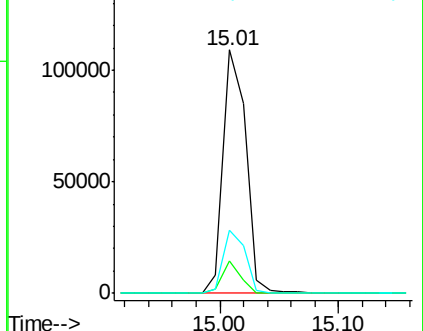

#78

Terphenyl-d14

Concen: 67.44 ng

RT: 13.65 min Scan# 924

Delta R.T. -0.02 min

Lab File: BF080234.D

Acq: 30 Jun 2015 14:13


Tgt Ion:244 Resp: 417976

Ion Ratio Lower Upper

244 100

212 7.3 4.3 6.5#



122 13.4 17.4 26.2#

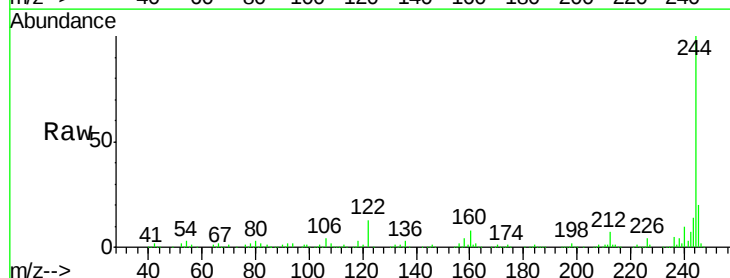


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

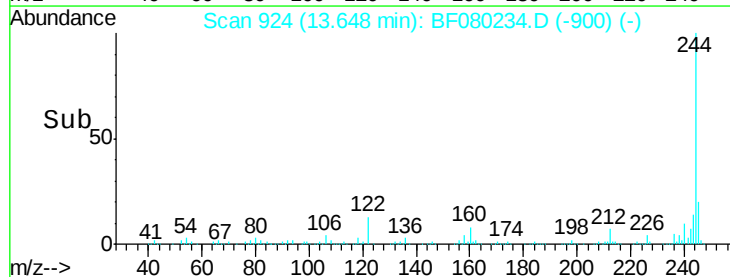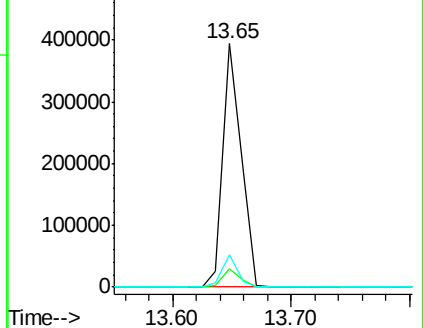


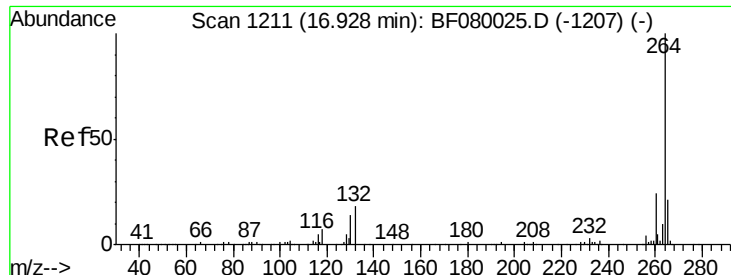

#86
Perylene-d12
Concen: 20.00 ng
RT: 16.99 min Scan# 1216
Delta R.T. 0.06 min
Lab File: BF080234.D
Acq: 30 Jun 2015 14:13

Instrument :
BNA_F
ClientSampleId :
PB84280BL

Tgt Ion: 264 Resp: 141243
Ion Ratio Lower Upper
264 100
260 23.9 16.7 25.1
265 21.0 17.2 25.8

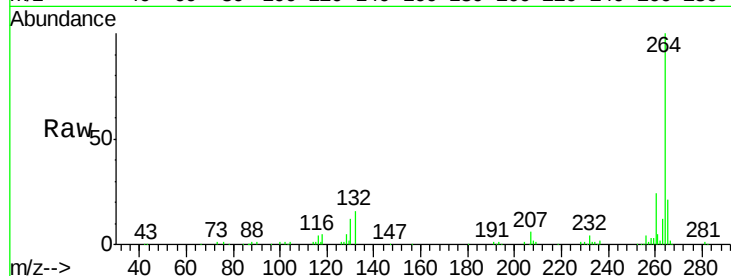

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

