
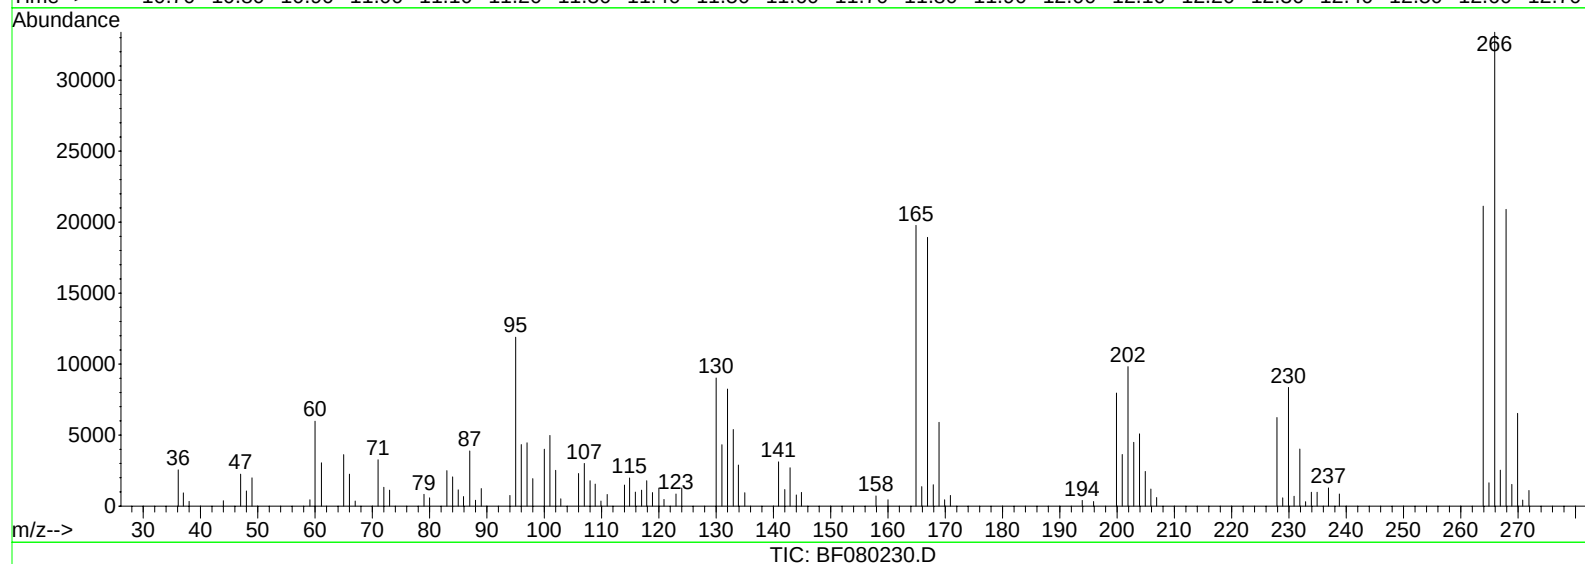


Data Path : Z:\HPCHEM1\BNA F\Data\BF063015\
Data File : BF080230.D
Acq On : 30 Jun 2015 11:00
Operator : TP/IZ
Sample : DF TPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 11:40:47 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 23 00:53:56 2015
Response via : Initial Calibration

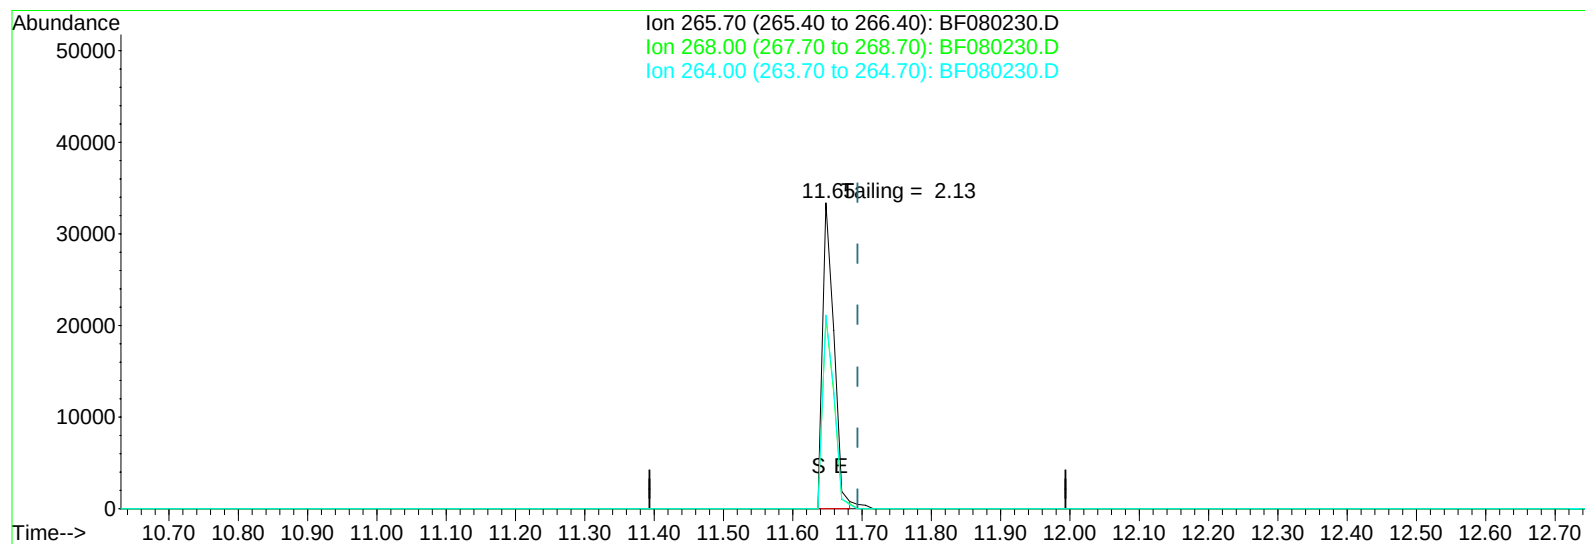

(69) Pentachlorophenol (C)



11.648min (-0.046) 0.00ng

response 38632

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.62
264.00	62.70	63.29
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF063015\
Data File : BF080230.D
Acq On : 30 Jun 2015 11:00
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 11:40:47 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 23 00:53:56 2015
Response via : Initial Calibration

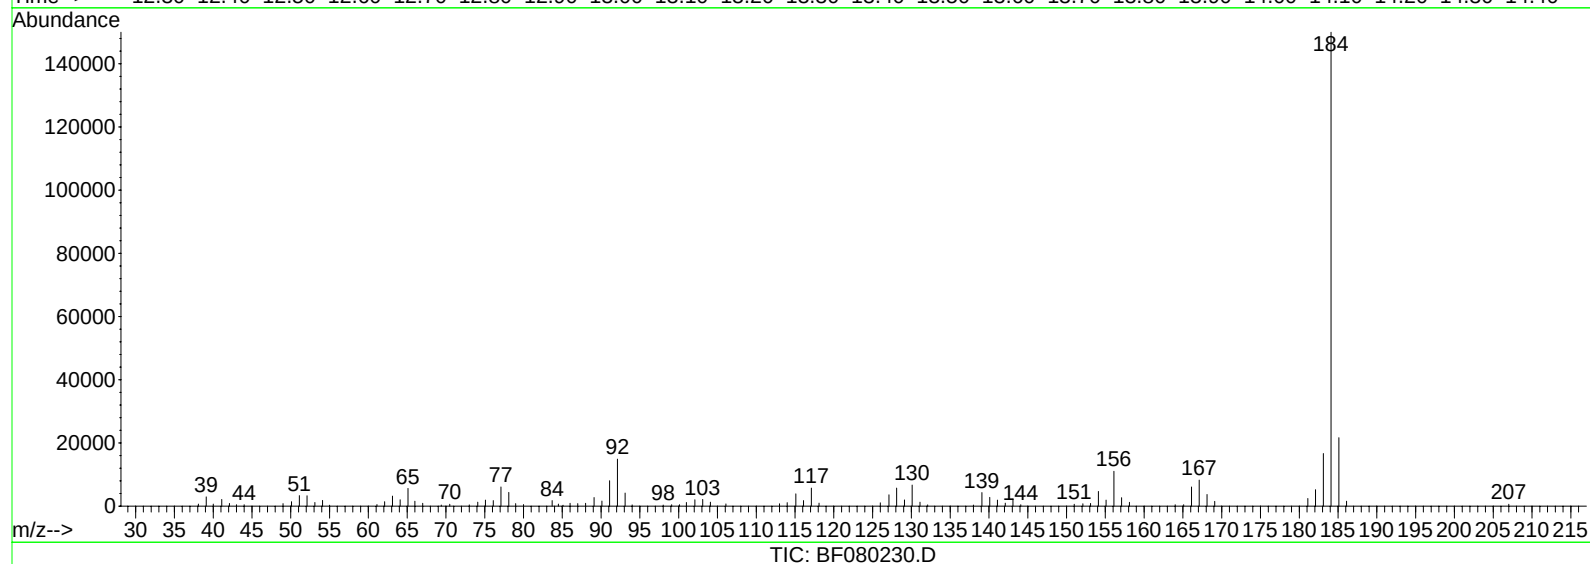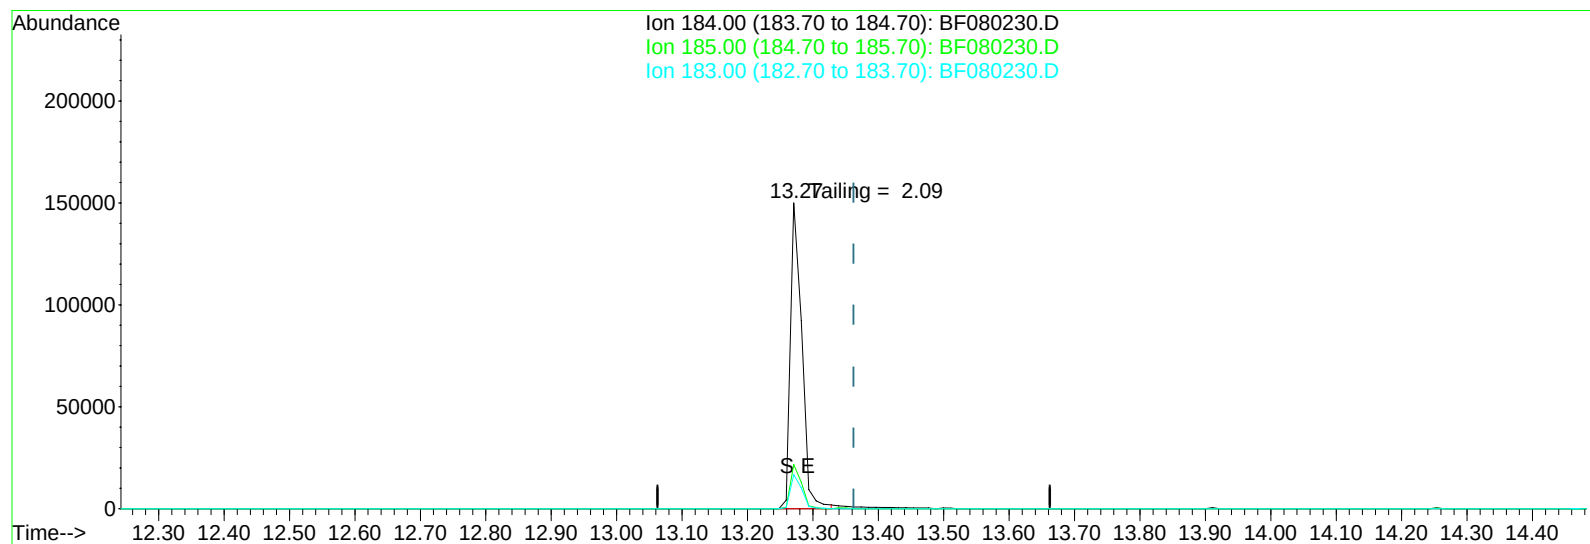

(76) Benzidine

13.271min (-0.091) 27970.18ng

response 186857

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.44
183.00	9.50	11.11
0.00	0.00	0.00